

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
 Data File : PL071856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2022 17:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:09:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.494	8983263	24575264	19.446	20.002
28)	SA Decachlor...	10.321	11.390	14561133	24123083	20.139	20.357
Target Compounds							
7)	B delta-BHC	0.000	6.973f	0	491711	N.D.	0.320 #
8)	B Heptachlo...	0.000	7.965	0	1919392	N.D.	1.374 #
9)	A Endosulfan I	0.000	8.327f	0	396543	N.D.	0.320 #
10)	B gamma-Chl...	0.000	8.251f	0	2620582	N.D.	1.916 #
11)	B alpha-Chl...	0.000	8.305	0	904384	N.D.	0.680 #
13)	MA Dieldrin	7.684	0.000	83741	0	0.139	N.D. #
15)	B Endosulfa...	0.000	9.107	0	111516	N.D.	0.099 #
16)	A 4,4'-DDD	0.000	9.028	0	51280	N.D.	0.053 #
17)	MA 4,4'-DDT	0.000	9.350	0	62594	N.D.	0.066 #
21)	B Endrin ke...	0.000	9.977	0	165994	N.D.	0.147 #
25)	Chlordane-3	0.000	8.251f	0	2620582	N.D.	12.839 #
26)	Chlordane-4	0.000	8.305	0	904384	N.D.	3.715 #
27)	Chlordane-5	0.000	9.189	0	13551	N.D.	0.338 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
Data File : PL071856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2022 17:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:09:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

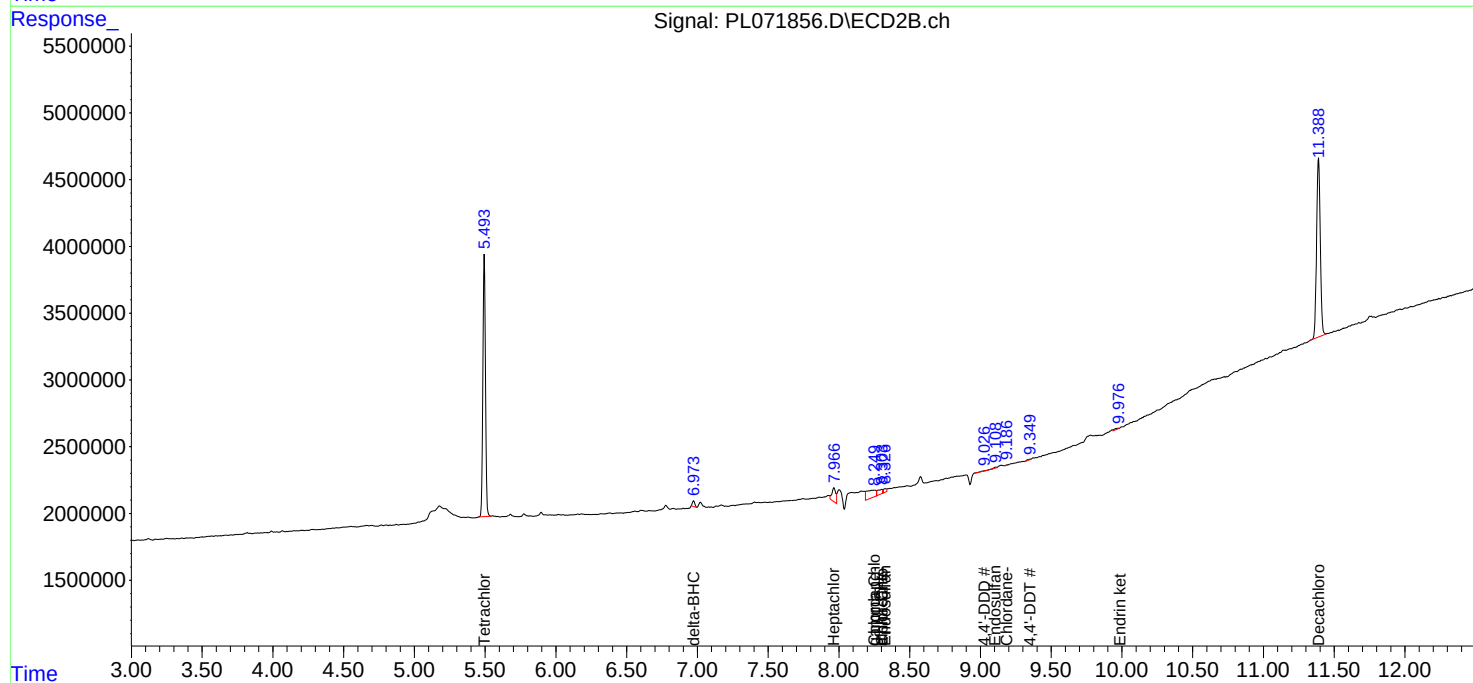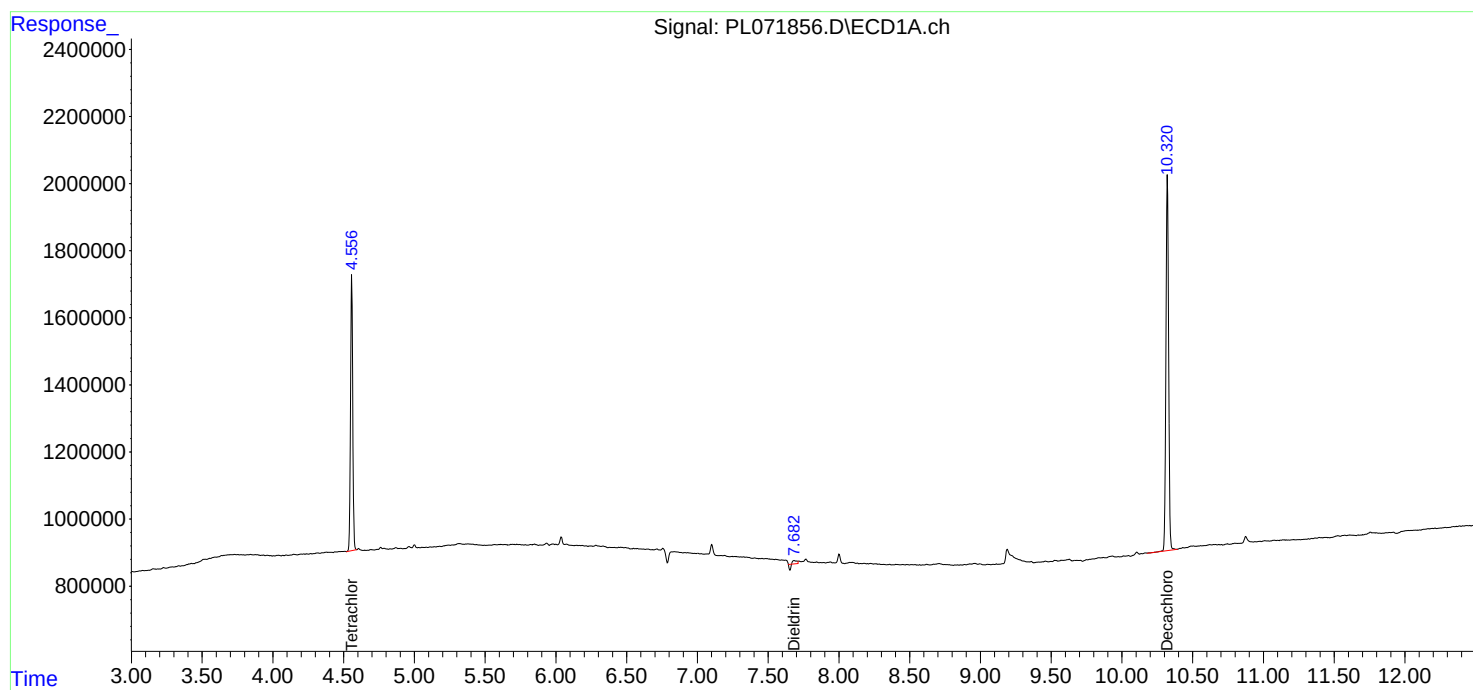


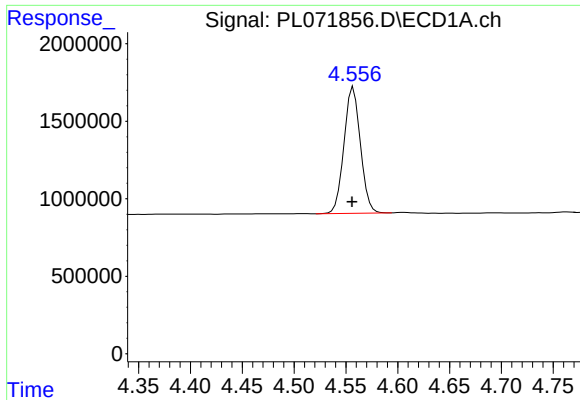

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 8983263
Conc: 19.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

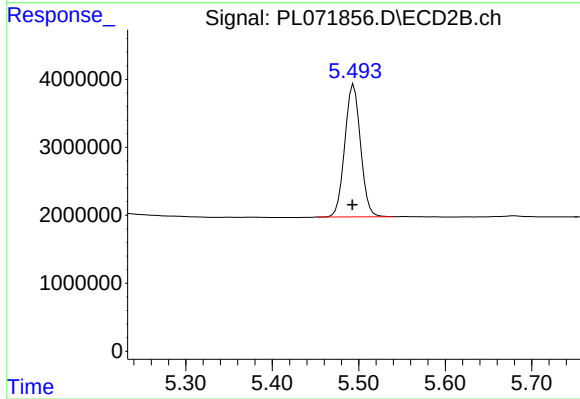


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 24575264
Conc: 20.00 ng/ml

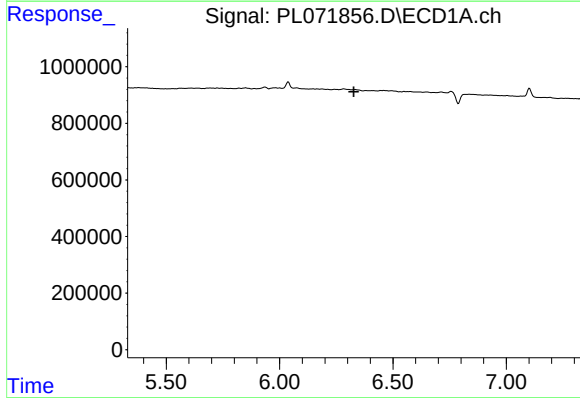


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

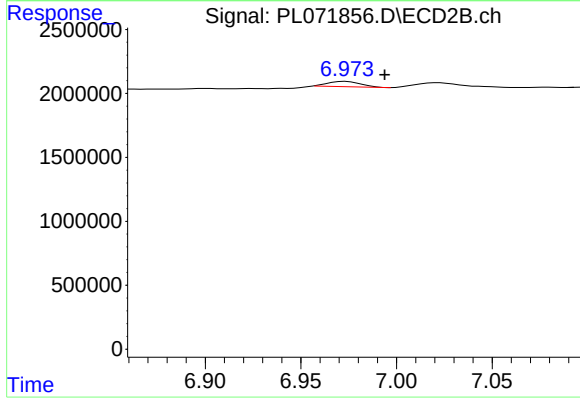

#7 delta-BHC


R.T.: 6.973 min
Delta R.T.: -0.020 min
Response: 491711
Conc: 0.32 ng/ml

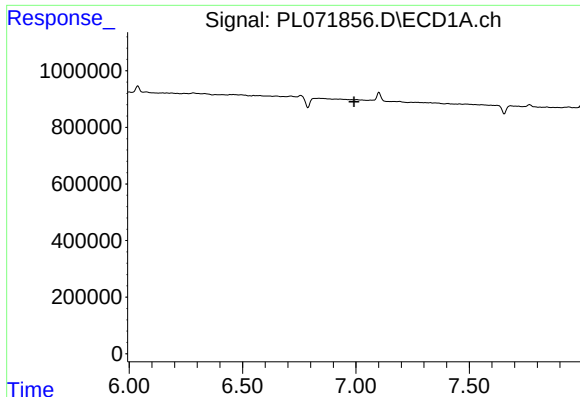

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

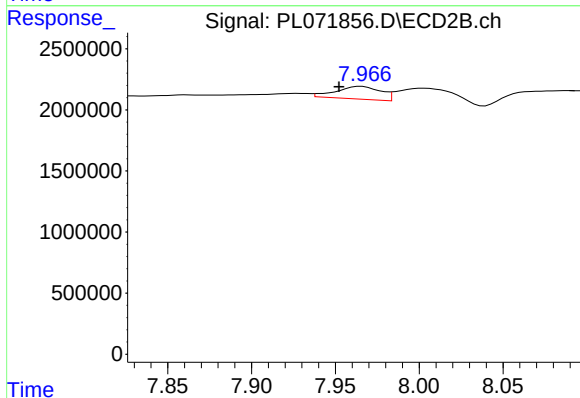


#8 Heptachlor epoxide

R.T.: 7.965 min
Delta R.T.: 0.013 min
Response: 1919392
Conc: 1.37 ng/ml

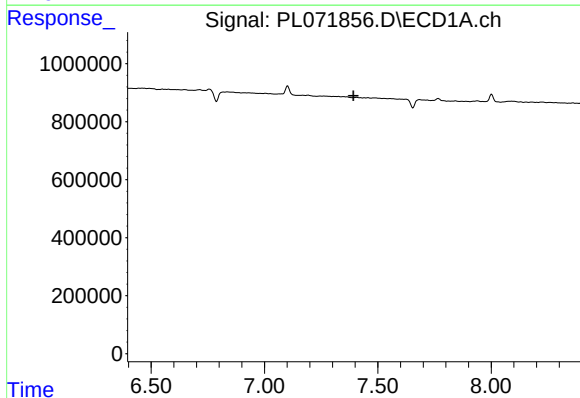


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

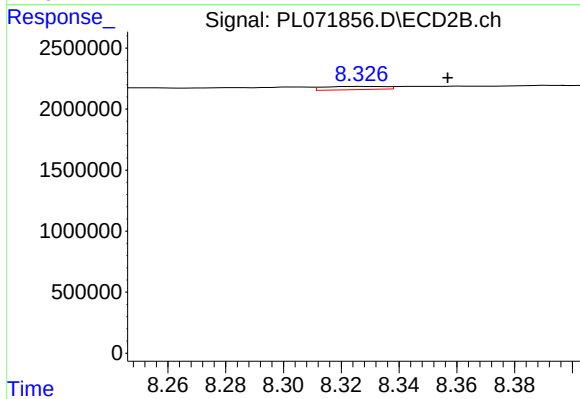

#9 Endosulfan I


R.T.: 8.327 min
Delta R.T.: -0.030 min
Response: 396543
Conc: 0.32 ng/ml

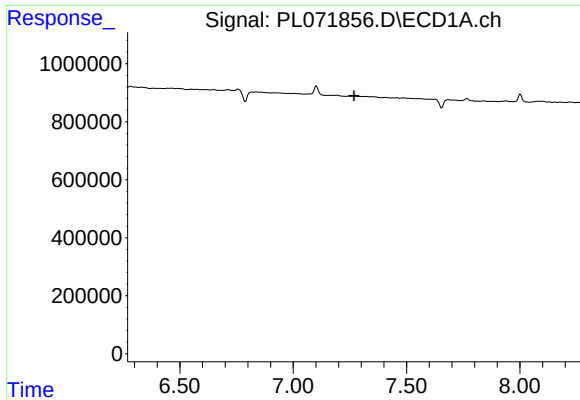

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

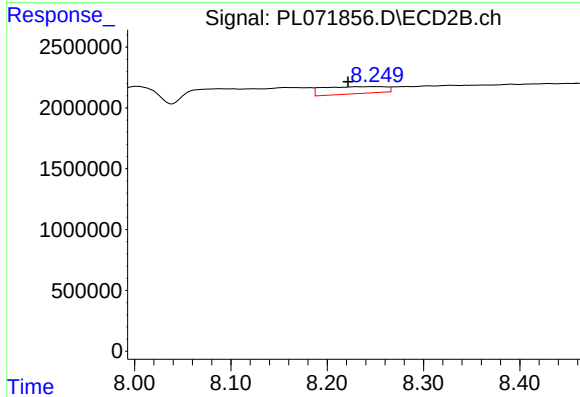


#10 gamma-Chlordane

R.T.: 8.251 min
Delta R.T.: 0.029 min
Response: 2620582
Conc: 1.92 ng/ml

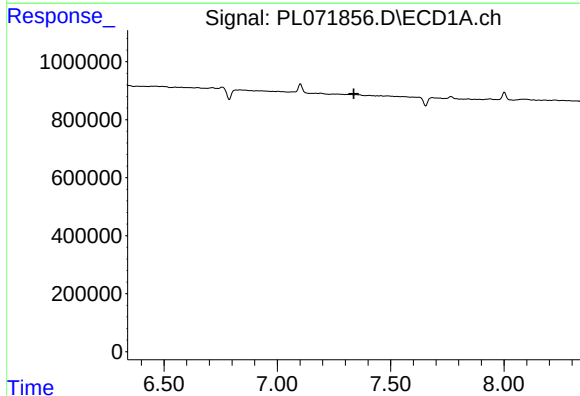


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

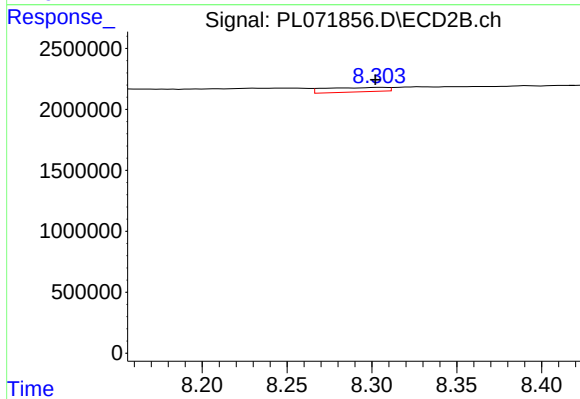

#11 alpha-Chlordane


R.T.: 8.305 min
Delta R.T.: 0.003 min
Response: 904384
Conc: 0.68 ng/ml

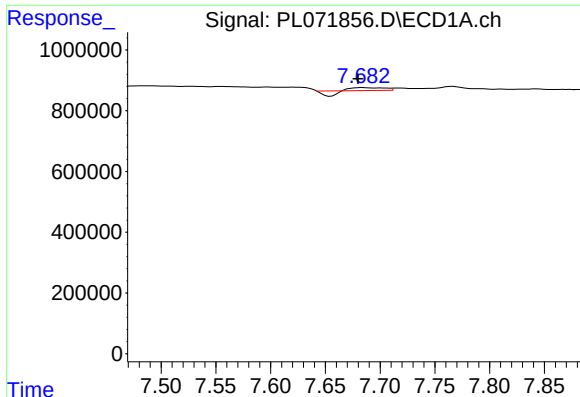

#13 Dieldrin


R.T.: 7.684 min
Delta R.T.: 0.004 min
Response: 83741
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

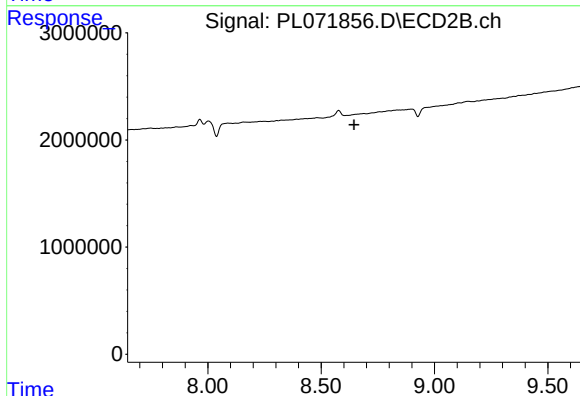


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.646 min
Response: 0
Conc: N.D.

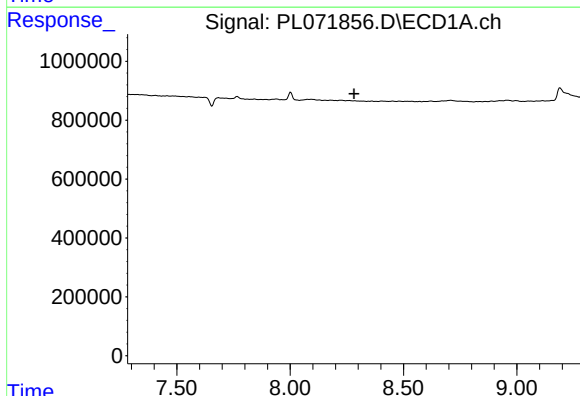


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.283 min
Response: 0
Conc: N.D.

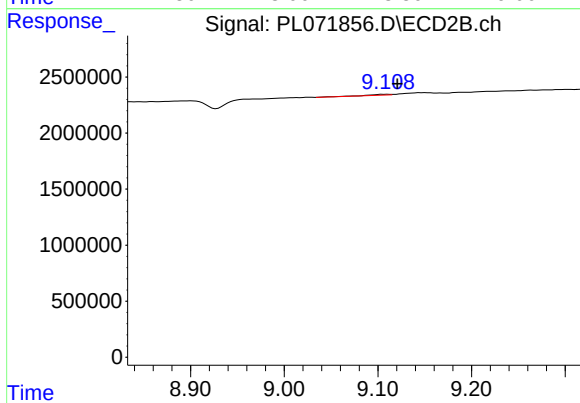

#15 Endosulfan II


R.T.: 9.107 min
Delta R.T.: -0.013 min
Response: 111516
Conc: 0.10 ng/ml

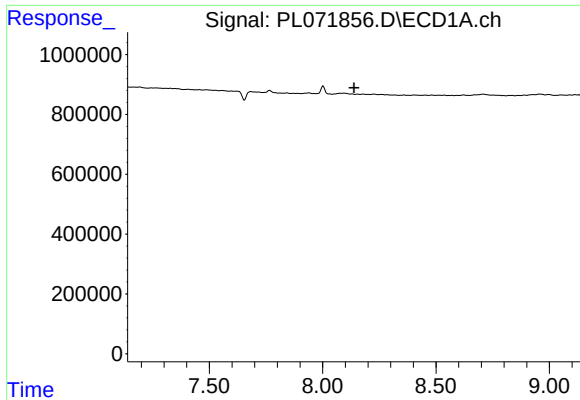

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

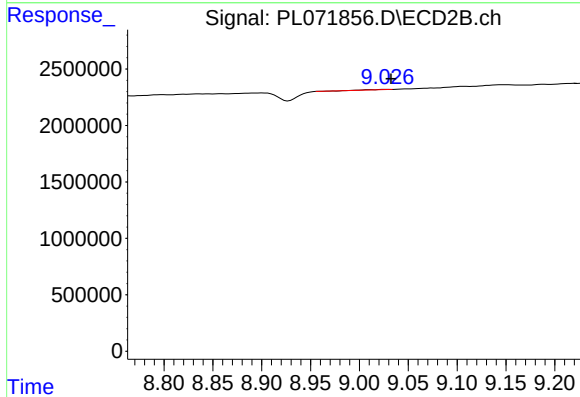


#16 4,4'-DDD

R.T.: 9.028 min
Delta R.T.: -0.004 min
Response: 51280
Conc: 0.05 ng/ml

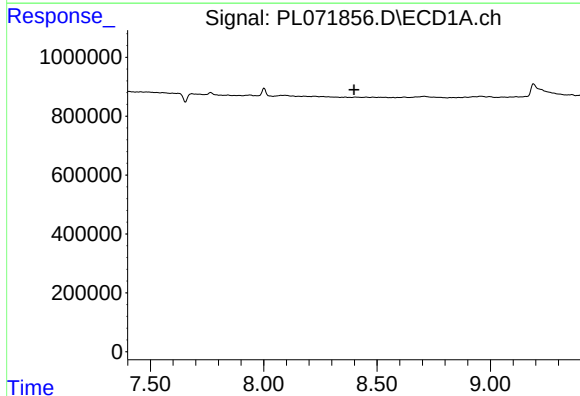


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

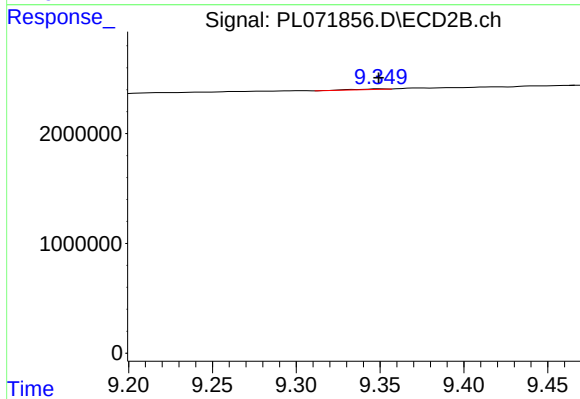

#17 4,4'-DDT


R.T.: 9.350 min
Delta R.T.: 0.001 min
Response: 62594
Conc: 0.07 ng/ml

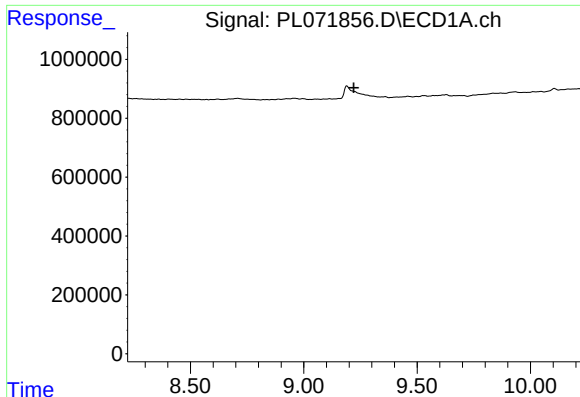

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

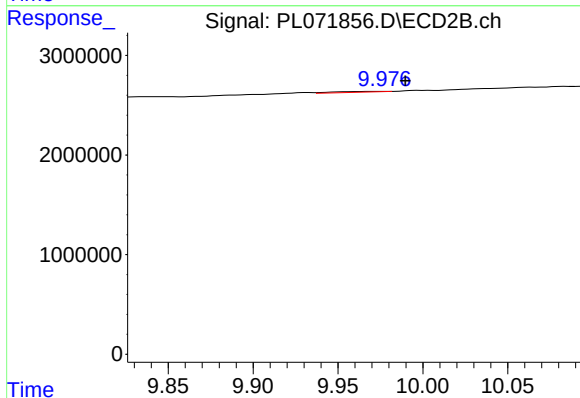


#21 Endrin ketone

R.T.: 9.977 min
Delta R.T.: -0.013 min
Response: 165994
Conc: 0.15 ng/ml

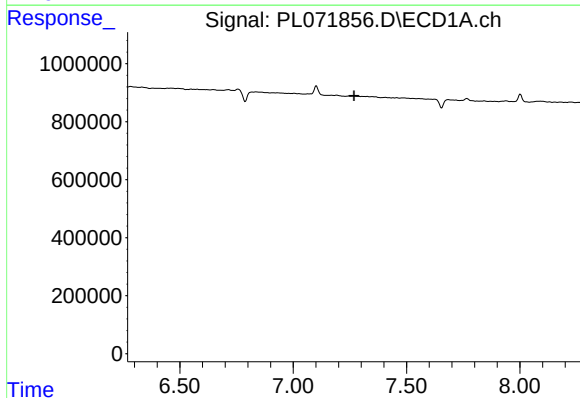


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

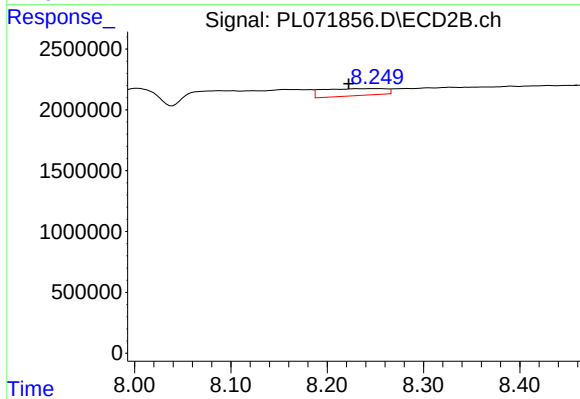

#25 Chlordane-3


R.T.: 8.251 min
Delta R.T.: 0.028 min
Response: 2620582
Conc: 12.84 ng/ml

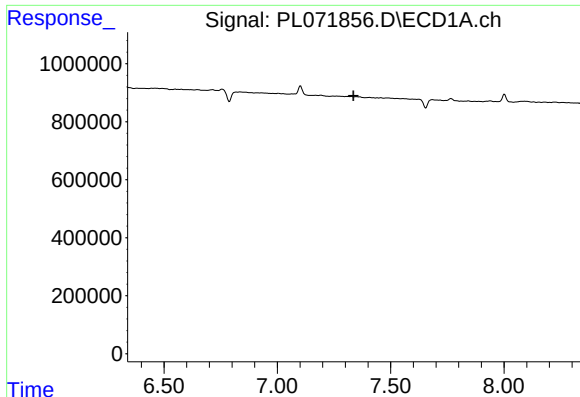

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

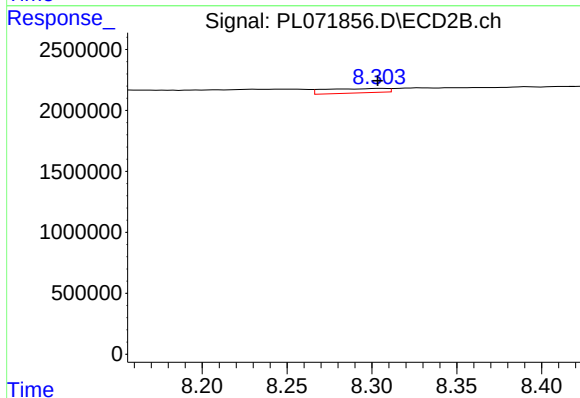


#26 Chlordane-4

R.T.: 8.305 min
Delta R.T.: 0.002 min
Response: 904384
Conc: 3.72 ng/ml

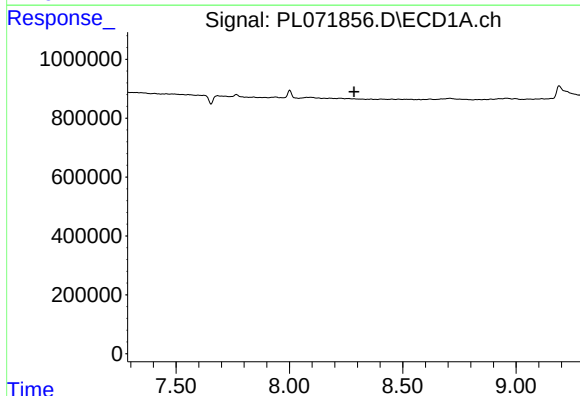


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

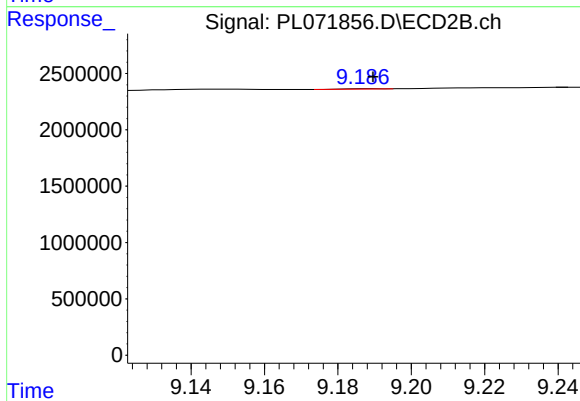

#27 Chlordane-5


R.T.: 9.189 min
Delta R.T.: 0.000 min
Response: 13551
Conc: 0.34 ng/ml

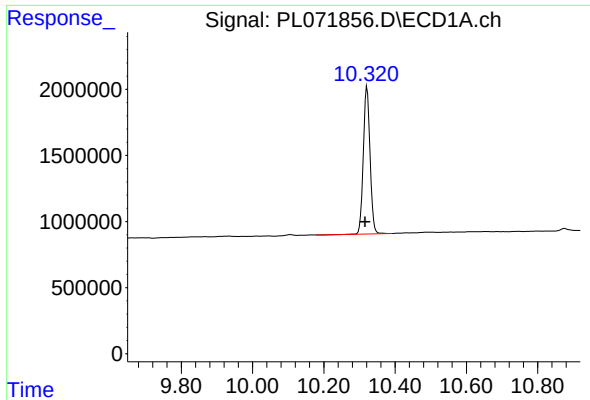

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: 0.005 min
Response: 14561133
Conc: 20.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

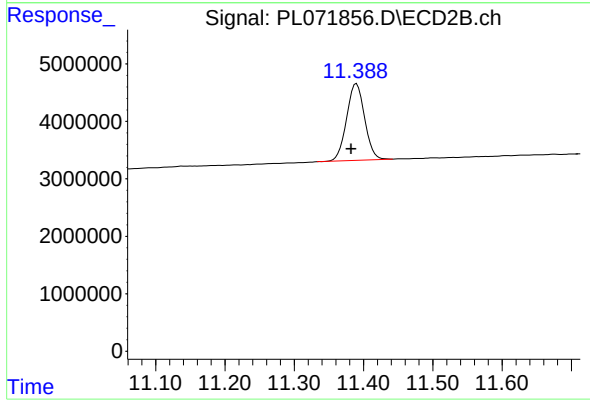

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.008 min
Response: 24123083
Conc: 20.36 ng/ml