

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010719\
 Data File : PL043656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2019 17:16
 Operator : AJ\SJ
 Sample : K1041-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OS-1-5-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 00:18:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.463	4.098	69457284	31262765	10.871	10.700
28) SA	Decachlor...	8.198	9.228	66907125	25649324	13.277	11.603
Target Compounds							
2) A	alpha-BHC	3.858f	4.451f	1250996	1500009	0.129	0.355 #
7) B	delta-BHC	0.000	5.166	0	3464132	N.D.	0.819 #
8) B	Heptachlo...	5.111f	5.998	2063879	4816057	0.268	1.317 #
20) A	Methoxychlor	6.899	0.000	1376074	0	0.498	N.D. #
23)	Chlordane-1	4.327	5.166	1164661	3464132	4.327	25.895 #
24)	Chlordane-2	0.000	5.539	0	749078	N.D.	6.066 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010719\
Data File : PL043656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2019 17:16
Operator : AJ\SJ
Sample : K1041-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
OS-1-5-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:18:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

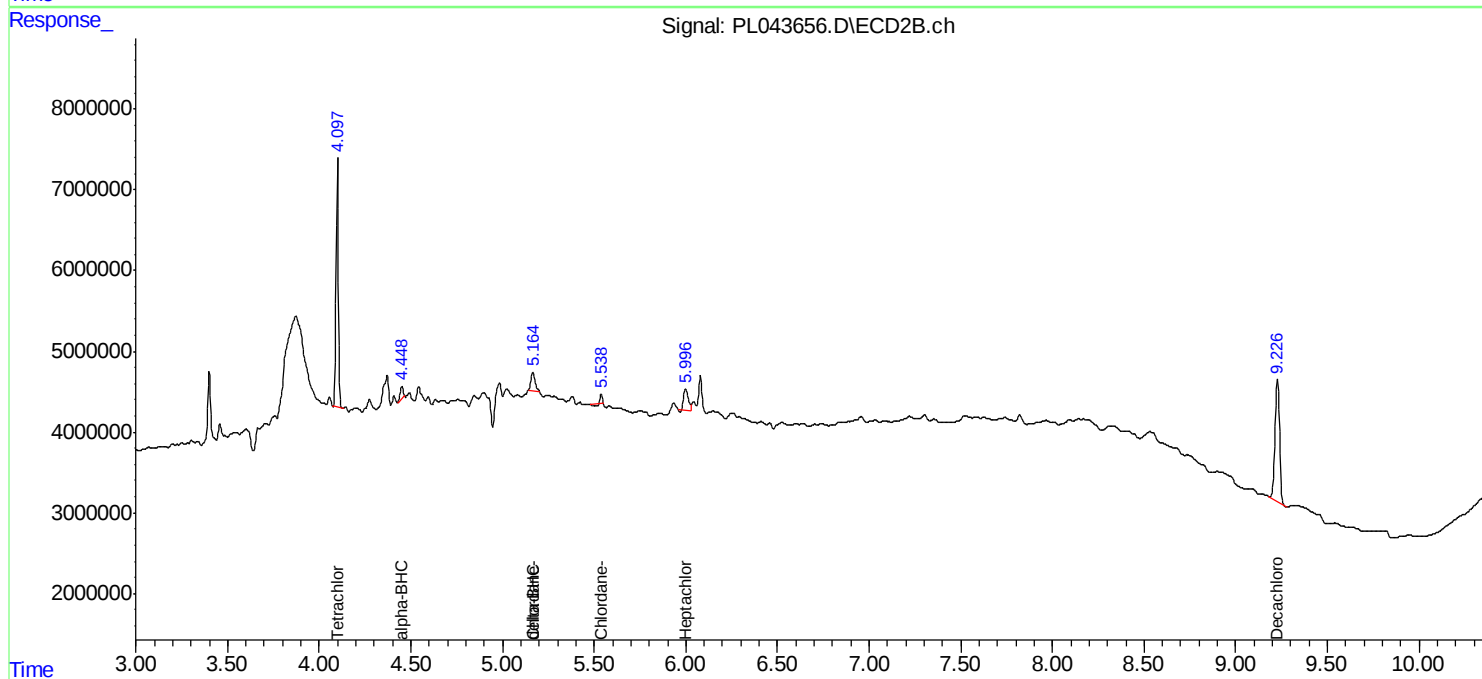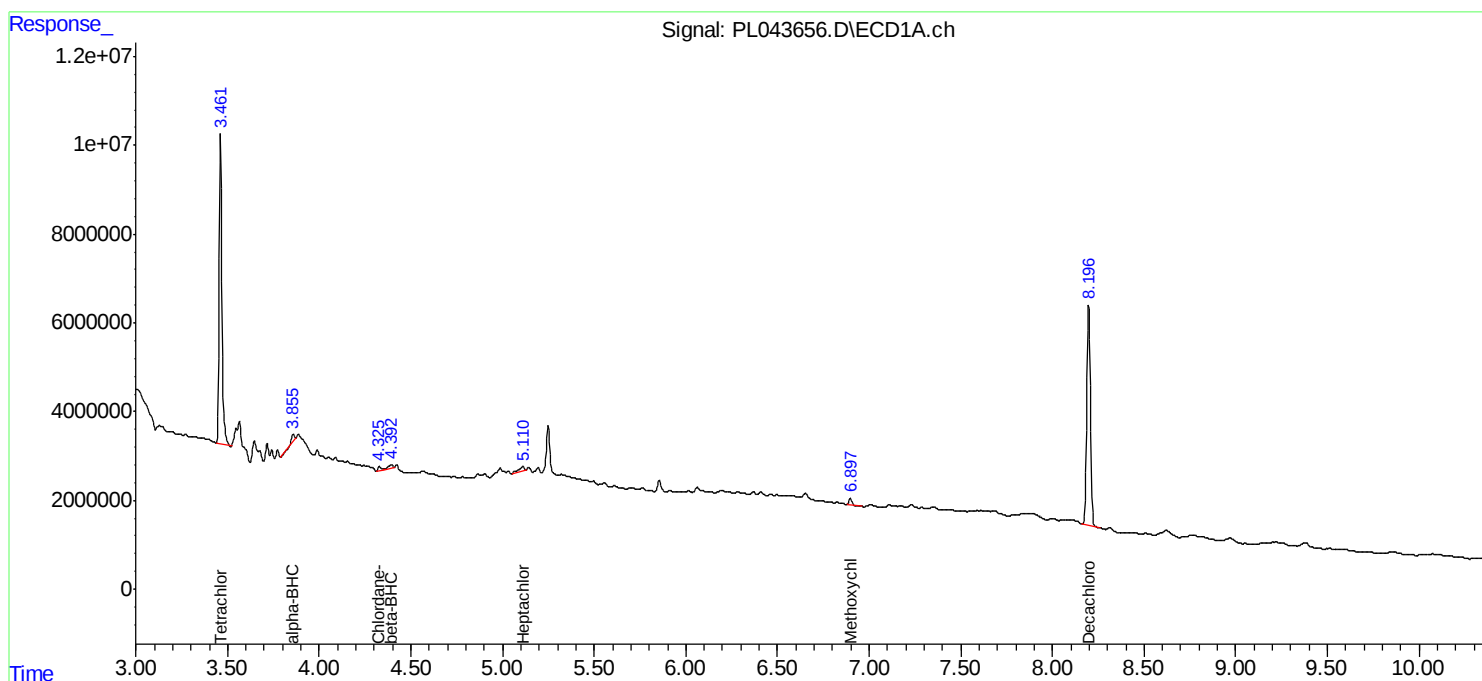


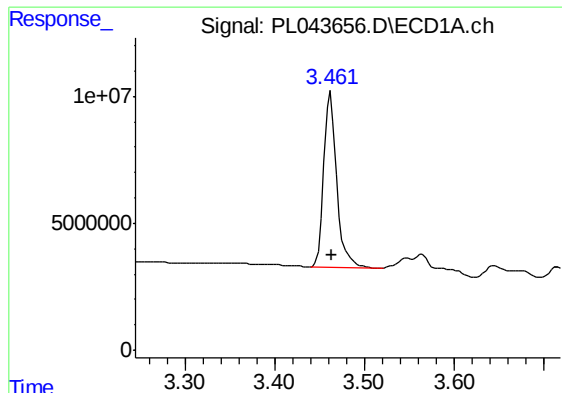

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: -0.001 min
Response: 69457284
Conc: 10.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
OS-1-5-COMP

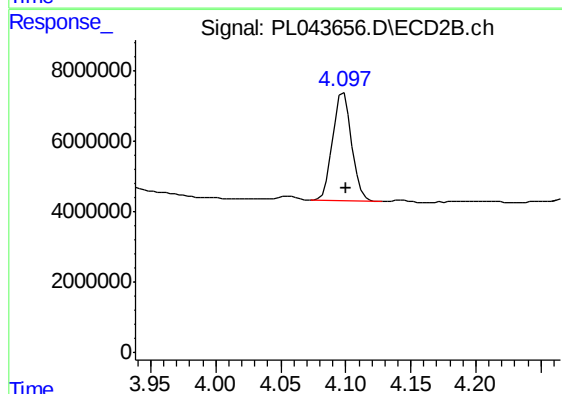


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.002 min
Response: 31262765
Conc: 10.70 ng/ml

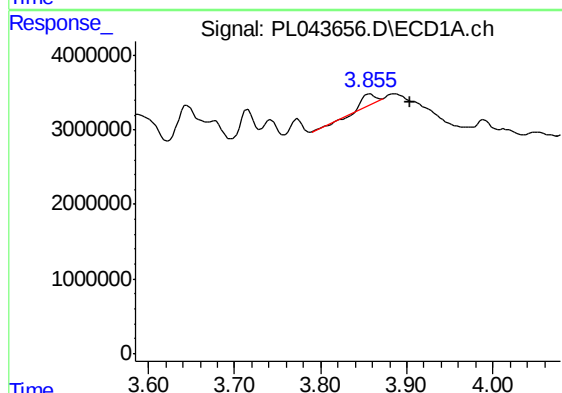


#2 alpha-BHC

R.T.: 3.858 min
Delta R.T.: -0.046 min
Response: 1250996
Conc: 0.13 ng/ml

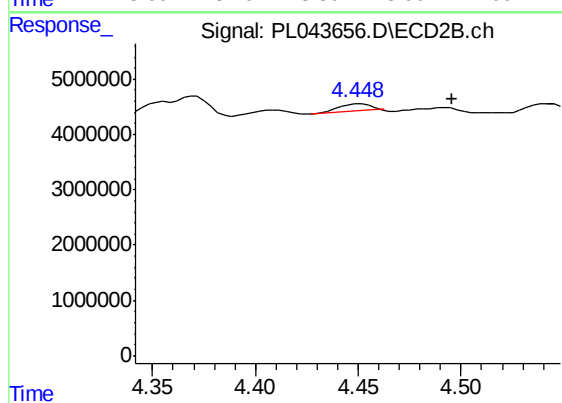

#2 alpha-BHC


R.T.: 4.451 min
Delta R.T.: -0.045 min
Response: 1500009
Conc: 0.35 ng/ml

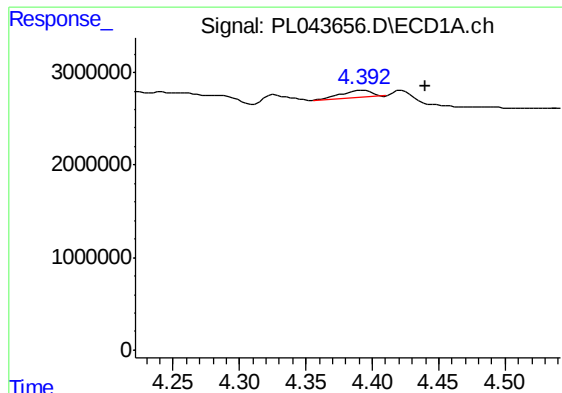

#6 beta-BHC


R.T.: 4.393 min
Delta R.T.: -0.047 min
Response: 1265073
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
OS-1-5-COMP

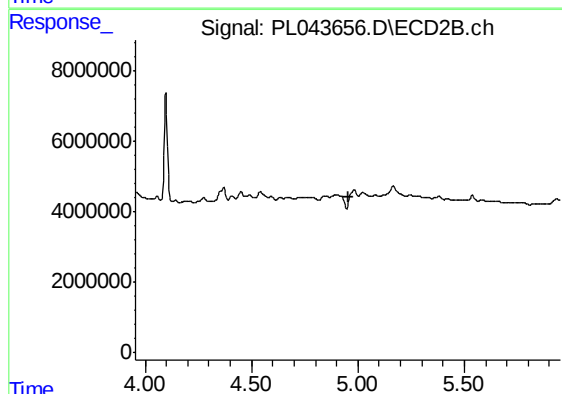


#6 beta-BHC

R.T.: 4.984 min
Delta R.T.: 0.030 min
Response: -1445368
Conc: N.D.

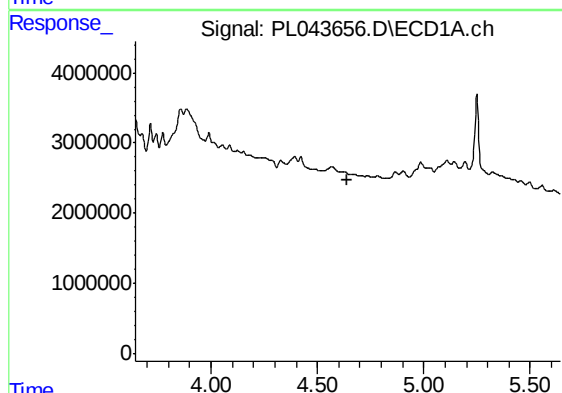


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.642 min
Response: 0
Conc: N.D.

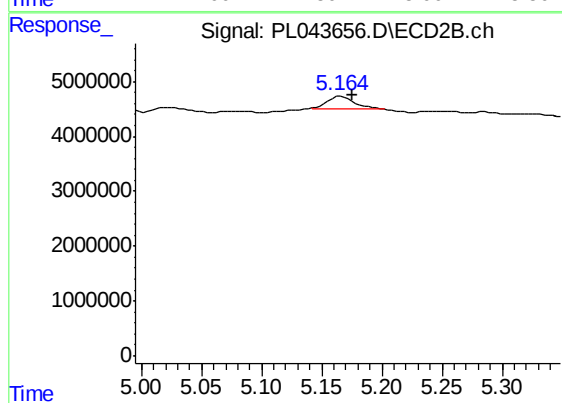

#7 delta-BHC


R.T.: 5.166 min
Delta R.T.: -0.009 min
Response: 3464132
Conc: 0.82 ng/ml

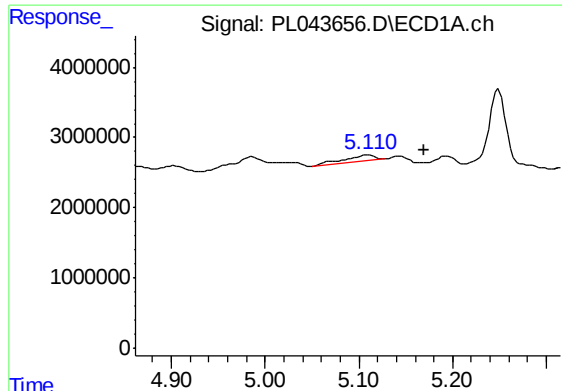

#8 Heptachlor epoxide


R.T.: 5.111 min
Delta R.T.: -0.058 min
Response: 2063879
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
OS-1-5-COMP

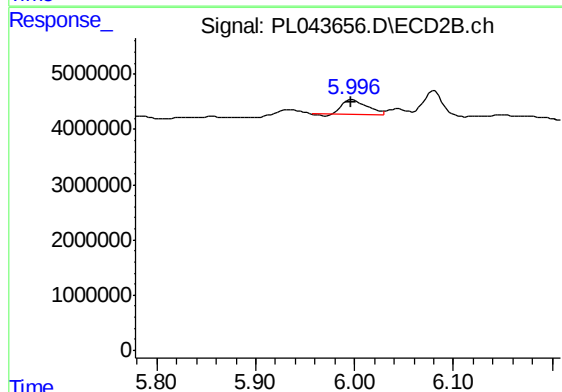


#8 Heptachlor epoxide

R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 4816057
Conc: 1.32 ng/ml

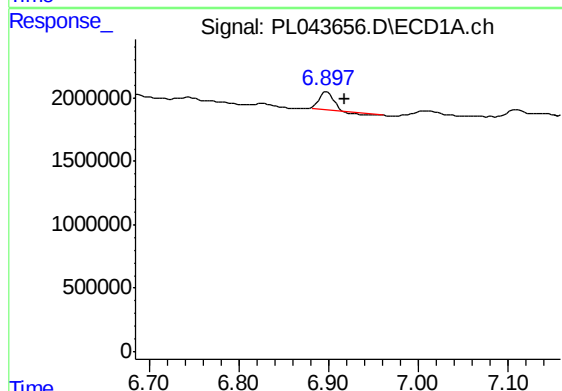


#20 Methoxychlor

R.T.: 6.899 min
Delta R.T.: -0.020 min
Response: 1376074
Conc: 0.50 ng/ml

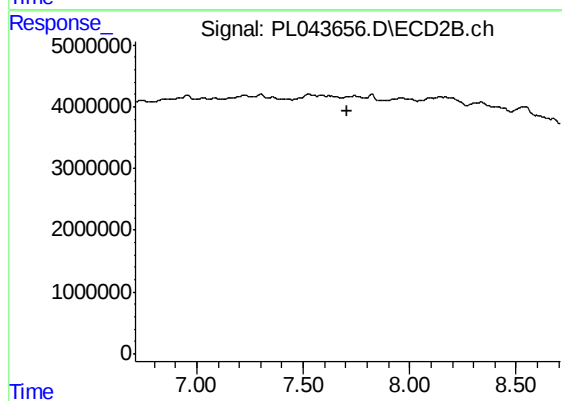

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

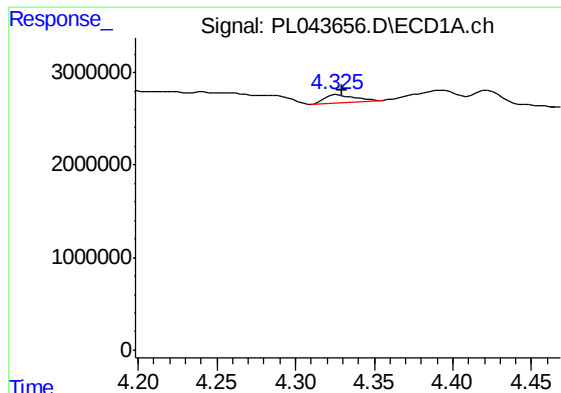

#23 Chlordane-1


R.T.: 4.327 min
Delta R.T.: -0.002 min
Response: 1164661
Conc: 4.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
OS-1-5-COMP

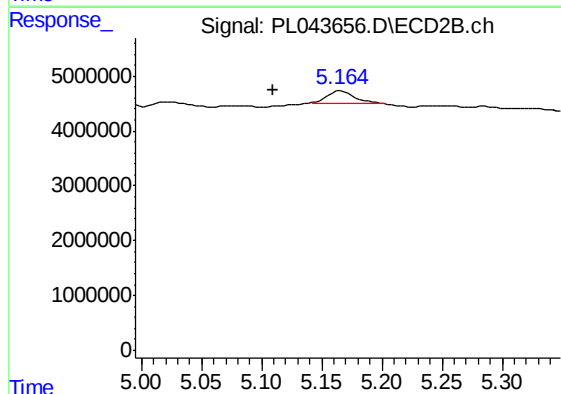


#23 Chlordane-1

R.T.: 5.166 min
Delta R.T.: 0.057 min
Response: 3464132
Conc: 25.90 ng/ml

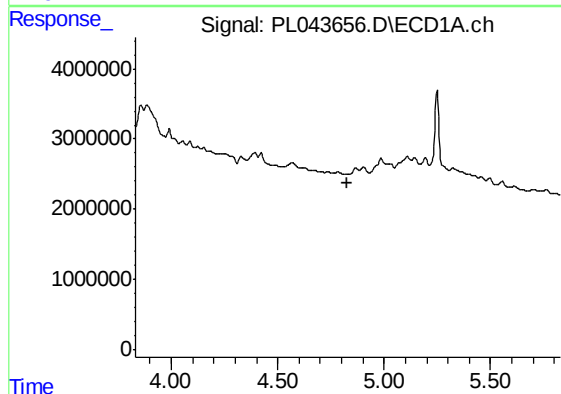


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.829 min
Response: 0
Conc: N.D.

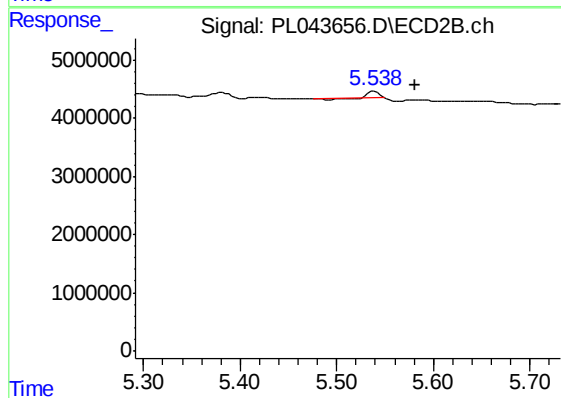

#24 Chlordane-2


R.T.: 5.539 min
Delta R.T.: -0.042 min
Response: 749078
Conc: 6.07 ng/ml

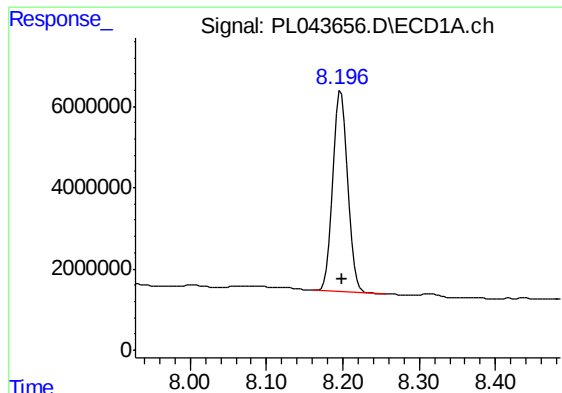

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: 0.000 min
Response: 66907125
Conc: 13.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
OS-1-5-COMP

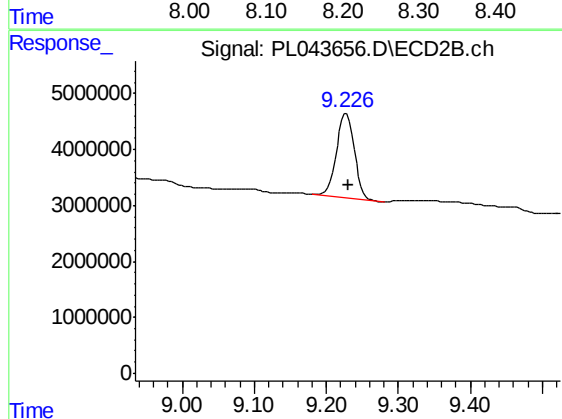

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: -0.004 min
Response: 25649324
Conc: 11.60 ng/ml