

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010719\
 Data File : PL043680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2019 22:54
 Operator : AJ\SJ
 Sample : K1010-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-010419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 00:26:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.100	108.1E6	51085088	16.919	17.484
28)	SA Decachlor...	8.195	9.227	112.3E6	49774418	22.284	22.516
Target Compounds							
2)	A alpha-BHC	3.933f	0.000	1219009	0	0.126	N.D. #
3)	MA gamma-BHC...	4.194	0.000	2222359	0	0.254	N.D. #
6)	B beta-BHC	4.395f	0.000	5478813	0	1.497	N.D. #
8)	B Heptachlo...	5.237f	6.001	4403954	4417385	0.573	1.208 #
9)	A Endosulfan I	5.535	0.000	1348146	0	0.190	N.D. #
13)	MA Dieldrin	5.733	0.000	4052746	0	0.571	N.D. #
16)	A 4,4'-DDD	6.093f	0.000	1314721	0	0.248	N.D. #
23)	Chlordane-1	4.373	0.000	1652705	0	6.140	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010719\
Data File : PL043680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2019 22:54
Operator : AJ\SJ
Sample : K1010-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-03-010419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:26:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

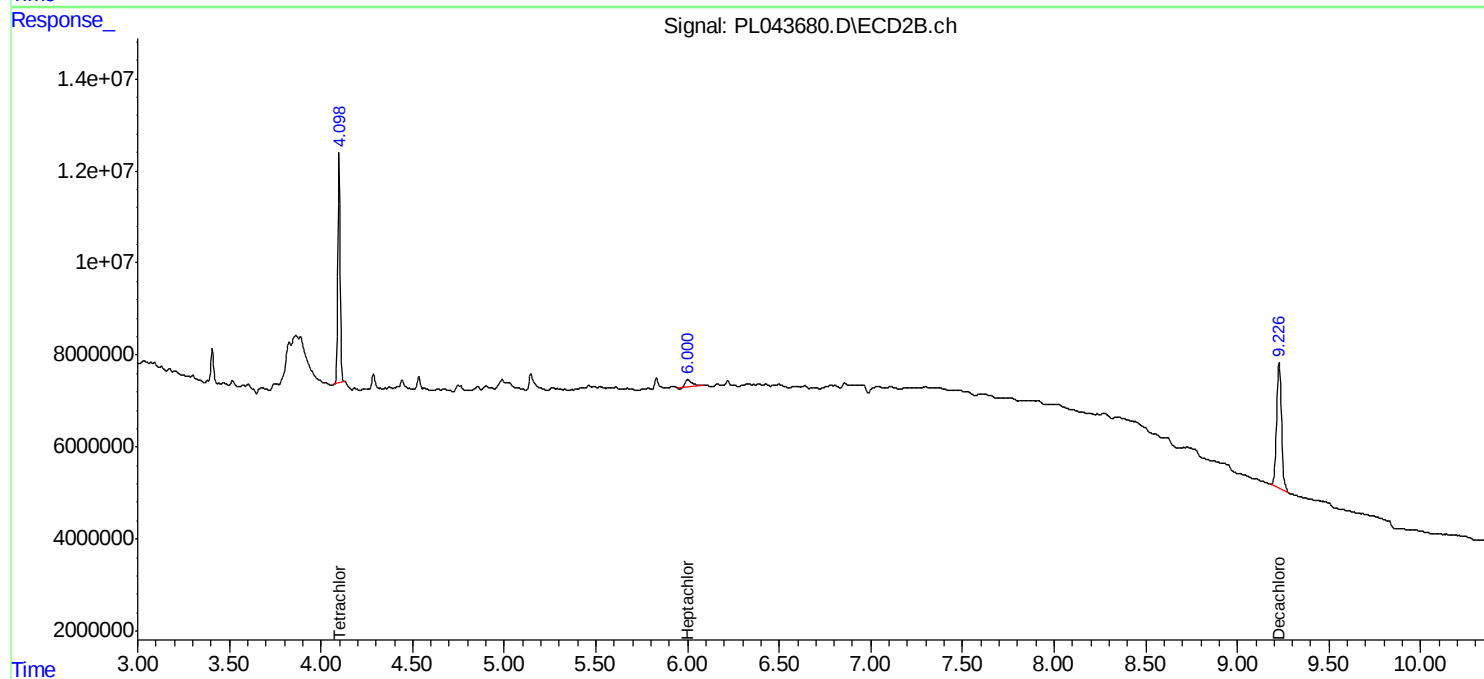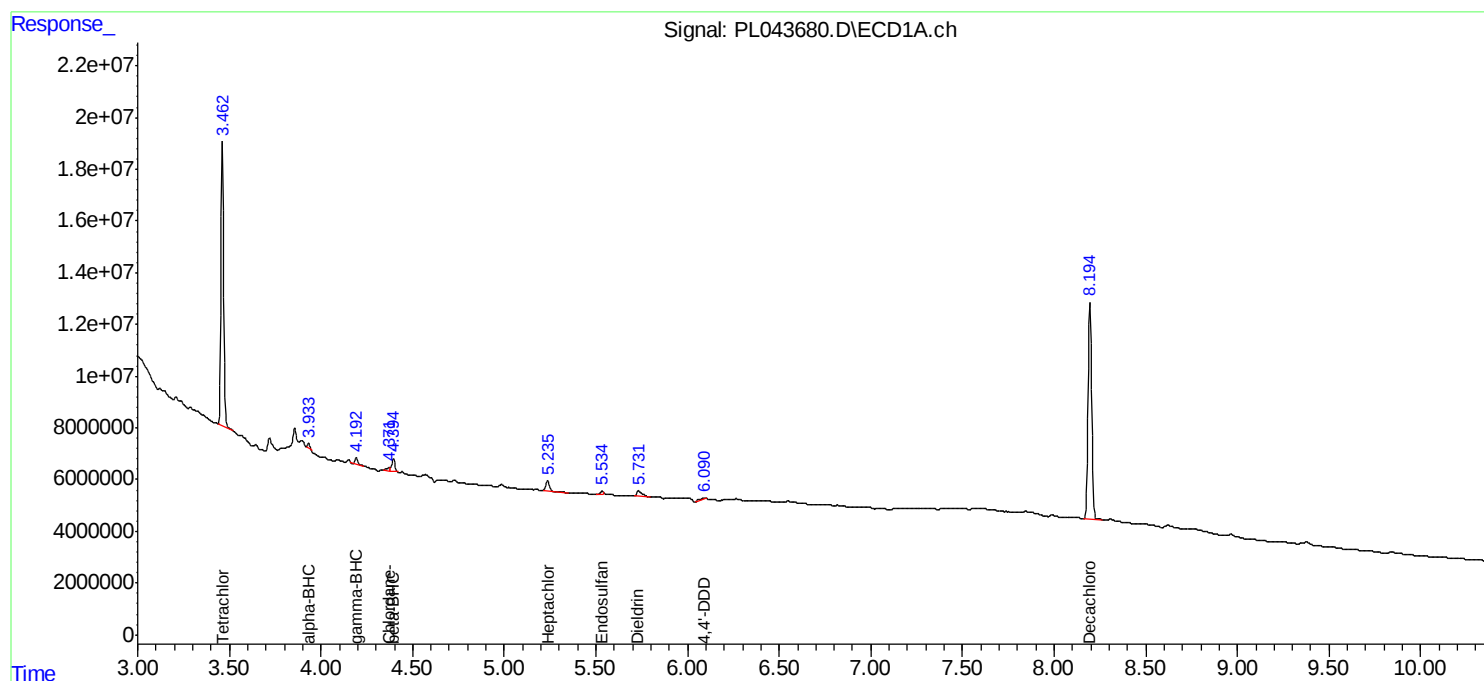


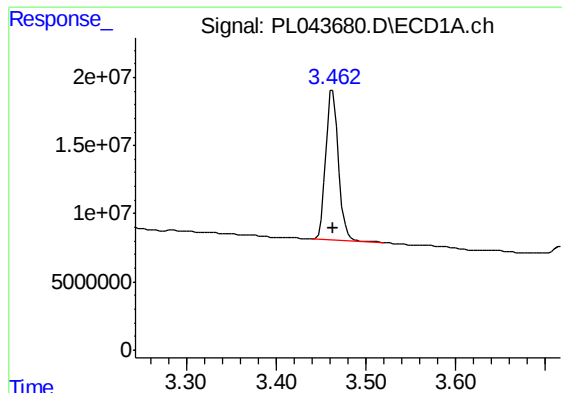

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: -0.001 min
Response: 108101659
Conc: 16.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-010419

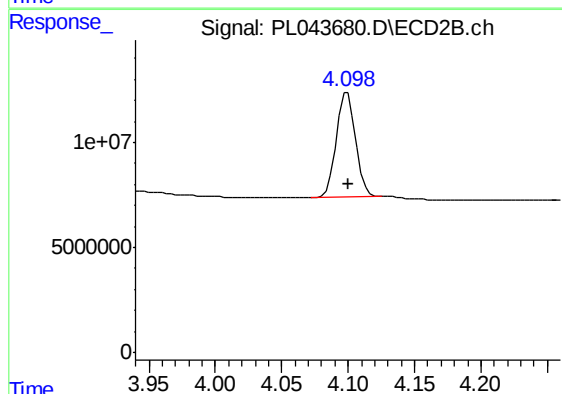


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 51085088
Conc: 17.48 ng/ml

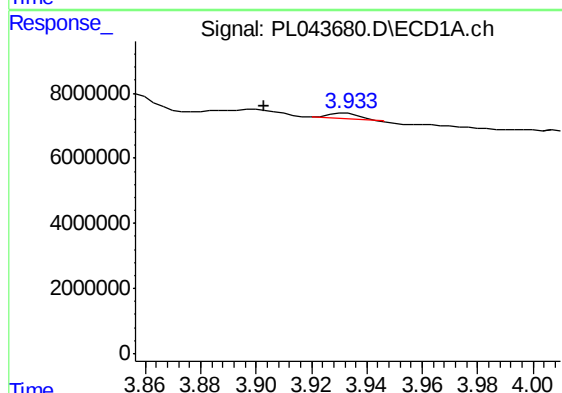


#2 alpha-BHC

R.T.: 3.933 min
Delta R.T.: 0.029 min
Response: 1219009
Conc: 0.13 ng/ml

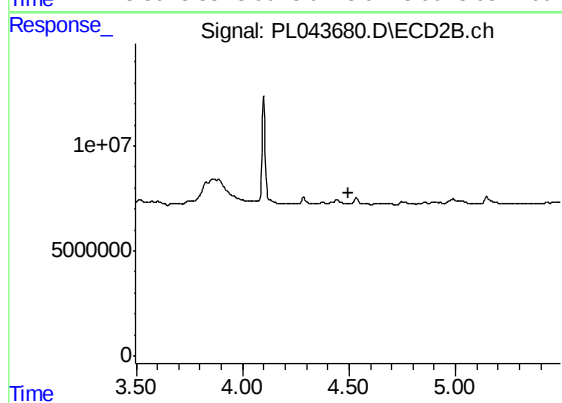

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.496 min
Response: 0
Conc: N.D.

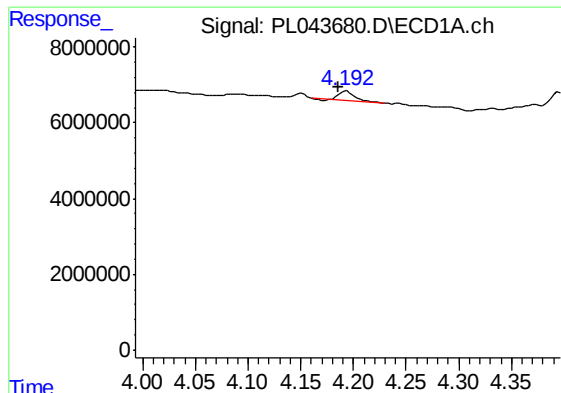

#3 gamma-BHC (Lindane)


R.T.: 4.194 min
Delta R.T.: 0.008 min
Response: 2222359
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-010419

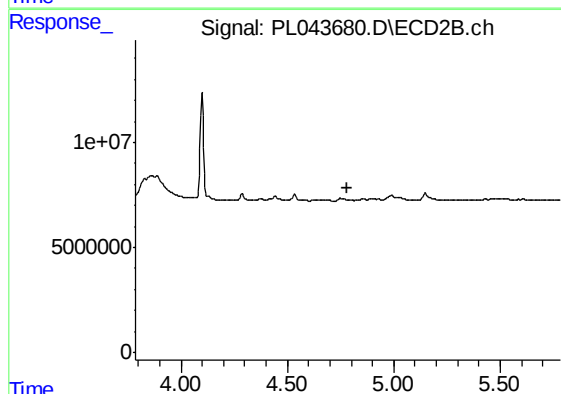


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.784 min
Response: 0
Conc: N.D.

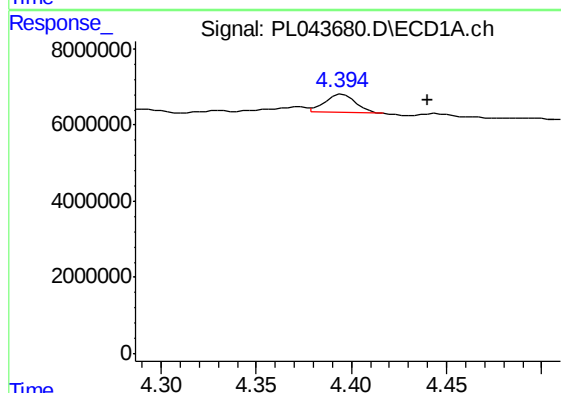


#6 beta-BHC

R.T.: 4.395 min
Delta R.T.: -0.045 min
Response: 5478813
Conc: 1.50 ng/ml

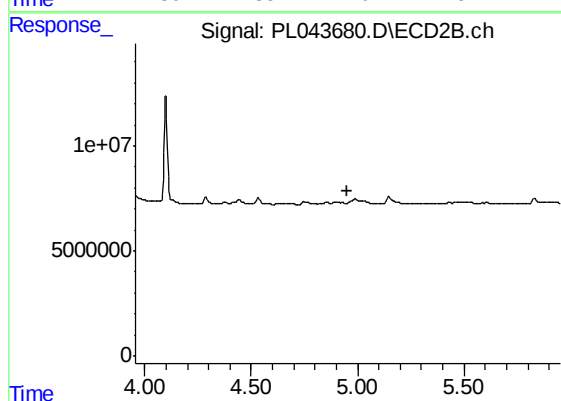

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

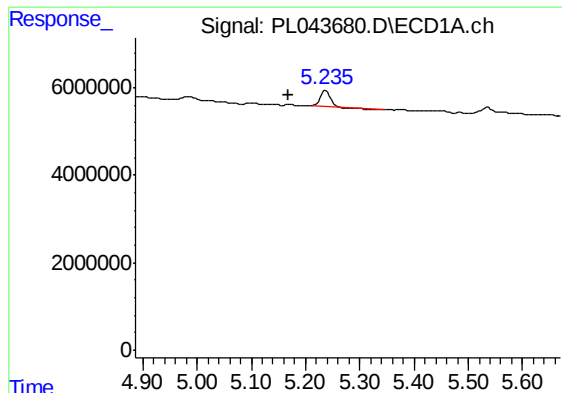

#8 Heptachlor epoxide


R.T.: 5.237 min
Delta R.T.: 0.067 min
Response: 4403954
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-010419

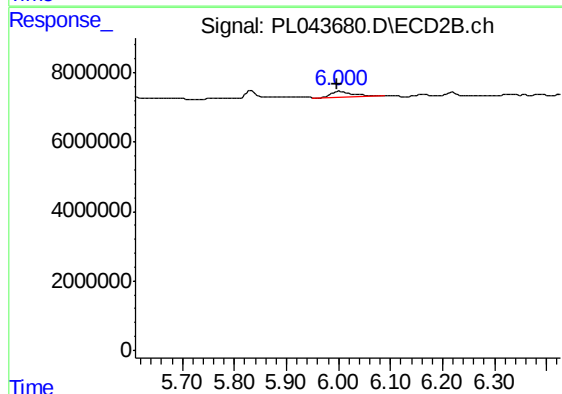


#8 Heptachlor epoxide

R.T.: 6.001 min
Delta R.T.: 0.004 min
Response: 4417385
Conc: 1.21 ng/ml

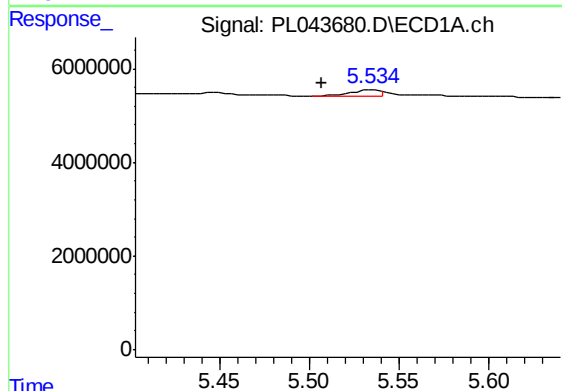


#9 Endosulfan I

R.T.: 5.535 min
Delta R.T.: 0.028 min
Response: 1348146
Conc: 0.19 ng/ml

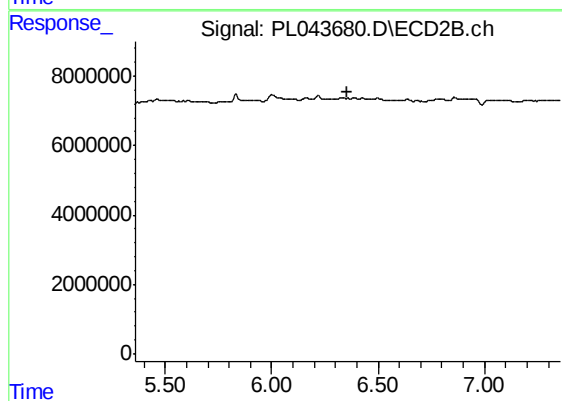

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

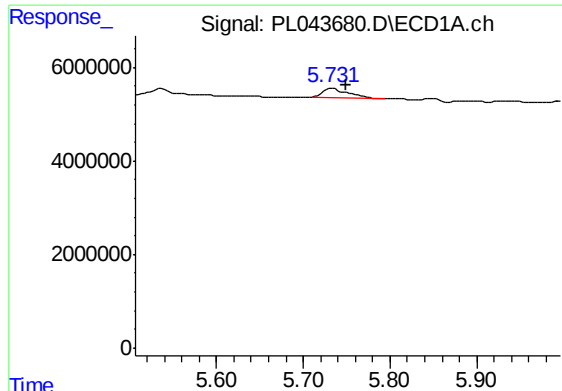

#13 Dieldrin


R.T.: 5.733 min
Delta R.T.: -0.017 min
Response: 4052746
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-010419

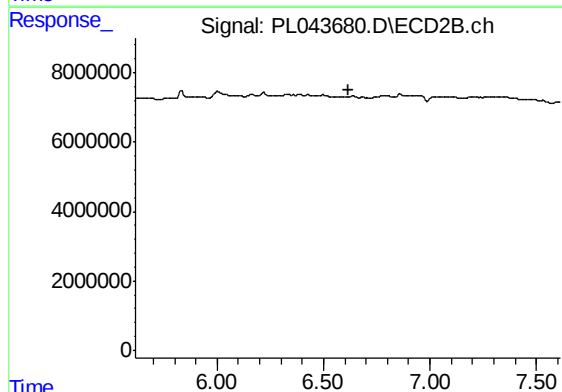


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.616 min
Response: 0
Conc: N.D.

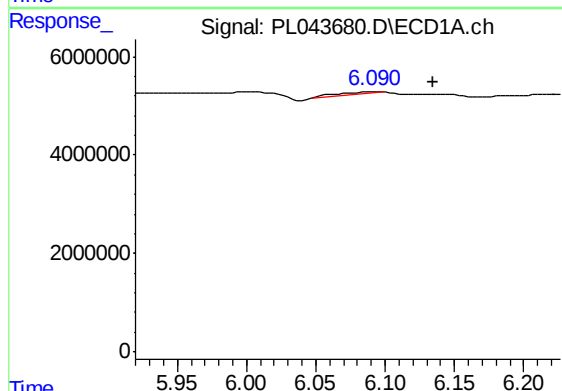


#16 4,4'-DDD

R.T.: 6.093 min
Delta R.T.: -0.042 min
Response: 1314721
Conc: 0.25 ng/ml

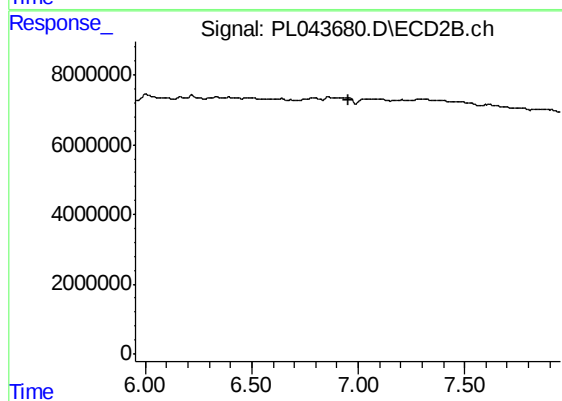

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

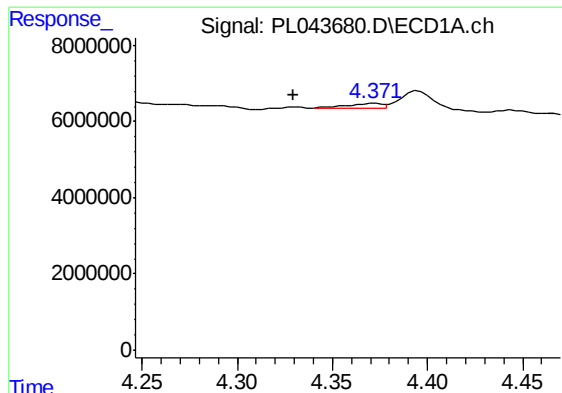

#23 Chlordane-1


R.T.: 4.373 min
Delta R.T.: 0.043 min
Response: 1652705
Conc: 6.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-010419

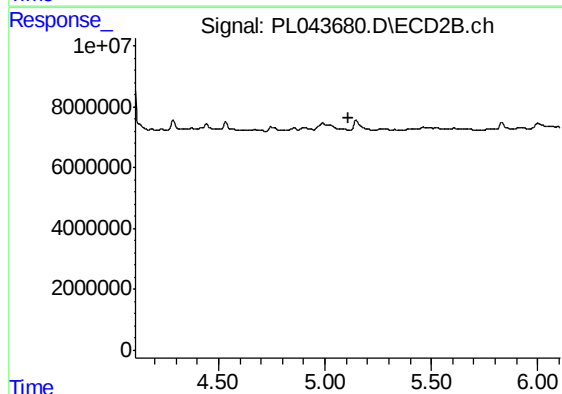


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

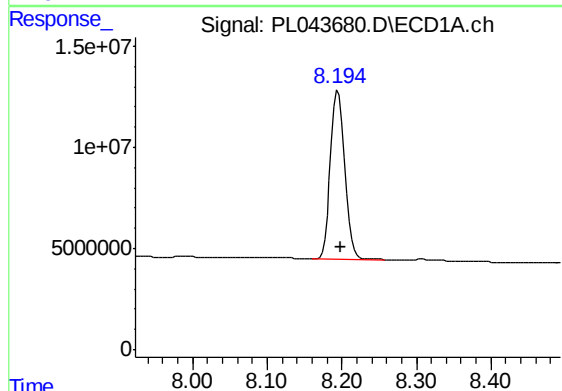

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: -0.003 min
Response: 112298381
Conc: 22.28 ng/ml

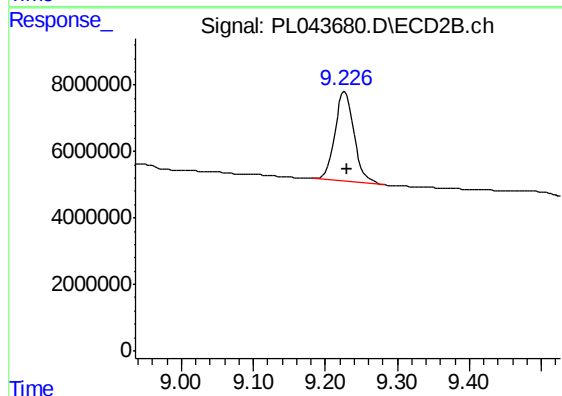

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: -0.004 min
Response: 49774418
Conc: 22.52 ng/ml