

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
 Data File : PL063964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 12:07
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 12:20:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 12:20:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.111	62843785	48114035	20.000	20.000
27)	SA Decachlor...	8.170	9.272	121.5E6	73713891	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.870	4.512	94335874	60984498	20.000	20.000
3)	MA gamma-BHC...	4.150	4.804	88453050	58229208	20.000	20.000
4)	MA Heptachlor	4.450	5.317	87207376	57098892	20.000	20.000
9)	A Endosulfan I	5.473	6.383	71725365	44661073	20.000	20.000
13)	MA Dieldrin	5.715	6.644	155.4E6	93362434	40.000	40.000
14)	MA Endrin	5.969	6.866	122.0E6	68685568	40.000	40.000
16)	A 4,4'-DDD	6.101	6.983	121.4E6	72159364	40.000	40.000
17)	MA 4,4'-DDT	6.341	7.283	118.4E6	68474296	40.000	40.000
20)	A Methoxychlor	6.889	7.743	286.1E6	188.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
Data File : PL063964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 12:07
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 12:20:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 12:20:27 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

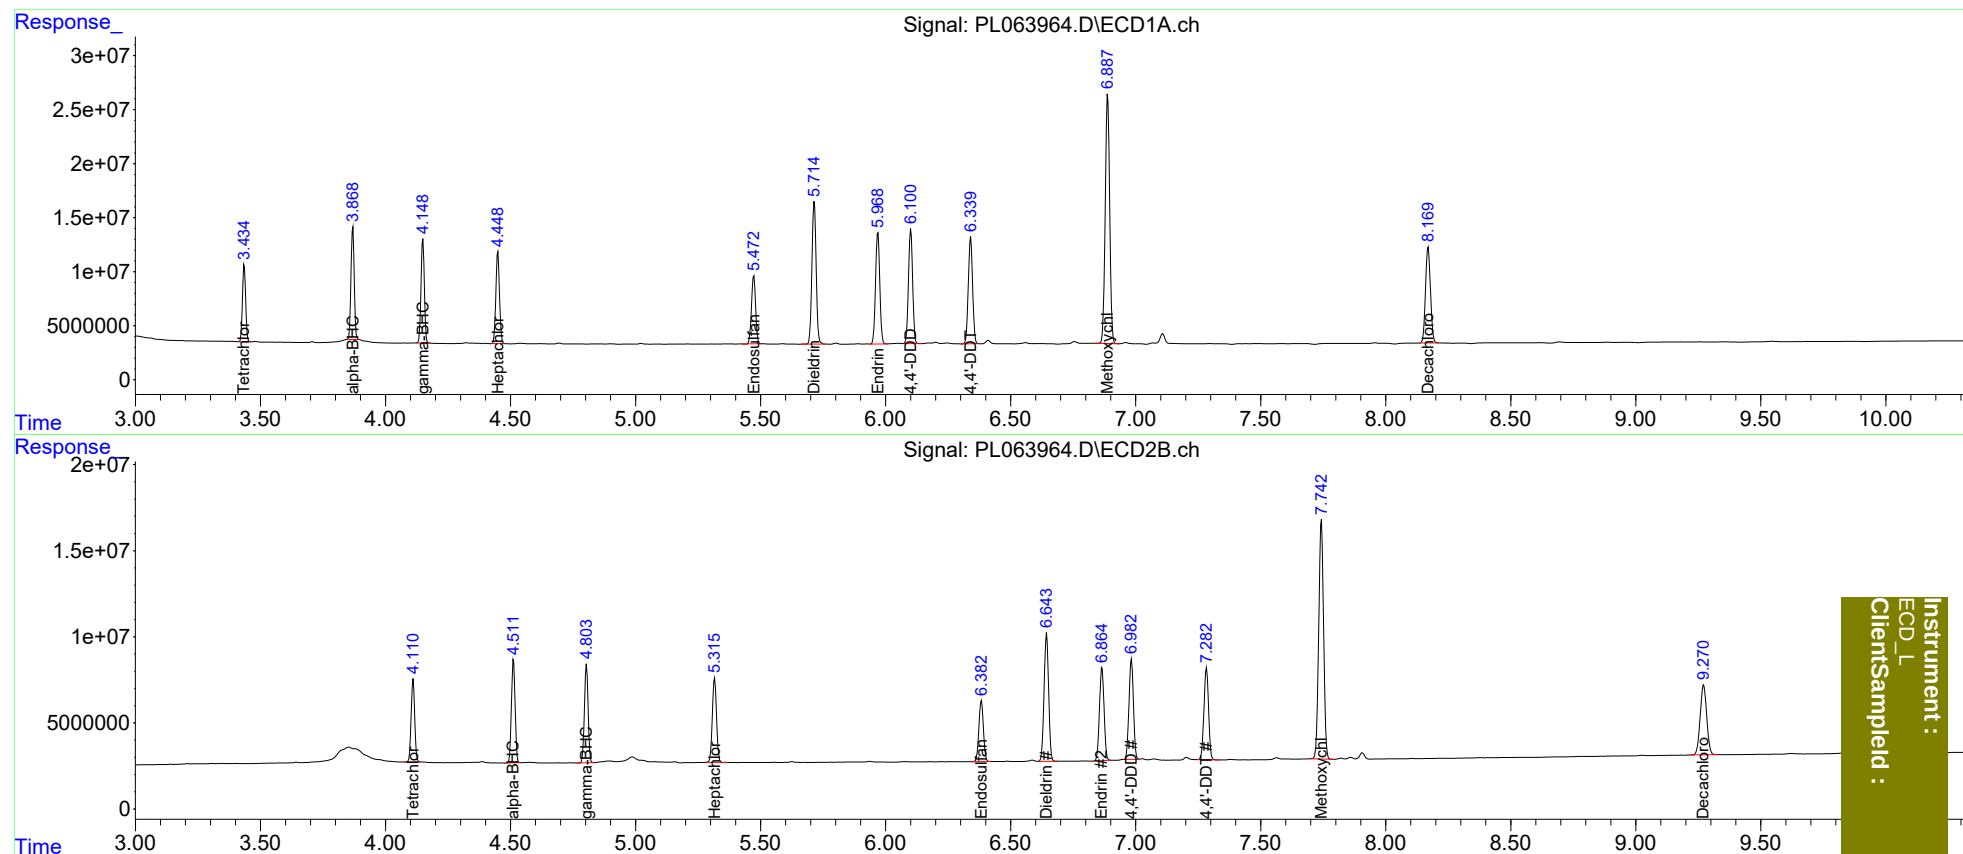


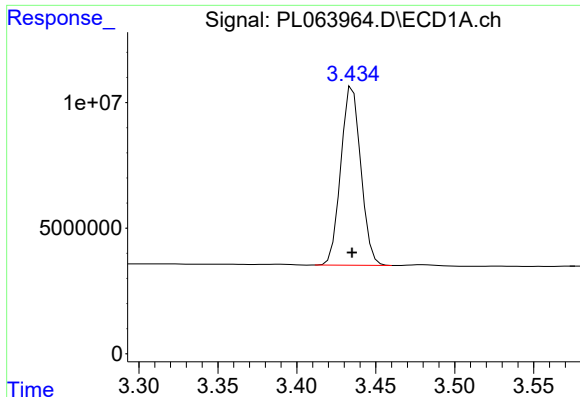

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 62843785
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

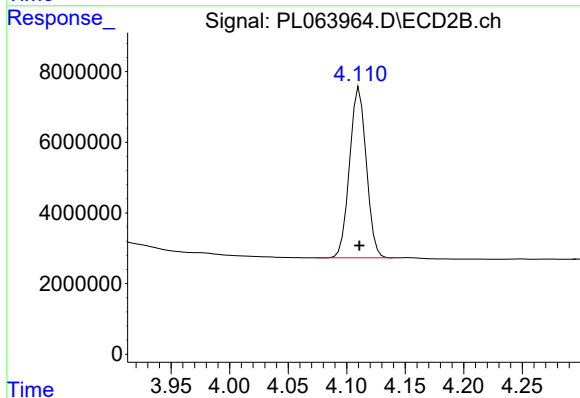


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: 0.000 min
Response: 48114035
Conc: 20.00 ng/ml

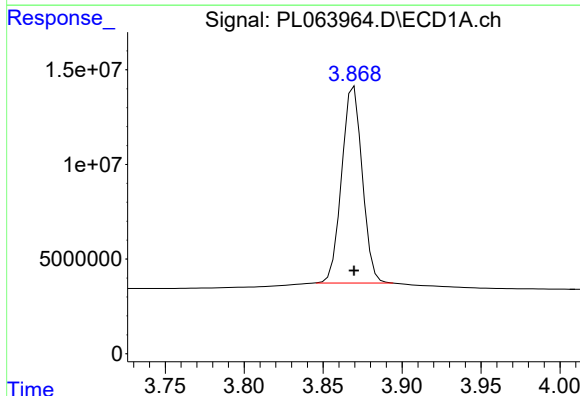


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: 0.000 min
Response: 94335874
Conc: 20.00 ng/ml

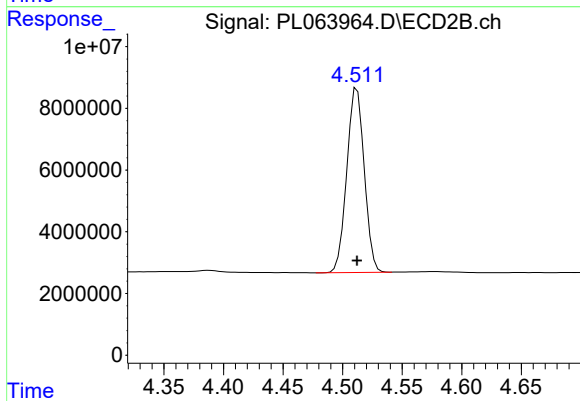

#2 alpha-BHC


R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 60984498
Conc: 20.00 ng/ml

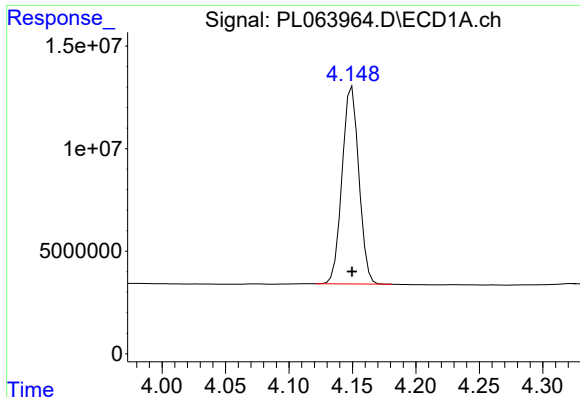

#3 gamma-BHC (Lindane)


R.T.: 4.150 min
Delta R.T.: 0.000 min
Response: 88453050
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

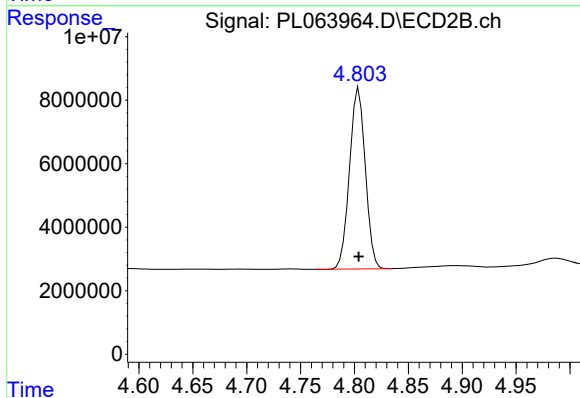


#3 gamma-BHC (Lindane)

R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 58229208
Conc: 20.00 ng/ml

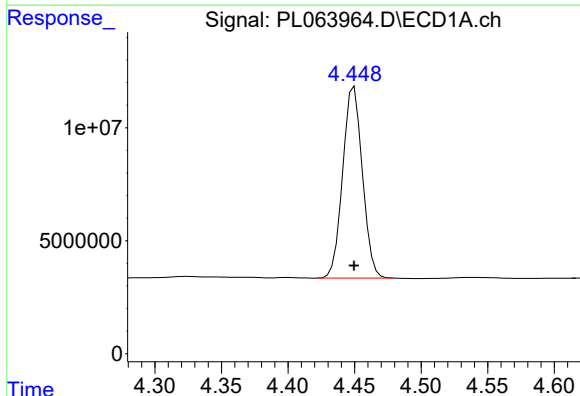


#4 Heptachlor

R.T.: 4.450 min
Delta R.T.: 0.000 min
Response: 87207376
Conc: 20.00 ng/ml

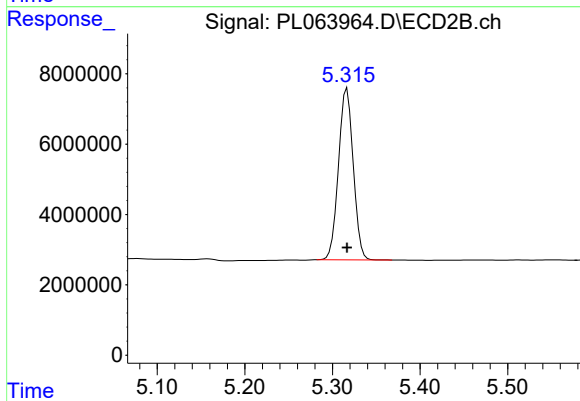

#4 Heptachlor


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 57098892
Conc: 20.00 ng/ml

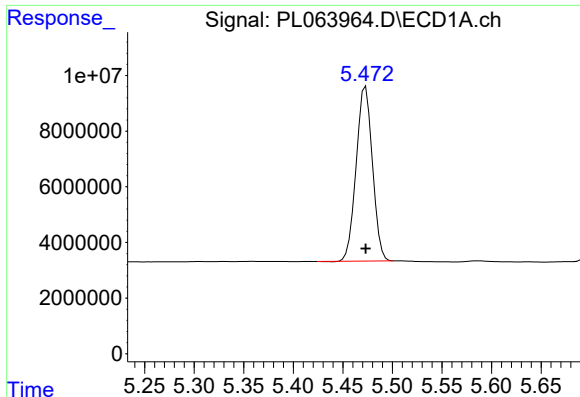

#9 Endosulfan I


R.T.: 5.473 min
Delta R.T.: 0.000 min
Response: 71725365
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

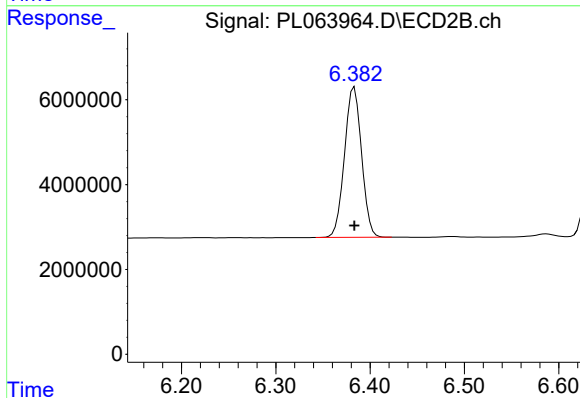


#9 Endosulfan I

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 44661073
Conc: 20.00 ng/ml

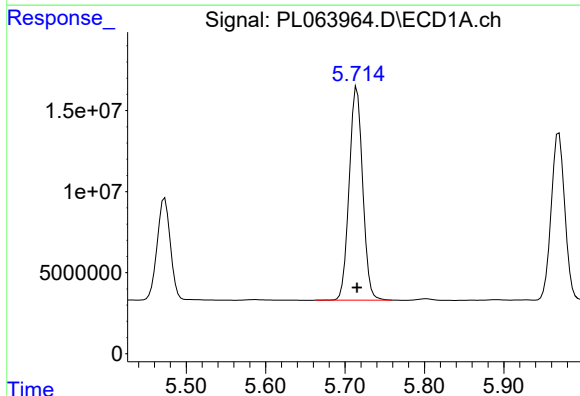


#13 Dieldrin

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 155402246
Conc: 40.00 ng/ml

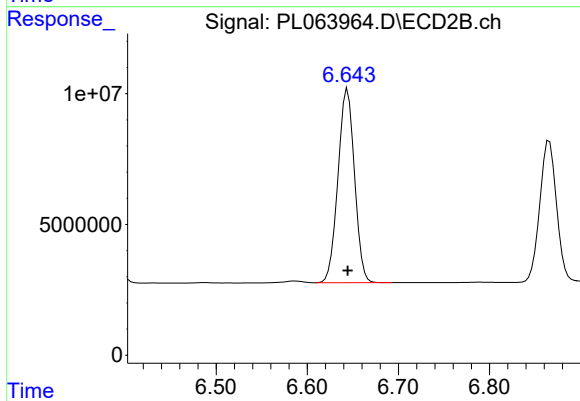

#13 Dieldrin


R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 93362434
Conc: 40.00 ng/ml

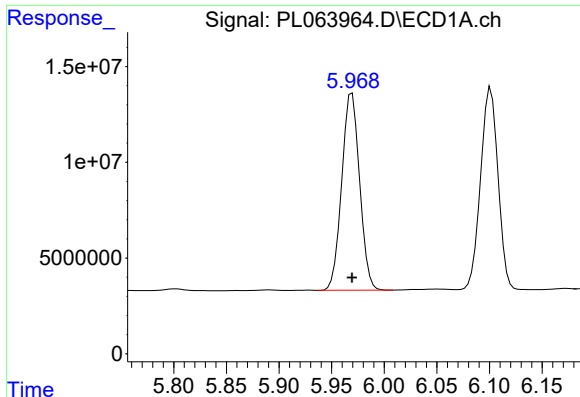

#14 Endrin


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 121954835
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

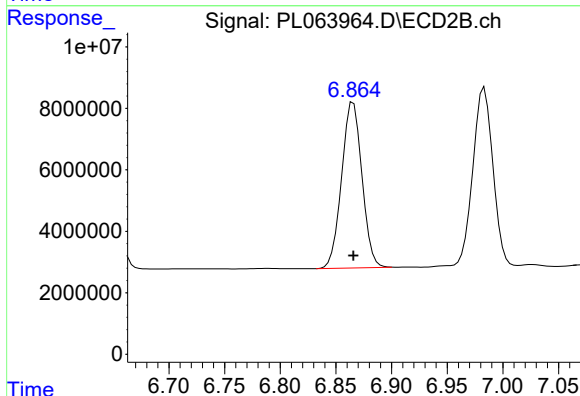


#14 Endrin

R.T.: 6.866 min
Delta R.T.: 0.000 min
Response: 68685568
Conc: 40.00 ng/ml

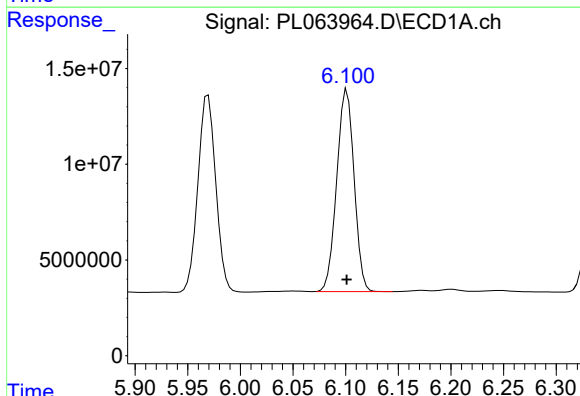


#16 4,4'-DDD

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 121420622
Conc: 40.00 ng/ml

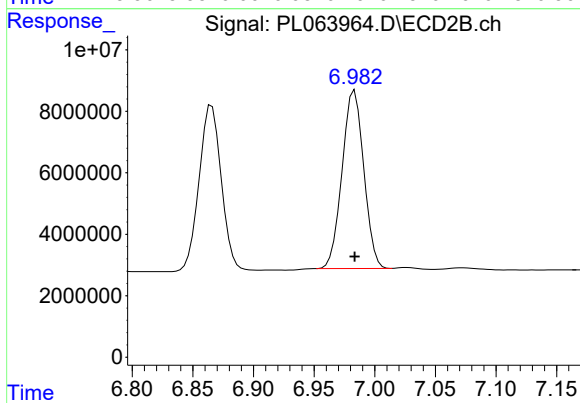

#16 4,4'-DDD


R.T.: 6.983 min
Delta R.T.: 0.000 min
Response: 72159364
Conc: 40.00 ng/ml

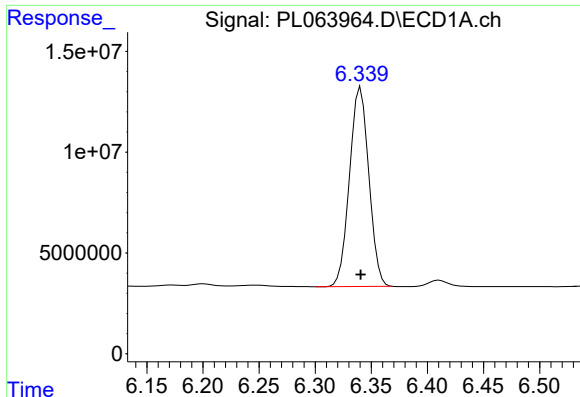

#17 4,4'-DDT


R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 118394825
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

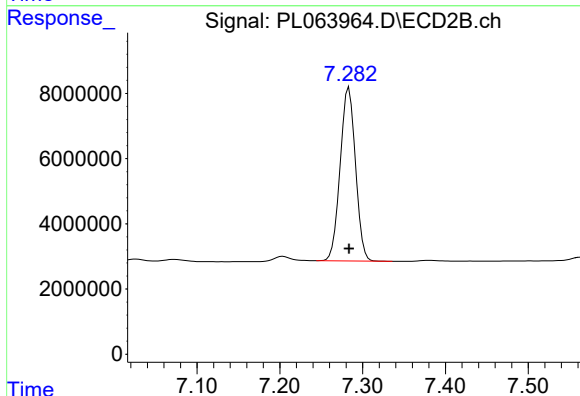


#17 4,4'-DDT

R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 68474296
Conc: 40.00 ng/ml

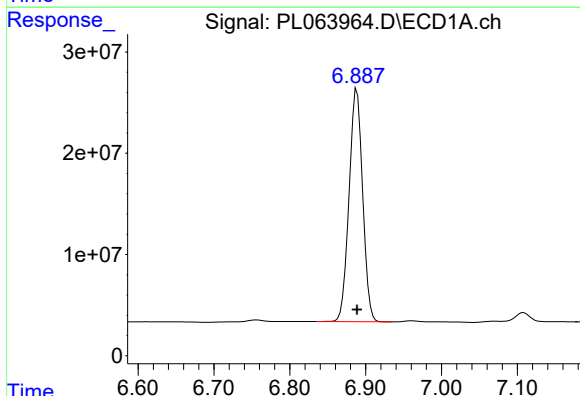


#20 Methoxychlor

R.T.: 6.889 min
Delta R.T.: 0.000 min
Response: 286107333
Conc: 200.00 ng/ml

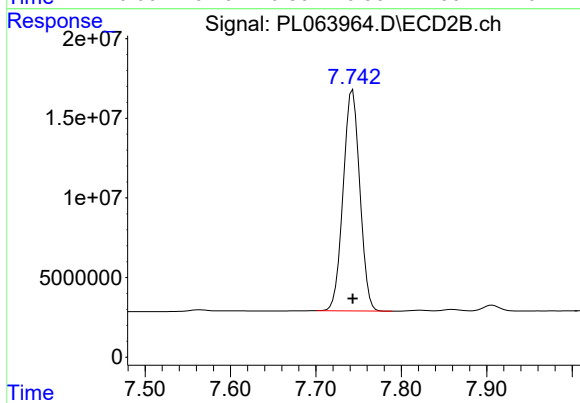

#20 Methoxychlor

R.T.: 7.743 min
Delta R.T.: 0.000 min
Response: 188168217
Conc: 200.00 ng/ml

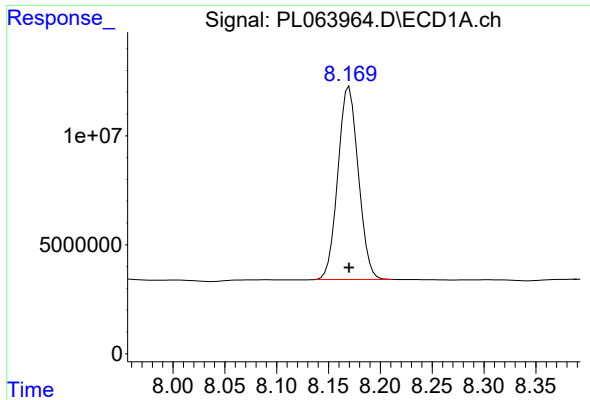

#27 Decachlorobiphenyl


R.T.: 8.170 min

Delta R.T.: 0.000 min

Response: 121481930

Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

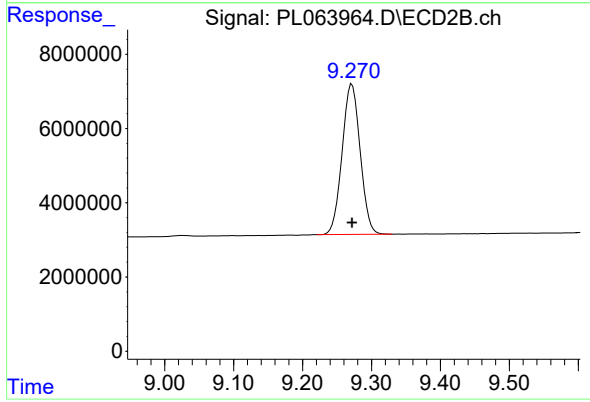

#27 Decachlorobiphenyl

R.T.: 9.272 min

Delta R.T.: 0.000 min

Response: 73713891

Conc: 40.00 ng/ml