

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
 Data File : PL063966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 12:36
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 13:03:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 12:24:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	4.111	122.3E6	94039838	38.220	38.375
27)	SA Decachlor...	8.171	9.271	226.9E6	138.3E6	69.585	69.774
Target Compounds							
2)	A alpha-BHC	3.870	4.513	192.2E6	126.1E6	41.651	42.363
3)	MA gamma-BHC...	4.150	4.805	178.8E6	118.1E6	40.903	40.970
4)	MA Heptachlor	4.450	5.317	172.0E6	111.7E6	38.809	37.782
9)	A Endosulfan I	5.472	6.383	139.9E6	86662527	38.437	37.866
13)	MA Dieldrin	5.715	6.644	311.2E6	187.5E6	80.299	79.724
14)	MA Endrin	5.969	6.866	243.0E6	137.4E6	77.832	77.614
16)	A 4,4'-DDD	6.100	6.984	242.4E6	145.3E6	80.729	82.086
17)	MA 4,4'-DDT	6.340	7.284	240.4E6	139.1E6	82.006	80.703
20)	A Methoxychlor	6.888	7.743	548.3E6	364.9E6	366.757	371.272


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
Data File : PL063966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 12:36
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 13:03:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 12:24:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

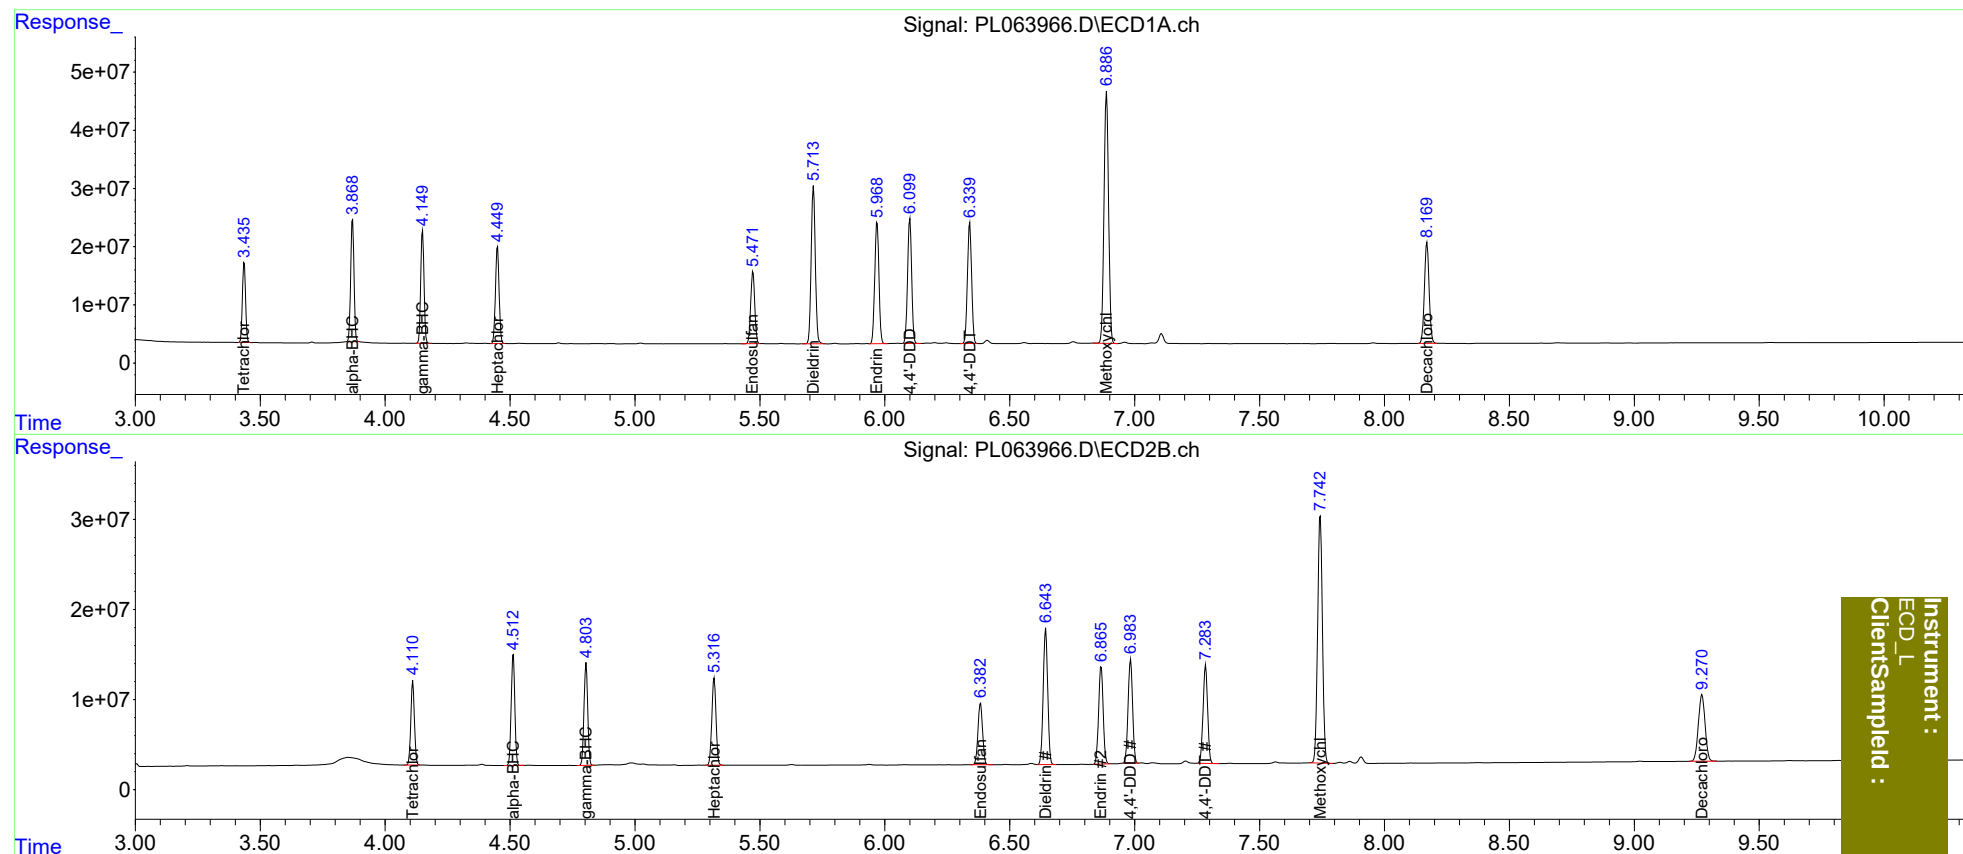


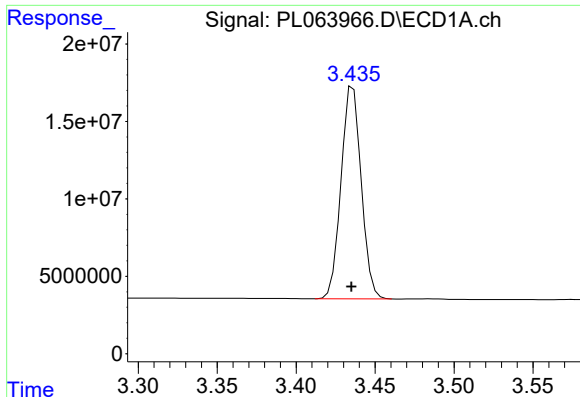

#1 Tetrachloro-m-xylene


R.T.: 3.436 min
Delta R.T.: 0.001 min
Response: 122328994
Conc: 38.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

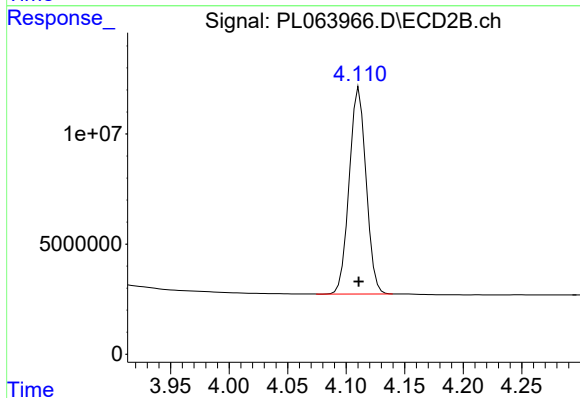


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: 0.000 min
Response: 94039838
Conc: 38.38 ng/ml

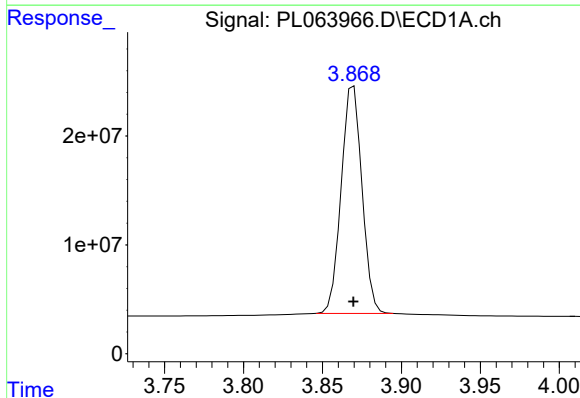


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: 0.000 min
Response: 192212443
Conc: 41.65 ng/ml

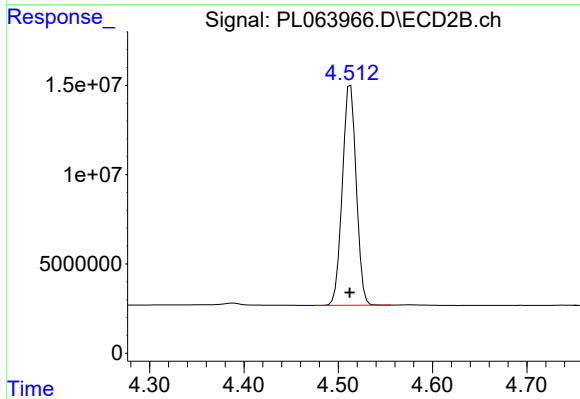

#2 alpha-BHC


R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 126136788
Conc: 42.36 ng/ml

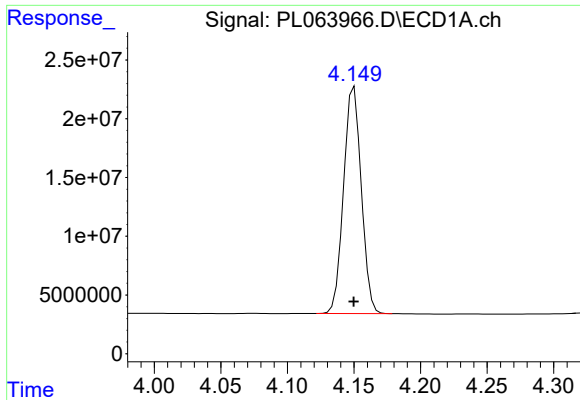

#3 gamma-BHC (Lindane)


R.T.: 4.150 min
Delta R.T.: 0.000 min
Response: 178797005
Conc: 40.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

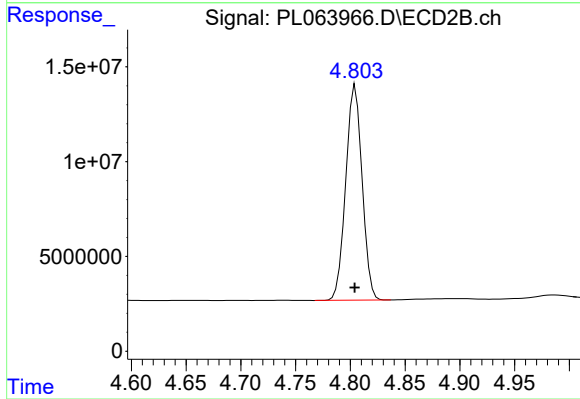


#3 gamma-BHC (Lindane)

R.T.: 4.805 min
Delta R.T.: 0.000 min
Response: 118137662
Conc: 40.97 ng/ml

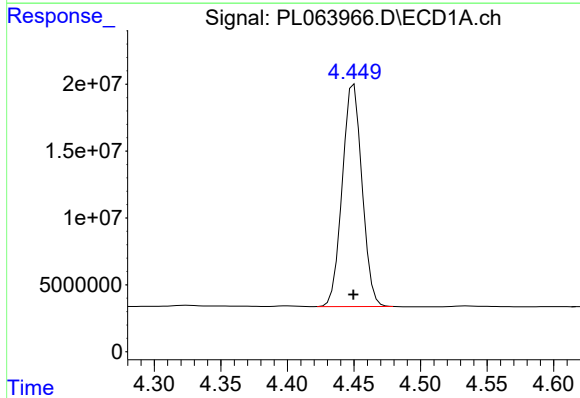


#4 Heptachlor

R.T.: 4.450 min
Delta R.T.: 0.000 min
Response: 172033654
Conc: 38.81 ng/ml

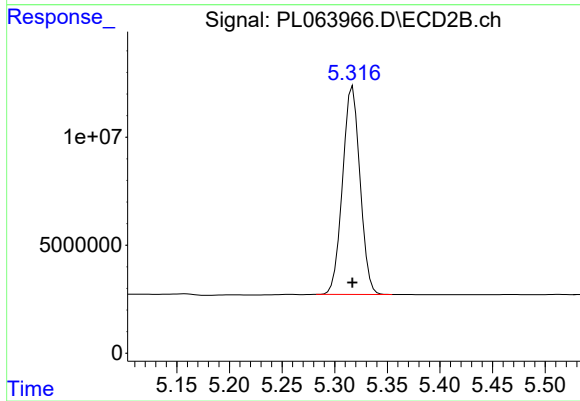

#4 Heptachlor


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 111704418
Conc: 37.78 ng/ml

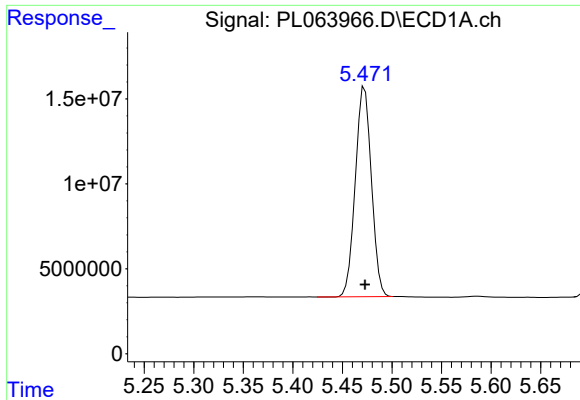

#9 Endosulfan I


R.T.: 5.472 min
Delta R.T.: 0.000 min
Response: 139911431
Conc: 38.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

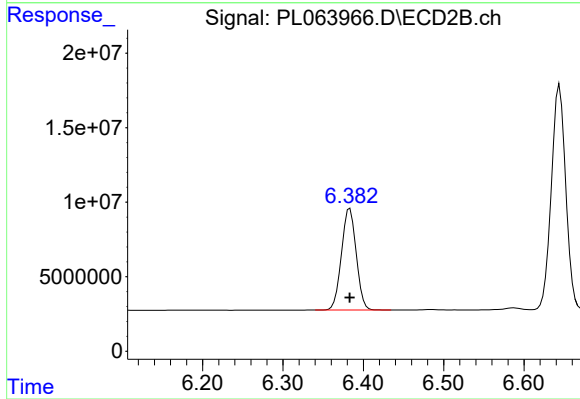


#9 Endosulfan I

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 86662527
Conc: 37.87 ng/ml

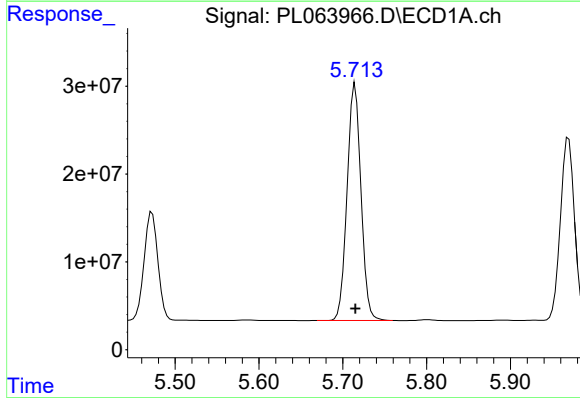


#13 Dieldrin

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 311234182
Conc: 80.30 ng/ml

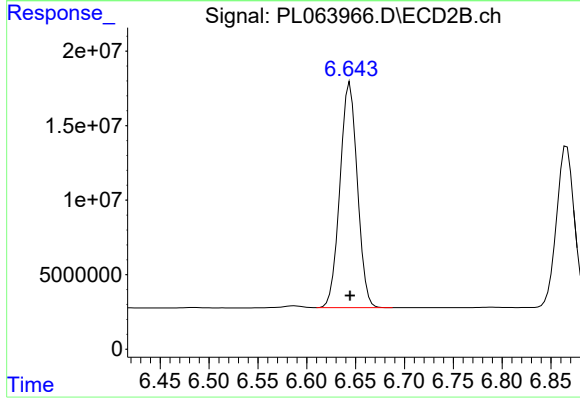

#13 Dieldrin


R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 187490234
Conc: 79.72 ng/ml

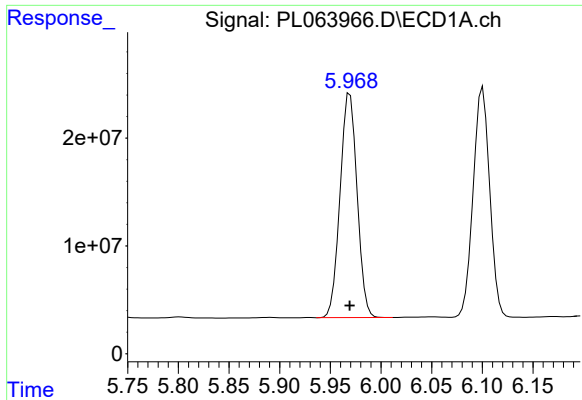

#14 Endrin


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 242991963
Conc: 77.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

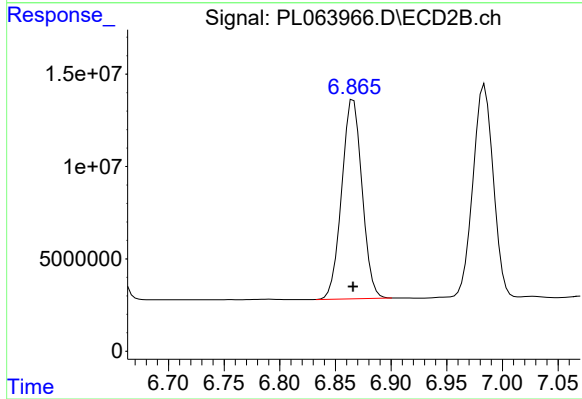


#14 Endrin

R.T.: 6.866 min
Delta R.T.: 0.000 min
Response: 137392081
Conc: 77.61 ng/ml

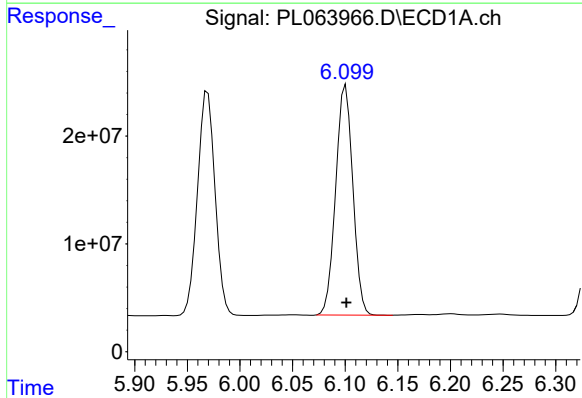


#16 4,4'-DDD

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 242423039
Conc: 80.73 ng/ml

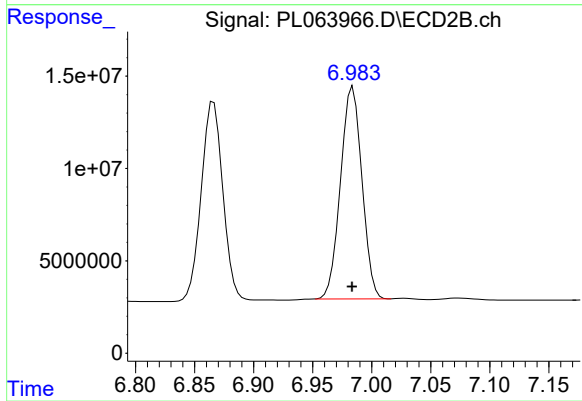

#16 4,4'-DDD


R.T.: 6.984 min
Delta R.T.: 0.000 min
Response: 145291988
Conc: 82.09 ng/ml

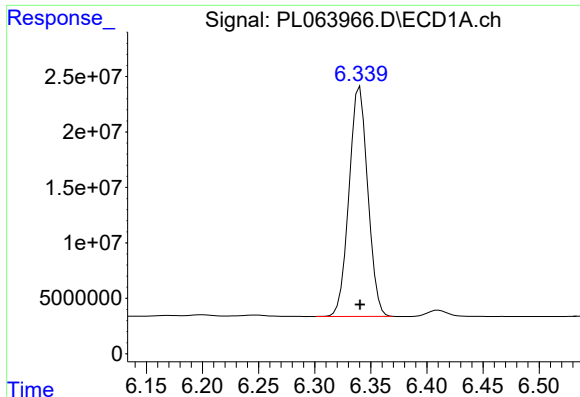

#17 4,4'-DDT


R.T.: 6.340 min
Delta R.T.: 0.000 min
Response: 240408786
Conc: 82.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

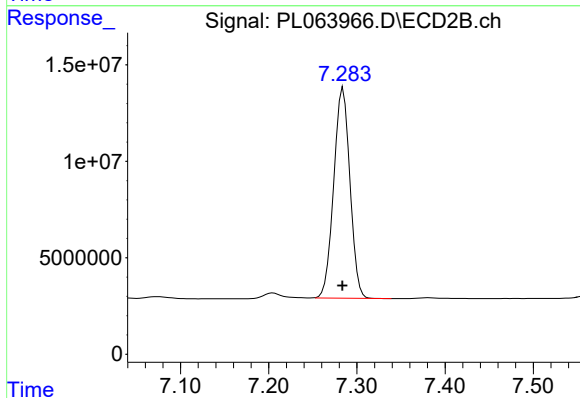


#17 4,4'-DDT

R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 139131282
Conc: 80.70 ng/ml

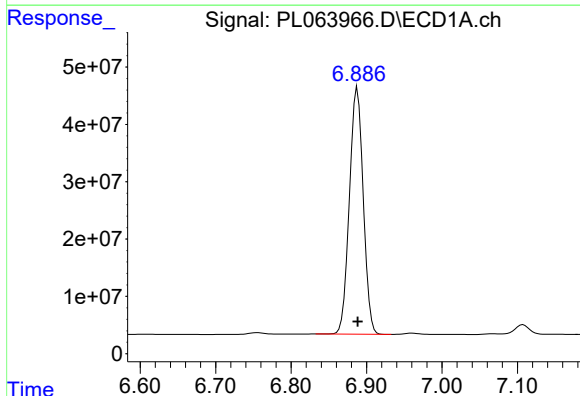


#20 Methoxychlor

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 548334244
Conc: 366.76 ng/ml

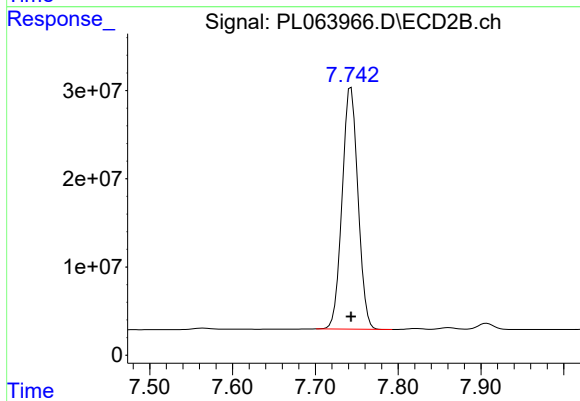

#20 Methoxychlor


R.T.: 7.743 min
Delta R.T.: 0.000 min
Response: 364943499
Conc: 371.27 ng/ml

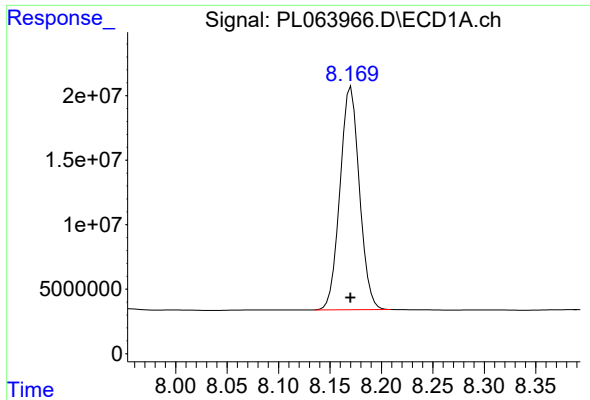

#27 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.000 min
Response: 226868087
Conc: 69.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

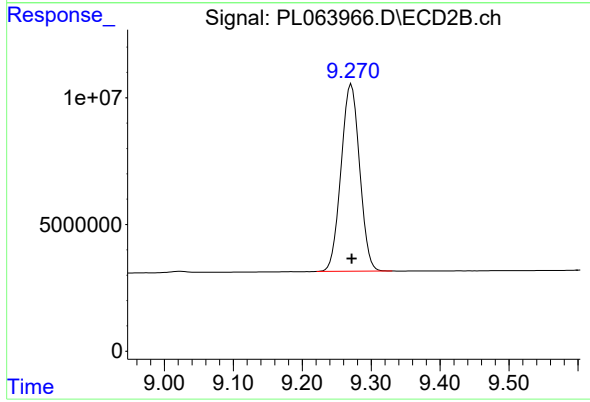

#27 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.000 min
Response: 138292386
Conc: 69.77 ng/ml