

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
 Data File : PL063967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 12:50
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 05:34:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 08 05:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	4.111	116.0E6	89639969	37.575	38.098
27)	SA Decachlor...	8.171	9.272	222.5E6	135.7E6	72.178	72.526
Target Compounds							
5)	MB Aldrin	4.696	5.627	158.2E6	98926455	38.564	38.721
6)	B beta-BHC	4.399	4.980	76473848	57956622	36.520	35.603
7)	B delta-BHC	4.601	5.202	176.3E6	111.7E6	38.747	39.003
8)	B Heptachlo...	5.136	6.021	146.7E6	91234421	37.765	37.659
10)	B trans-Chl...	5.363	6.256	151.5E6	94900303	37.853	37.816
11)	B cis-Chlor...	5.421	6.329	146.6E6	92625340	37.630	37.583
12)	B 4,4'-DDE	5.588	6.486	287.6E6	176.0E6	78.101	78.697
15)	B Endosulfa...	6.242	7.079	242.0E6	146.2E6	75.199	75.550
18)	B Endrin al...	6.410	7.204	203.1E6	124.4E6	74.185	74.880
19)	B Endosulfa...	6.623	7.428	244.4E6	144.0E6	74.772	74.752
21)	B Endrin ke...	7.110	7.907	261.6E6	153.7E6	75.612	76.032

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
Data File : PL063967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 12:50
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 05:34:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 08 05:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

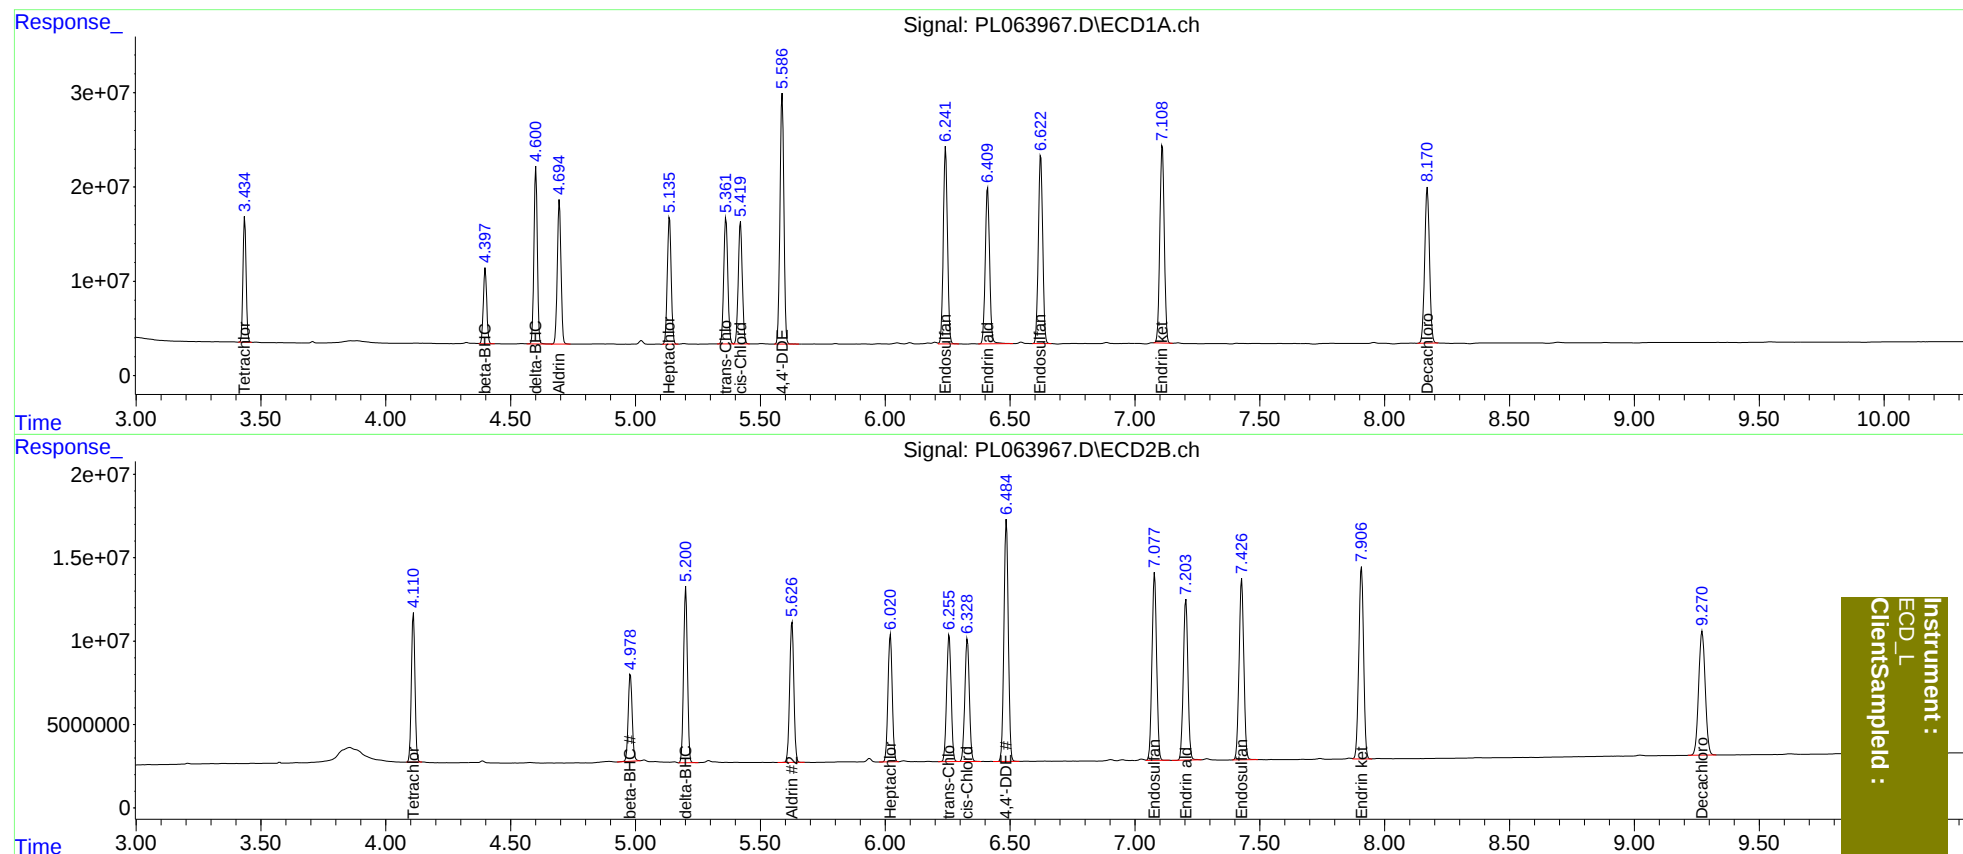


Instrument :
ECD_L
ClientSampled :

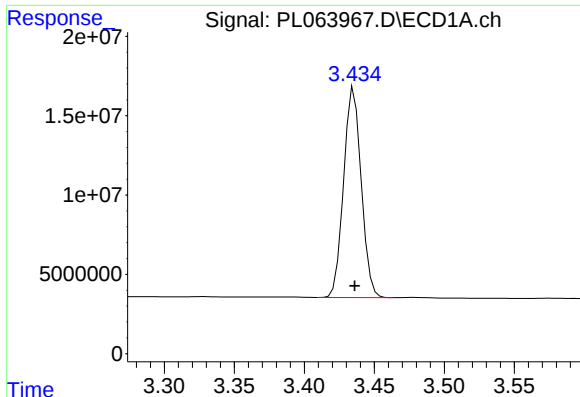

#1 Tetrachloro-m-xylene


R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 116005806
Conc: 37.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

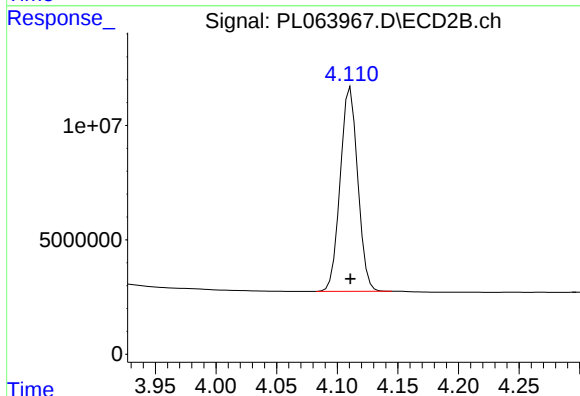


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: 0.000 min
Response: 89639969
Conc: 38.10 ng/ml

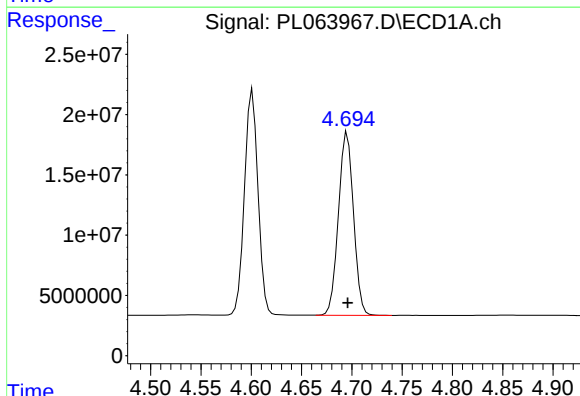


#5 Aldrin

R.T.: 4.696 min
Delta R.T.: 0.000 min
Response: 158242479
Conc: 38.56 ng/ml

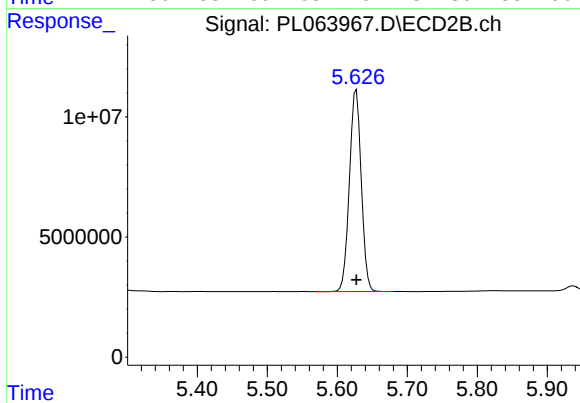

#5 Aldrin


R.T.: 5.627 min
Delta R.T.: 0.000 min
Response: 98926455
Conc: 38.72 ng/ml

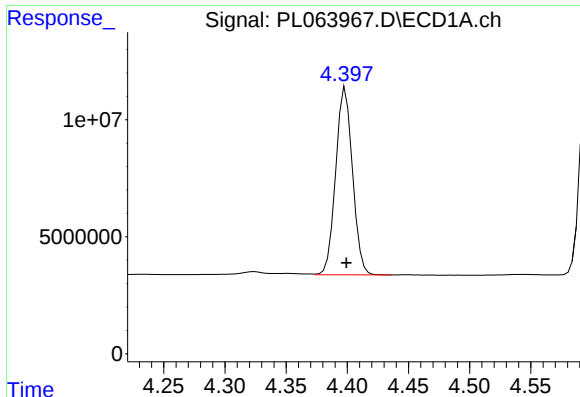

#6 beta-BHC


R.T.: 4.399 min
Delta R.T.: 0.000 min
Response: 76473848
Conc: 36.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

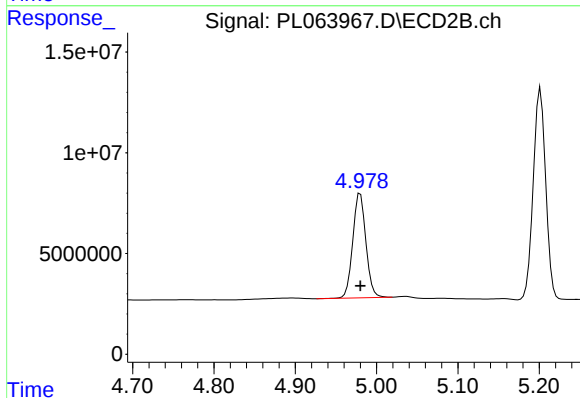


#6 beta-BHC

R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 57956622
Conc: 35.60 ng/ml

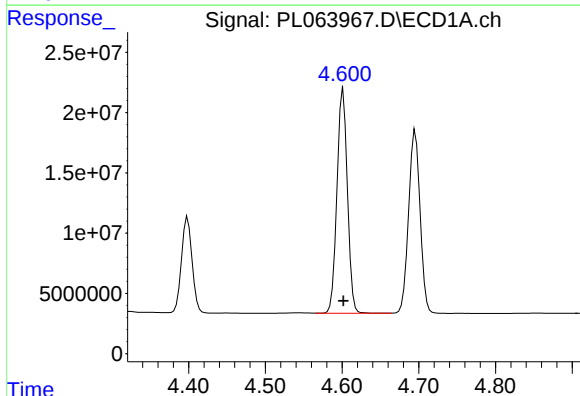


#7 delta-BHC

R.T.: 4.601 min
Delta R.T.: 0.000 min
Response: 176321514
Conc: 38.75 ng/ml

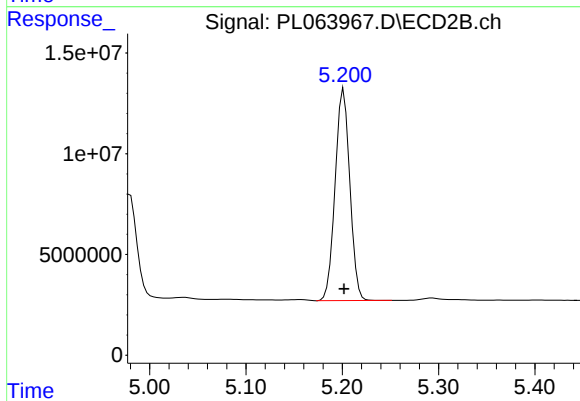

#7 delta-BHC


R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 111721987
Conc: 39.00 ng/ml

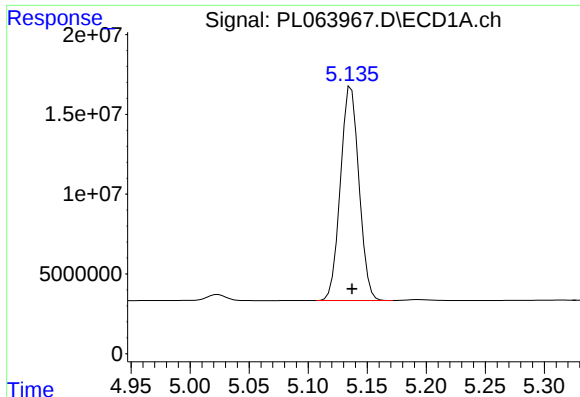

#8 Heptachlor epoxide


R.T.: 5.136 min
Delta R.T.: 0.000 min
Response: 146701970
Conc: 37.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

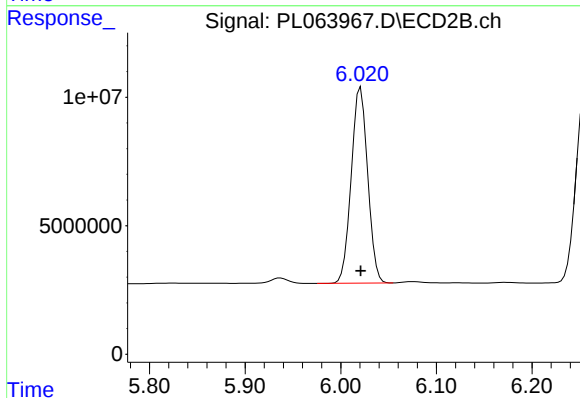


#8 Heptachlor epoxide

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 91234421
Conc: 37.66 ng/ml

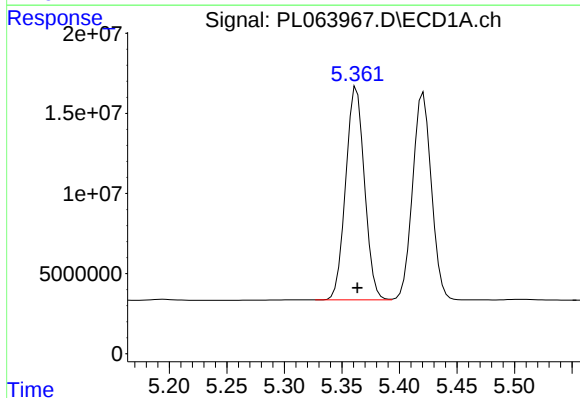


#10 trans-Chlordane

R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 151544912
Conc: 37.85 ng/ml

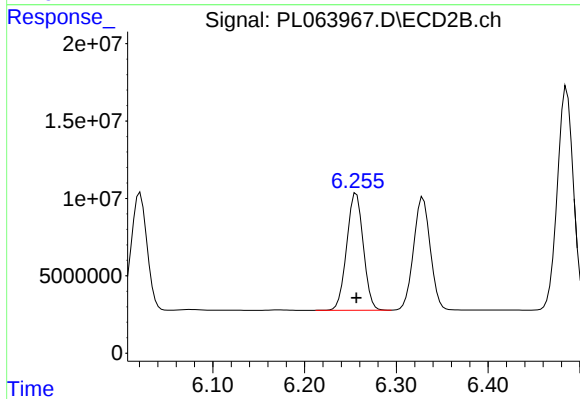

#10 trans-Chlordane


R.T.: 6.256 min
Delta R.T.: 0.000 min
Response: 94900303
Conc: 37.82 ng/ml

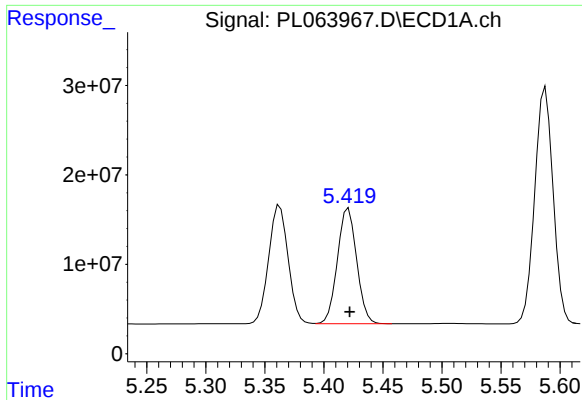

#11 cis-Chlordane


R.T.: 5.421 min
Delta R.T.: 0.000 min
Response: 146643137
Conc: 37.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

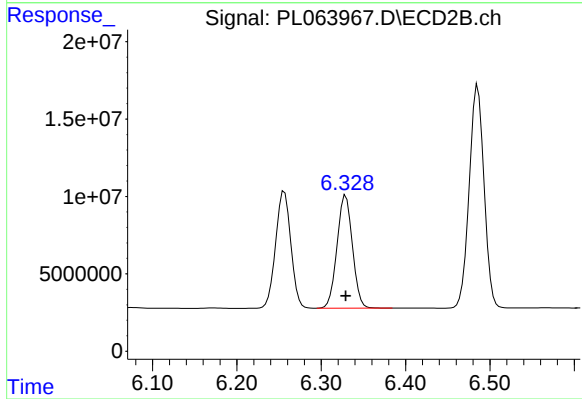


#11 cis-Chlordane

R.T.: 6.329 min
Delta R.T.: 0.000 min
Response: 92625340
Conc: 37.58 ng/ml

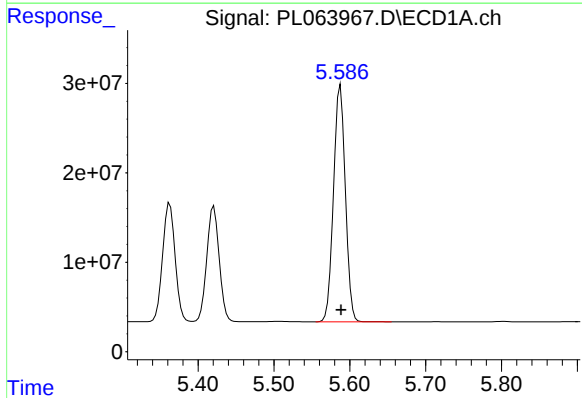


#12 4,4'-DDE

R.T.: 5.588 min
Delta R.T.: 0.000 min
Response: 287594338
Conc: 78.10 ng/ml

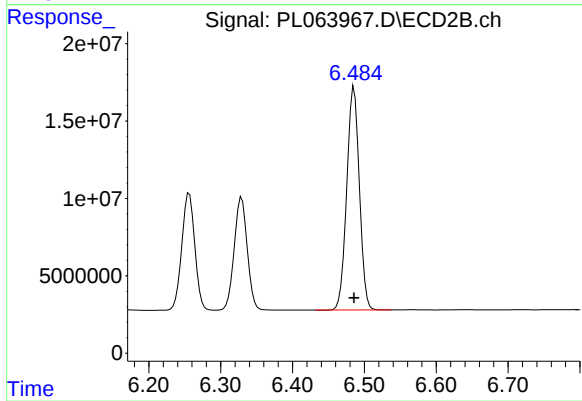

#12 4,4'-DDE


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 175956055
Conc: 78.70 ng/ml

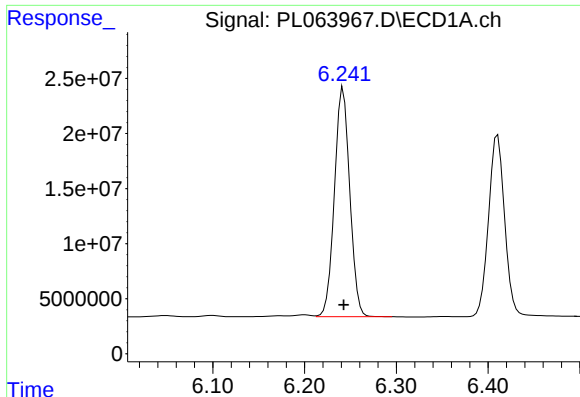

#15 Endosulfan II


R.T.: 6.242 min
Delta R.T.: 0.000 min
Response: 242044240
Conc: 75.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

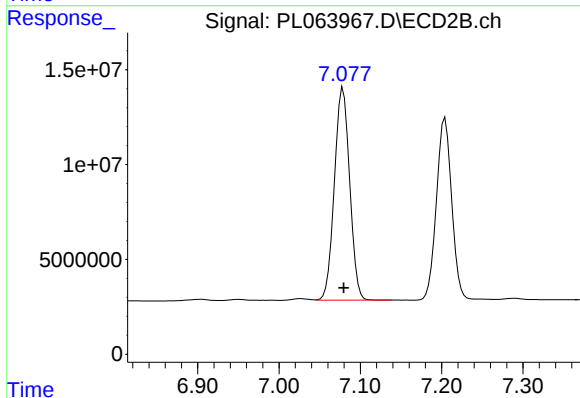


#15 Endosulfan II

R.T.: 7.079 min
Delta R.T.: 0.000 min
Response: 146187898
Conc: 75.55 ng/ml

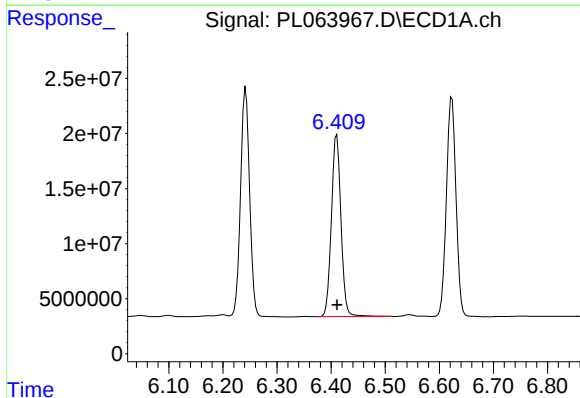


#18 Endrin aldehyde

R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 203109639
Conc: 74.19 ng/ml

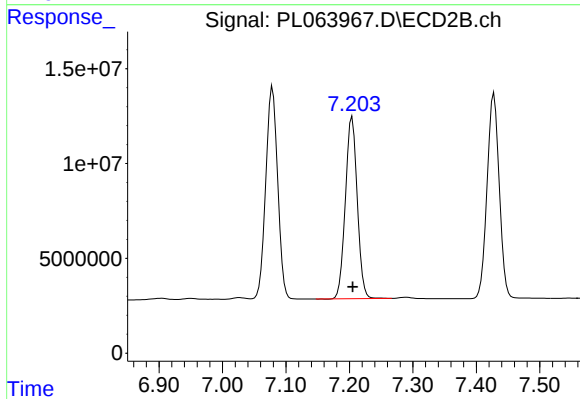

#18 Endrin aldehyde


R.T.: 7.204 min
Delta R.T.: 0.000 min
Response: 124412273
Conc: 74.88 ng/ml

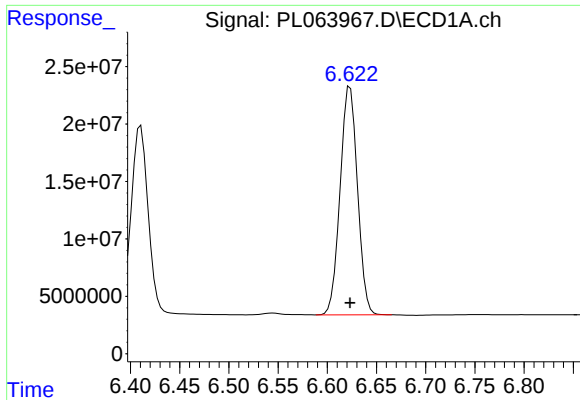

#19 Endosulfan Sulfate


R.T.: 6.623 min
Delta R.T.: 0.000 min
Response: 244439059
Conc: 74.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

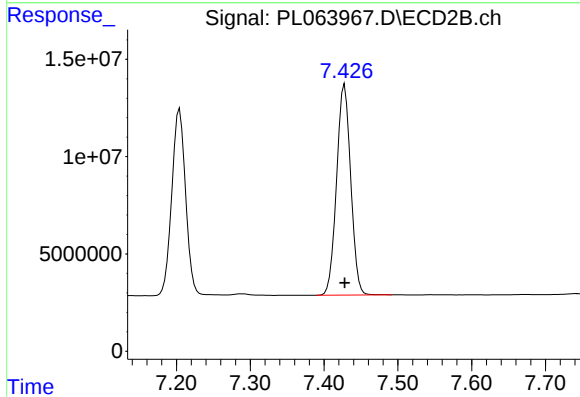


#19 Endosulfan Sulfate

R.T.: 7.428 min
Delta R.T.: 0.000 min
Response: 143967785
Conc: 74.75 ng/ml

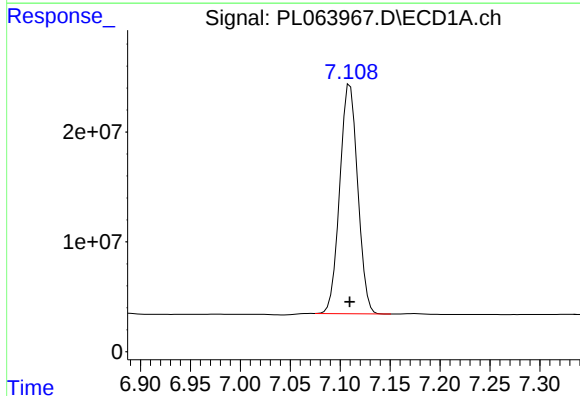


#21 Endrin ketone

R.T.: 7.110 min
Delta R.T.: 0.000 min
Response: 261636303
Conc: 75.61 ng/ml

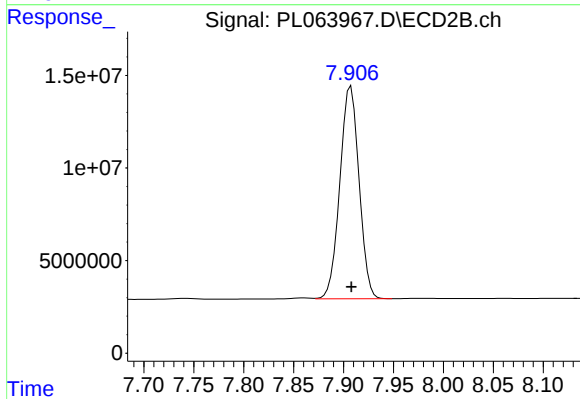

#21 Endrin ketone


R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 153686779
Conc: 76.03 ng/ml

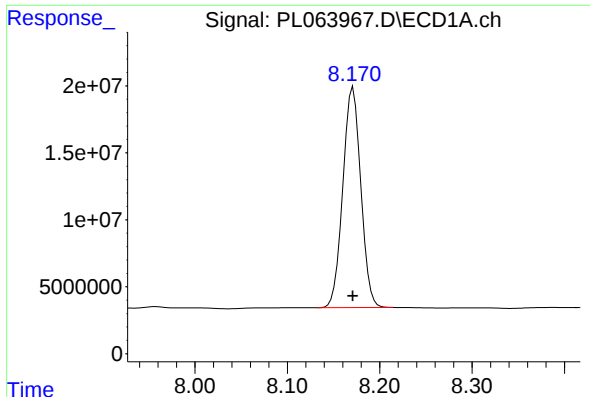

#27 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.000 min
Response: 222493091
Conc: 72.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

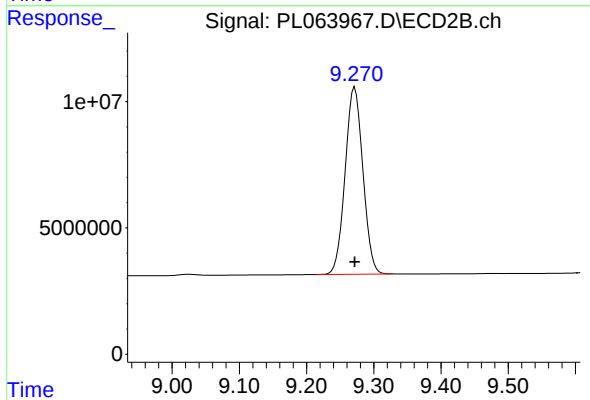

#27 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 135719983
Conc: 72.53 ng/ml