

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
 Data File : PL063975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 15:14
 Operator : AR\AJ
 Sample : PB133915BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 02:02:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 13:41:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.111	60493280	46324358	19.290	19.261
27)	SA Decachlor...	8.171	9.272	119.0E6	72792402	38.876	39.103
Target Compounds							
6)	B beta-BHC	0.000	4.991	0	2953388	N.D.	1.708
15)	B Endosulfa...	6.200f	0.000	1749515	0	0.542	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
Data File : PL063975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 15:14
Operator : AR\AJ
Sample : PB133915BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 02:02:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 13:41:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

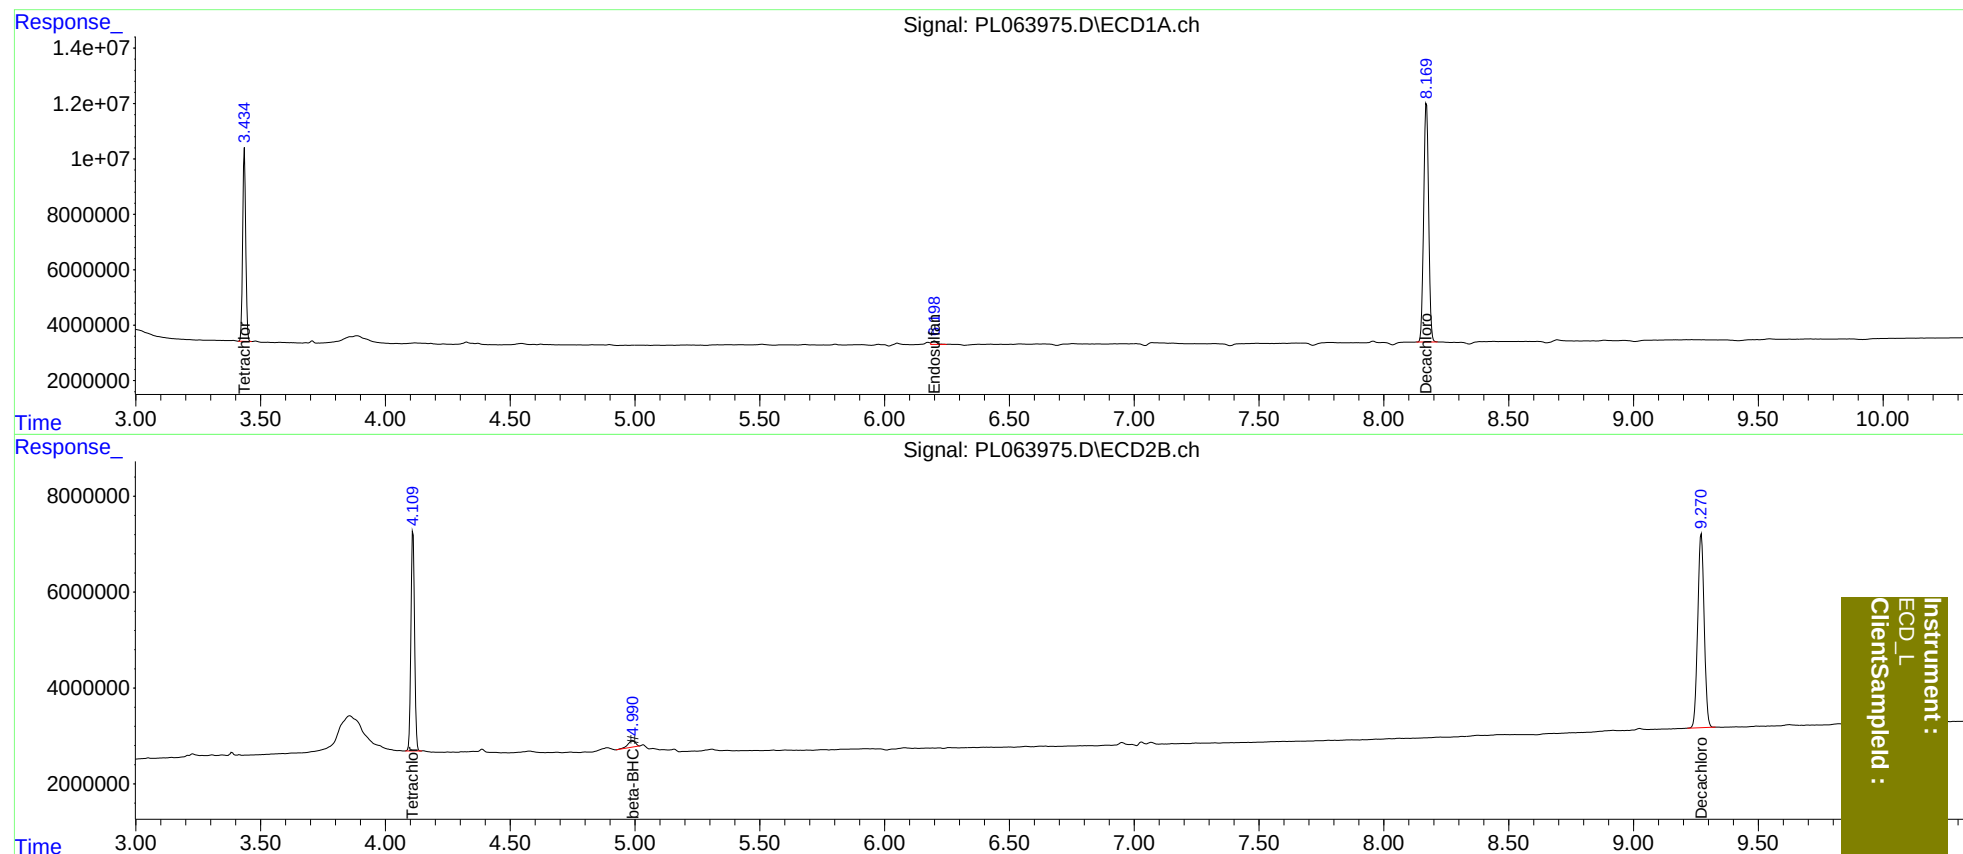


Instrument :
ECD_L
ClientSampleId :

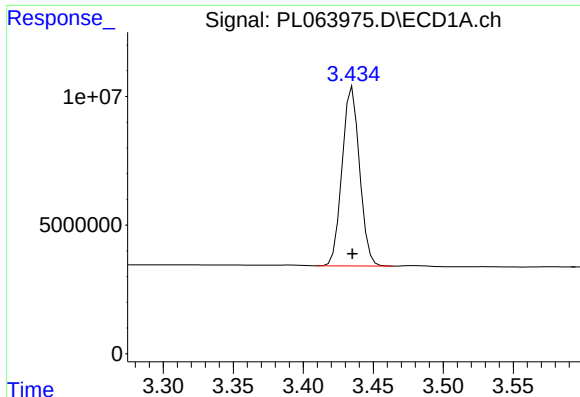

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 60493280
Conc: 19.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

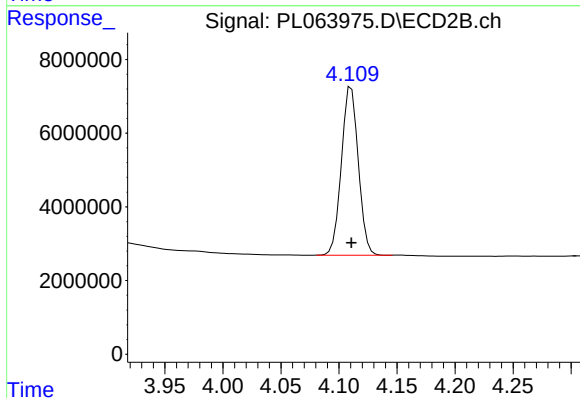


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: 0.000 min
Response: 46324358
Conc: 19.26 ng/ml

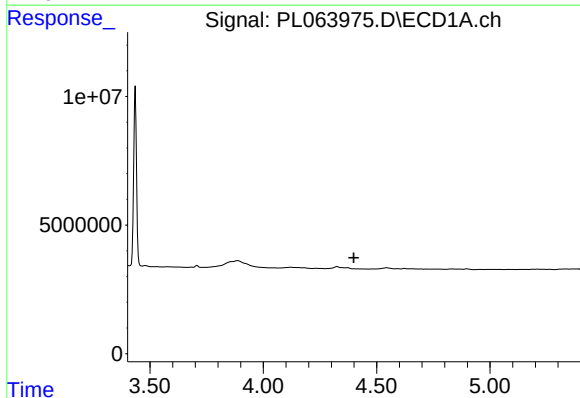


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.399 min
Response: 0
Conc: N.D.

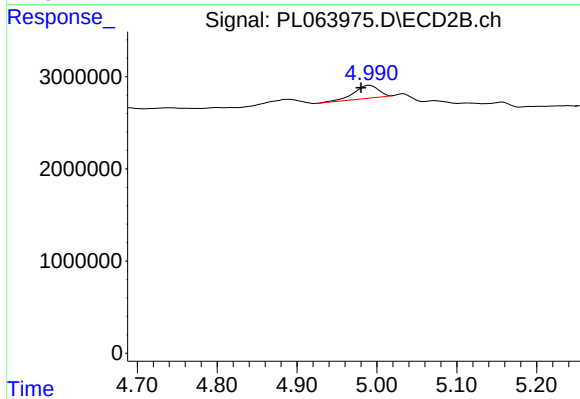

#6 beta-BHC


R.T.: 4.991 min
Delta R.T.: 0.011 min
Response: 2953388
Conc: 1.71 ng/ml

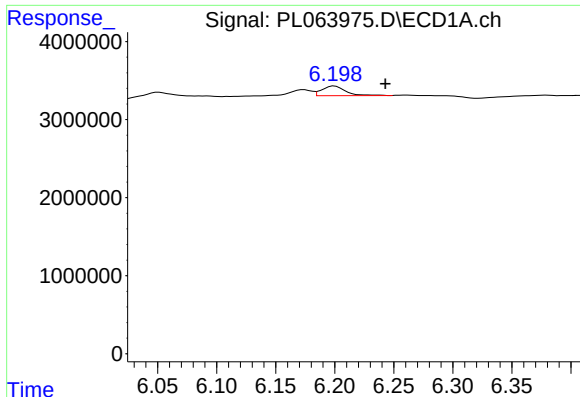

#15 Endosulfan II


R.T.: 6.200 min
Delta R.T.: -0.043 min
Response: 1749515
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

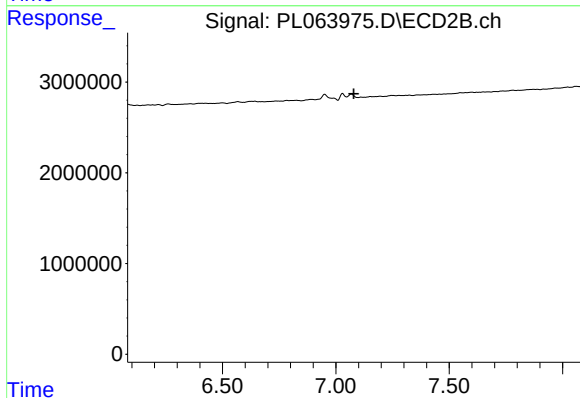


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.080 min
Response: 0
Conc: N.D.

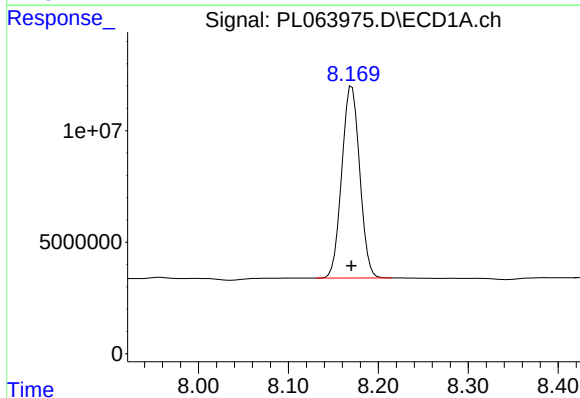

#27 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.000 min
Response: 119049075
Conc: 38.88 ng/ml

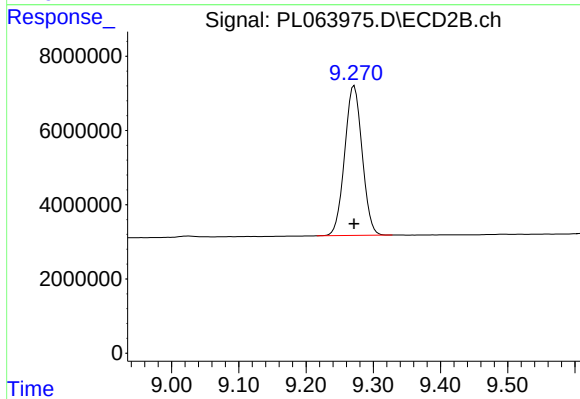

#27 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 72792402
Conc: 39.10 ng/ml