

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\
 Data File : PL063976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 15:28
 Operator : AR\AJ
 Sample : L5214-01
 Misc : PEST MDL 1 PPB
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT1-2021-01

Manual Integrations
 APPROVED

Ankita
 1/8/2021 10:14:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 09:34:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 08 05:48:24 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.111	56987160	43645509	18.172	18.147
27)	SA Decachlor...	8.170	9.270	113.1E6	68970205	36.918	37.050
Target Compounds							
2)	A alpha-BHC	3.868	4.512	4524477	2486843	0.959	0.808
3)	MA gamma-BHC...	4.149	4.803	3993166	2477688	0.902	0.846
4)	MA Heptachlor	4.449	5.316	4463891	2855832	1.020	0.987
5)	MB Aldrin	4.694	5.626	3623369	2101278	0.879	0.808
6)	B beta-BHC	4.398	4.981	1906413	2714950	0.911	1.547 #
7)	B delta-BHC	4.600	5.200	4049666	2075039	0.884	0.717
8)	B Heptachlo...	5.136	6.020	3815106	2517460	0.978	1.048
9)	A Endosulfan I	5.472	6.383	3406235	2196540	0.953	0.982
10)	B trans-Chl...	5.362	6.255	3886739	2444784	0.964	0.967
11)	B cis-Chlor...	5.420	6.328	3992621	2357689	1.019	0.951
12)	B 4,4'-DDE	5.585	6.484	3429772	2024501	0.929m	0.895
13)	MA Dieldrin	5.712	6.643	3583409	2216591	0.923m	0.941
14)	MA Endrin	5.969	6.866	4262658	1611908	1.381m	0.919 #
15)	B Endosulfa...	6.241	7.075	3555267	2504983	1.097	1.271m
16)	A 4,4'-DDD	6.099	6.982	2761880	2179607	0.916	1.214 #
17)	MA 4,4'-DDT	6.338	7.281	2532180	1292951	0.852m	0.742m
18)	B Endrin al...	6.410	7.203	3065787	1950131	1.116	1.168
19)	B Endosulfa...	6.622	7.427	3578880	1957505	1.091	1.004
20)	A Methoxychlor	6.886	7.743	1440588	976509	1.007m	1.028
21)	B Endrin ke...	7.107	7.906	3563814	1902350	1.031m	0.935

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

```
Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010721\  
Data File : PL063976.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On    : 07 Jan 2021 15:28  
Operator  : AR\AJ  
Sample    : L5214-01  
Misc      : PEST MDL 1 PPB  
ALS Vial  : 25 Sample Multiplier: 1
```

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 09:34:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010721CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 08 05:48:24 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

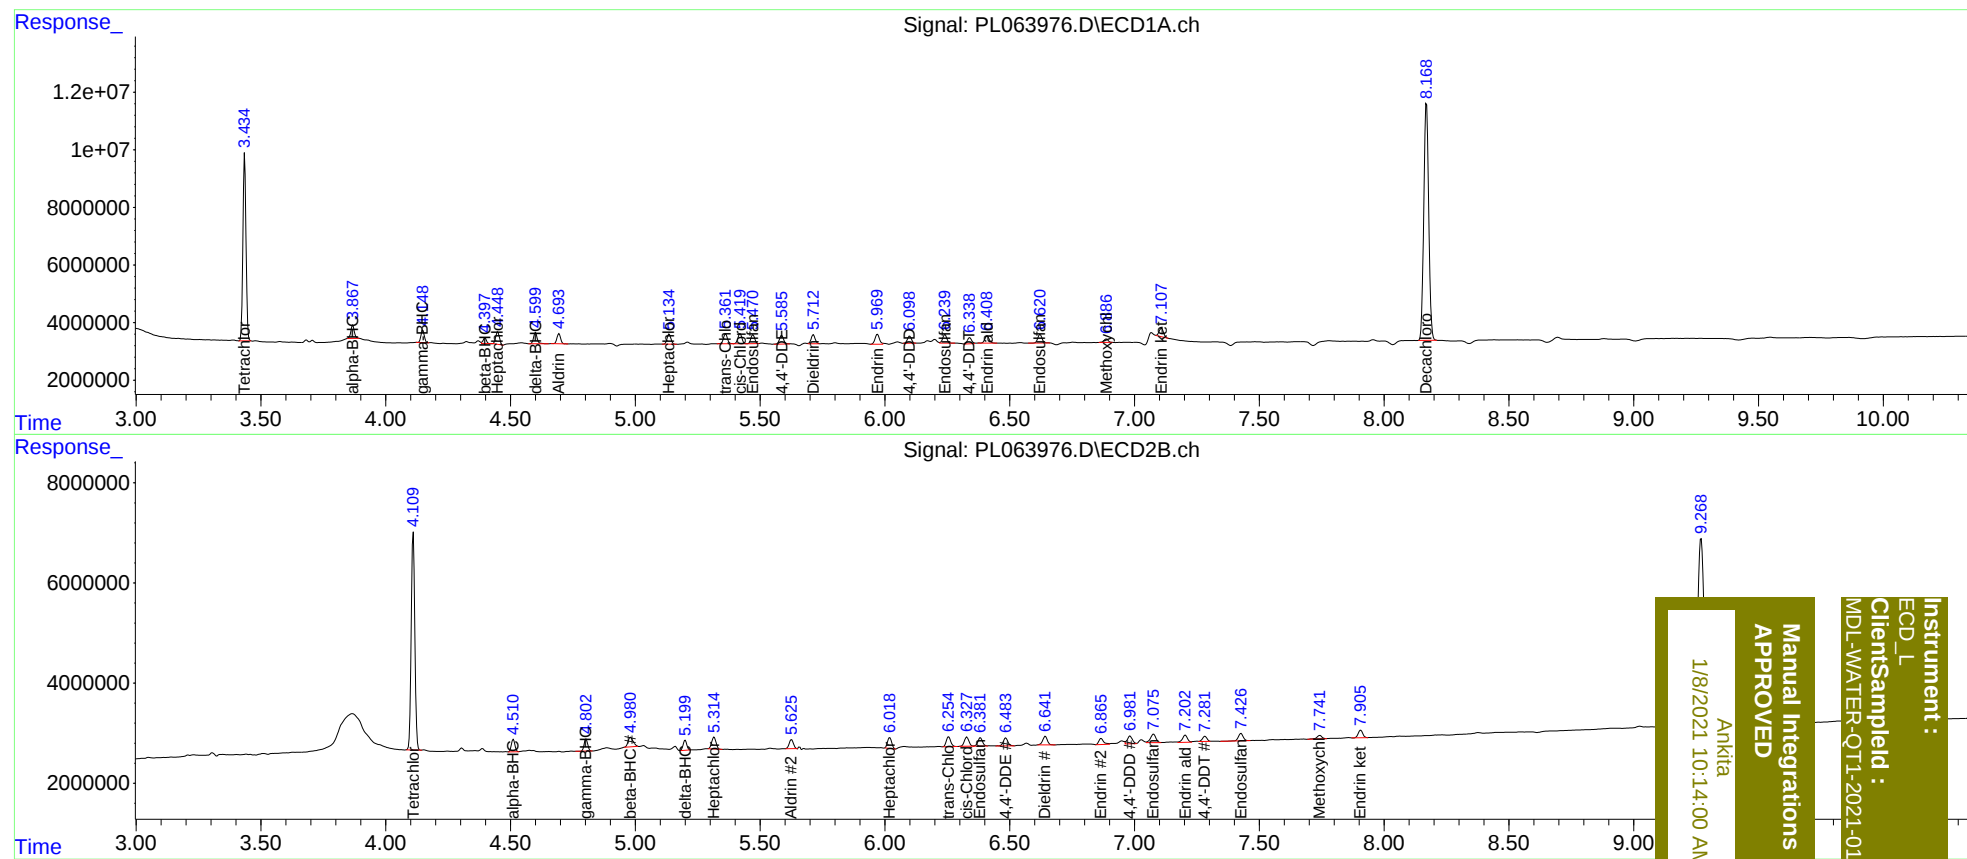

1/8/2021 10:14:00 AM 892.6

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientsSampled :
MDL-WATER-QT1-2021-01