

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010820\
 Data File : PL055607.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2020 16:57
 Operator : AJ\MA
 Sample : K6474-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 03:36:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010820.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 08 12:19:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.500	4.013	199.5E6	60558923	17.883	19.698
28) SA Decachlor...	8.260	9.085	195.4E6	47536483	20.145	20.548
Target Compounds						
7) B delta-BHC	0.000	5.048f	0	3254721	N.D.	0.953 #
23) Chlordane-1	4.405f	0.000	11051836	0	27.559	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010820\
Data File : PL055607.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2020 16:57
Operator : AJ\MA
Sample : K6474-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:36:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010820.M
Quant Title : GC Extractables
QLast Update : Wed Jan 08 12:19:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

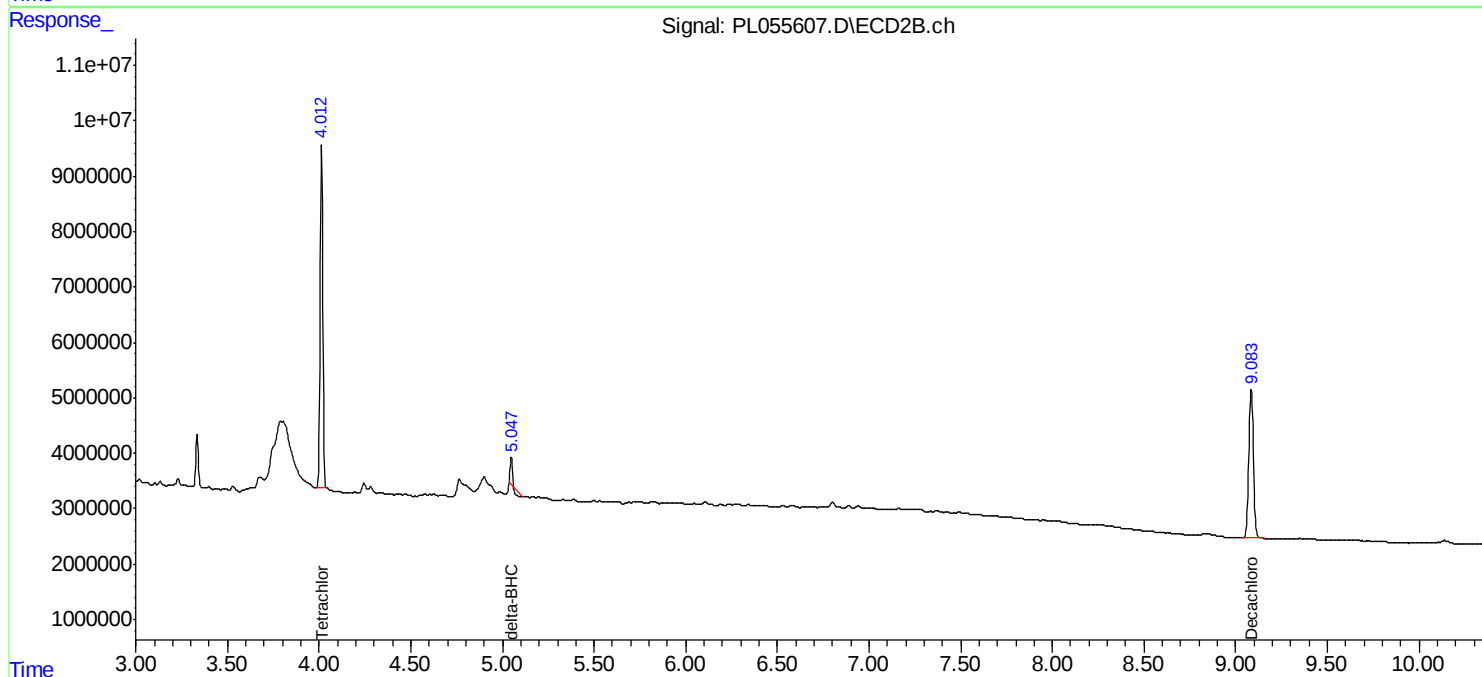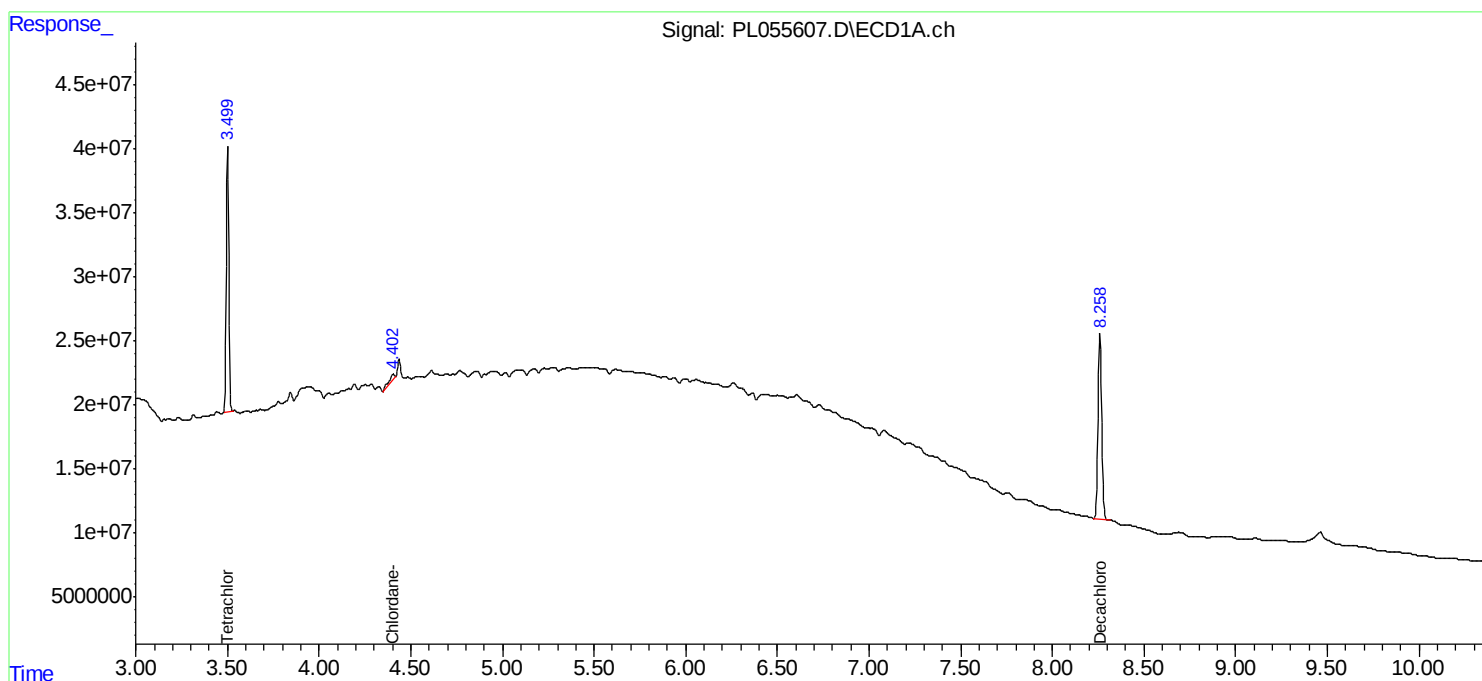


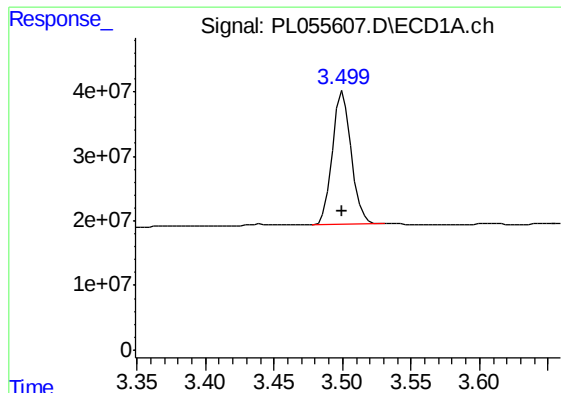

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 199452467
Conc: 17.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

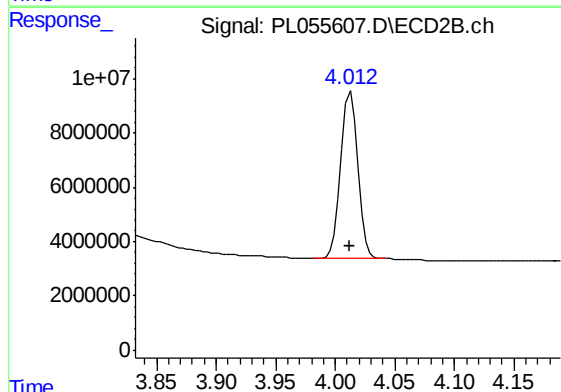


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 60558923
Conc: 19.70 ng/ml

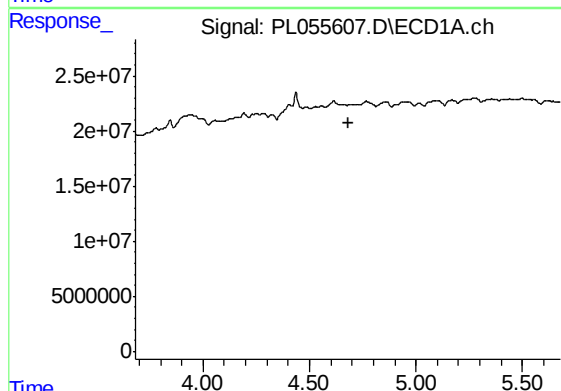


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.681 min
Response: 0
Conc: N.D.

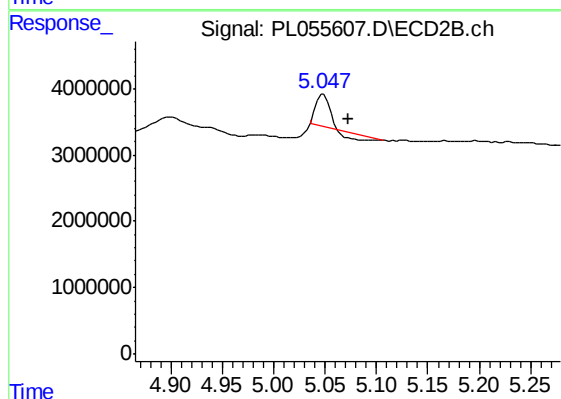

#7 delta-BHC


R.T.: 5.048 min
Delta R.T.: -0.025 min
Response: 3254721
Conc: 0.95 ng/ml

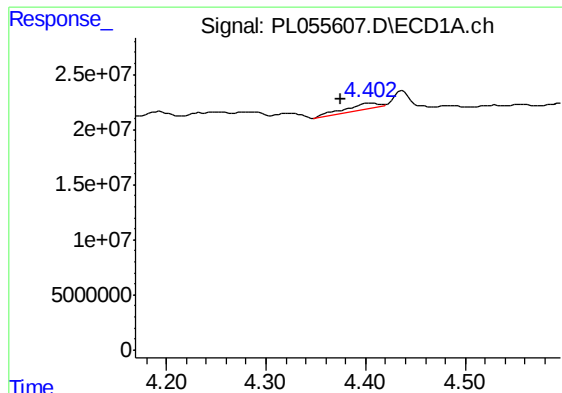

#23 Chlordane-1


R.T.: 4.405 min
Delta R.T.: 0.030 min
Response: 11051836
Conc: 27.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

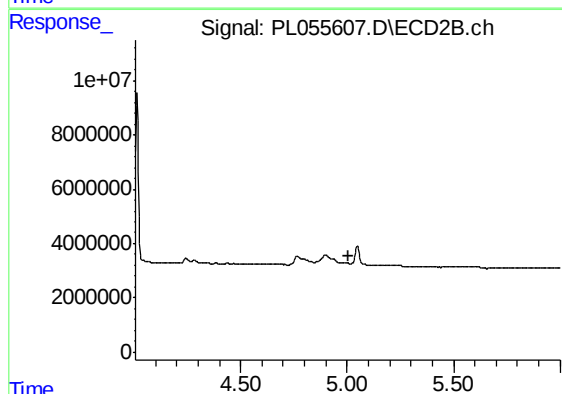


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

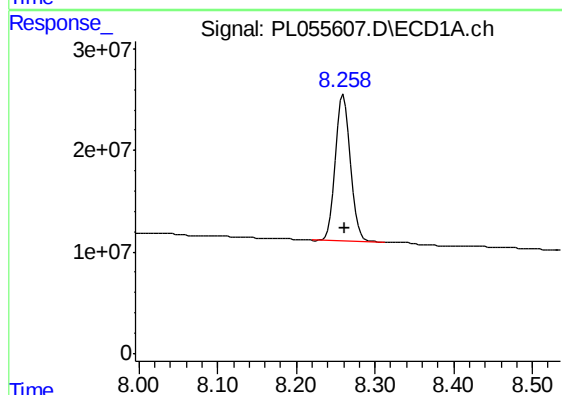

#28 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: 0.000 min
Response: 195438419
Conc: 20.14 ng/ml

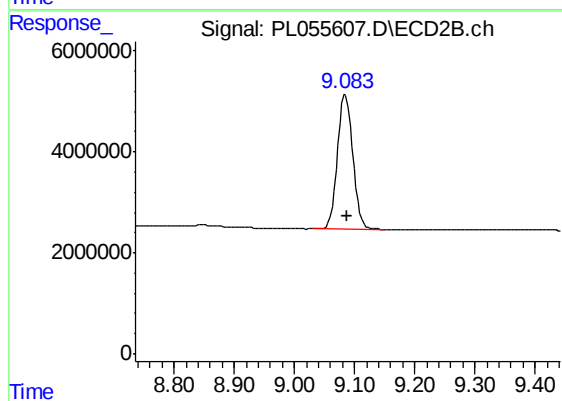

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.004 min
Response: 47536483
Conc: 20.55 ng/ml