

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010820\
 Data File : PL055580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2020 10:20
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 11:49:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010820.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 08 11:49:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.013	231.4E6	64876266	20.747	21.102
28)	SA Decachlor...	8.261	9.087	201.9E6	49487038	20.813	21.391
Target Compounds							
9)	A Endosulfan I	5.560	6.240	147.4E6	31504011	9.722	10.206
10)	B gamma-Chl...	5.447	6.117	155.3E6	33069794	9.449	10.079
12)	B 4,4'-DDE	5.668	6.347	299.6E6	61194240	19.882	19.829
13)	MA Dieldrin	5.803	6.497	317.5E6	63241879	19.808	19.959
19)	B Endosulfa...	6.715	7.274	212.8E6	49339927	18.993	19.571
20)	A Methoxychlor	6.970	7.599	549.0E6	121.5E6	99.889	94.541
21)	B Endrin ke...	7.207	7.747	240.5E6	52910513	19.659	20.110



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010820\
Data File : PL055580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2020 10:20
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 11:49:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010820.M
Quant Title : GC Extractables
QLast Update : Wed Jan 08 11:49:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

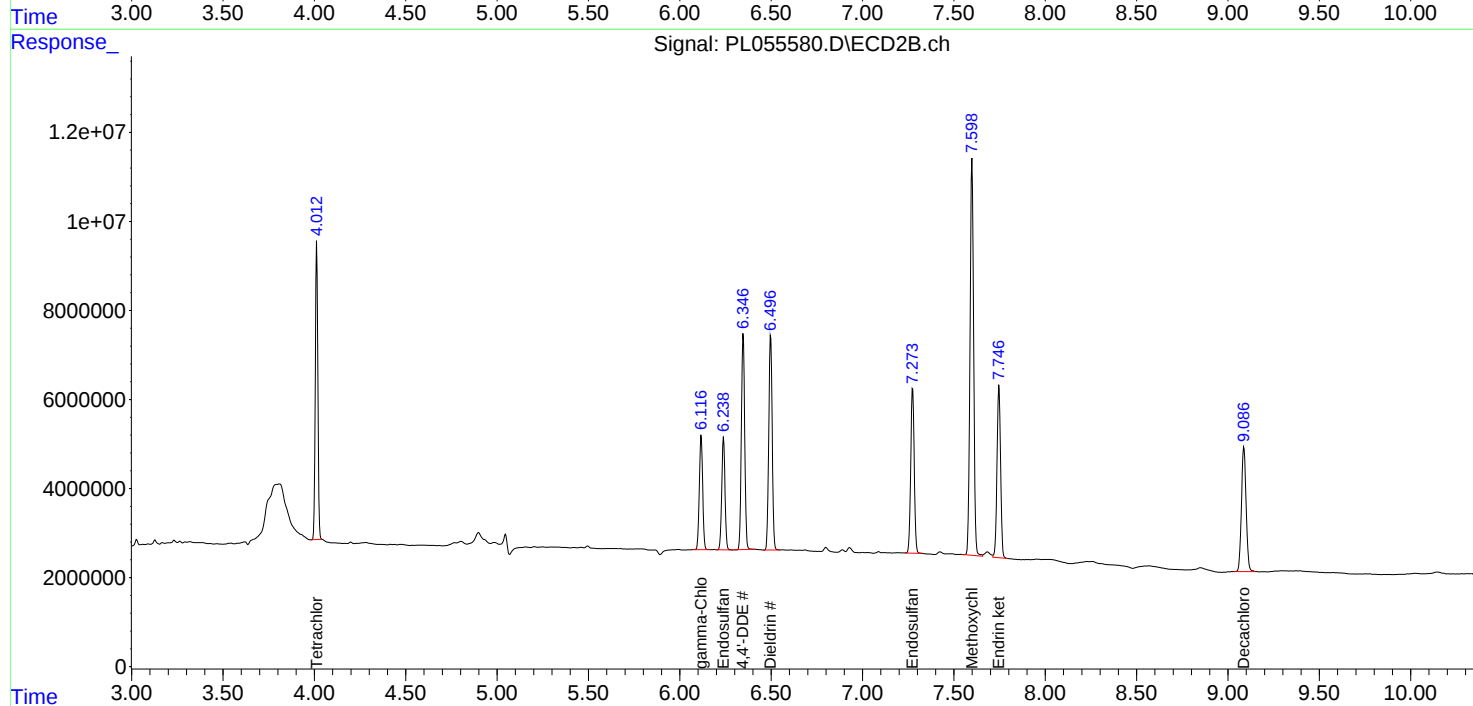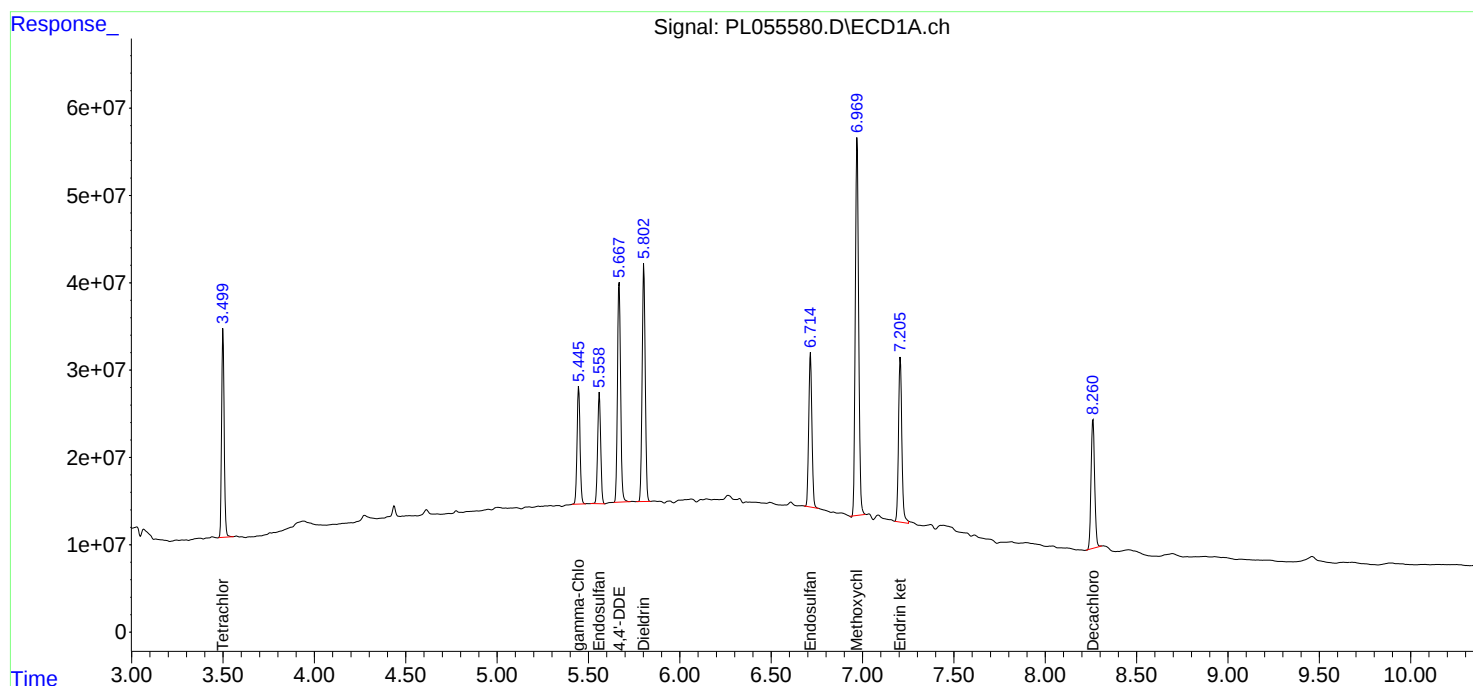


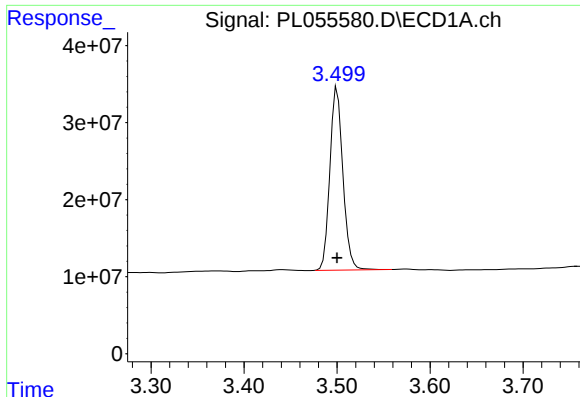

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 231385097
Conc: 20.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

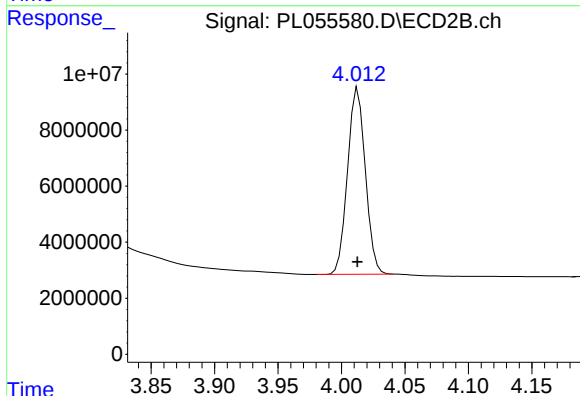


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 64876266
Conc: 21.10 ng/ml

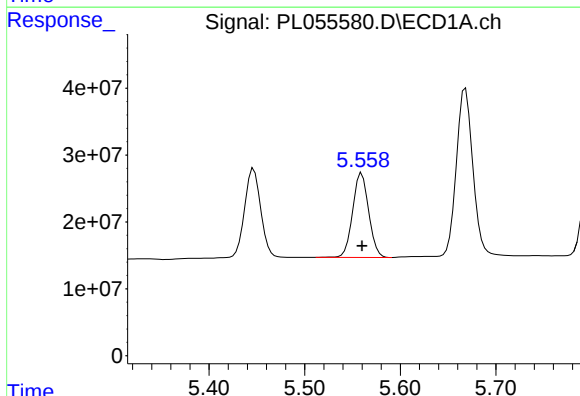


#9 Endosulfan I

R.T.: 5.560 min
Delta R.T.: 0.000 min
Response: 147449259
Conc: 9.72 ng/ml

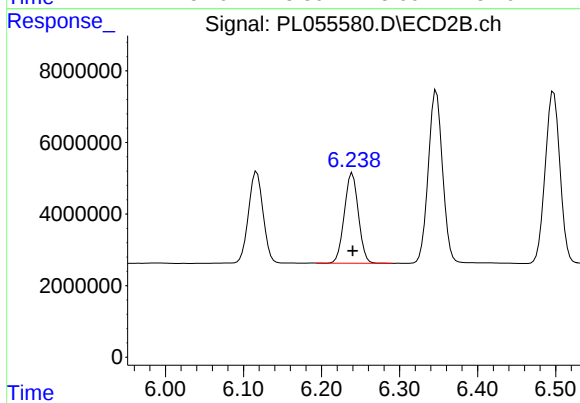

#9 Endosulfan I


R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 31504011
Conc: 10.21 ng/ml

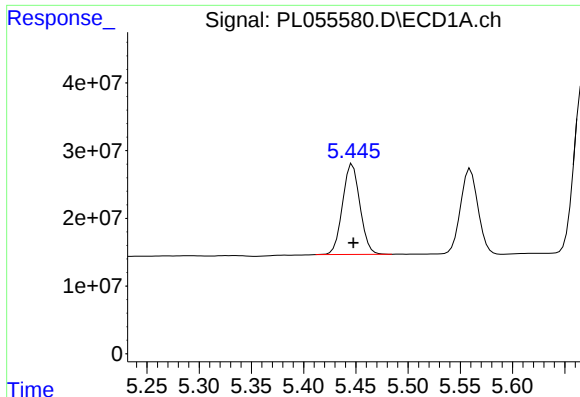

#10 gamma-Chlordane


R.T.: 5.447 min
Delta R.T.: 0.000 min
Response: 155293057
Conc: 9.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

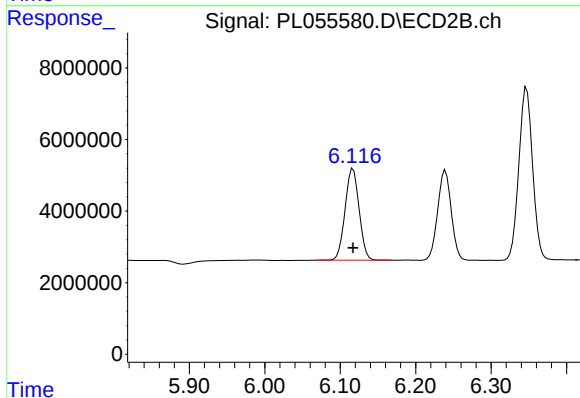


#10 gamma-Chlordane

R.T.: 6.117 min
Delta R.T.: 0.000 min
Response: 33069794
Conc: 10.08 ng/ml

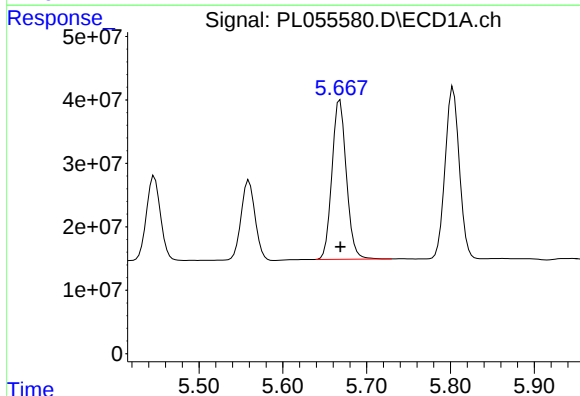


#12 4,4'-DDE

R.T.: 5.668 min
Delta R.T.: 0.000 min
Response: 299616268
Conc: 19.88 ng/ml

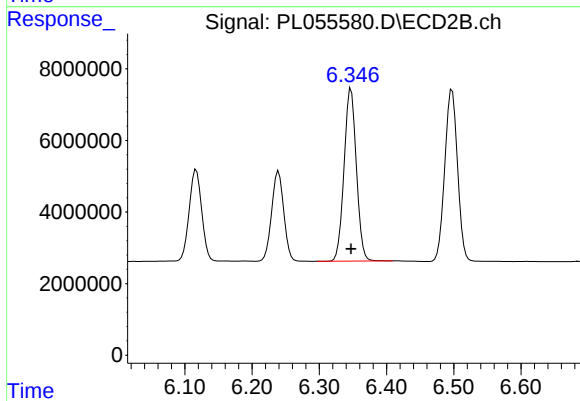

#12 4,4'-DDE


R.T.: 6.347 min
Delta R.T.: 0.000 min
Response: 61194240
Conc: 19.83 ng/ml

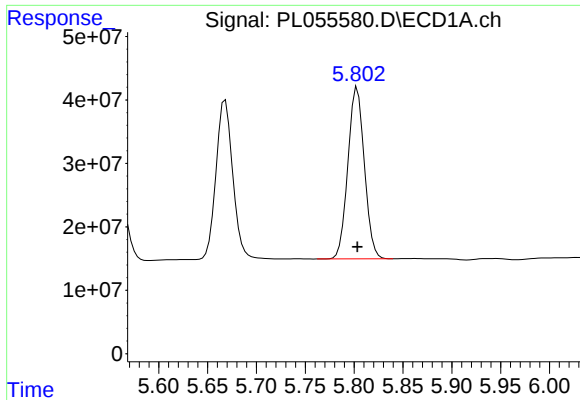

#13 Dieldrin


R.T.: 5.803 min
Delta R.T.: 0.000 min
Response: 317494285
Conc: 19.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

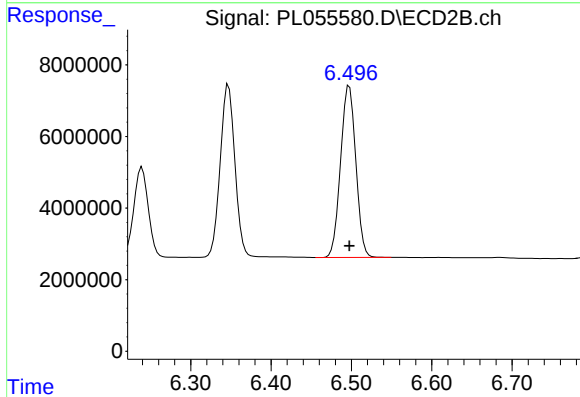


#13 Dieldrin

R.T.: 6.497 min
Delta R.T.: 0.000 min
Response: 63241879
Conc: 19.96 ng/ml

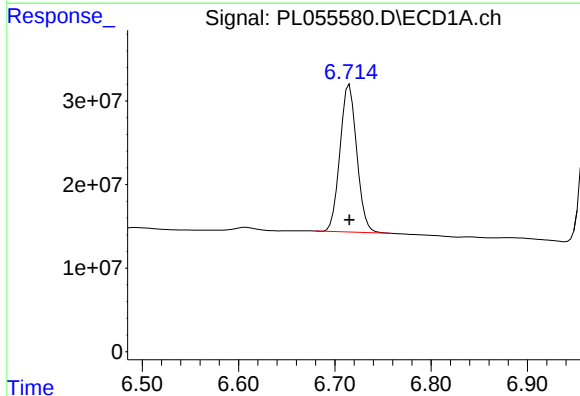


#19 Endosulfan Sulfate

R.T.: 6.715 min
Delta R.T.: 0.000 min
Response: 212789521
Conc: 18.99 ng/ml

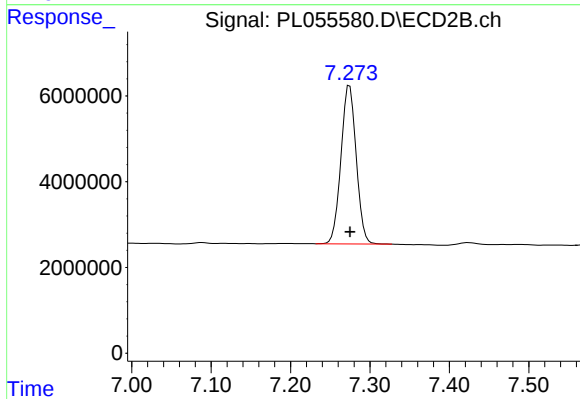

#19 Endosulfan Sulfate


R.T.: 7.274 min
Delta R.T.: 0.000 min
Response: 49339927
Conc: 19.57 ng/ml

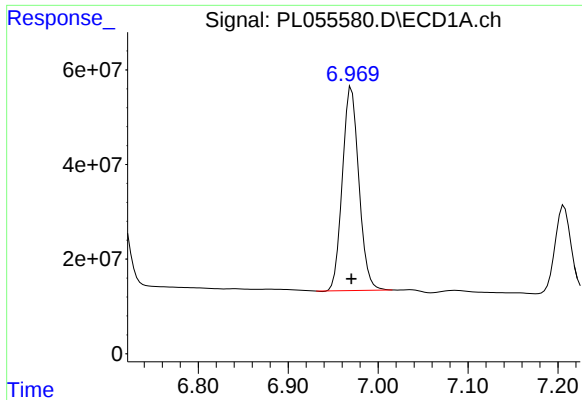

#20 Methoxychlor


R.T.: 6.970 min
Delta R.T.: 0.000 min
Response: 548990876
Conc: 99.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

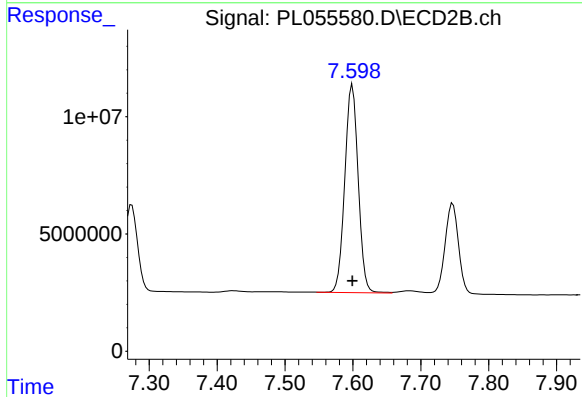


#20 Methoxychlor

R.T.: 7.599 min
Delta R.T.: 0.000 min
Response: 121546721
Conc: 94.54 ng/ml

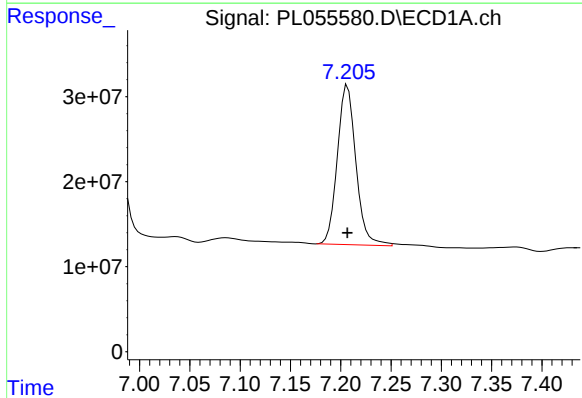


#21 Endrin ketone

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 240500190
Conc: 19.66 ng/ml

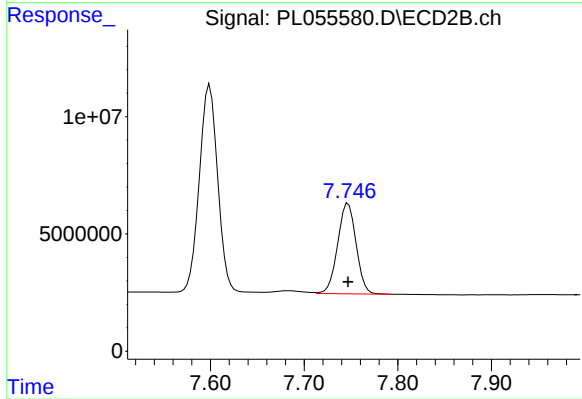

#21 Endrin ketone


R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 52910513
Conc: 20.11 ng/ml

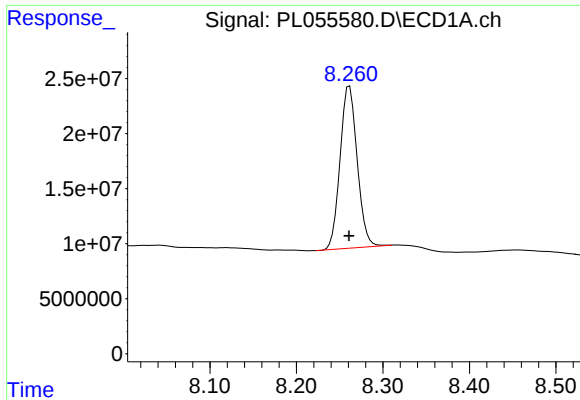

#28 Decachlorobiphenyl

R.T.: 8.261 min
Delta R.T.: 0.000 min
Response: 201925427
Conc: 20.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

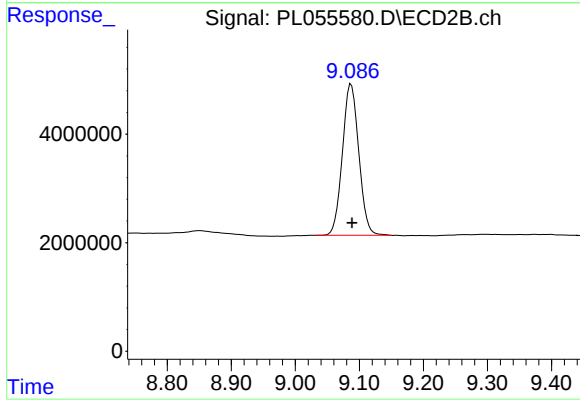

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: -0.001 min
Response: 49487038
Conc: 21.39 ng/ml