

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010820\
 Data File : PL055586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2020 11:44
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 12:18:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010820.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 08 12:17:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.012	635.2E6	147.0E6	50.000	50.000
28)	SA Decachlor...	8.261	9.087	471.0E6	110.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.375	5.004	200.5E6	53557935	500.000	500.000
24)	Chlordane-2	4.877	5.470	238.5E6	54530445	500.000	500.000
25)	Chlordane-3	5.448	6.117	703.1E6	195.4E6	500.000	500.000
26)	Chlordane-4	5.506	6.192	593.3E6	231.0E6	500.000	500.000
27)	Chlordane-5	6.344	6.997	183.8E6	39289362	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010820\
Data File : PL055586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2020 11:44
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 12:18:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010820.M
Quant Title : GC Extractables
QLast Update : Wed Jan 08 12:17:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

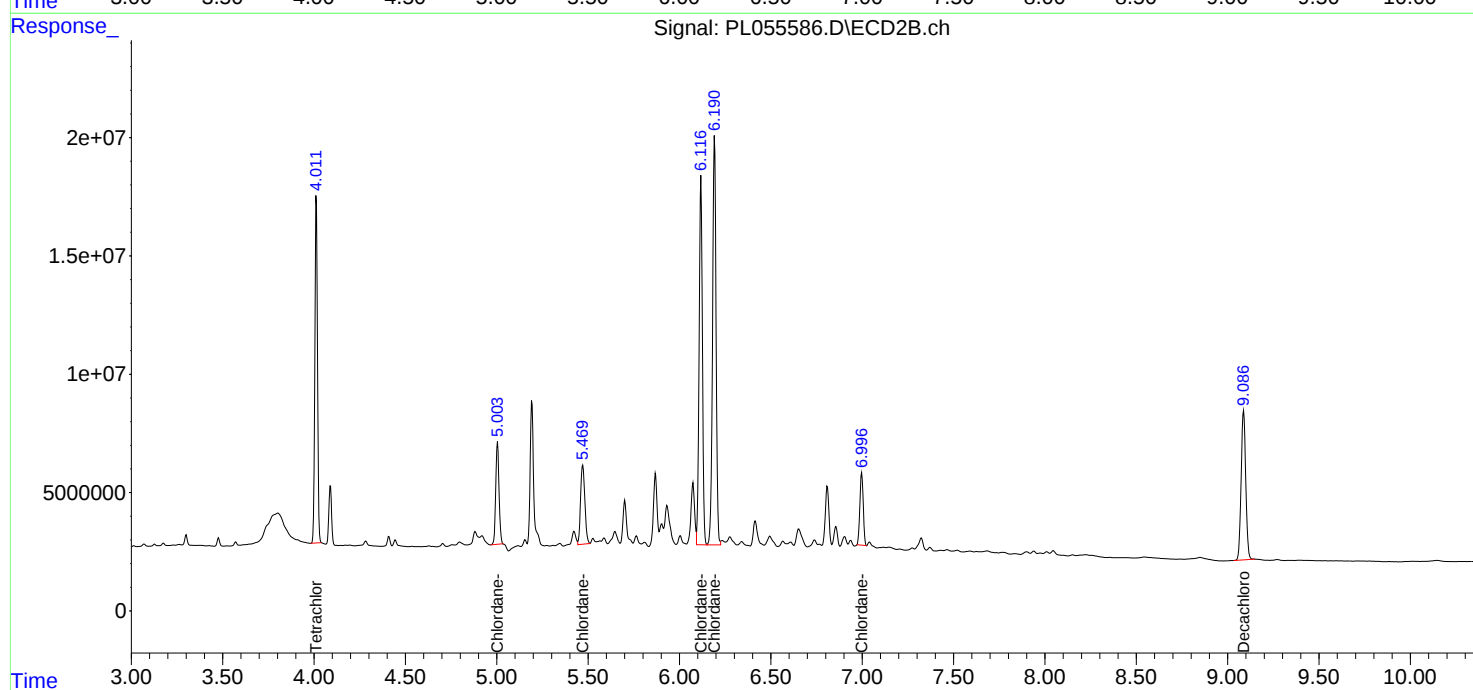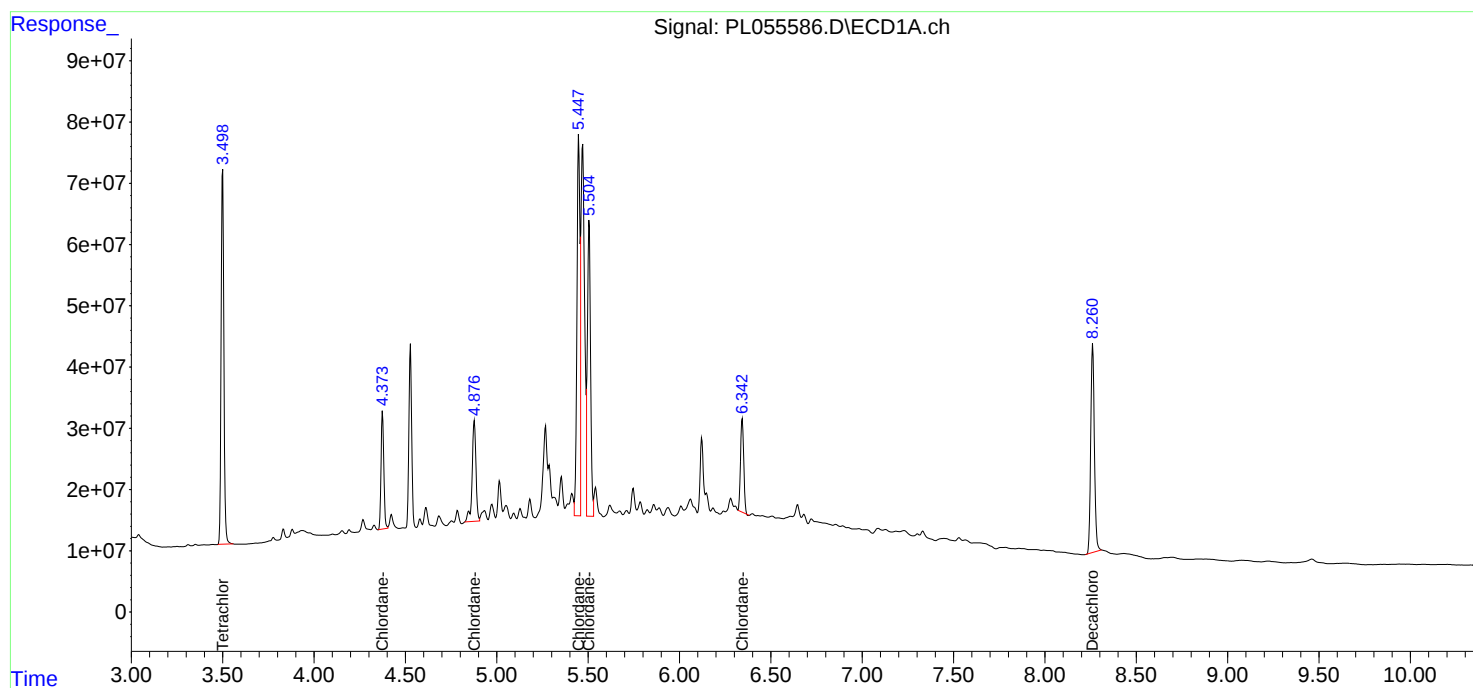


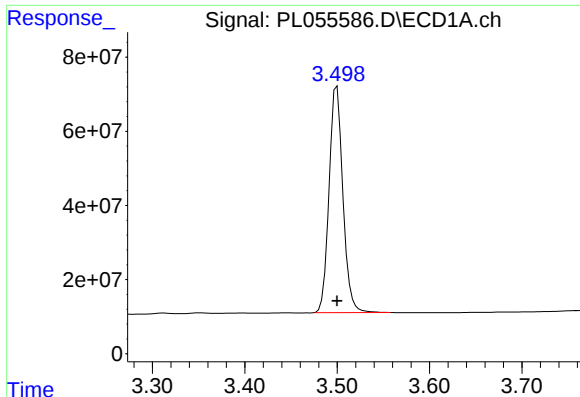

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 635170685
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

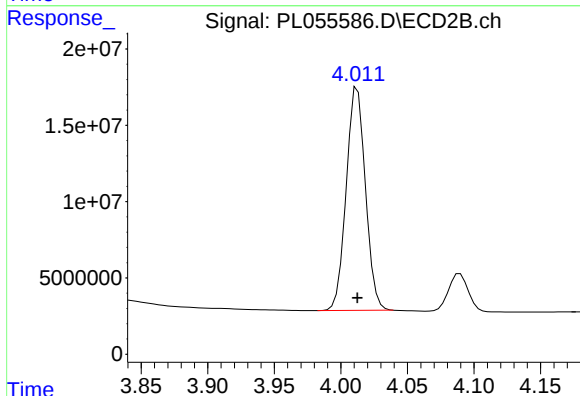


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 147001195
Conc: 50.00 ng/ml

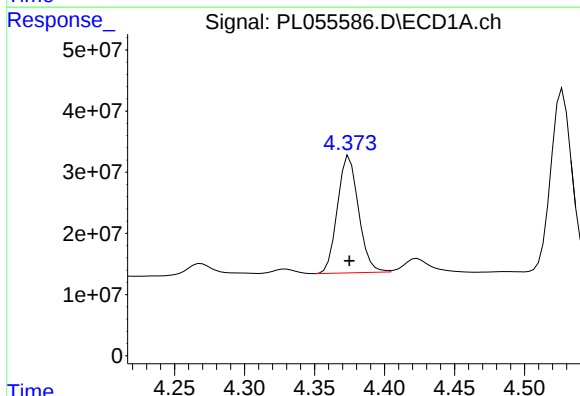


#23 Chlordane-1

R.T.: 4.375 min
Delta R.T.: 0.000 min
Response: 200510010
Conc: 500.00 ng/ml

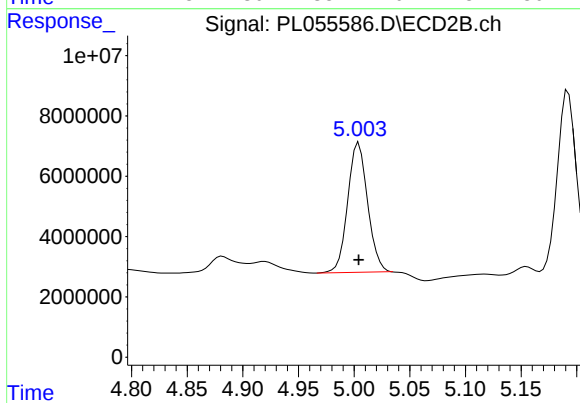

#23 Chlordane-1


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 53557935
Conc: 500.00 ng/ml

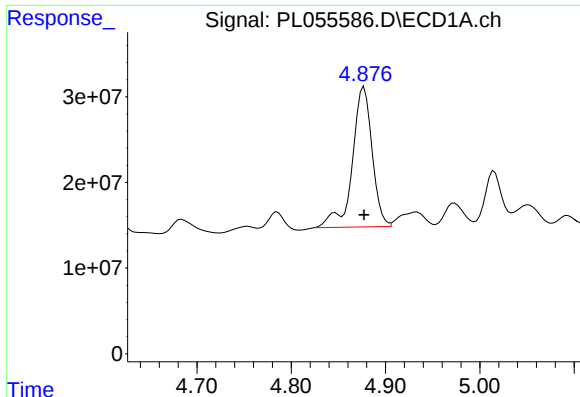

#24 Chlordane-2


R.T.: 4.877 min
Delta R.T.: 0.000 min
Response: 238520444
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

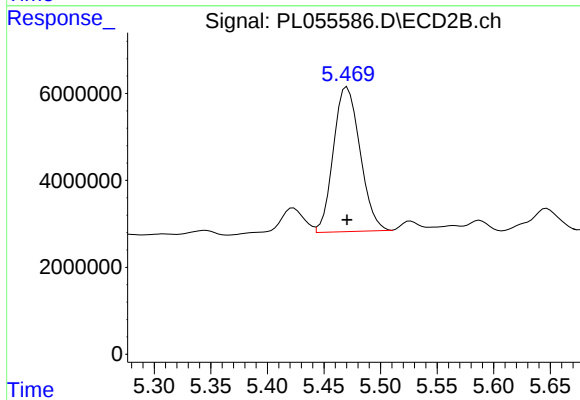


#24 Chlordane-2

R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 54530445
Conc: 500.00 ng/ml

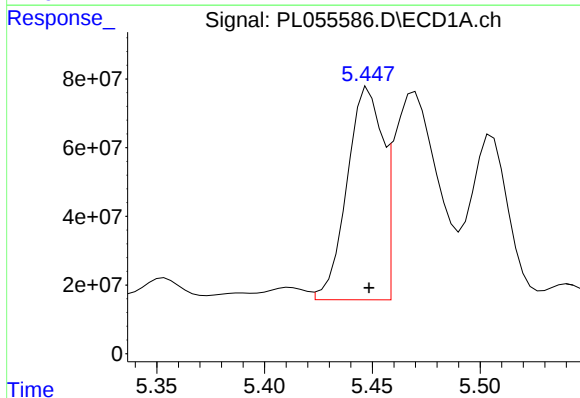


#25 Chlordane-3

R.T.: 5.448 min
Delta R.T.: 0.000 min
Response: 703144812
Conc: 500.00 ng/ml

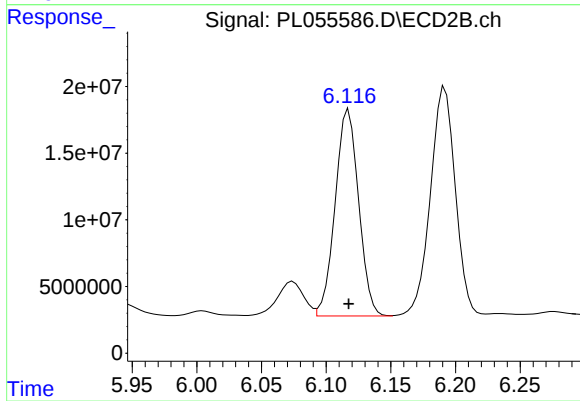

#25 Chlordane-3


R.T.: 6.117 min
Delta R.T.: 0.000 min
Response: 195412349
Conc: 500.00 ng/ml

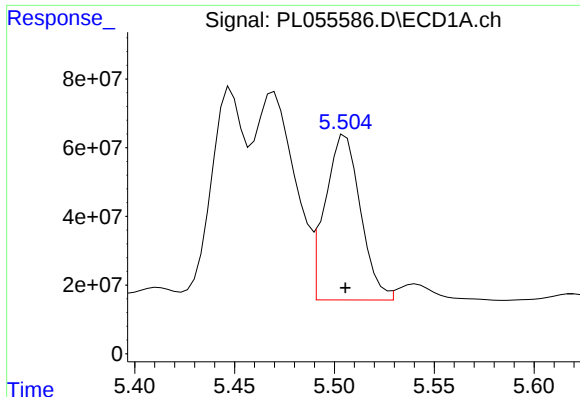

#26 Chlordane-4


R.T.: 5.506 min
Delta R.T.: 0.000 min
Response: 593261408
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

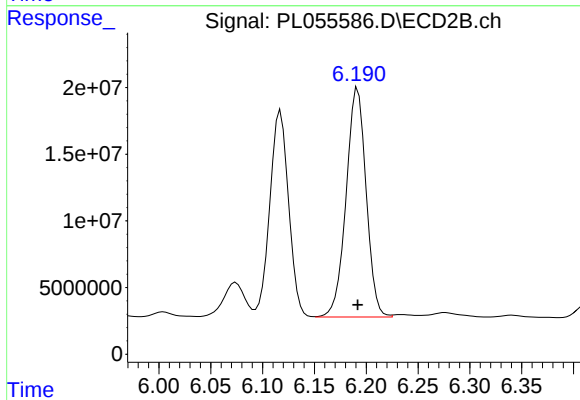


#26 Chlordane-4

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 230971203
Conc: 500.00 ng/ml

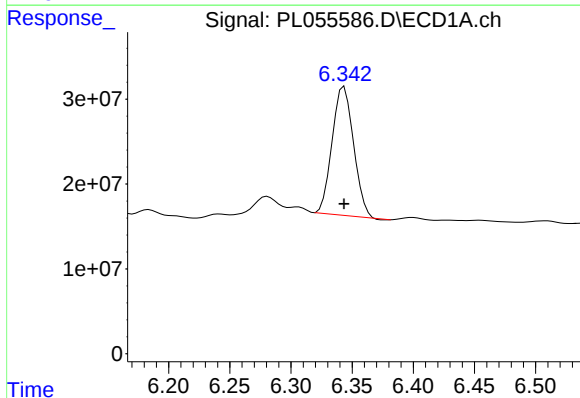


#27 Chlordane-5

R.T.: 6.344 min
Delta R.T.: 0.000 min
Response: 183775462
Conc: 500.00 ng/ml

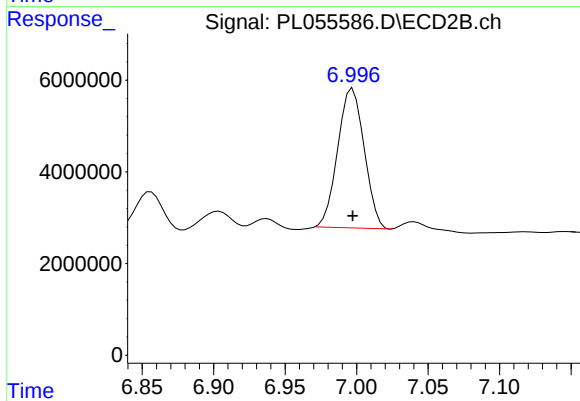

#27 Chlordane-5


R.T.: 6.997 min
Delta R.T.: 0.000 min
Response: 39289362
Conc: 500.00 ng/ml

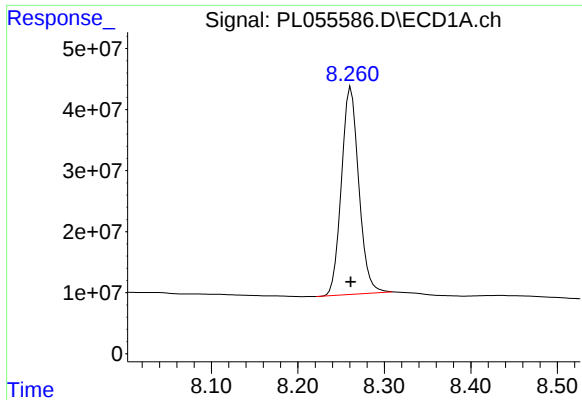

#28 Decachlorobiphenyl

R.T.: 8.261 min
Delta R.T.: 0.000 min
Response: 471025097
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

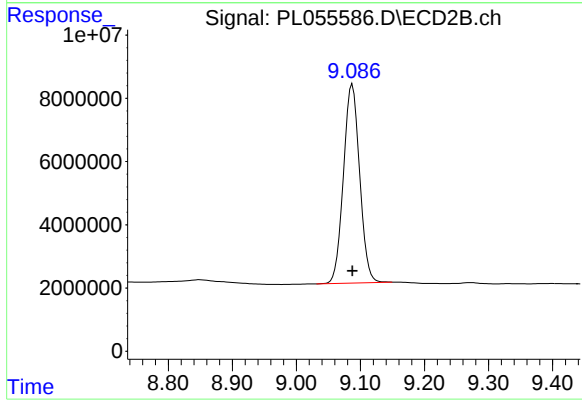

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.000 min
Response: 110258481
Conc: 50.00 ng/ml