

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
 Data File : PL064021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2021 21:18
 Operator : AR\AJ
 Sample : M1042-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 01:19:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.111	31068493	23724884	10.363	9.293
28)	SA Decachlor...	8.171	9.275	31189737	19831581	11.321	10.059
Target Compounds							
10)	B gamma-Chl...	5.386f	0.000	4645587	0	1.222	N.D. #
11)	B alpha-Chl...	0.000	6.330	0	4383989	N.D.	1.588 #
17)	MA 4,4'-DDT	6.339	0.000	2474592	0	0.934	N.D. #
25)	Chlordane-3	5.386f	0.000	4645587	0	14.217	N.D. #
26)	Chlordane-4	0.000	6.330	0	4383989	N.D.	10.666 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
Data File : PL064021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2021 21:18
Operator : AR\AJ
Sample : M1042-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 01:19:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

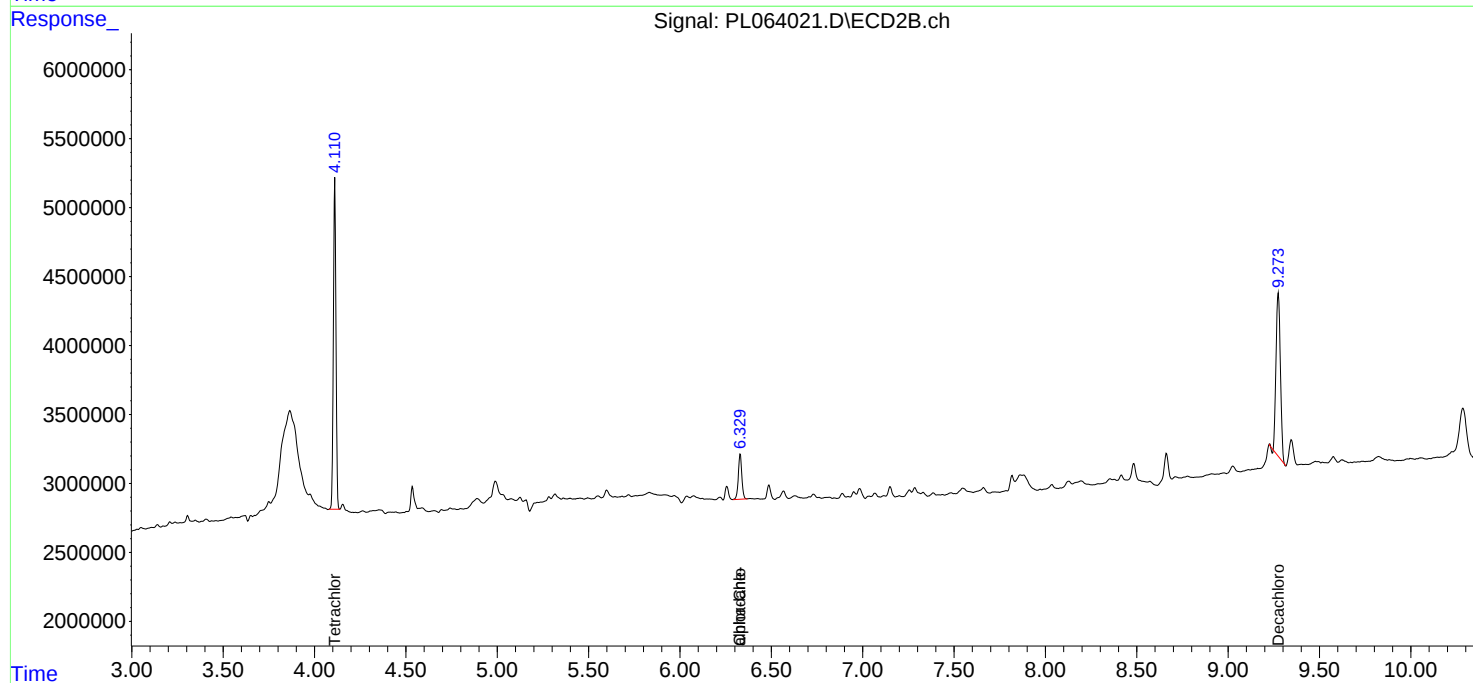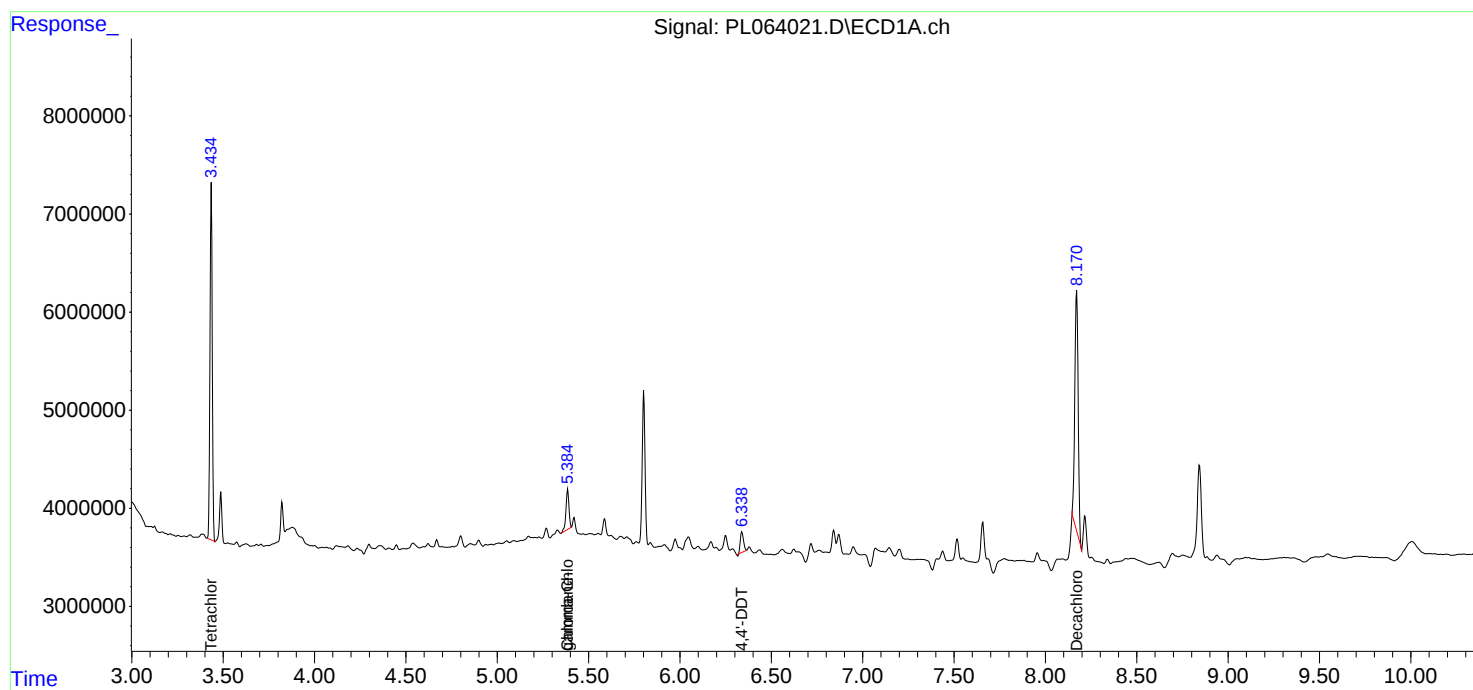


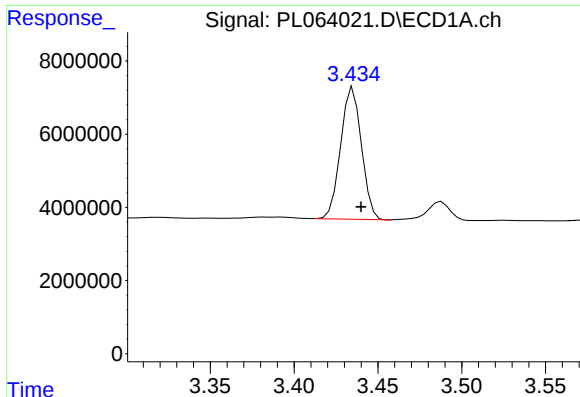

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: -0.005 min
Response: 31068493
Conc: 10.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

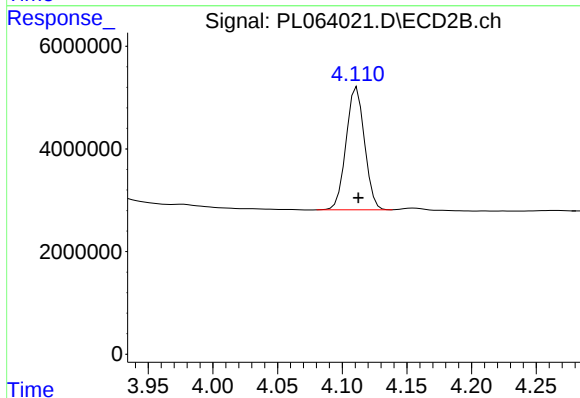


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.001 min
Response: 23724884
Conc: 9.29 ng/ml

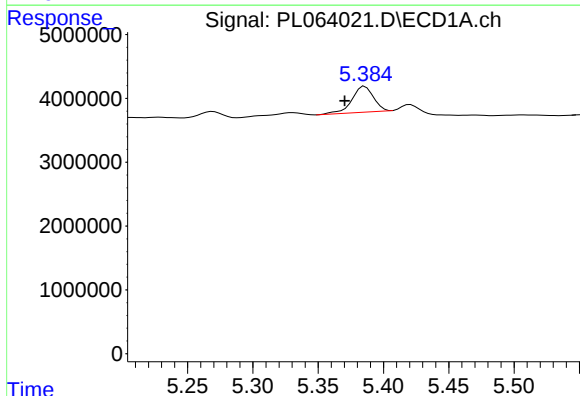


#10 gamma-Chlordane

R.T.: 5.386 min
Delta R.T.: 0.016 min
Response: 4645587
Conc: 1.22 ng/ml

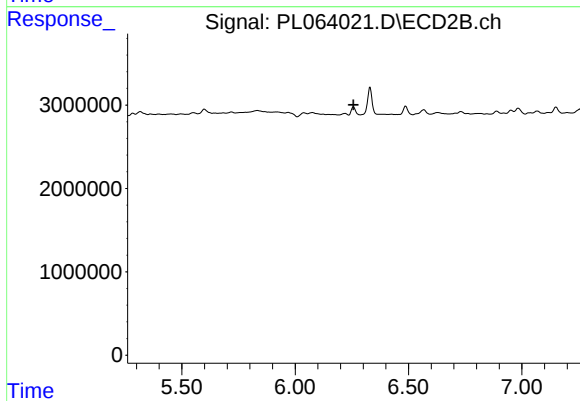

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.258 min
Response: 0
Conc: N.D.

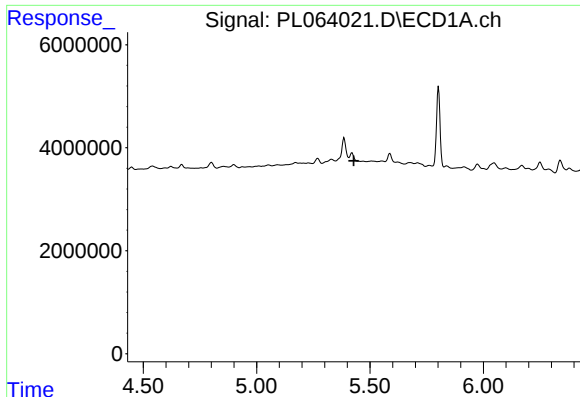

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

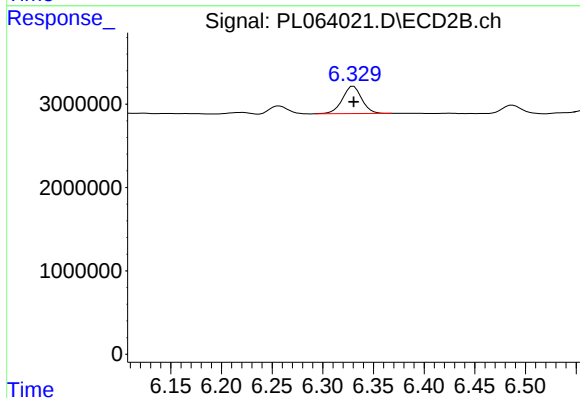


#11 alpha-Chlordane

R.T.: 6.330 min
Delta R.T.: 0.000 min
Response: 4383989
Conc: 1.59 ng/ml

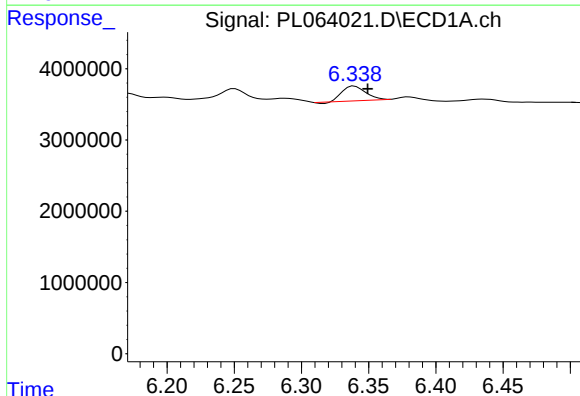


#17 4,4'-DDT

R.T.: 6.339 min
Delta R.T.: -0.010 min
Response: 2474592
Conc: 0.93 ng/ml

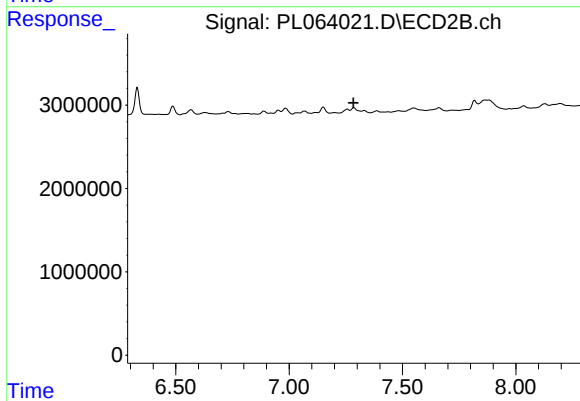

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

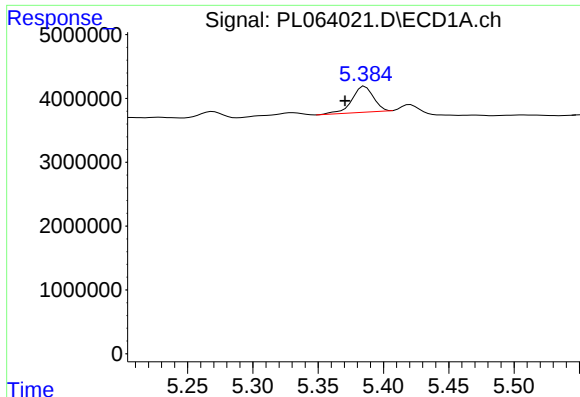

#25 Chlordane-3


R.T.: 5.386 min
Delta R.T.: 0.015 min
Response: 4645587
Conc: 14.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

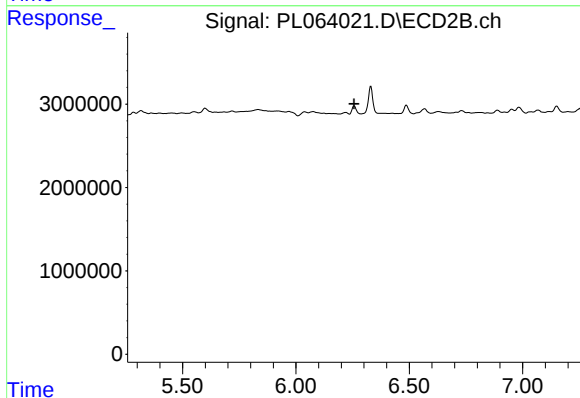


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.257 min
Response: 0
Conc: N.D.

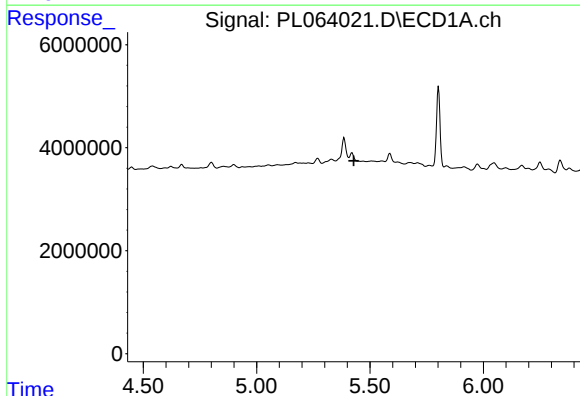


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.428 min
Response: 0
Conc: N.D.

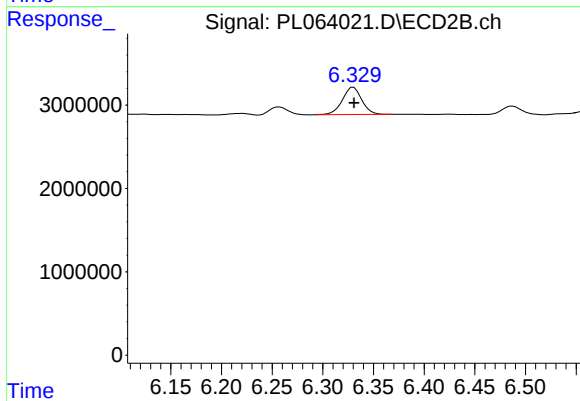

#26 Chlordane-4


R.T.: 6.330 min
Delta R.T.: 0.000 min
Response: 4383989
Conc: 10.67 ng/ml

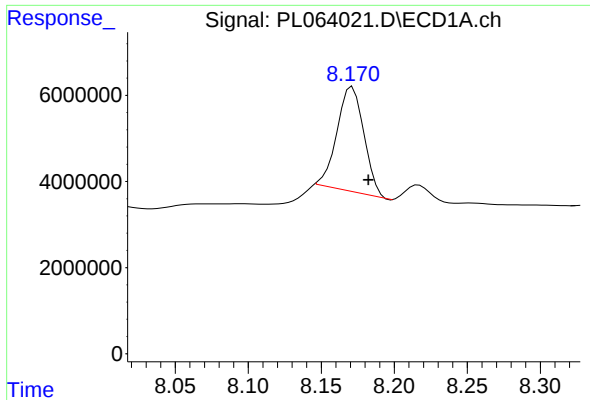

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: -0.011 min
Response: 31189737
Conc: 11.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

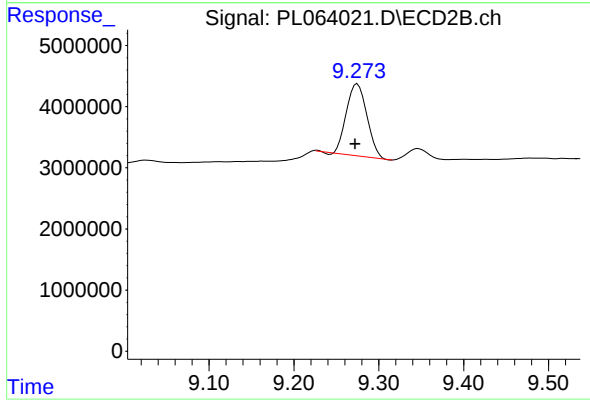

#28 Decachlorobiphenyl

R.T.: 9.275 min
Delta R.T.: 0.003 min
Response: 19831581
Conc: 10.06 ng/ml