

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
 Data File : PL063992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2021 11:38
 Operator : AR\AJ
 Sample : M1023-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-04-010621

Manual Integrations
 APPROVED

Ankita
 1/11/2021 10:32:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 00:48:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	4.111	35452794	27861216	11.826	10.913
28)	SA Decachlor...	8.171	9.273	33277738	24590304	12.078	12.472
Target Compounds							
17)	MA 4,4'-DDT	6.336	7.282	1927243	829845	0.727m	0.427m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
Data File : PL063992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2021 11:38
Operator : AR\AJ
Sample : M1023-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SU-04-010621


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 00:48:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

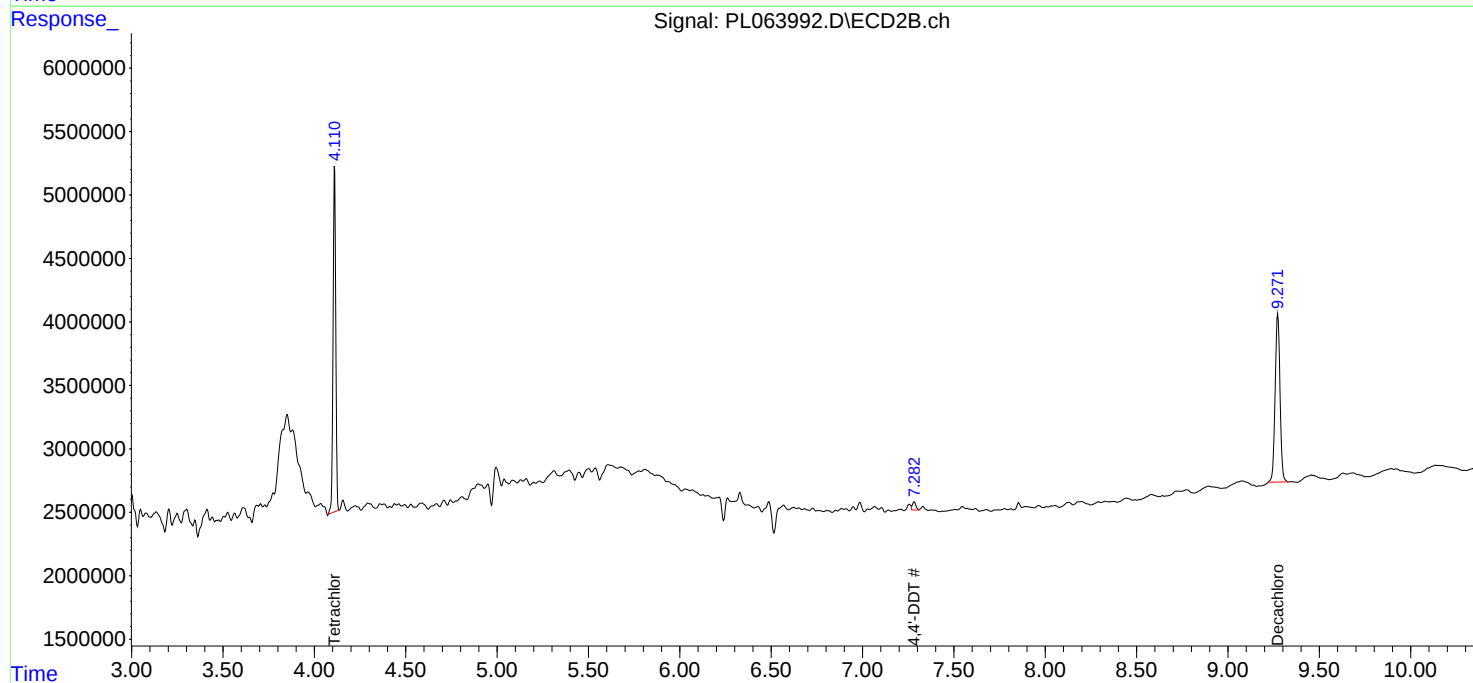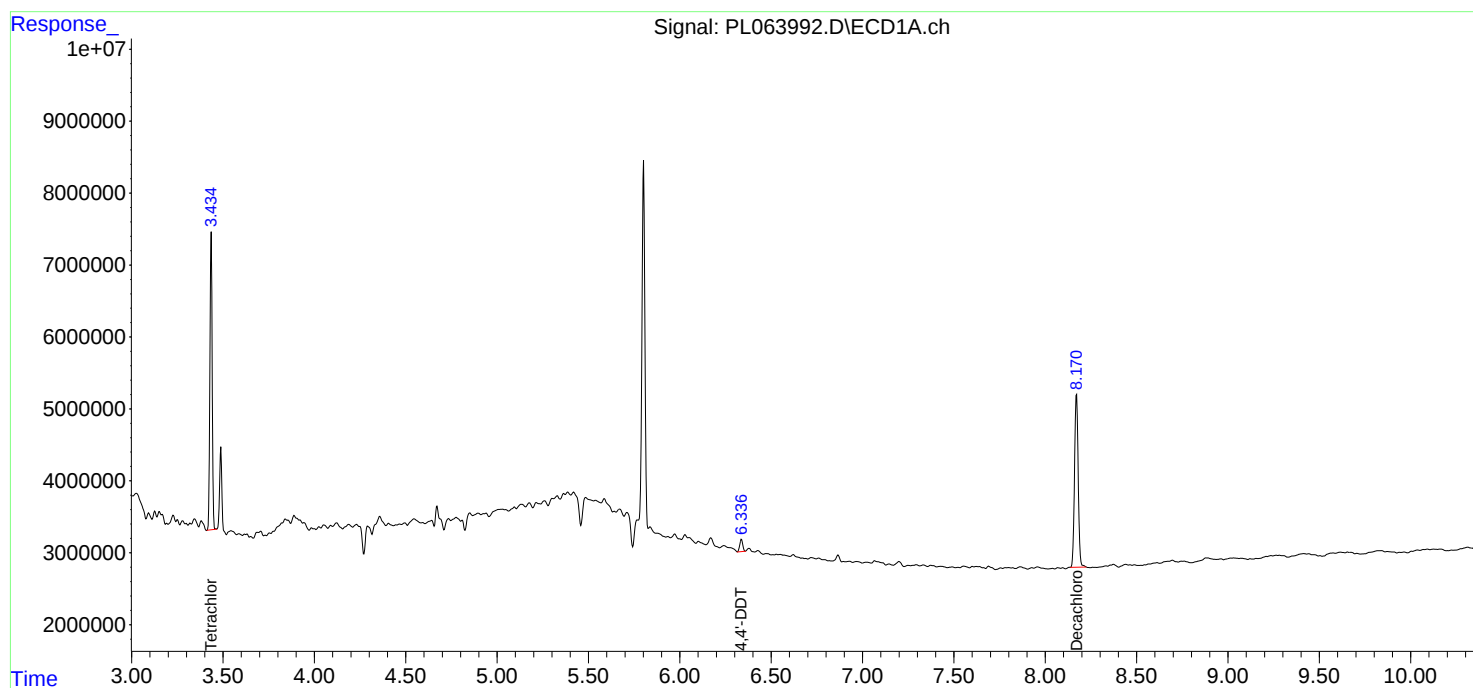

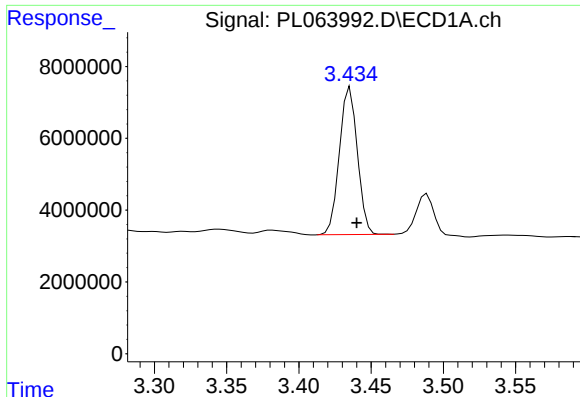


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: -0.004 min
Response: 35452794
Conc: 11.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-010621


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:28 AM

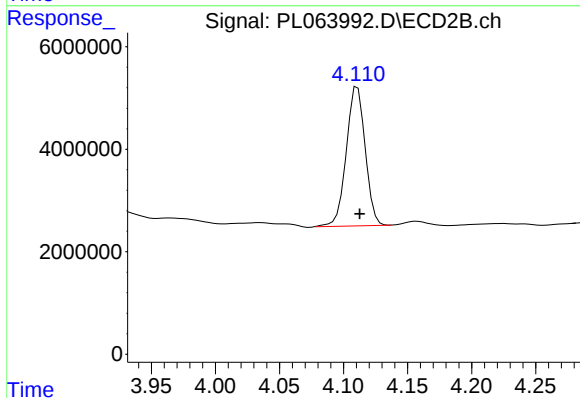


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 27861216
Conc: 10.91 ng/ml

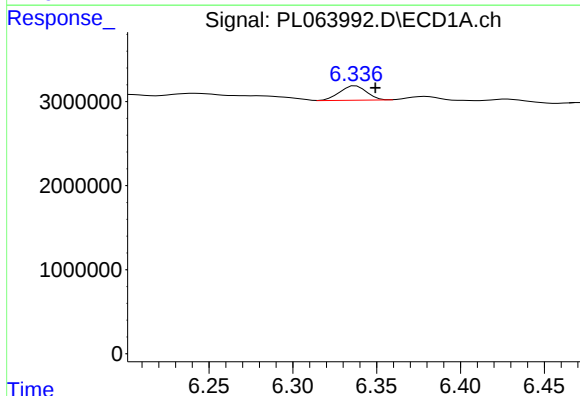


#17 4,4'-DDT

R.T.: 6.336 min
Delta R.T.: -0.013 min
Response: 1927243
Conc: 0.73 ng/ml m

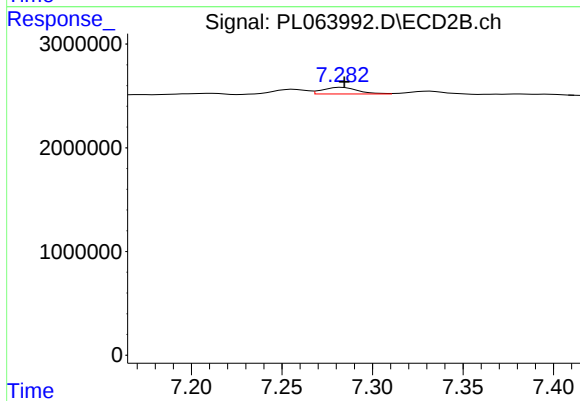

#17 4,4'-DDT

R.T.: 7.282 min
Delta R.T.: -0.003 min
Response: 829845
Conc: 0.43 ng/ml m

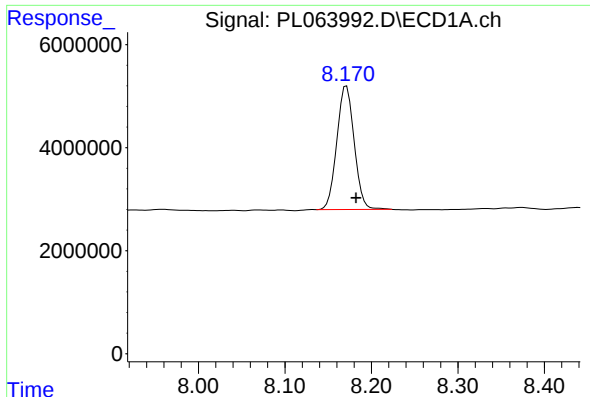


#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: -0.011 min
Response: 33277738
Conc: 12.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-010621

Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:28 AM

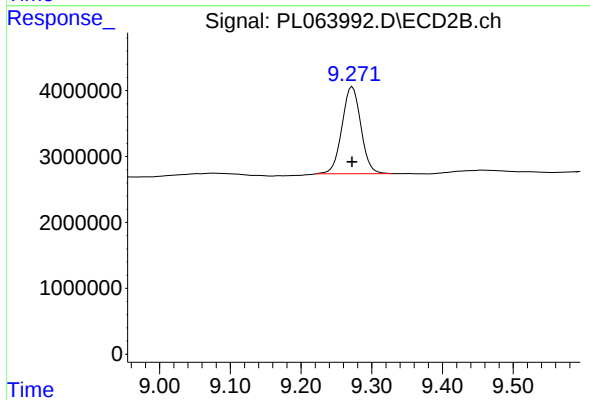

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 24590304
Conc: 12.47 ng/ml