

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
 Data File : PL064016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2021 20:07
 Operator : AR\AJ
 Sample : M1044-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-8

Manual Integrations
 APPROVED

Ankita
 1/11/2021 10:32:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 01:18:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	4.111	36961348	28510459	12.329	11.167
28)	SA Decachlor...	8.170	9.275	41724870	25783635	15.144m	13.077
Target Compounds							
12)	B 4,4'-DDE	5.587	6.487	8919142	7476811	2.594	3.027
17)	MA 4,4'-DDT	6.337	7.285	15422219	5939745	5.820m	3.053 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
Data File : PL064016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2021 20:07
Operator : AR\AJ
Sample : M1044-07
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-8


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 01:18:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

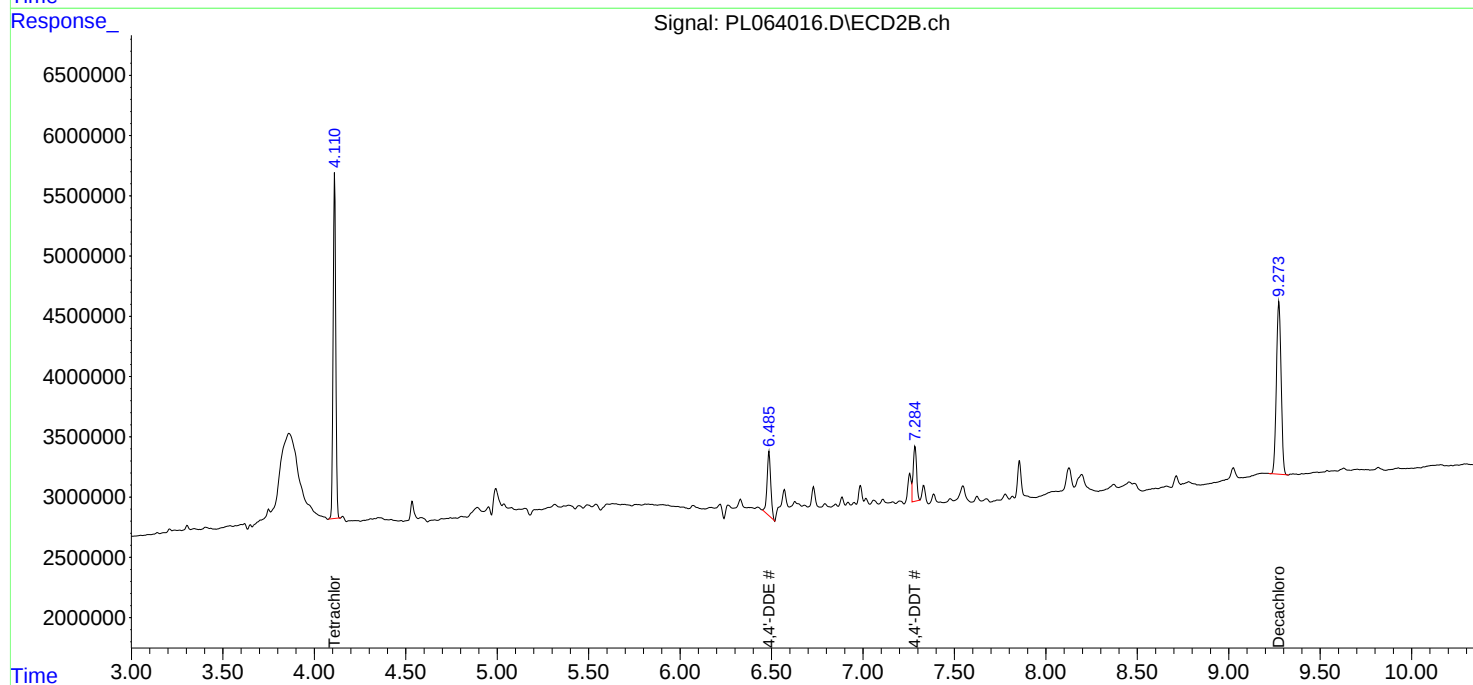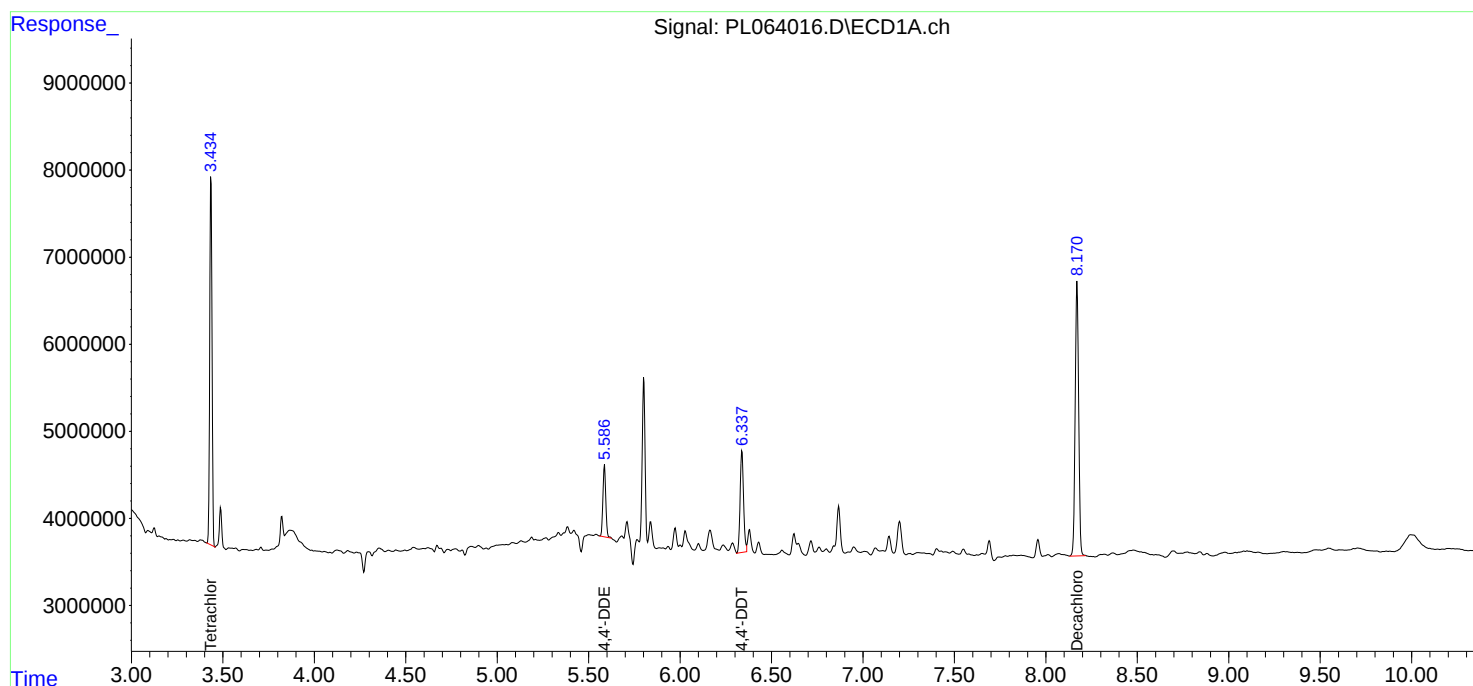

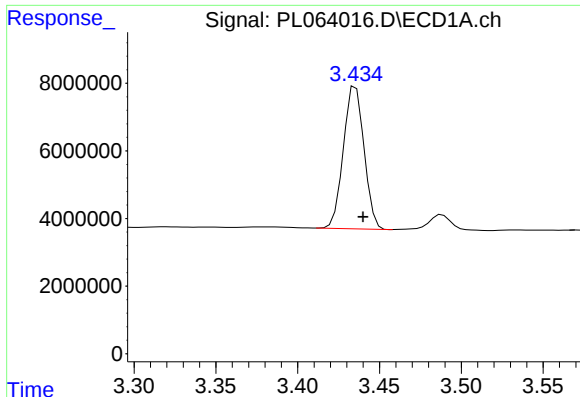


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: -0.004 min
Response: 36961348
Conc: 12.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:40 AM

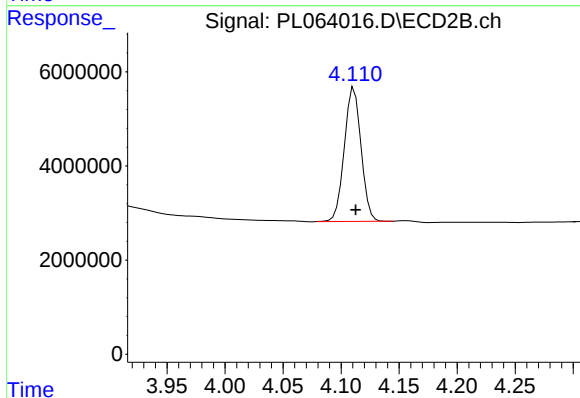


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.001 min
Response: 28510459
Conc: 11.17 ng/ml

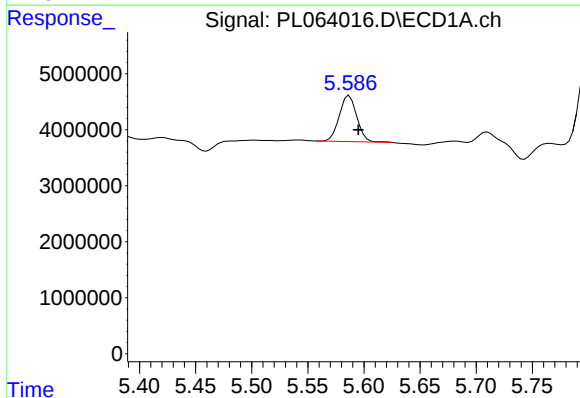


#12 4,4'-DDE

R.T.: 5.587 min
Delta R.T.: -0.008 min
Response: 8919142
Conc: 2.59 ng/ml

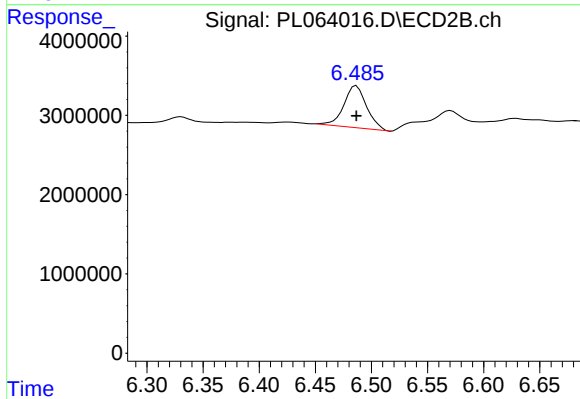

#12 4,4'-DDE

R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 7476811
Conc: 3.03 ng/ml

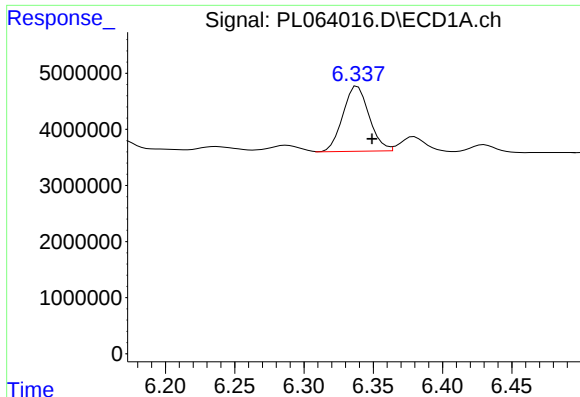


#17 4,4'-DDT

R.T.: 6.337 min
Delta R.T.: -0.012 min
Response: 15422219
Conc: 5.82 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-8


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:40 AM

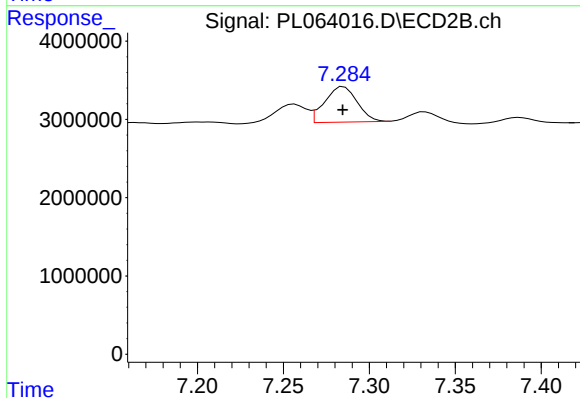


#17 4,4'-DDT

R.T.: 7.285 min
Delta R.T.: 0.000 min
Response: 5939745
Conc: 3.05 ng/ml

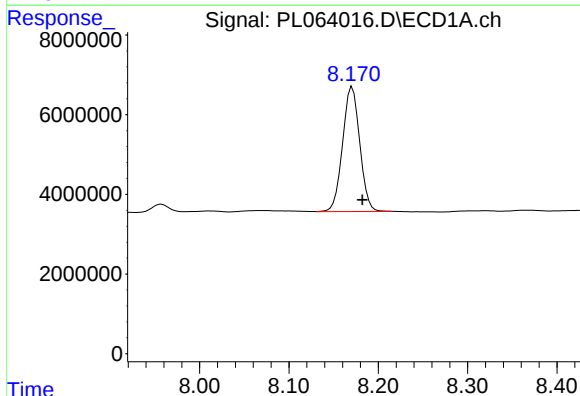

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: -0.013 min
Response: 41724870
Conc: 15.14 ng/ml m

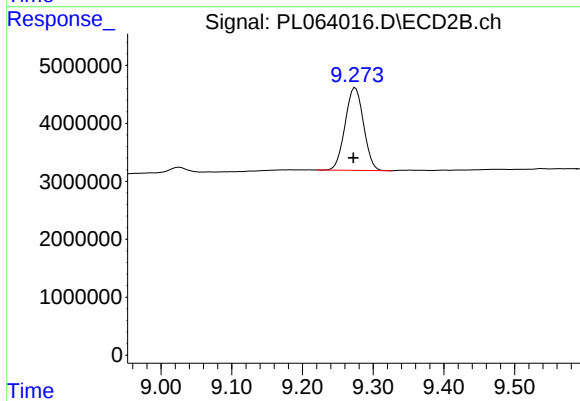

#28 Decachlorobiphenyl

R.T.: 9.275 min
Delta R.T.: 0.003 min
Response: 25783635
Conc: 13.08 ng/ml