

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
 Data File : PL064021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2021 21:18
 Operator : AR\AJ
 Sample : M1042-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 11939

Manual Integrations
 APPROVED

Ankita
 1/11/2021 10:32:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 02:33:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.111	31068493	23724884	10.363	9.293
28)	SA Decachlor...	8.170	9.273	40000191	22990612	14.518m	11.661m
Target Compounds							
11)	B alpha-Chl...	5.419	6.330	1892402	4383989	0.504m	1.588 #
12)	B 4,4'-DDE	5.586	6.486	1825177	1339127	0.531m	0.542m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
Data File : PL064021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2021 21:18
Operator : AR\AJ
Sample : M1042-02
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
11939


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 02:33:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

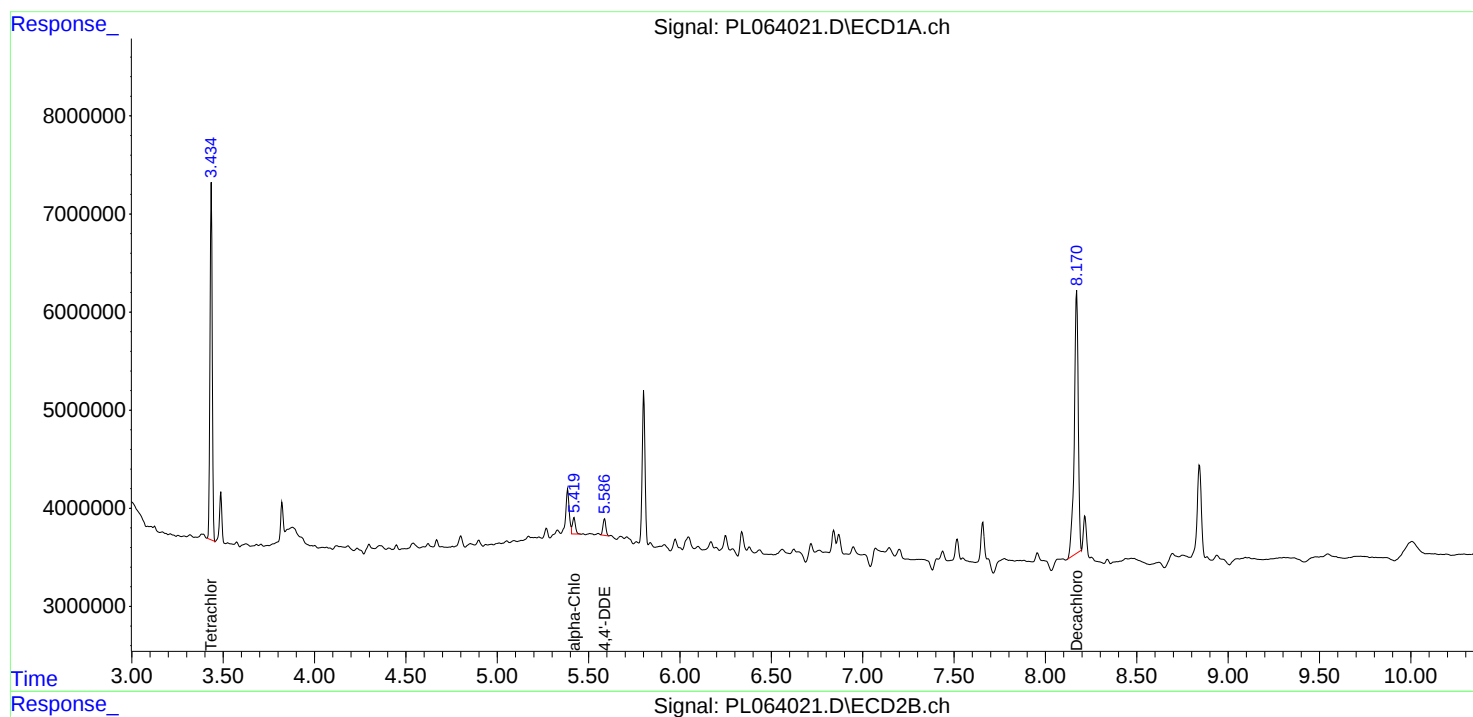

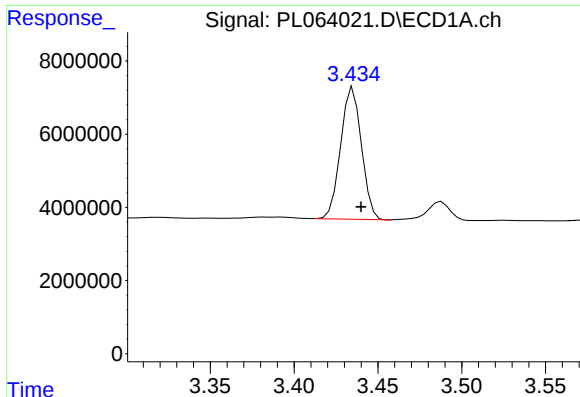


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: -0.005 min
Response: 31068493
Conc: 10.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
11939


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:46 AM

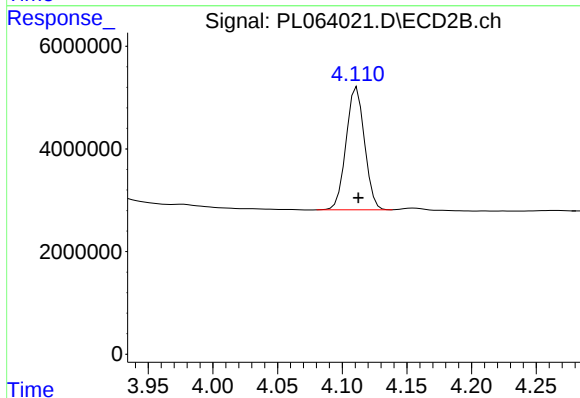


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.001 min
Response: 23724884
Conc: 9.29 ng/ml

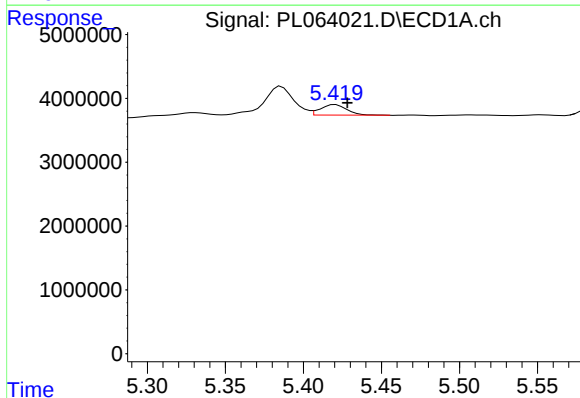


#11 alpha-Chlordane

R.T.: 5.419 min
Delta R.T.: -0.009 min
Response: 1892402
Conc: 0.50 ng/ml m

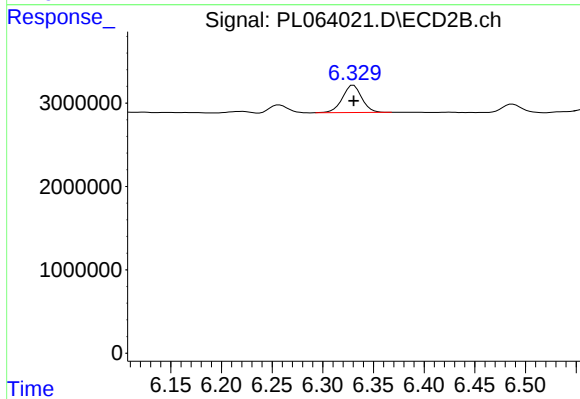

#11 alpha-Chlordane

R.T.: 6.330 min
Delta R.T.: 0.000 min
Response: 4383989
Conc: 1.59 ng/ml

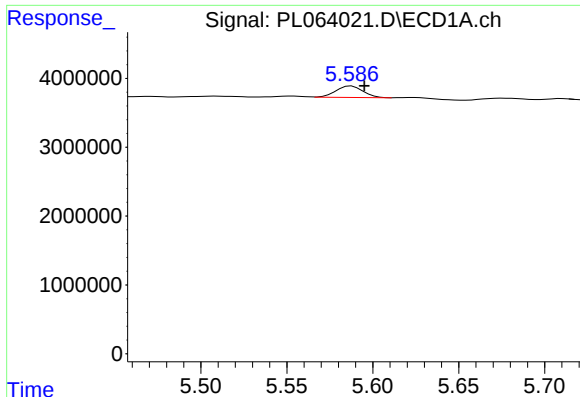


#12 4,4'-DDE

R.T.: 5.586 min
Delta R.T.: -0.009 min
Response: 1825177
Conc: 0.53 ng/ml m

Instrument :
ECD_L
ClientSampleId :
11939


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:46 AM

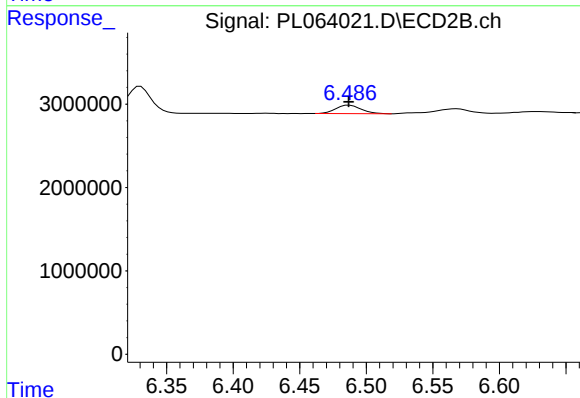


#12 4,4'-DDE

R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 1339127
Conc: 0.54 ng/ml m

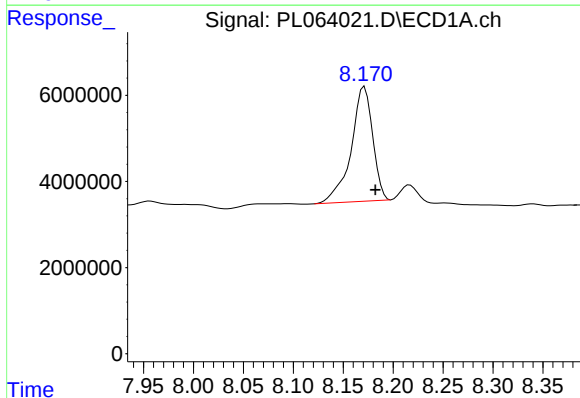

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: -0.012 min
Response: 40000191
Conc: 14.52 ng/ml m

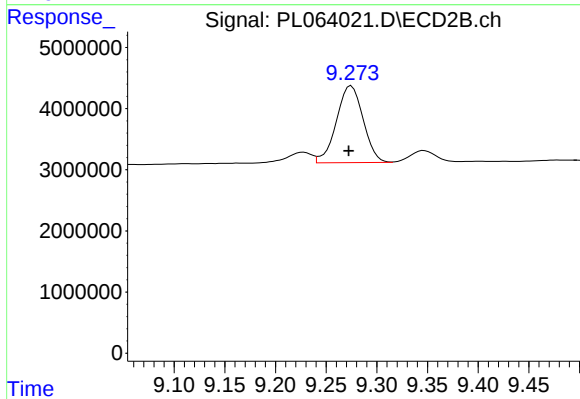

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.001 min
Response: 22990612
Conc: 11.66 ng/ml m