

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
 Data File : PL064022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2021 21:32
 Operator : AR\AJ
 Sample : M1043-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BALL-1

Manual Integrations
 APPROVED

Ankita
 1/11/2021 10:32:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 02:40:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.111	30050148	23567848	10.024	9.231
28)	SA Decachlor...	8.171	9.274	36412665	22709301	13.216	11.518
Target Compounds							
7)	B delta-BHC	4.615	5.207	4365614	6346121	0.963	1.930 #
12)	B 4,4'-DDE	5.586	6.488	4621679	6788505	1.344m	2.749 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
Data File : PL064022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2021 21:32
Operator : AR\AJ
Sample : M1043-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BALL-1


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 02:40:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

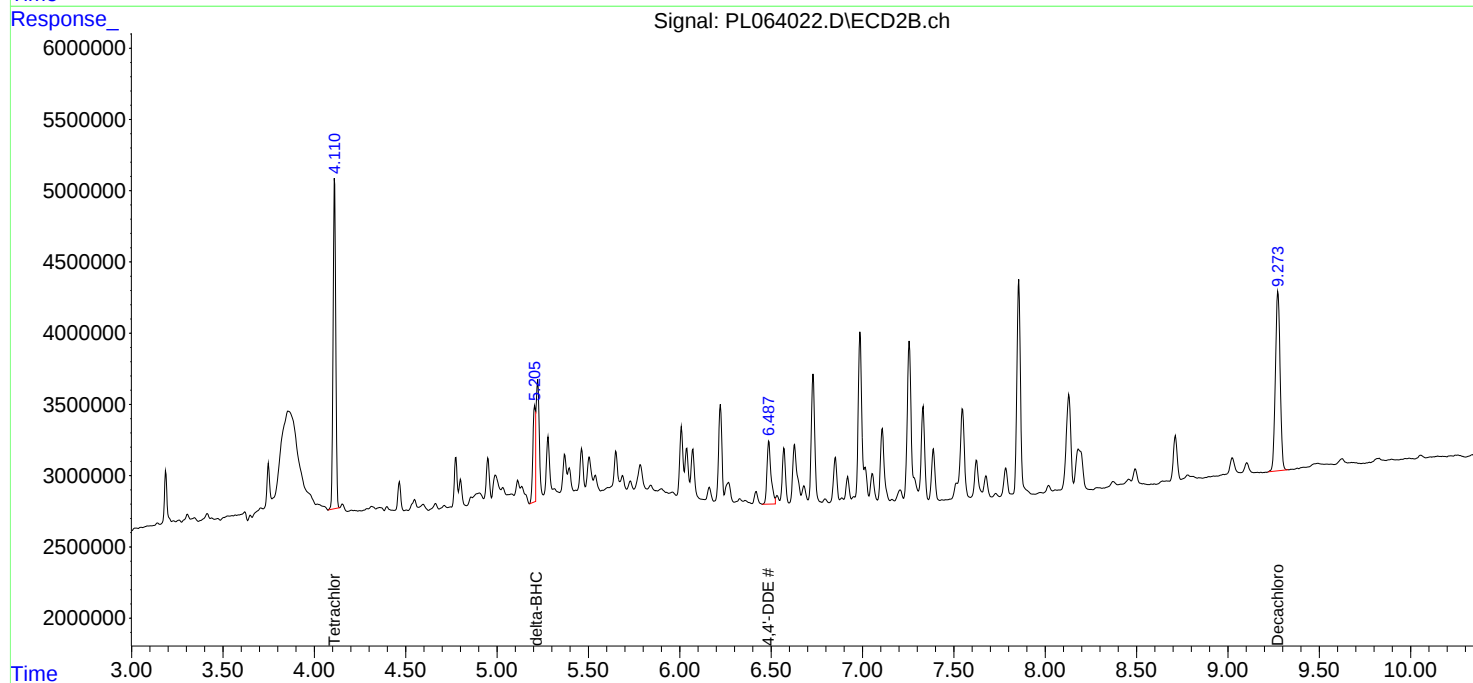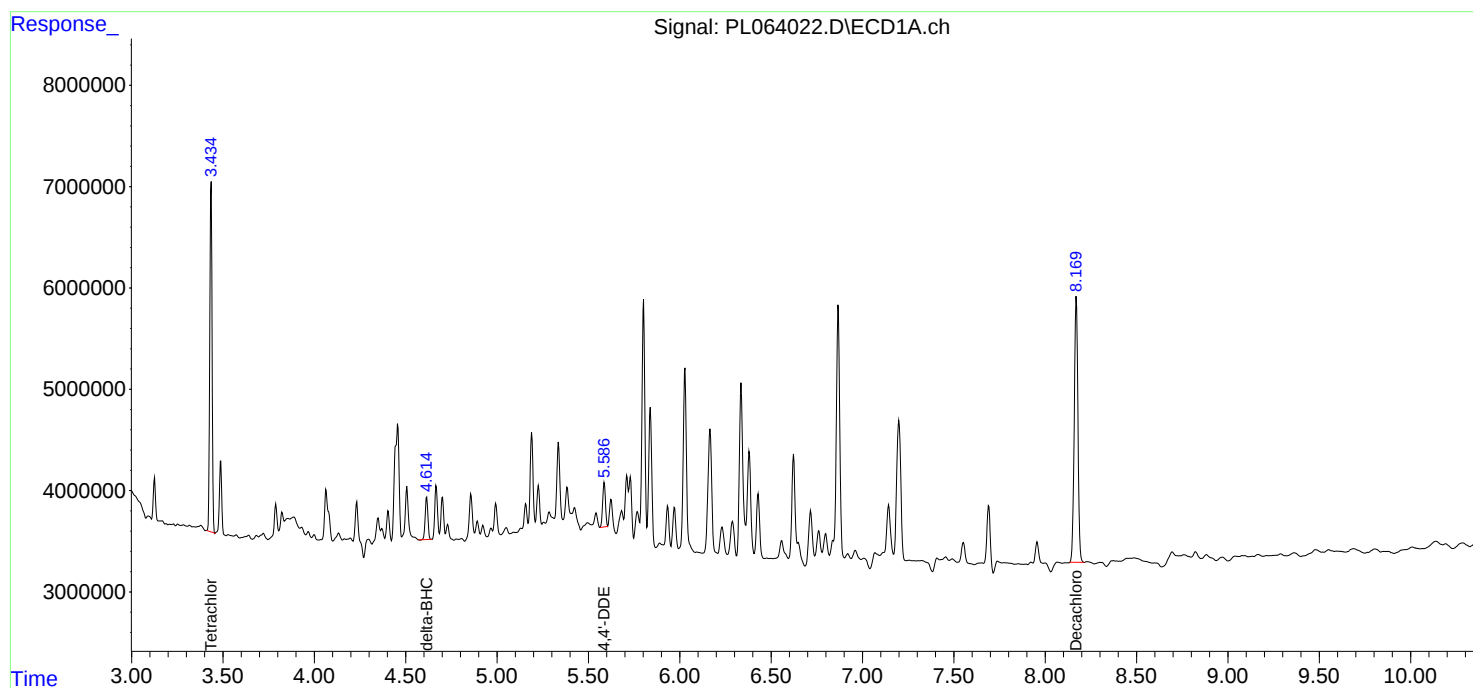

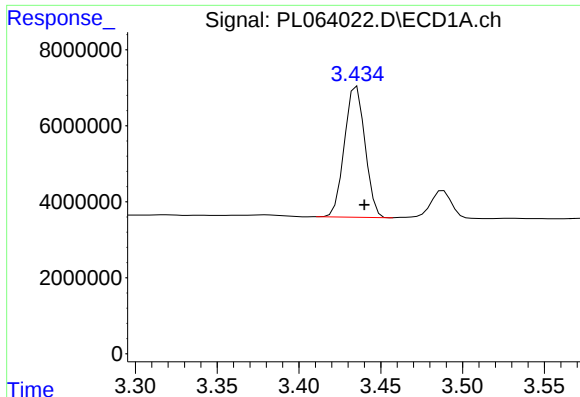


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: -0.005 min
Response: 30050148
Conc: 10.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
BALL-1


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:48 AM

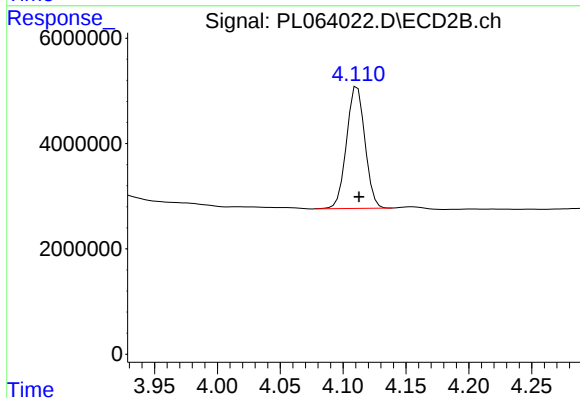


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.001 min
Response: 23567848
Conc: 9.23 ng/ml

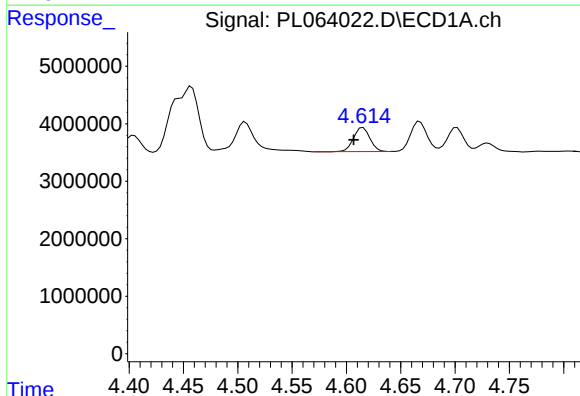


#7 delta-BHC

R.T.: 4.615 min
Delta R.T.: 0.009 min
Response: 4365614
Conc: 0.96 ng/ml

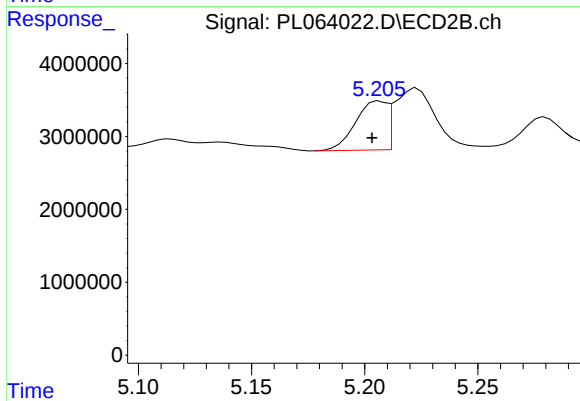

#7 delta-BHC

R.T.: 5.207 min
Delta R.T.: 0.003 min
Response: 6346121
Conc: 1.93 ng/ml

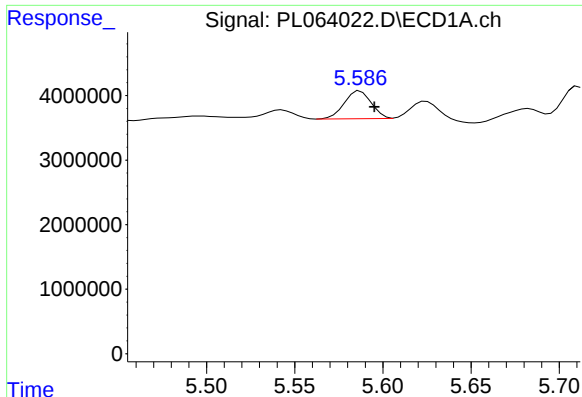


#12 4,4'-DDE

R.T.: 5.586 min
Delta R.T.: -0.009 min
Response: 4621679
Conc: 1.34 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BALL-1


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:48 AM

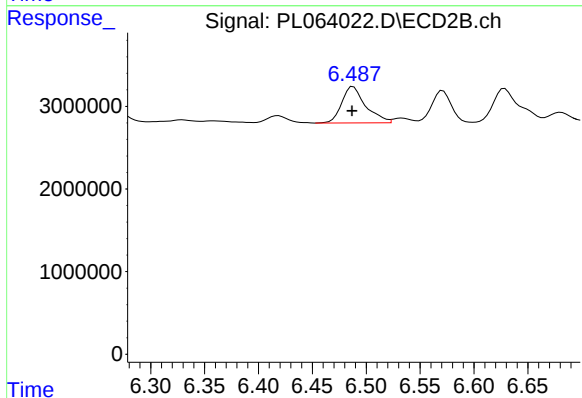


#12 4,4'-DDE

R.T.: 6.488 min
Delta R.T.: 0.001 min
Response: 6788505
Conc: 2.75 ng/ml

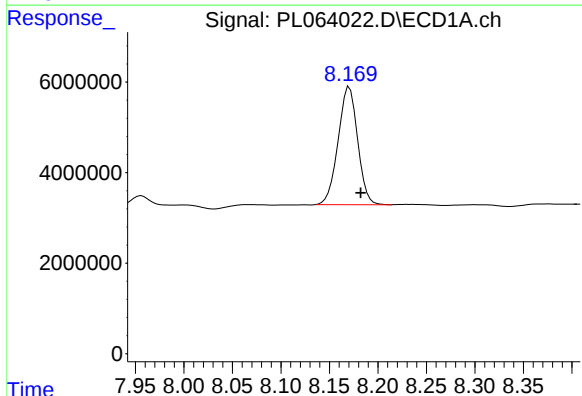

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: -0.012 min
Response: 36412665
Conc: 13.22 ng/ml

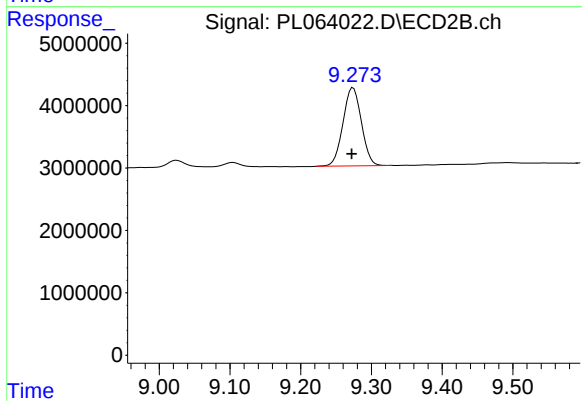

#28 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: 0.002 min
Response: 22709301
Conc: 11.52 ng/ml