

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
 Data File : PL064023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2021 21:46
 Operator : AR\AJ
 Sample : M1044-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 1/11/2021 10:32:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 02:43:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.436	4.111	30668902	23435816	10.230	9.180
28) SA Decachlor...	8.172	9.275	34903803	22702549	12.669	11.515
Target Compounds						
17) MA 4,4'-DDT	6.338	7.284	1753818	1001005	0.662m	0.515m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010821\
Data File : PL064023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2021 21:46
Operator : AR\AJ
Sample : M1044-01
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 02:43:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

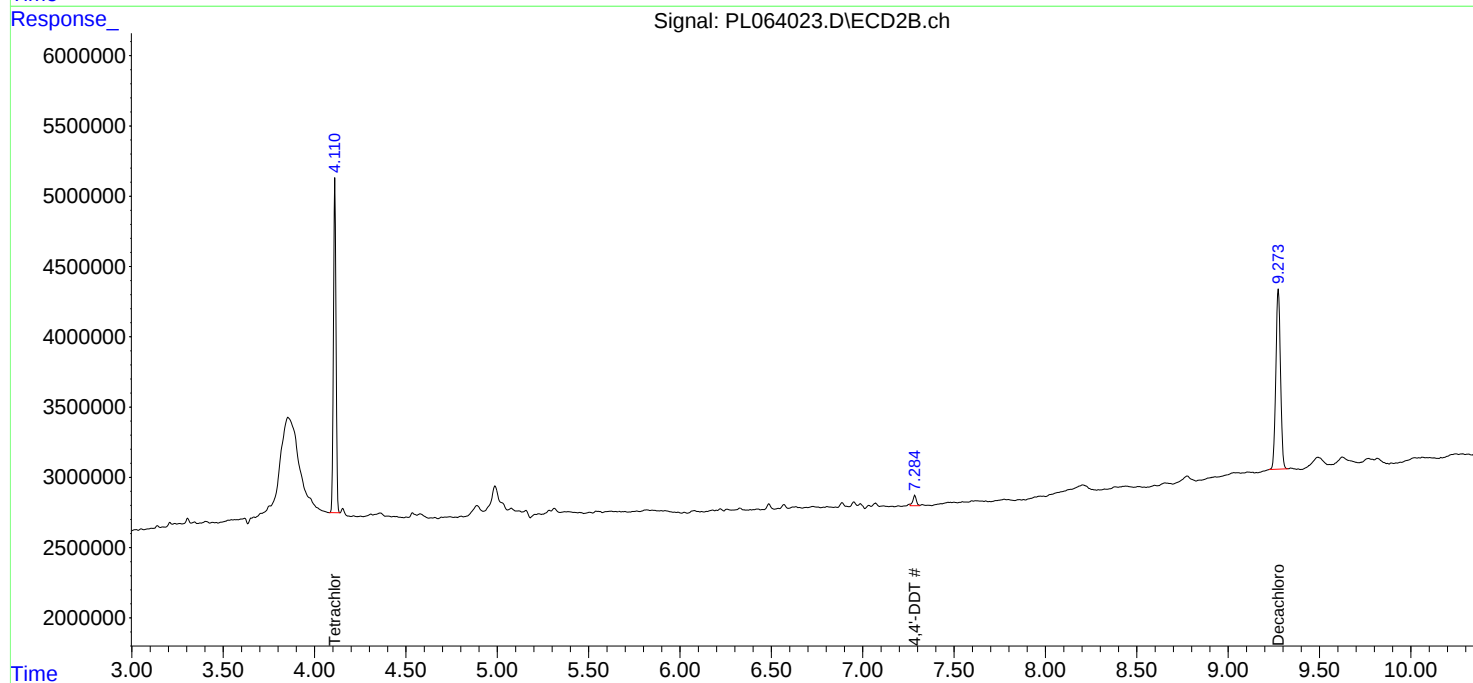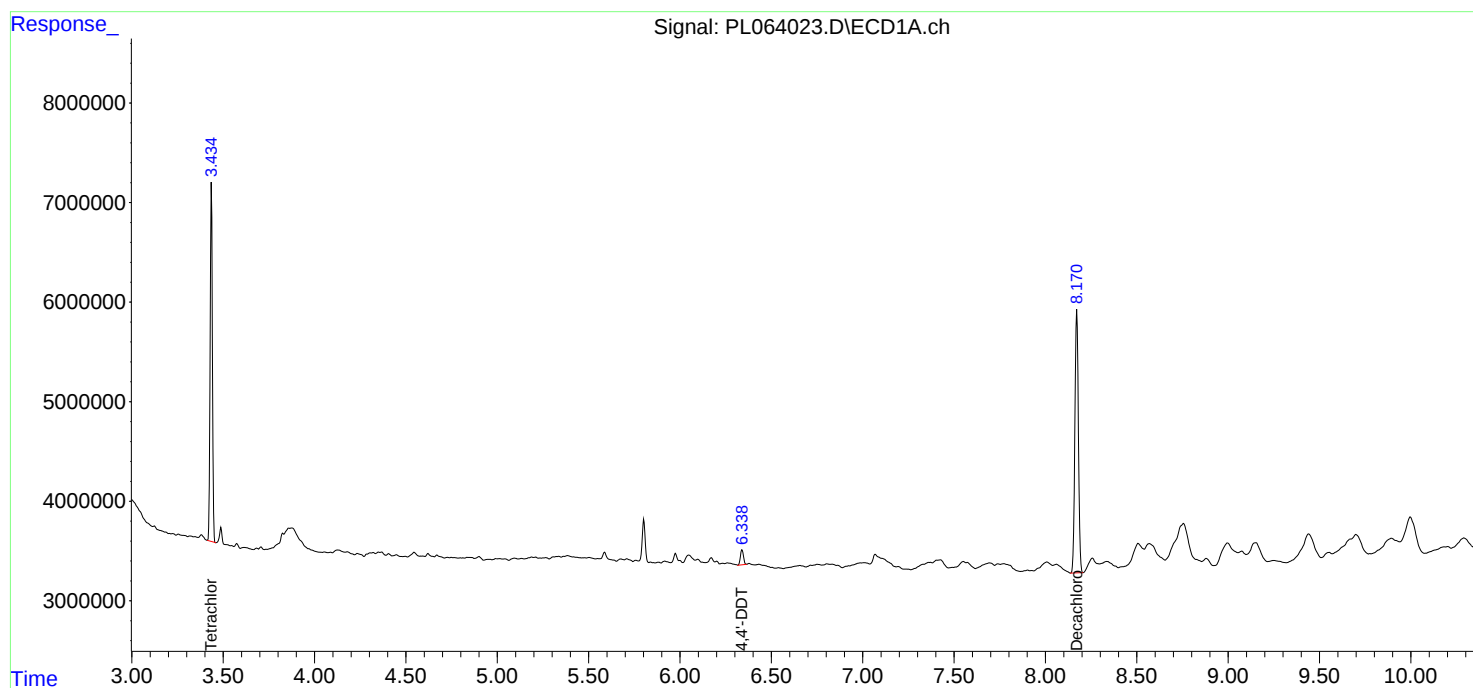

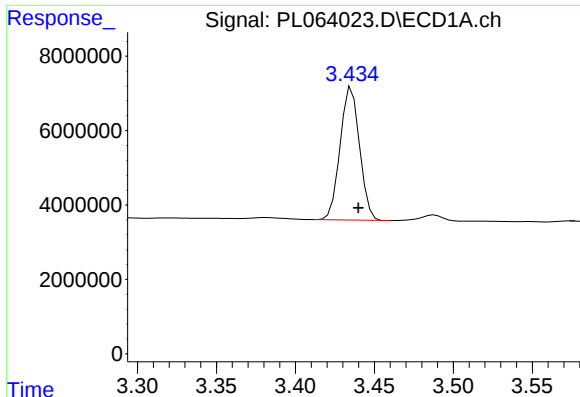


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: -0.004 min
Response: 30668902
Conc: 10.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:50 AM

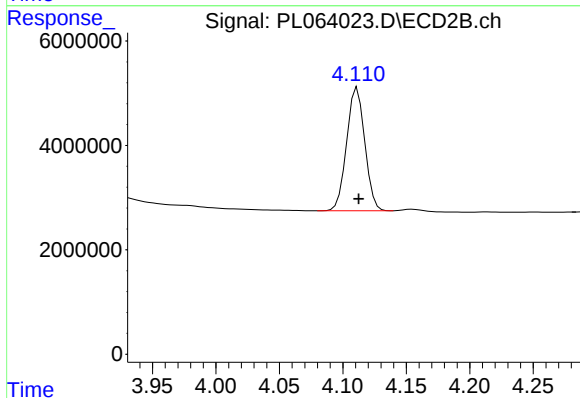


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.001 min
Response: 23435816
Conc: 9.18 ng/ml

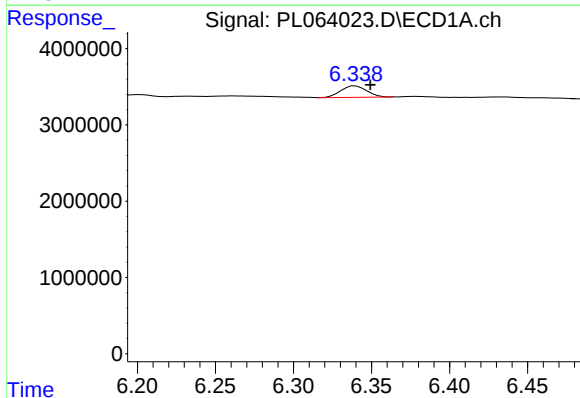


#17 4,4'-DDT

R.T.: 6.338 min
Delta R.T.: -0.011 min
Response: 1753818
Conc: 0.66 ng/ml m

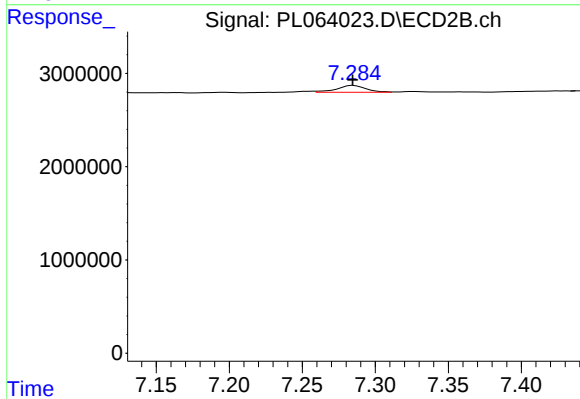

#17 4,4'-DDT

R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1001005
Conc: 0.51 ng/ml m

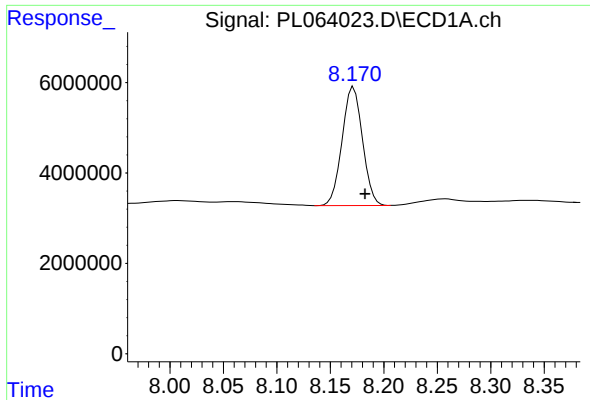


#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: -0.011 min
Response: 34903803
Conc: 12.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
1/11/2021 10:32:50 AM

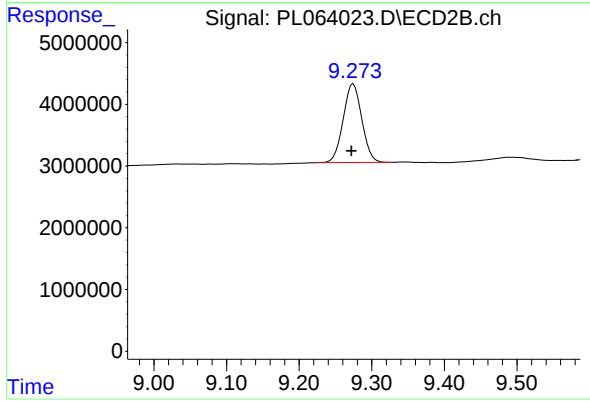

#28 Decachlorobiphenyl

R.T.: 9.275 min
Delta R.T.: 0.003 min
Response: 22702549
Conc: 11.51 ng/ml