

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010825\
 Data File : PL093598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2025 12:36
 Operator : AR\AJ
 Sample : PB165976BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB165976BL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/09/2025
 Supervised By :Ankita Jodhani 01/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 00:13:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.570f	2.776	50176821	57317060	20.268	19.688
28) SA Decachlor...	9.091f	7.916	44410892	70563171	24.019m	23.632

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010825\
Data File : PL093598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2025 12:36
Operator : AR\AJ
Sample : PB165976BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB165976BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/09/2025
Supervised By : Ankita Jodhani 01/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 00:13:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

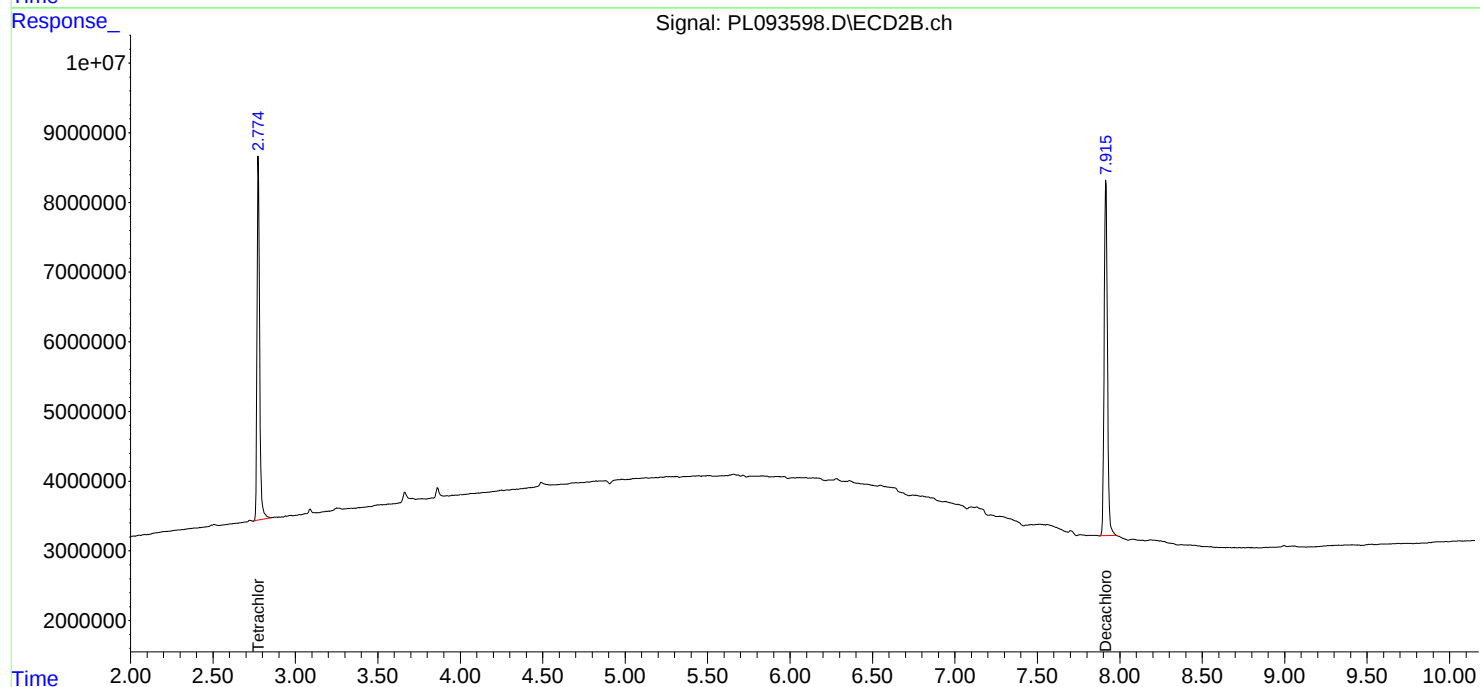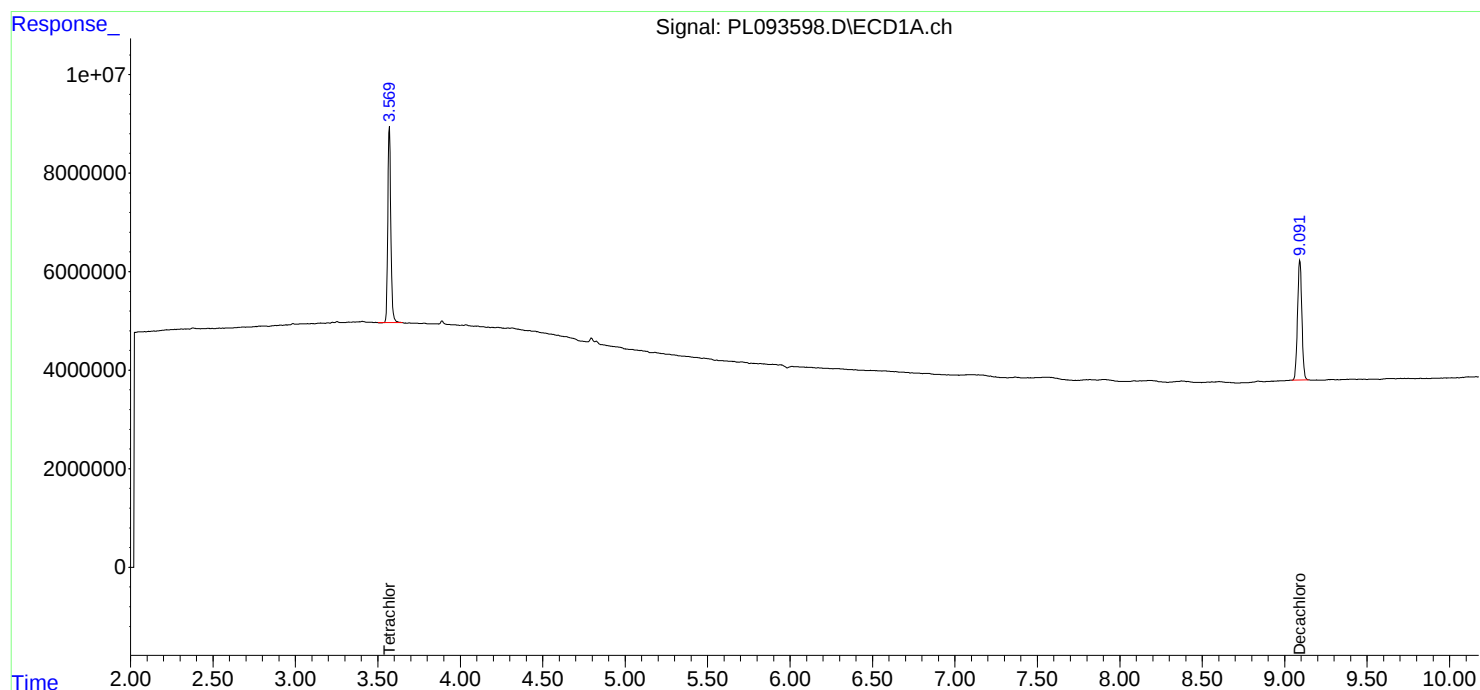

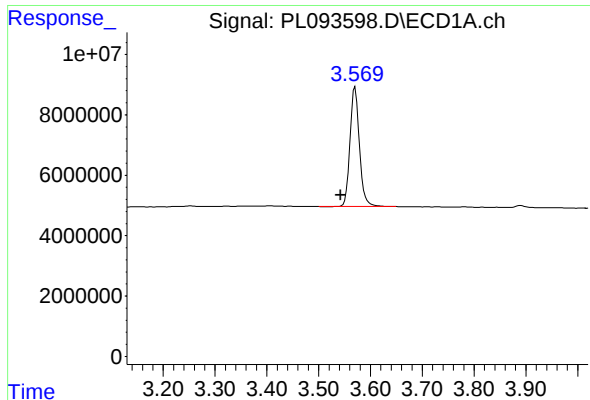


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: 0.028 min
Response: 50176821
Conc: 20.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB165976BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/09/2025
Supervised By :Ankita Jodhani 01/09/2025

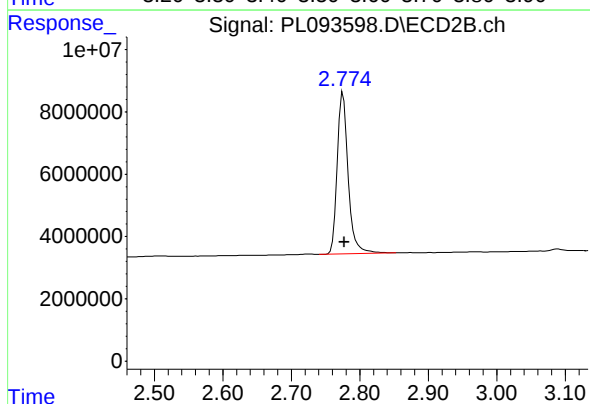


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: -0.002 min
Response: 57317060
Conc: 19.69 ng/ml

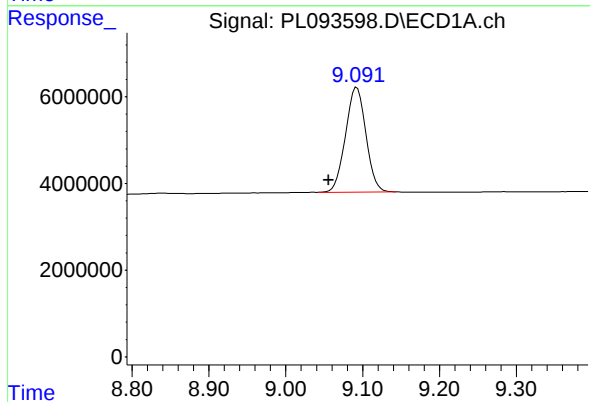

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.035 min
Response: 44410892
Conc: 24.02 ng/ml m

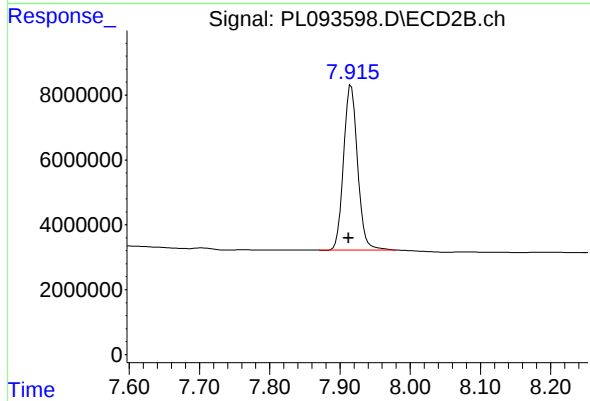

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.004 min
Response: 70563171
Conc: 23.63 ng/ml