

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010920\
 Data File : PL055619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2020 09:41
 Operator : AJ\MA
 Sample : L1017-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-010620

Manual Integrations
 APPROVED

Ankita
 1/9/2020 4:46:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 10:49:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010820.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 09 10:43:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	3.967	202.3E6	60042506	18.143m	19.530
28)	SA Decachlor...	8.235	8.951	181.7E6	40912054	18.727	17.685

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010920\
Data File : PL055619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2020 09:41
Operator : AJ\MA
Sample : L1017-03
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR-04-010620


Manual Integrations
APPROVED

Ankita
1/9/2020 4:46:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 10:49:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010820.M
Quant Title : GC Extractables
QLast Update : Thu Jan 09 10:43:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

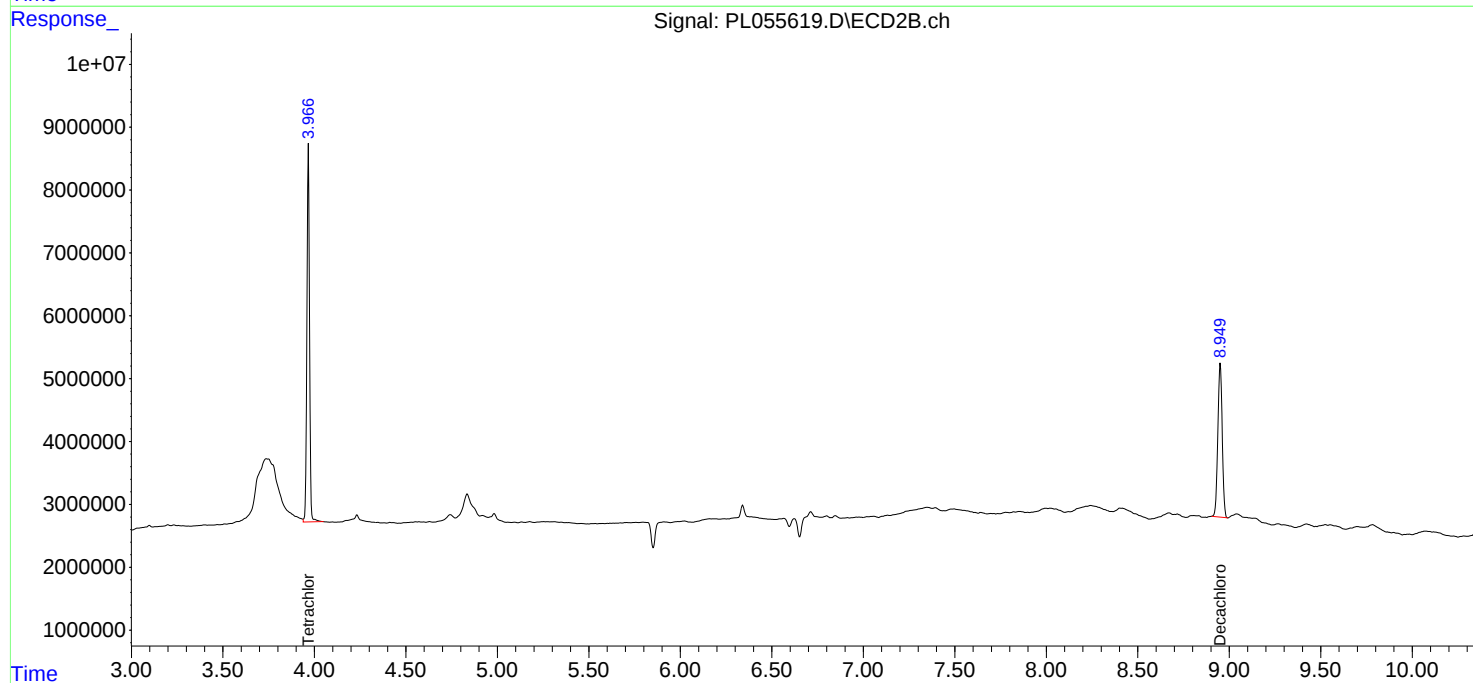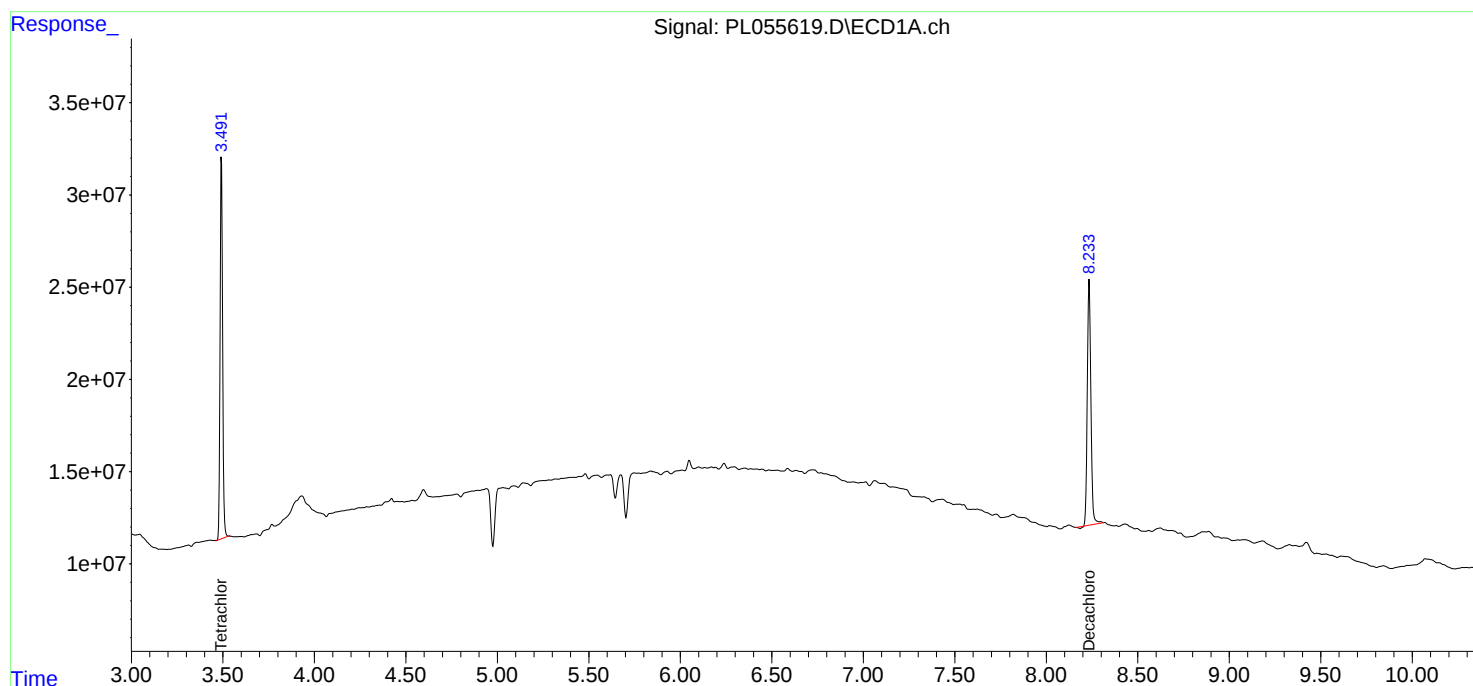

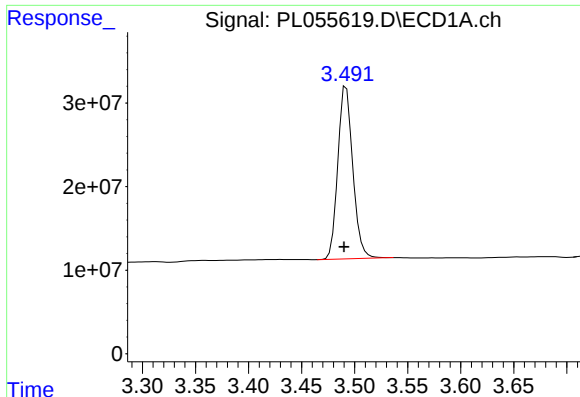


#1 Tetrachloro-m-xylene

R.T.: 3.491 min
Delta R.T.: 0.000 min
Response: 202349125
Conc: 18.14 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-04-010620


Manual Integrations
APPROVED

Ankita
1/9/2020 4:46:41 PM

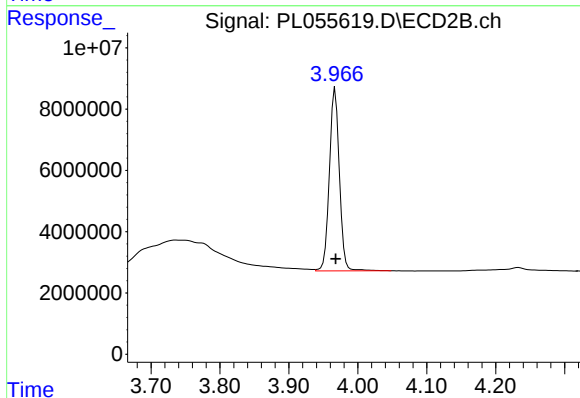


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 60042506
Conc: 19.53 ng/ml

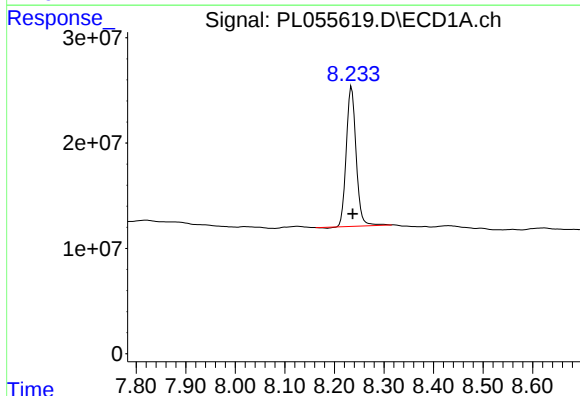

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: -0.002 min
Response: 181682427
Conc: 18.73 ng/ml

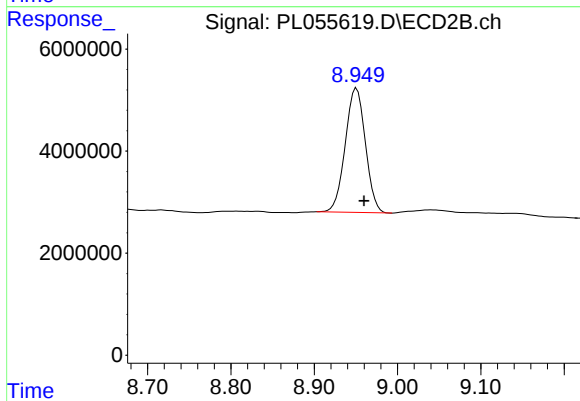

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.009 min
Response: 40912054
Conc: 17.68 ng/ml