

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010923\
 Data File : PL080169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2023 14:35
 Operator : AR\AJ
 Sample : PB150109BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB150109BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/10/2023
 Supervised By : Ankita Jodhani 01/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 20:33:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:11:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.378	2.692	35062632	36618988	17.627	16.105
2) SA Decachlor...	8.900	7.847	36265774	42189628	21.137m	18.674

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010923\
Data File : PL080169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2023 14:35
Operator : AR\AJ
Sample : PB150109BL
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
PB150109BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/10/2023
Supervised By : Ankita Jodhani 01/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 20:33:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:11:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

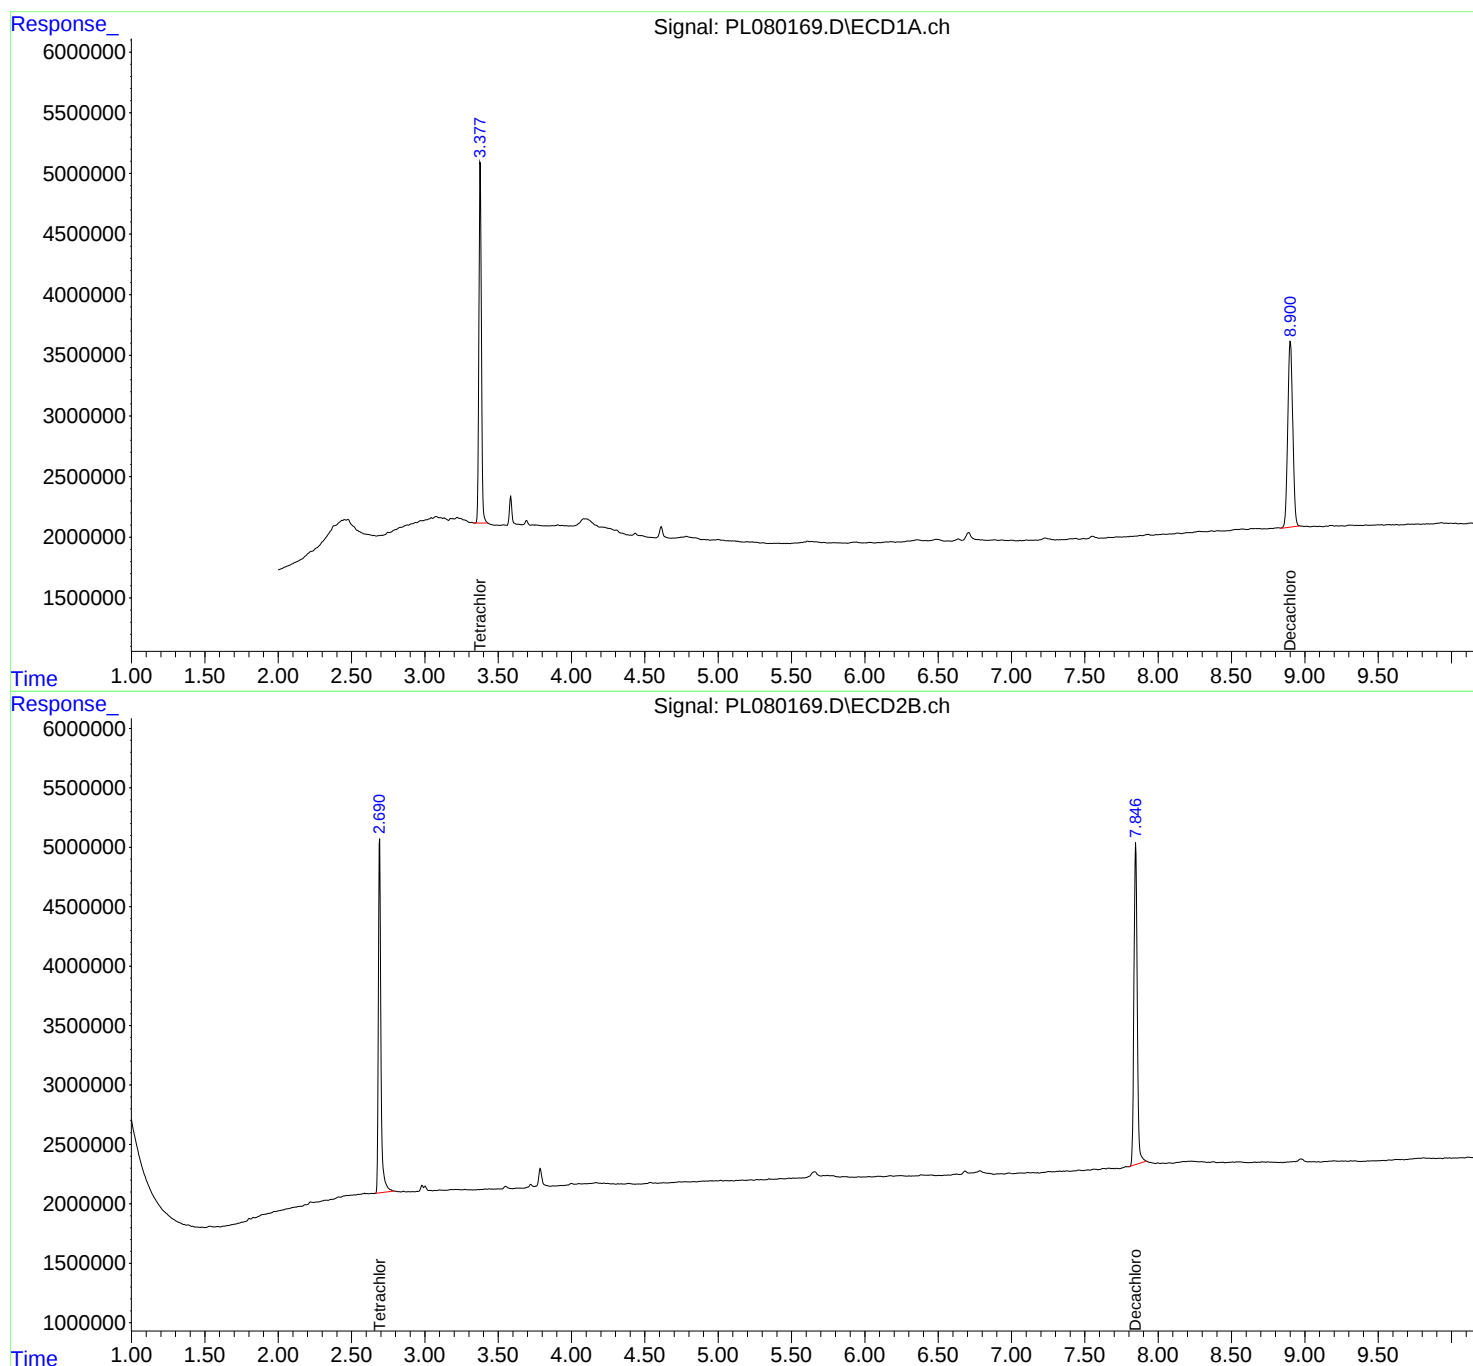

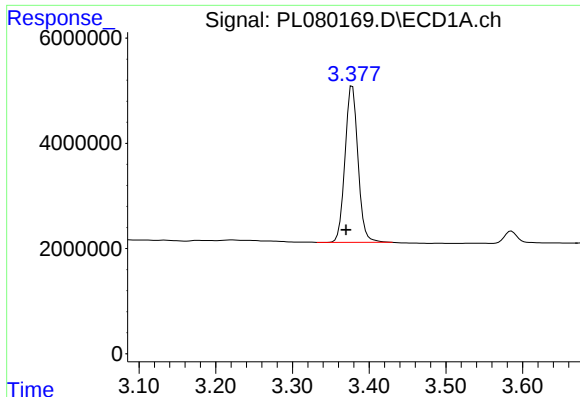


#1 Tetrachloro-m-xylene

R.T.: 3.378 min
Delta R.T.: 0.008 min
Response: 35062632
Conc: 17.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB150109BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/10/2023
Supervised By :Ankita Jodhani 01/10/2023

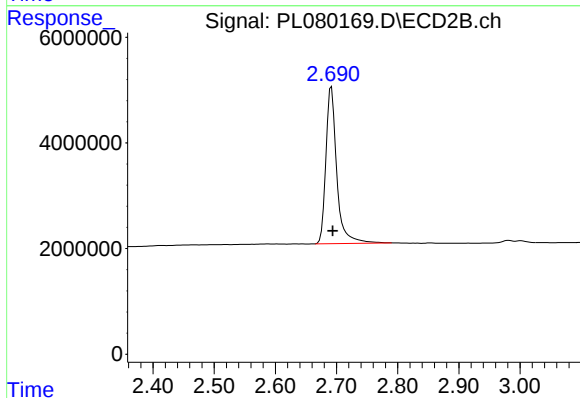


#1 Tetrachloro-m-xylene

R.T.: 2.692 min
Delta R.T.: -0.002 min
Response: 36618988
Conc: 16.10 ng/ml

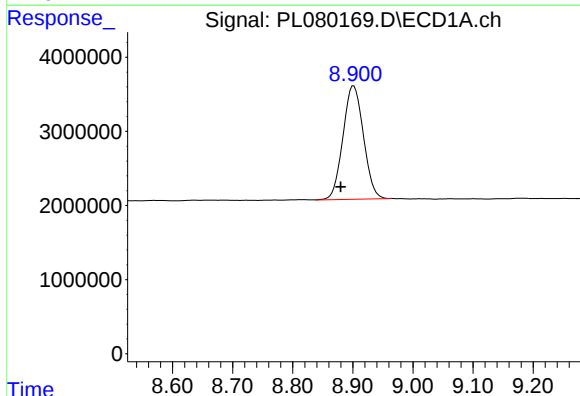

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.020 min
Response: 36265774
Conc: 21.14 ng/ml m

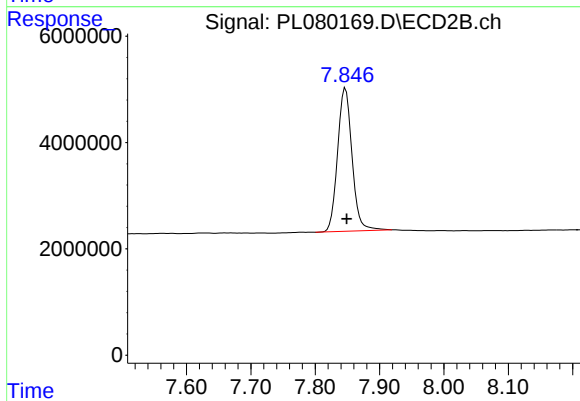

#28 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: -0.002 min
Response: 42189628
Conc: 18.67 ng/ml