

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011019\
 Data File : PL043746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2019 13:43
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 23:04:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011019.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 10 23:04:29 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	4.009	208.7E6	81272541	50.000	50.000
28)	SA Decachlor...	8.304	9.083	234.5E6	64508374	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.441	5.007	85019730	36331982	500.000	500.000
24)	Chlordane-2	4.943	5.475	98549620	35206081	500.000	500.000
25)	Chlordane-3	5.512	6.122	292.7E6	125.1E6	500.000	500.000
26)	Chlordane-4	5.568	6.196	243.4E6	148.2E6	500.000	500.000
27)	Chlordane-5	6.405	7.001	78824148	26282780	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011019\
Data File : PL043746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2019 13:43
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 23:04:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011019.M
Quant Title : GC Extractables
QLast Update : Thu Jan 10 23:04:29 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

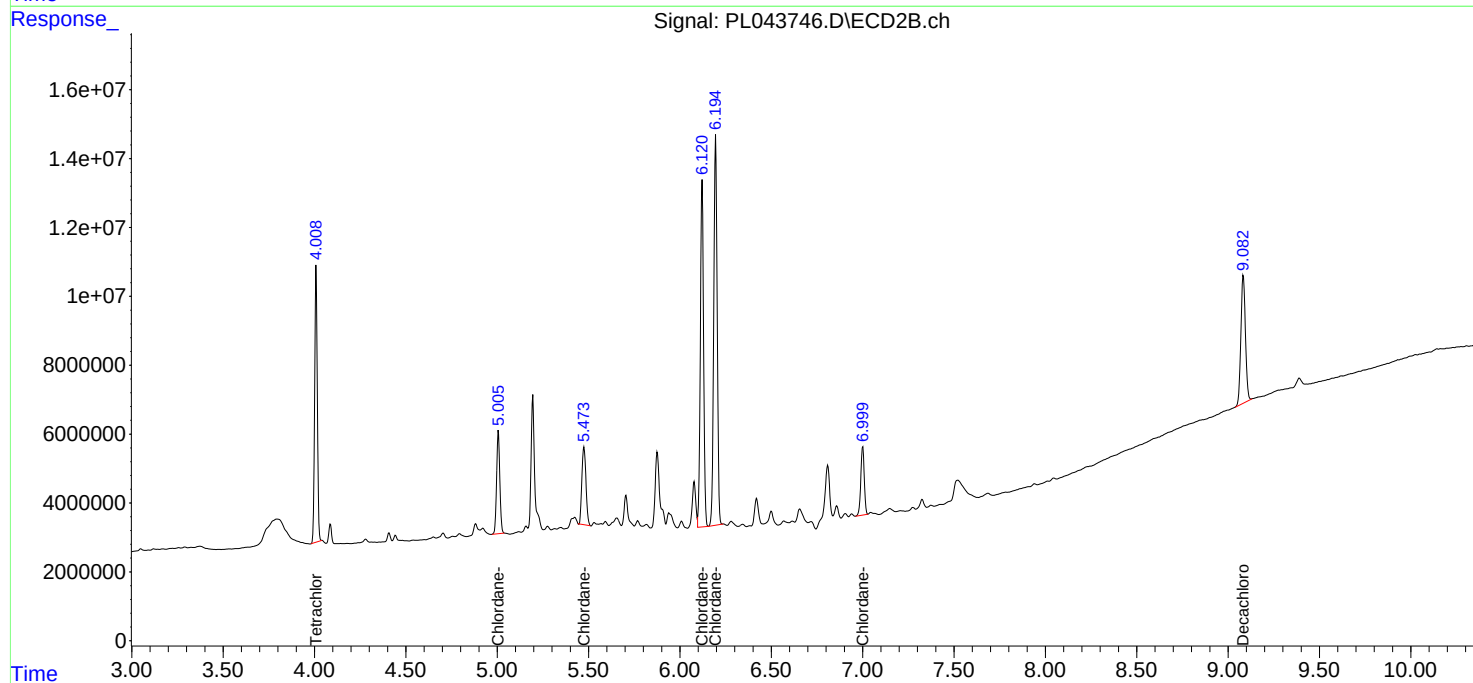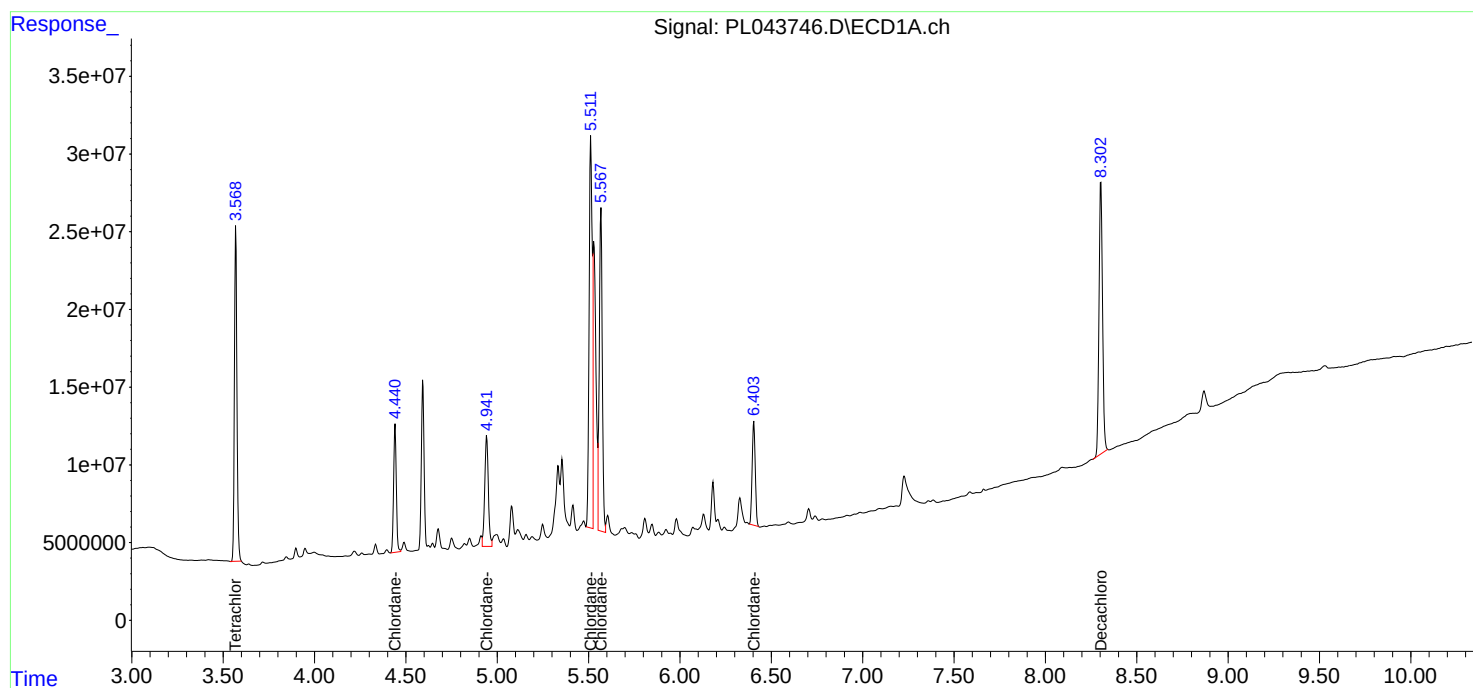


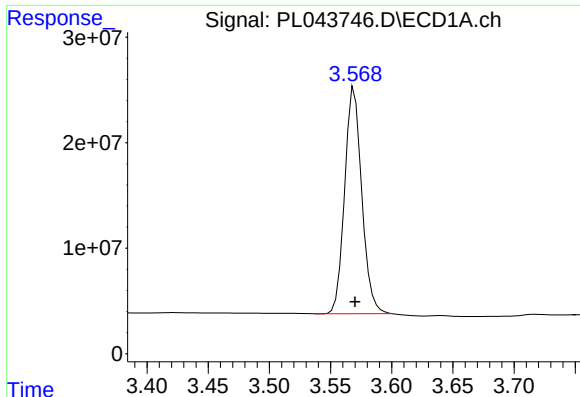

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 208652373
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

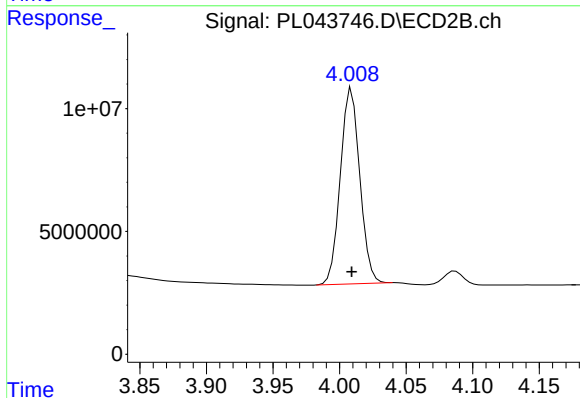


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 81272541
Conc: 50.00 ng/ml

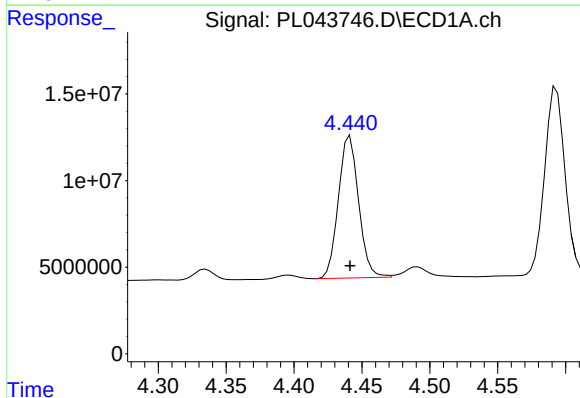


#23 Chlordane-1

R.T.: 4.441 min
Delta R.T.: 0.000 min
Response: 85019730
Conc: 500.00 ng/ml

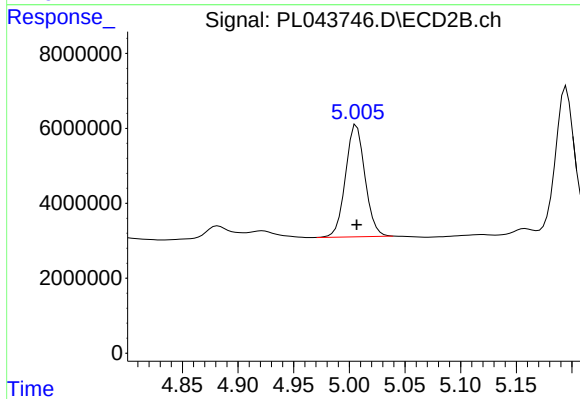

#23 Chlordane-1


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 36331982
Conc: 500.00 ng/ml

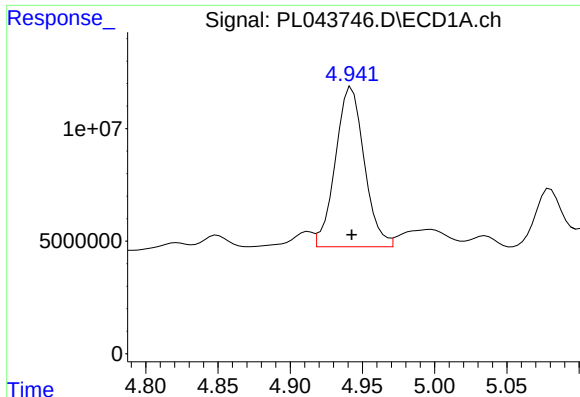

#24 Chlordane-2


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 98549620
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

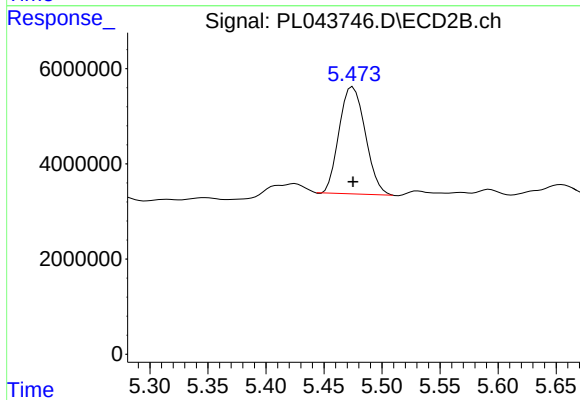


#24 Chlordane-2

R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 35206081
Conc: 500.00 ng/ml

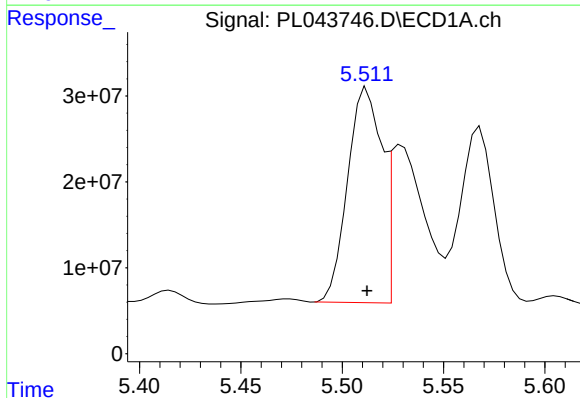


#25 Chlordane-3

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 292658380
Conc: 500.00 ng/ml

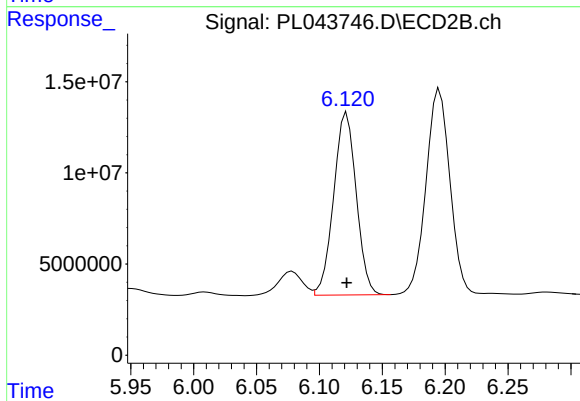

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 125075785
Conc: 500.00 ng/ml

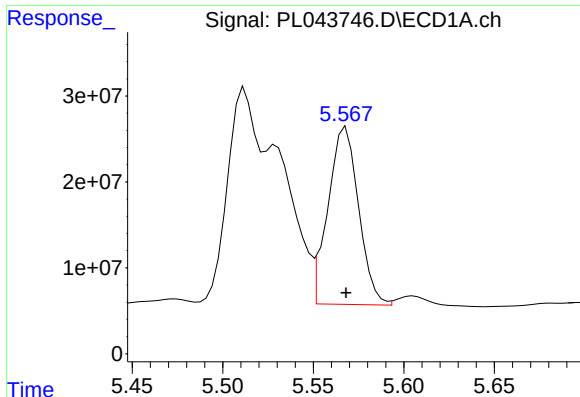

#26 Chlordane-4


R.T.: 5.568 min
Delta R.T.: 0.000 min
Response: 243422669
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

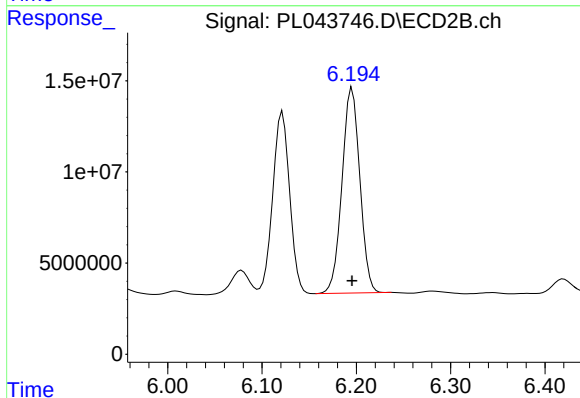


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 148239272
Conc: 500.00 ng/ml

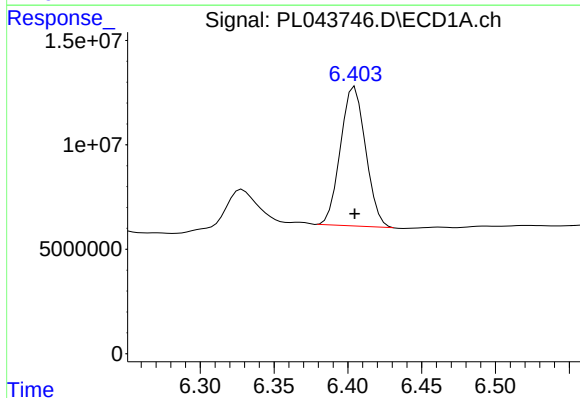


#27 Chlordane-5

R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 78824148
Conc: 500.00 ng/ml

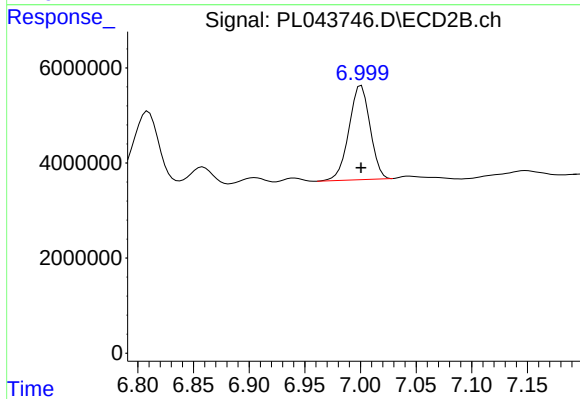

#27 Chlordane-5


R.T.: 7.001 min
Delta R.T.: 0.000 min
Response: 26282780
Conc: 500.00 ng/ml

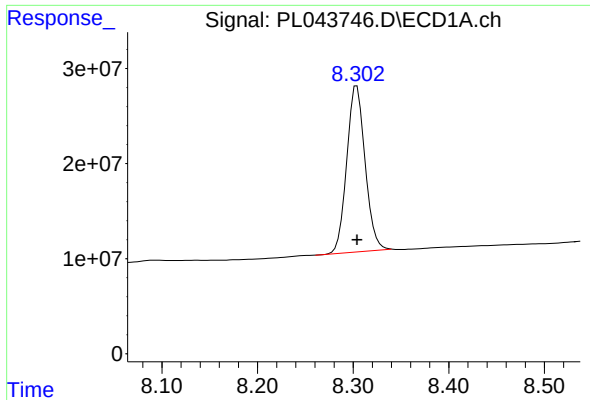

#28 Decachlorobiphenyl

R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 234536285
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

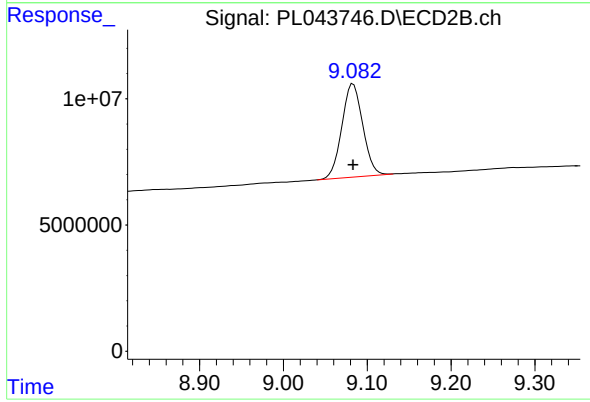

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 64508374
Conc: 50.00 ng/ml