

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011020\
 Data File : PL055630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2020 13:46
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 15:24:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 09 15:23:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	3.970	138.2E6	40678750	14.960	15.356
28)	SA Decachlor...	8.236	8.961	137.0E6	32380838	15.597	15.575
Target Compounds							
9)	A Endosulfan I	5.542	6.167	88861651	19851884	7.192	7.498
10)	B gamma-Chl...	5.430	6.046	93326511	20594292	6.971	7.315
12)	B 4,4'-DDE	5.651	6.272	180.3E6	38334980	14.502	14.429
13)	MA Dieldrin	5.786	6.422	187.9E6	40074426	14.336	14.656
19)	B Endosulfa...	6.695	7.188	141.7E6	32507521	14.485	14.611
20)	A Methoxychlor	6.950	7.508	317.0E6	74239614	73.847	70.917
21)	B Endrin ke...	7.184	7.656	153.5E6	34262264	13.542	14.390



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011020\
Data File : PL055630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2020 13:46
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 15:24:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Thu Jan 09 15:23:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

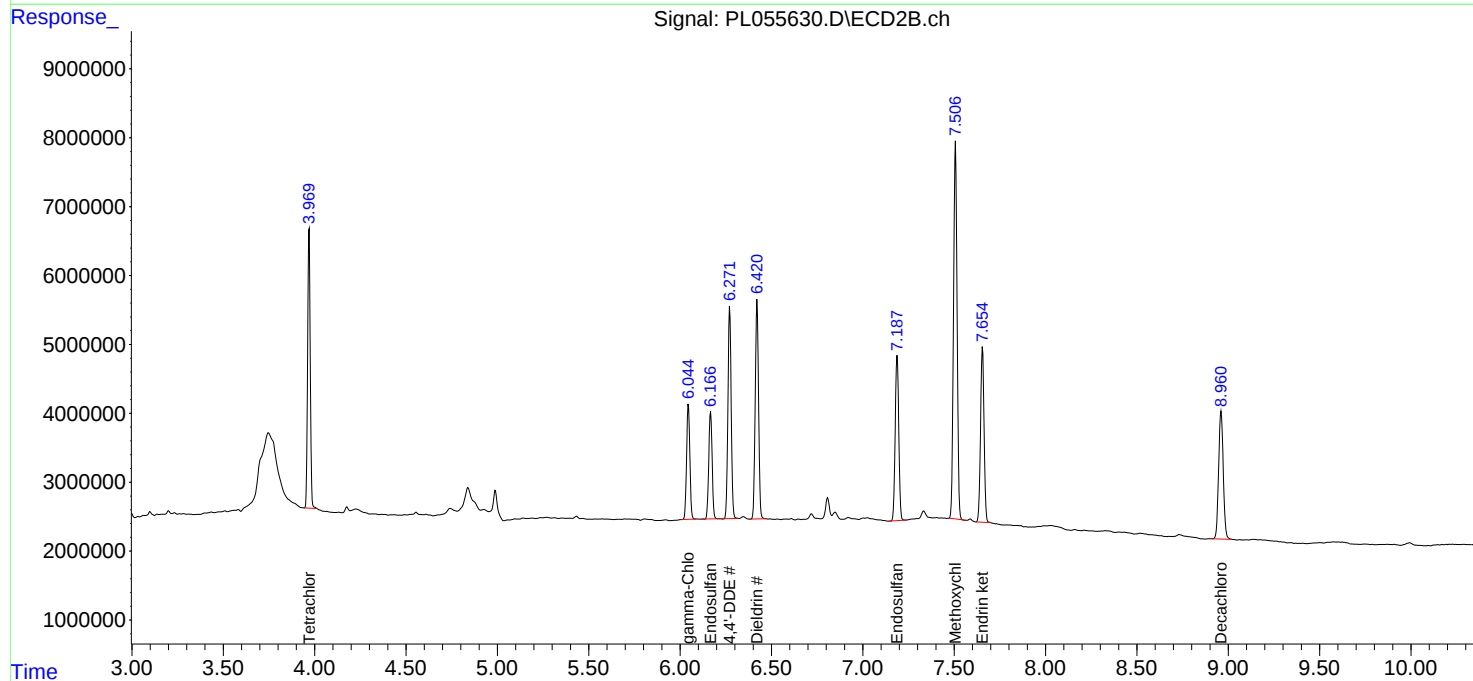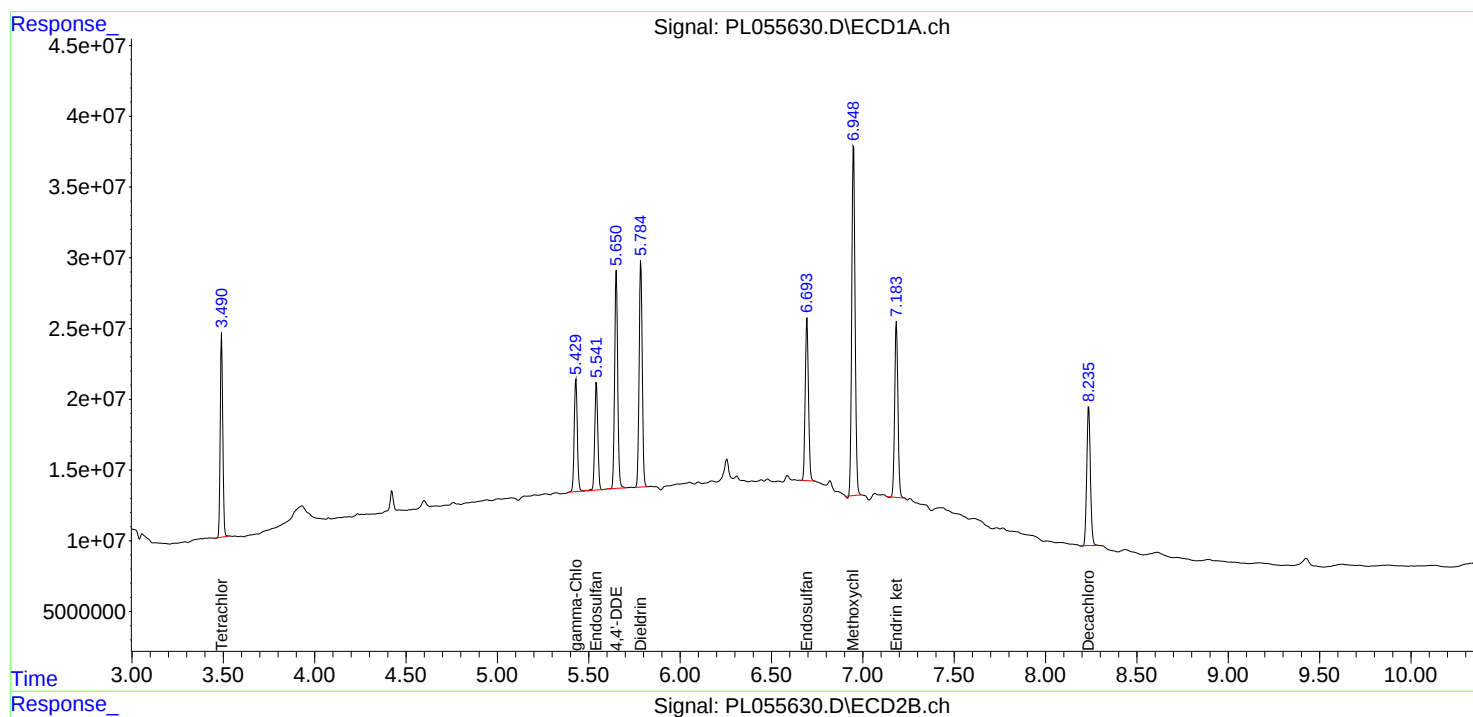


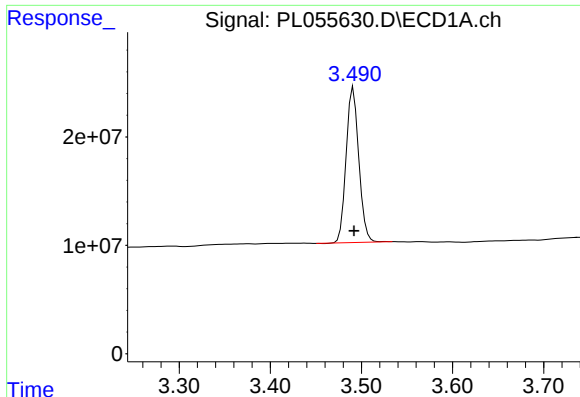

#1 Tetrachloro-m-xylene


R.T.: 3.491 min
Delta R.T.: 0.000 min
Response: 138238801
Conc: 14.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

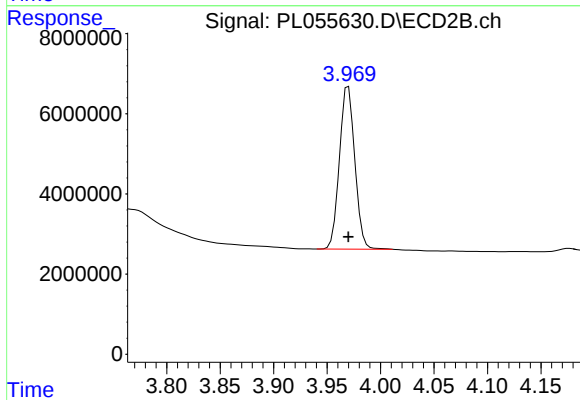


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 40678750
Conc: 15.36 ng/ml

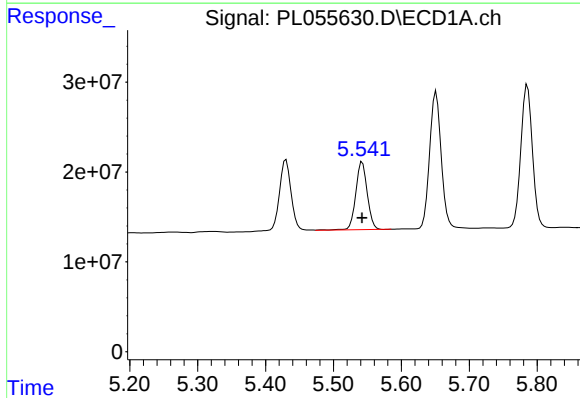


#9 Endosulfan I

R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 88861651
Conc: 7.19 ng/ml

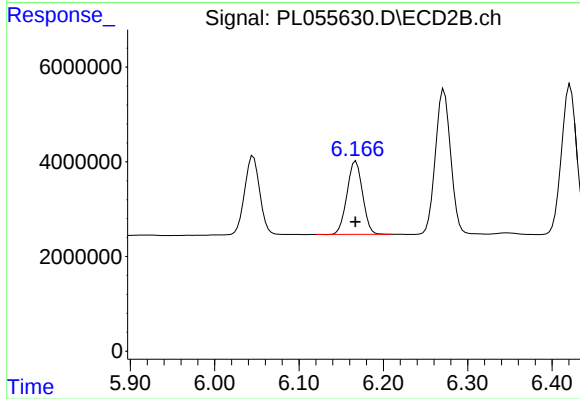

#9 Endosulfan I


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 19851884
Conc: 7.50 ng/ml

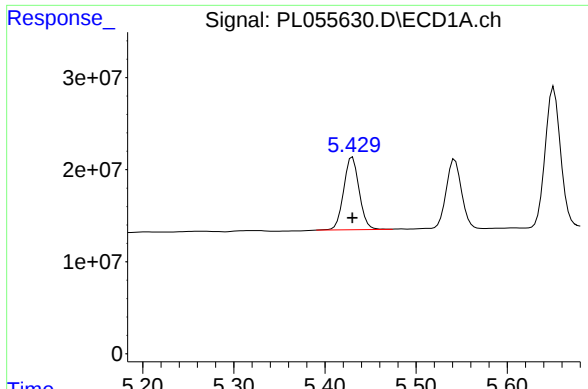

#10 gamma-Chlordane


R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 93326511
Conc: 6.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

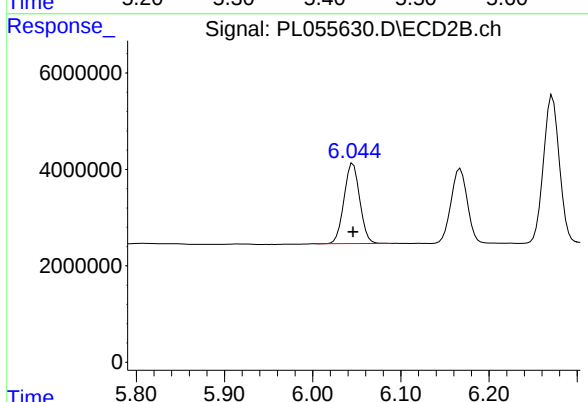


#10 gamma-Chlordane

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 20594292
Conc: 7.32 ng/ml

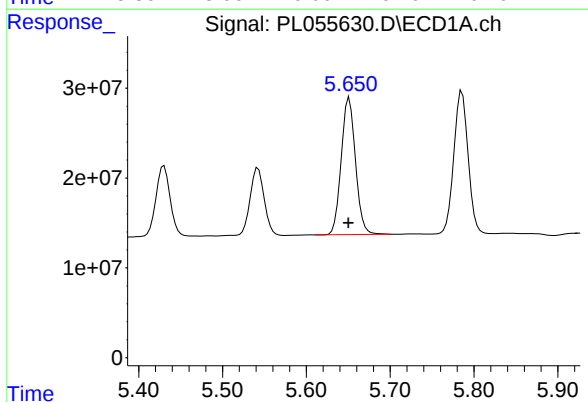


#12 4,4'-DDE

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 180327519
Conc: 14.50 ng/ml

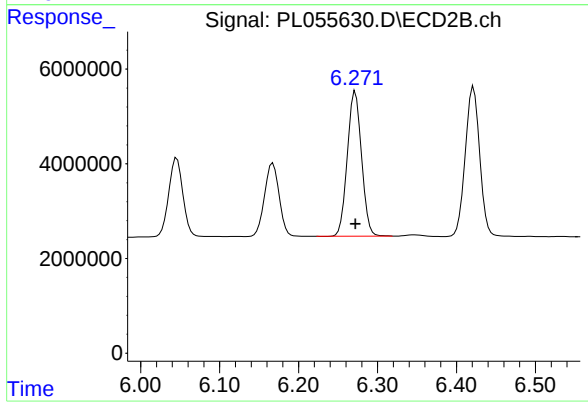

#12 4,4'-DDE


R.T.: 6.272 min
Delta R.T.: 0.000 min
Response: 38334980
Conc: 14.43 ng/ml

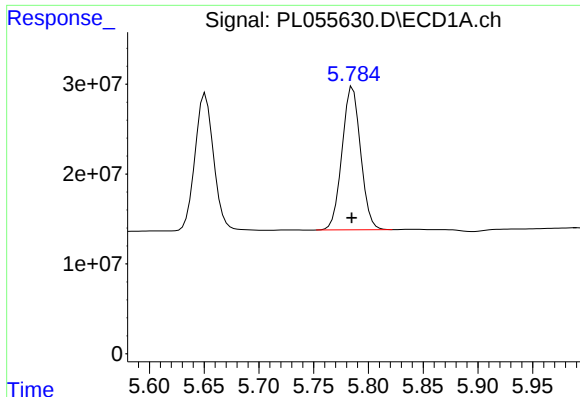

#13 Dieldrin


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 187924368
Conc: 14.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

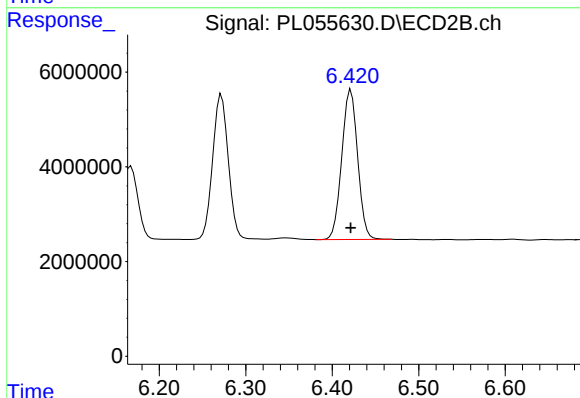


#13 Dieldrin

R.T.: 6.422 min
Delta R.T.: 0.000 min
Response: 40074426
Conc: 14.66 ng/ml

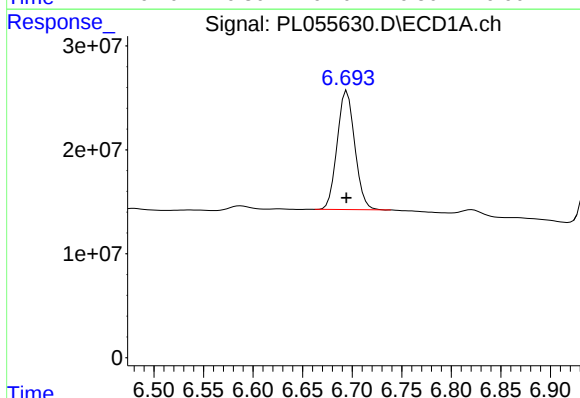


#19 Endosulfan Sulfate

R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 141696812
Conc: 14.49 ng/ml

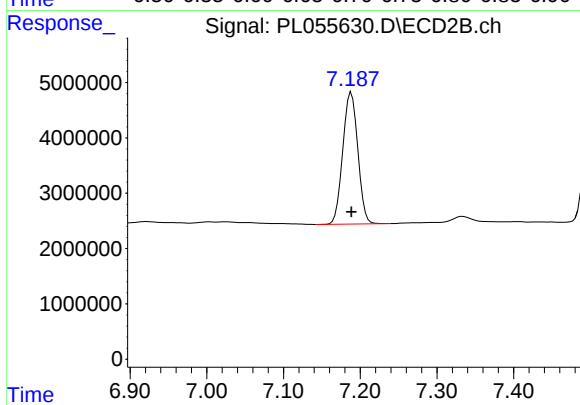

#19 Endosulfan Sulfate


R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 32507521
Conc: 14.61 ng/ml

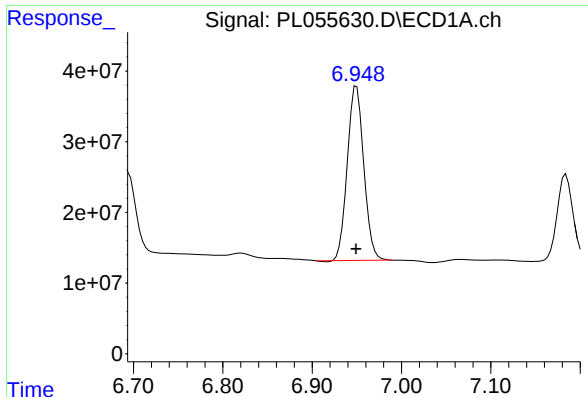

#20 Methoxychlor


R.T.: 6.950 min
Delta R.T.: 0.000 min
Response: 317018387
Conc: 73.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

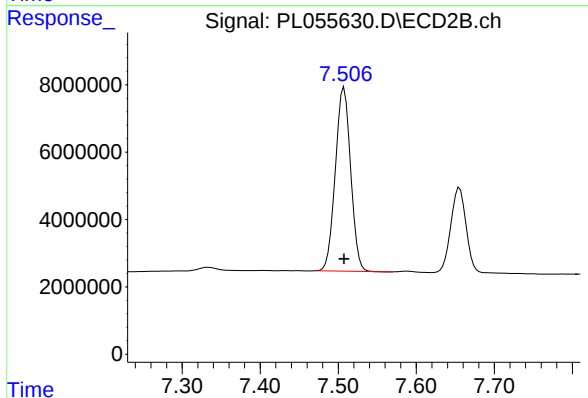


#20 Methoxychlor

R.T.: 7.508 min
Delta R.T.: 0.000 min
Response: 74239614
Conc: 70.92 ng/ml

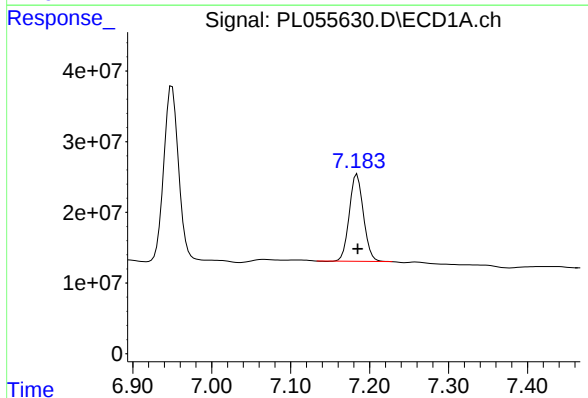


#21 Endrin ketone

R.T.: 7.184 min
Delta R.T.: 0.000 min
Response: 153510579
Conc: 13.54 ng/ml

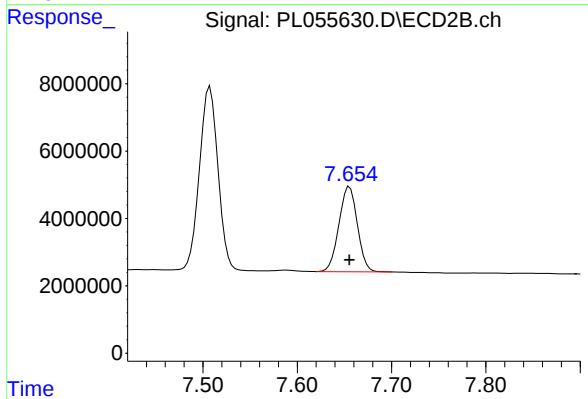

#21 Endrin ketone


R.T.: 7.656 min
Delta R.T.: 0.000 min
Response: 34262264
Conc: 14.39 ng/ml

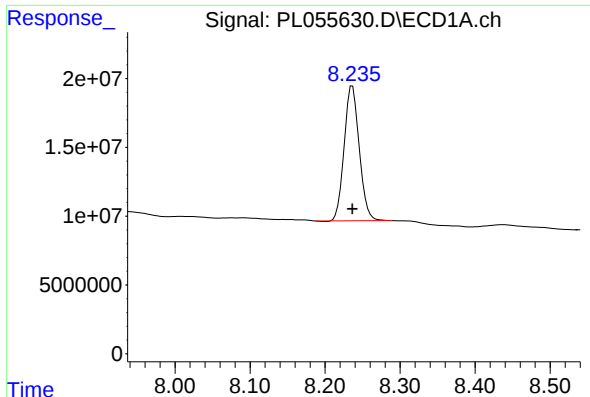

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 136970362
Conc: 15.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

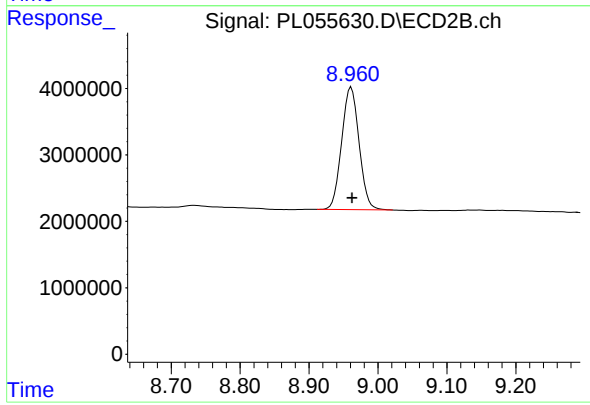

#28 Decachlorobiphenyl

R.T.: 8.961 min
Delta R.T.: 0.000 min
Response: 32380838
Conc: 15.57 ng/ml