

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011020\
 Data File : PL055636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2020 15:10
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 00:56:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:54:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	3.969	495.6E6	130.4E6	50.000	50.000
28)	SA Decachlor...	8.237	8.961	446.8E6	99828721	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.362	4.947	172.9E6	46206503	500.000	500.000
24)	Chlordane-2	4.862	5.407	203.4E6	47939944	500.000	500.000
25)	Chlordane-3	5.430	6.046	588.5E6	170.8E6	500.000	500.000
26)	Chlordane-4	5.488	6.119	488.2E6	200.6E6	500.000	500.000
27)	Chlordane-5	6.324	6.915	180.0E6	35094553	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011020\
Data File : PL055636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2020 15:10
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 00:56:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:54:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

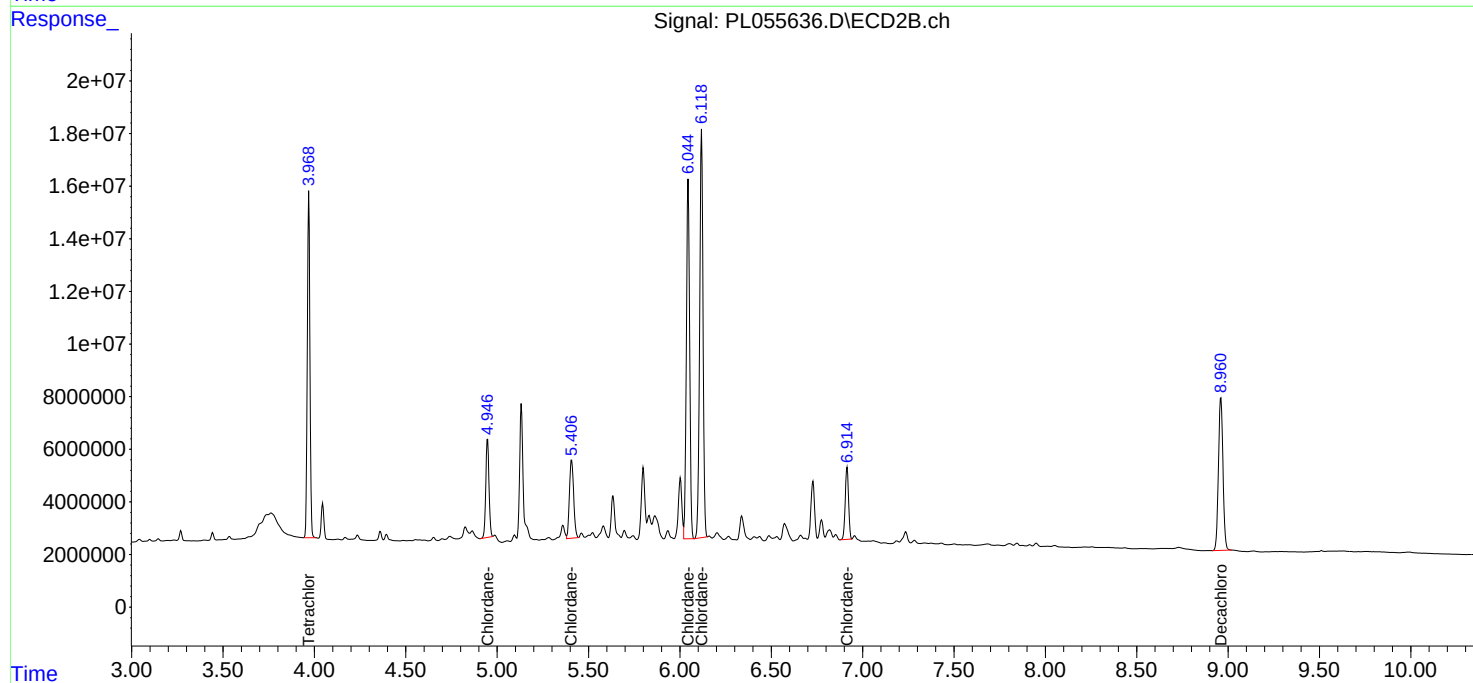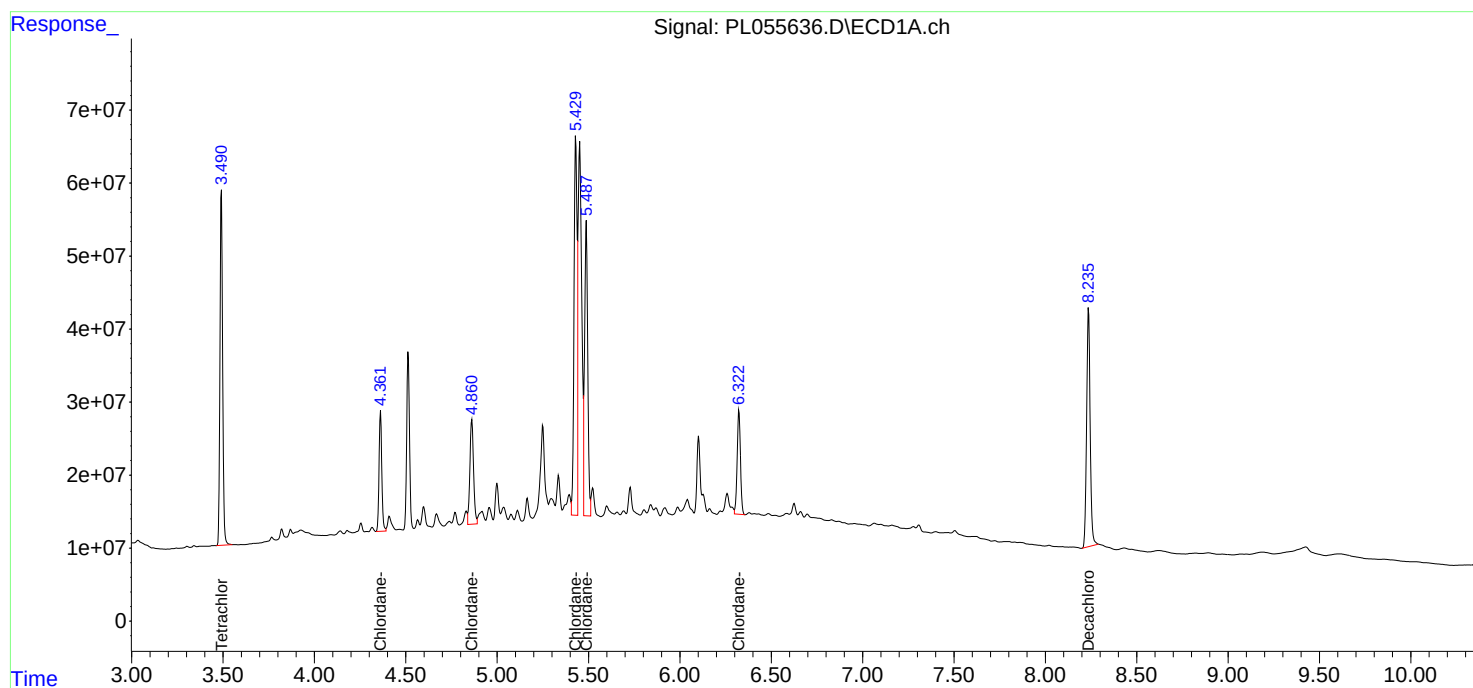


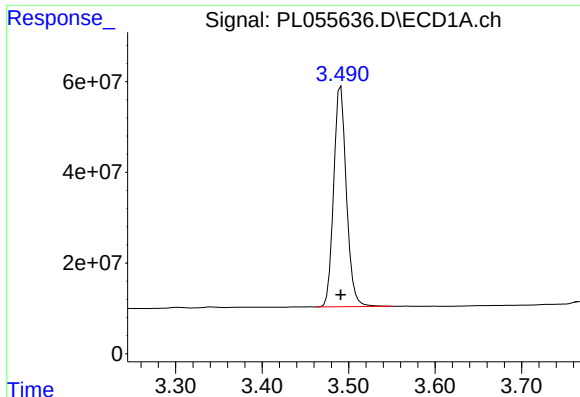

#1 Tetrachloro-m-xylene


R.T.: 3.491 min
Delta R.T.: 0.000 min
Response: 495594973
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

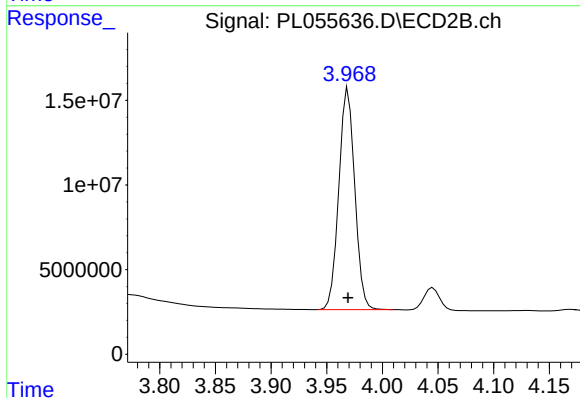


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 130383995
Conc: 50.00 ng/ml

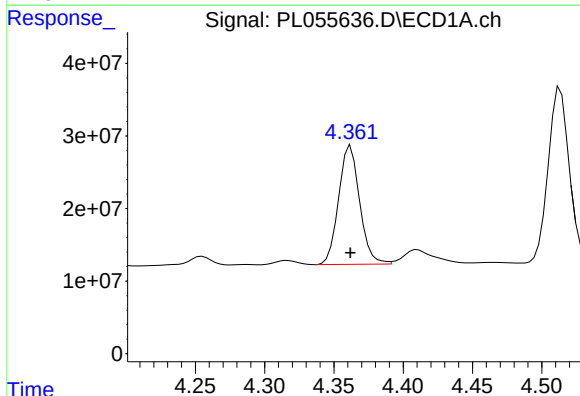


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 172940888
Conc: 500.00 ng/ml

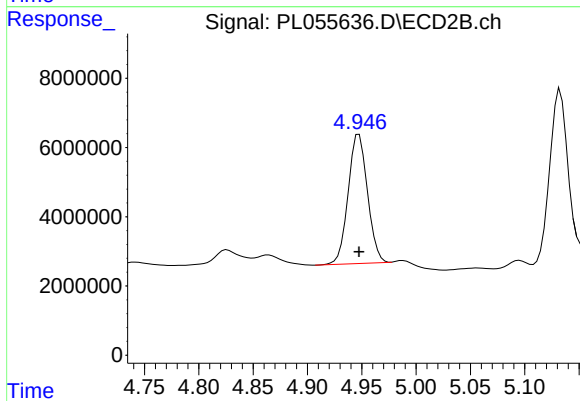

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 46206503
Conc: 500.00 ng/ml

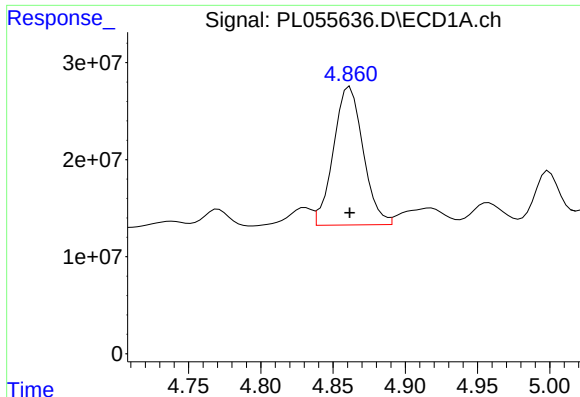

#24 Chlordane-2


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 203356407
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

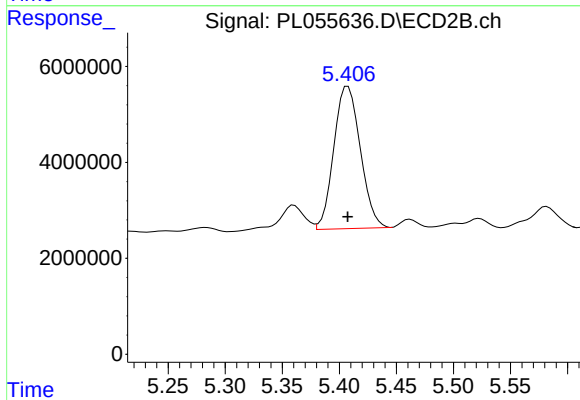


#24 Chlordane-2

R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 47939944
Conc: 500.00 ng/ml

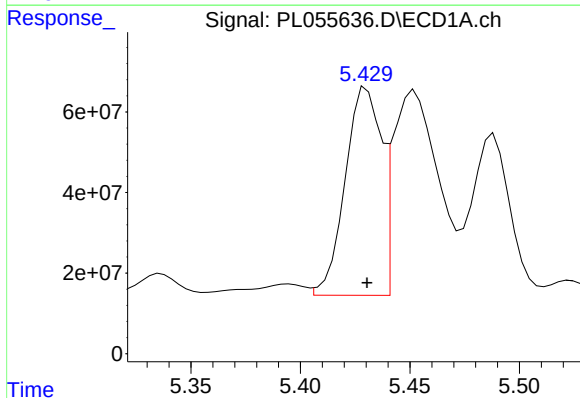


#25 Chlordane-3

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 588542447
Conc: 500.00 ng/ml

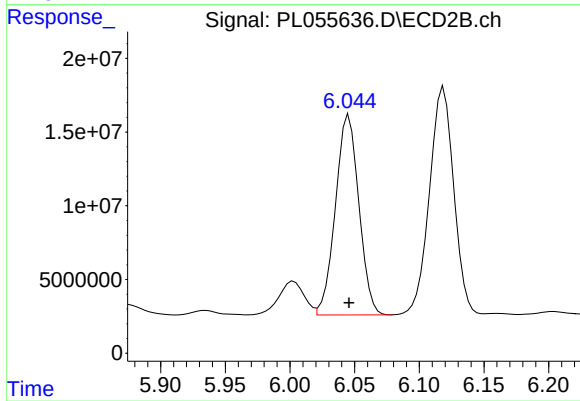

#25 Chlordane-3


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 170760093
Conc: 500.00 ng/ml

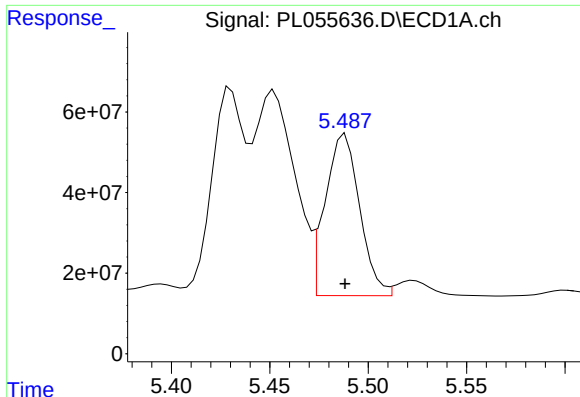

#26 Chlordane-4


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 488188535
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

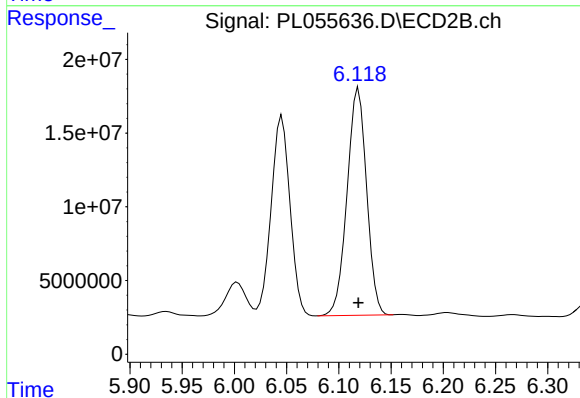


#26 Chlordane-4

R.T.: 6.119 min
Delta R.T.: 0.000 min
Response: 200558852
Conc: 500.00 ng/ml

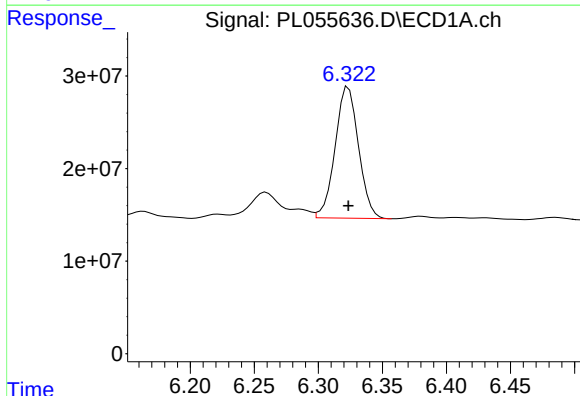


#27 Chlordane-5

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 179988873
Conc: 500.00 ng/ml

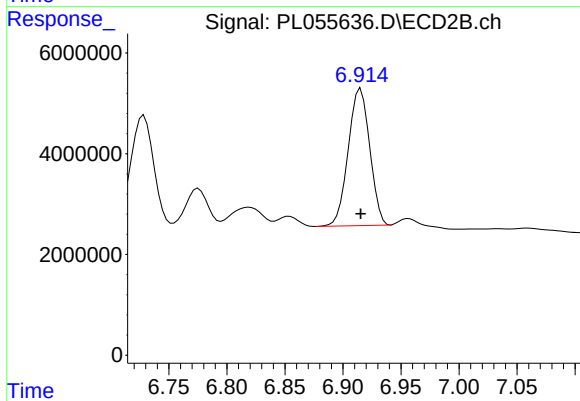

#27 Chlordane-5


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 35094553
Conc: 500.00 ng/ml

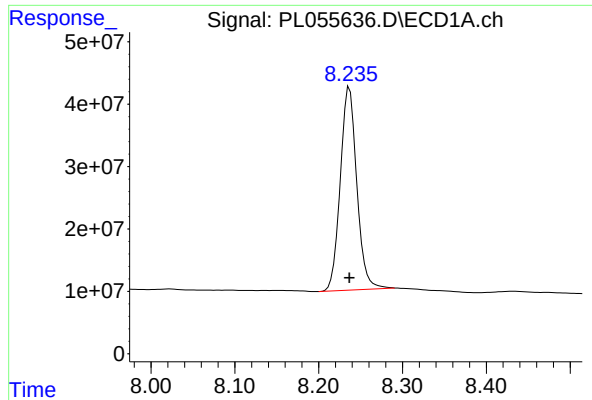

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 446751149
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

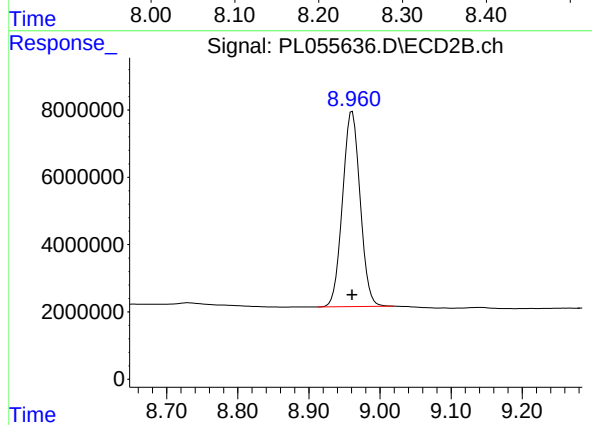

#28 Decachlorobiphenyl

R.T.: 8.961 min
Delta R.T.: 0.000 min
Response: 99828721
Conc: 50.00 ng/ml