

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
 Data File : PL071899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 13:23
 Operator : AR\AJ
 Sample : N1054-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:30:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.566	5.495	9248301	25021194	20.020	20.365
28)	SA Decachlor...	10.327	11.392	10326672	17076694	14.283	14.411
Target Compounds							
6)	B beta-BHC	6.045f	0.000	300896	0	1.112	N.D. #
7)	B delta-BHC	0.000	6.975f	0	429287	N.D.	0.280 #
9)	A Endosulfan I	0.000	8.351	0	81710	N.D.	0.066 #
10)	B gamma-Chl...	0.000	8.226	0	316513	N.D.	0.231 #
11)	B alpha-Chl...	0.000	8.299	0	42019	N.D.	0.032 #
15)	B Endosulfa...	0.000	9.098f	0	158604	N.D.	0.141 #
16)	A 4,4'-DDD	0.000	9.032	0	68929	N.D.	0.072 #
19)	B Endosulfa...	0.000	9.510f	0	134889	N.D.	0.130 #
21)	B Endrin ke...	0.000	10.019f	0	753523	N.D.	0.668 #
25)	Chlordane-3	0.000	8.226	0	316513	N.D.	1.551 #
26)	Chlordane-4	0.000	8.299	0	42019	N.D.	0.173 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
Data File : PL071899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 13:23
Operator : AR\AJ
Sample : N1054-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:30:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

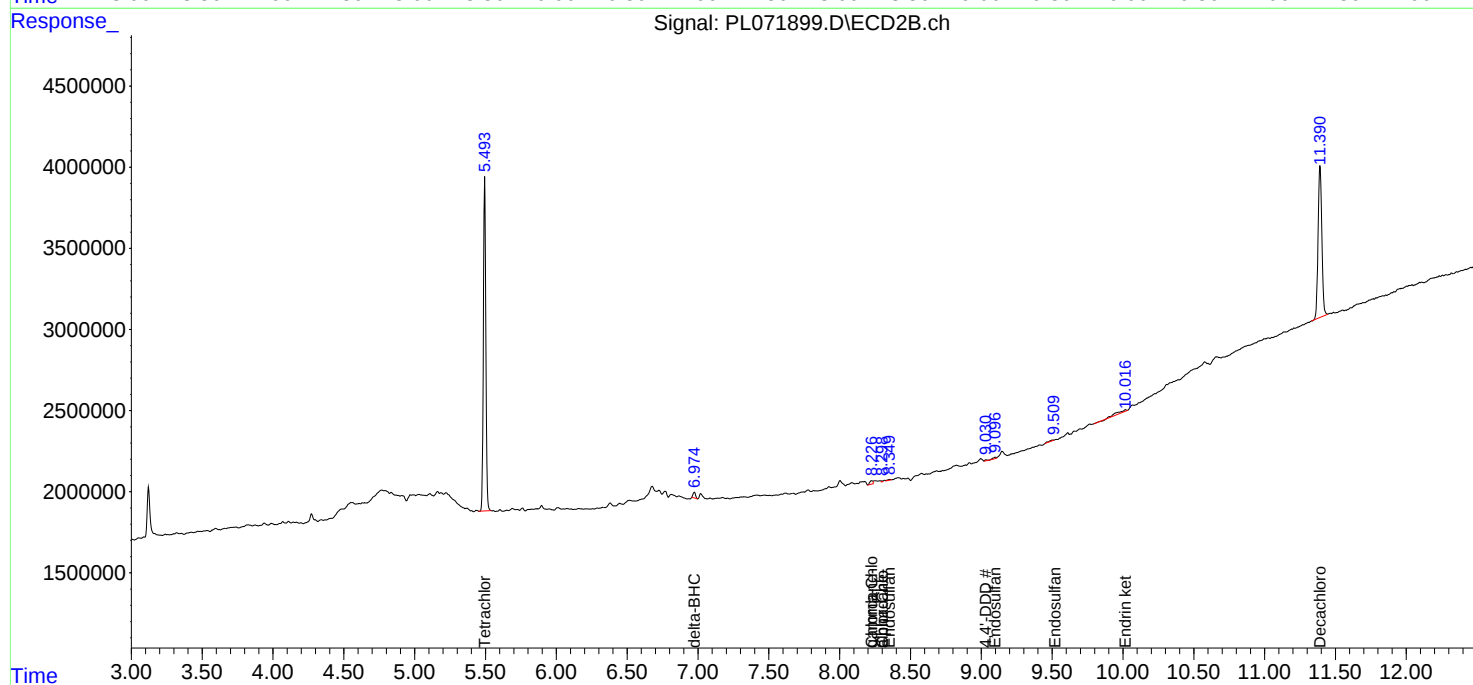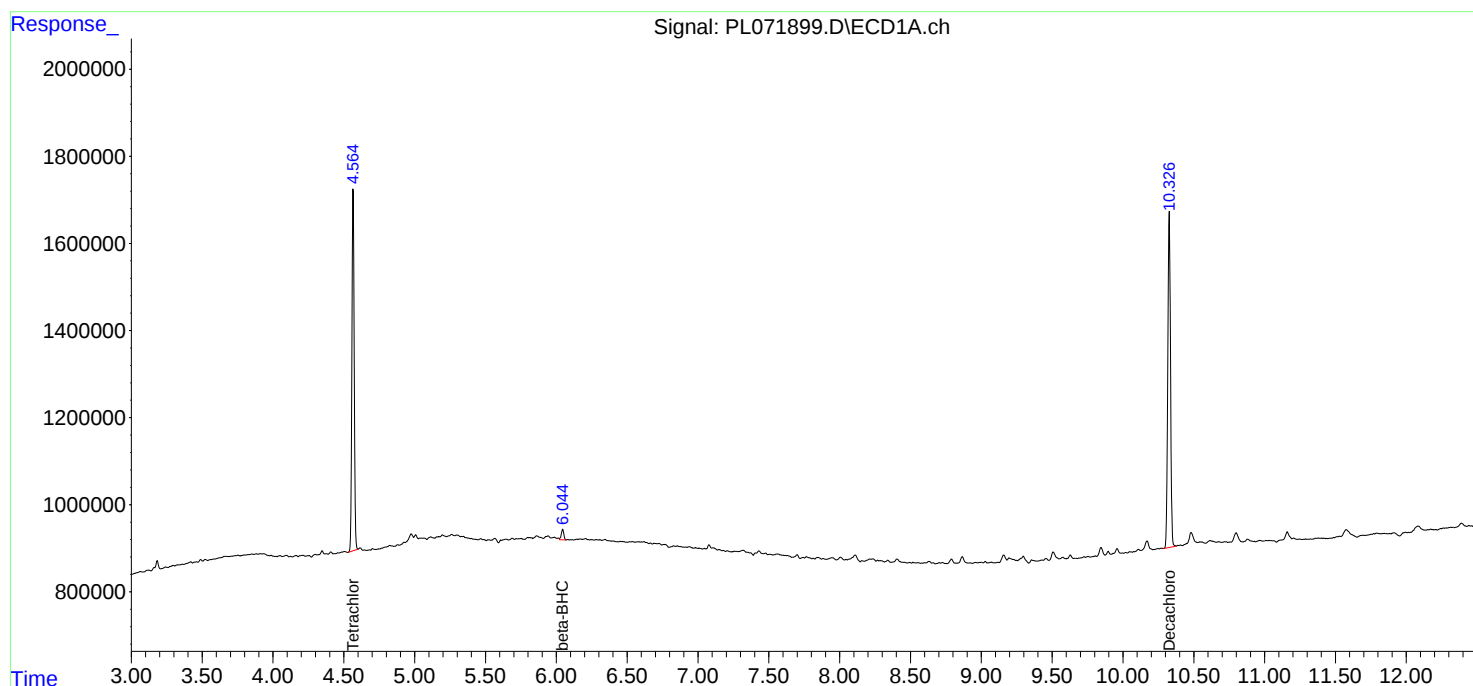


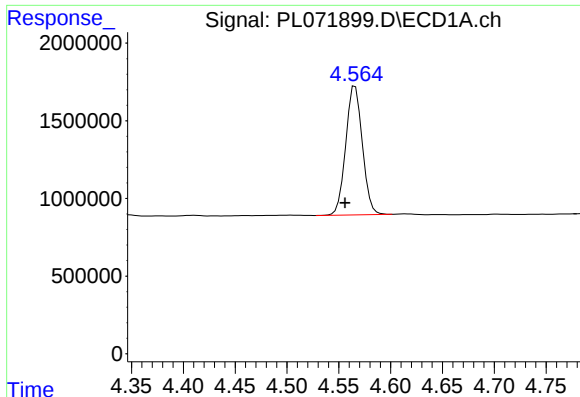

#1 Tetrachloro-m-xylene


R.T.: 4.566 min
Delta R.T.: 0.010 min
Response: 9248301
Conc: 20.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

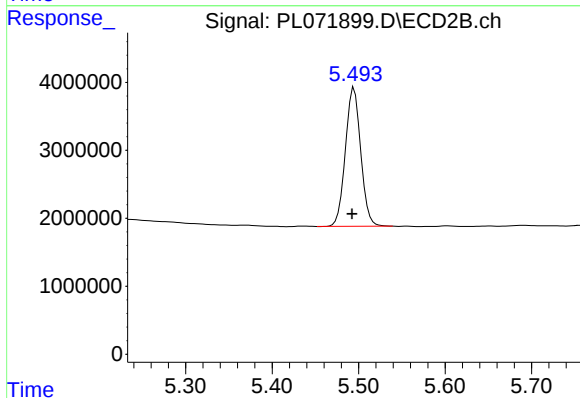


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: 0.002 min
Response: 25021194
Conc: 20.36 ng/ml

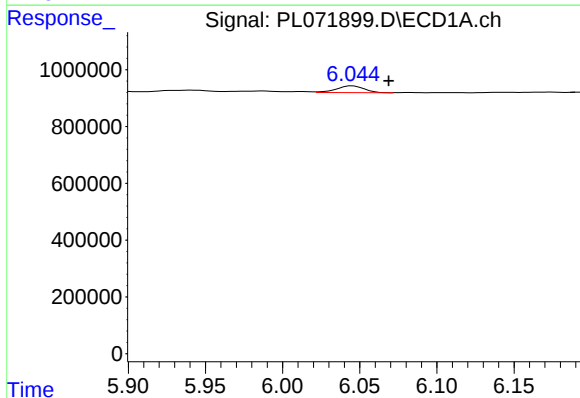


#6 beta-BHC

R.T.: 6.045 min
Delta R.T.: -0.023 min
Response: 300896
Conc: 1.11 ng/ml

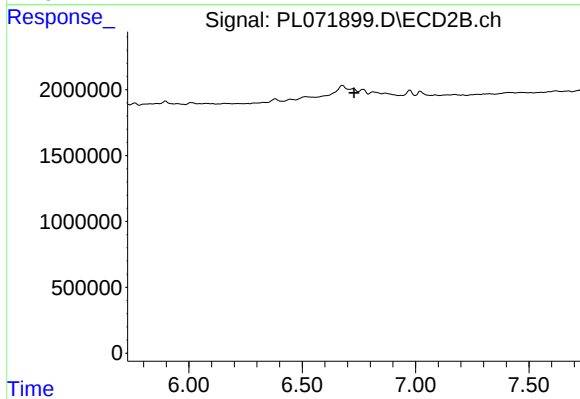

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.729 min
Response: 0
Conc: N.D.

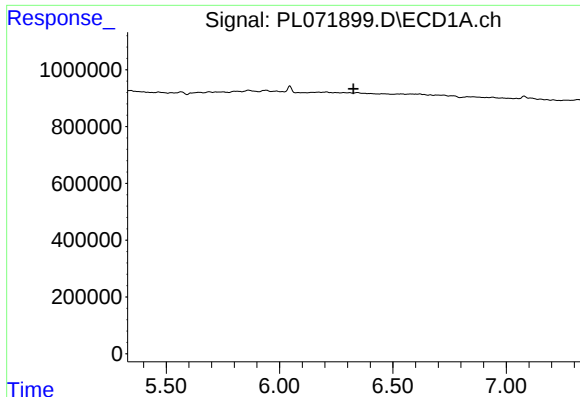

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

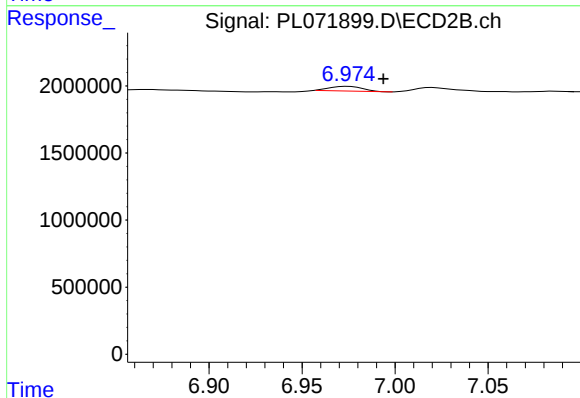


#7 delta-BHC

R.T.: 6.975 min
Delta R.T.: -0.019 min
Response: 429287
Conc: 0.28 ng/ml

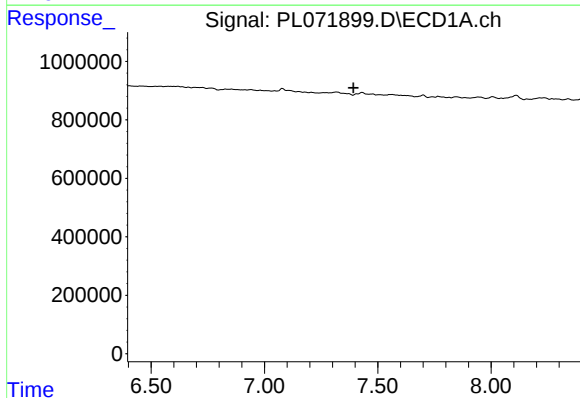


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

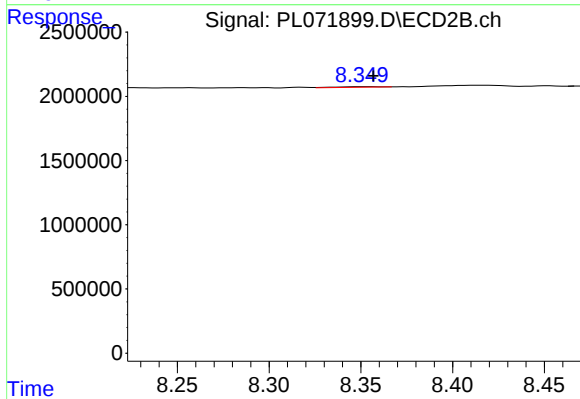

#9 Endosulfan I


R.T.: 8.351 min
Delta R.T.: -0.006 min
Response: 81710
Conc: 0.07 ng/ml

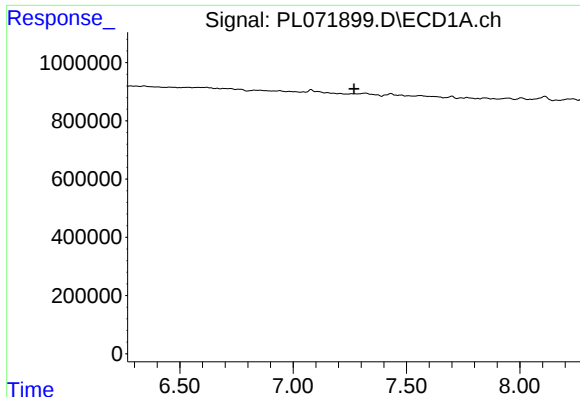

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

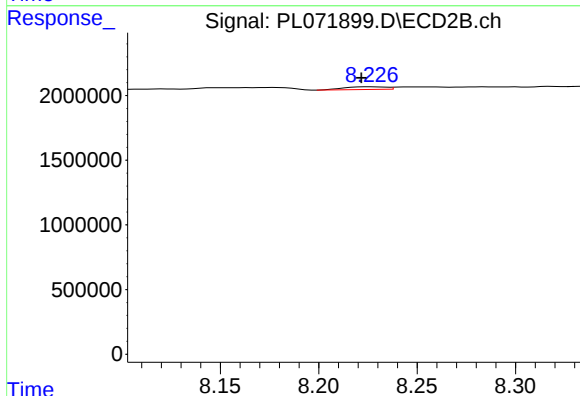


#10 gamma-Chlordane

R.T.: 8.226 min
Delta R.T.: 0.005 min
Response: 316513
Conc: 0.23 ng/ml

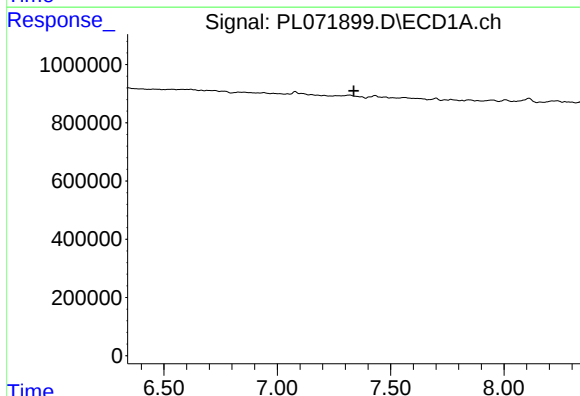


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

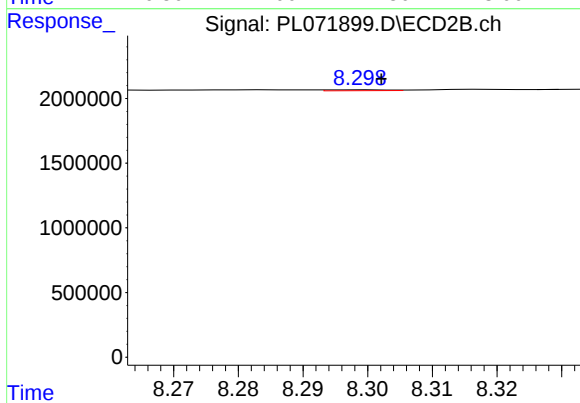

#11 alpha-Chlordane


R.T.: 8.299 min
Delta R.T.: -0.003 min
Response: 42019
Conc: 0.03 ng/ml

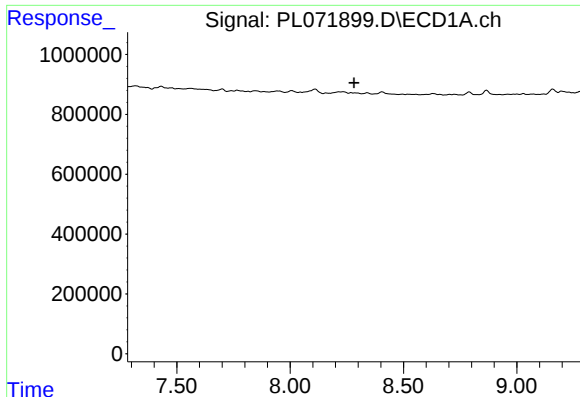

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

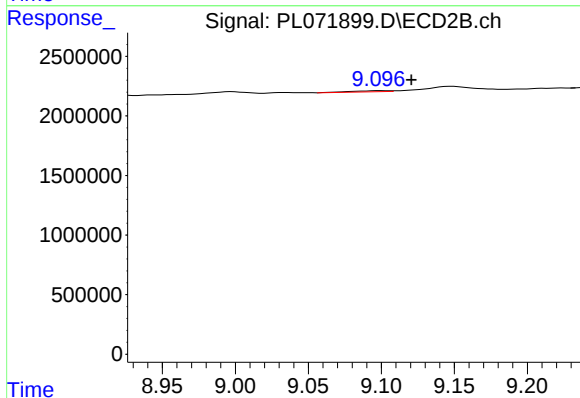


#15 Endosulfan II

R.T.: 9.098 min
Delta R.T.: -0.022 min
Response: 158604
Conc: 0.14 ng/ml

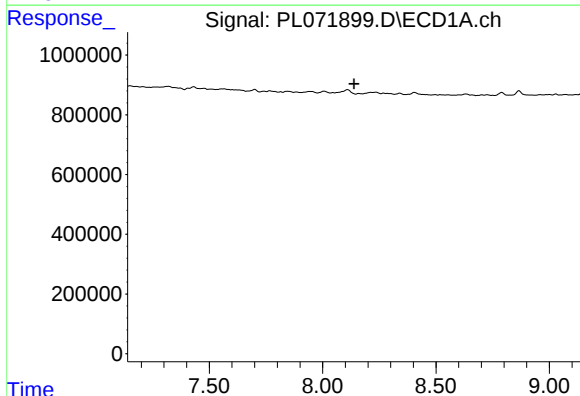


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

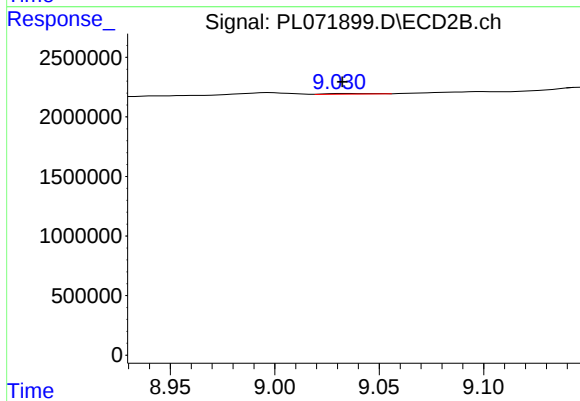

#16 4,4'-DDD


R.T.: 9.032 min
Delta R.T.: 0.000 min
Response: 68929
Conc: 0.07 ng/ml

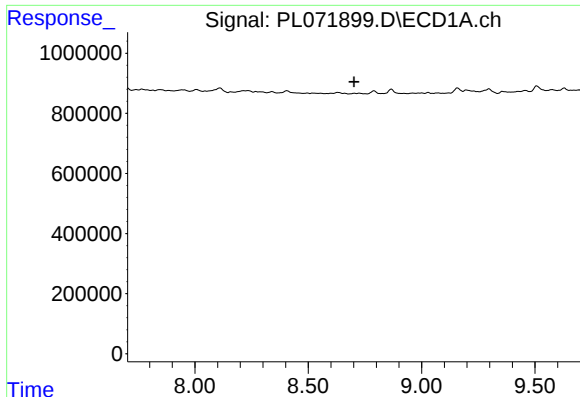

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

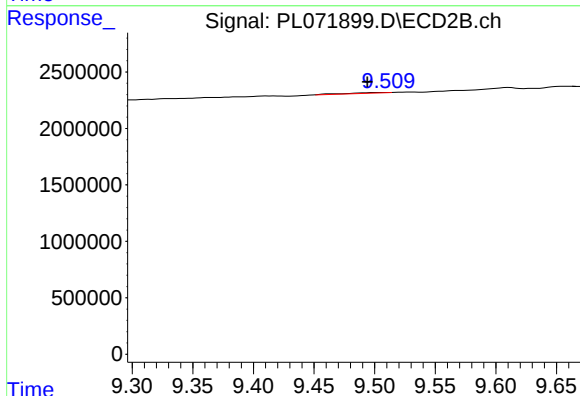


#19 Endosulfan Sulfate

R.T.: 9.510 min
Delta R.T.: 0.016 min
Response: 134889
Conc: 0.13 ng/ml

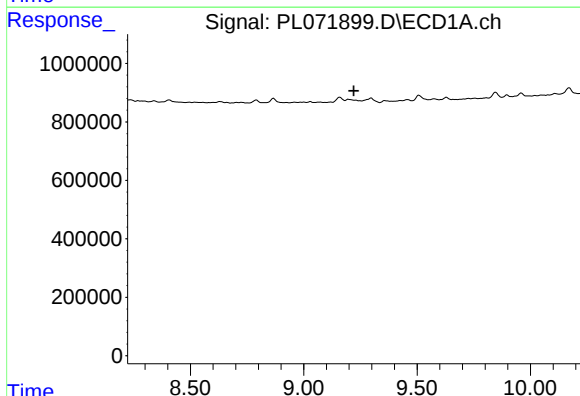


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

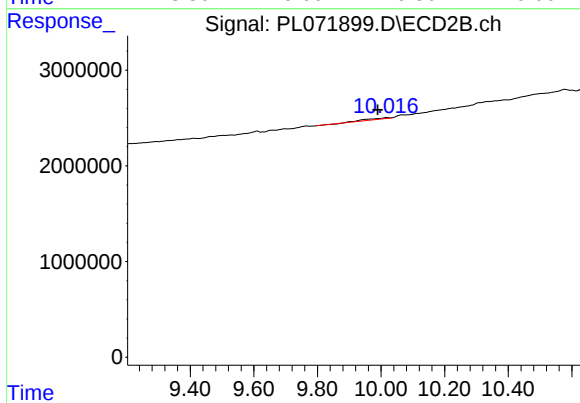

#21 Endrin ketone


R.T.: 10.019 min
Delta R.T.: 0.029 min
Response: 753523
Conc: 0.67 ng/ml

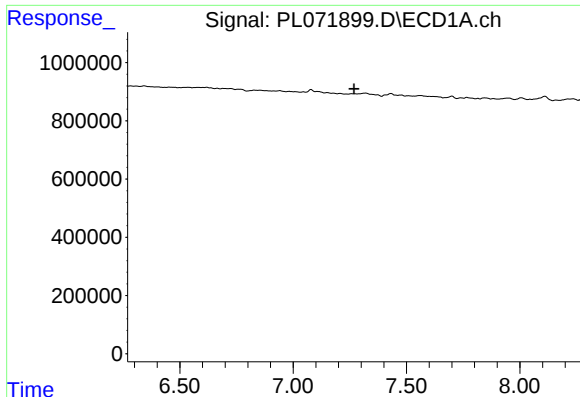

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

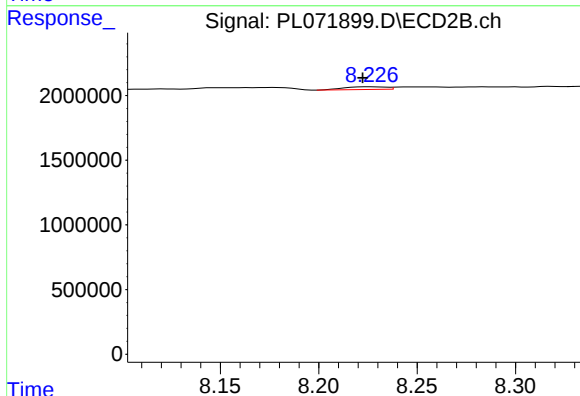


#25 Chlordane-3

R.T.: 8.226 min
Delta R.T.: 0.004 min
Response: 316513
Conc: 1.55 ng/ml

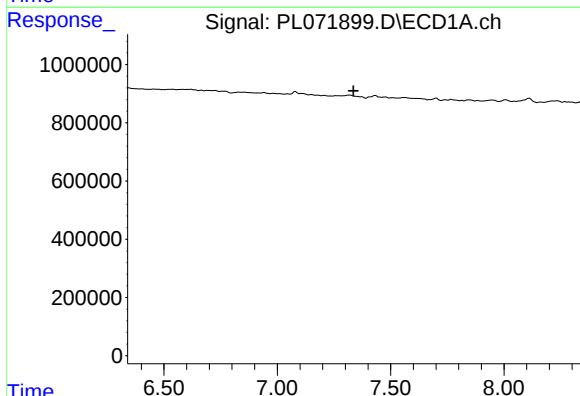


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

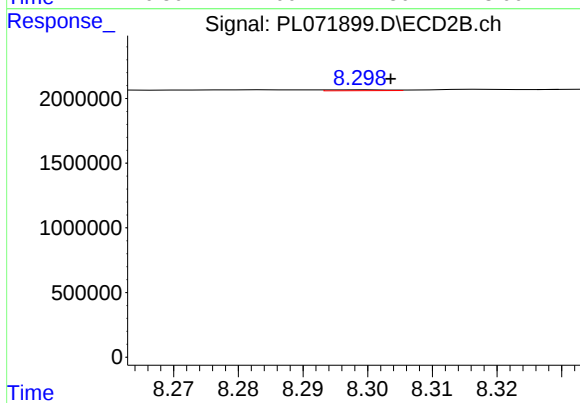

#26 Chlordane-4


R.T.: 8.299 min
Delta R.T.: -0.005 min
Response: 42019
Conc: 0.17 ng/ml

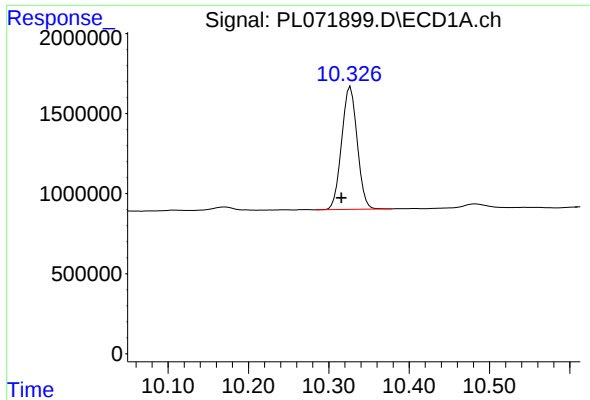

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.011 min
Response: 10326672
Conc: 14.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

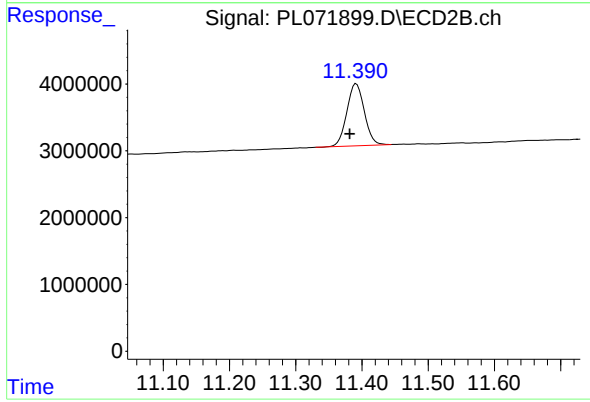

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.010 min
Response: 17076694
Conc: 14.41 ng/ml