

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
 Data File : PL071900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 13:39
 Operator : AR\AJ
 Sample : N1054-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:30:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	9540948	26293500	20.654	21.400
28)	SA Decachlor...	10.322	11.388	12688282	20948107	17.549	17.677
Target Compounds							
7)	B delta-BHC	0.000	6.972f	0	407105	N.D.	0.265 #
9)	A Endosulfan I	0.000	8.358	0	95432	N.D.	0.077 #
10)	B gamma-Chl...	0.000	8.234	0	307807	N.D.	0.225 #
15)	B Endosulfa...	0.000	9.100f	0	203584	N.D.	0.181 #
17)	MA 4,4'-DDT	0.000	9.363	0	36559	N.D.	0.039 #
18)	B Endrin al...	0.000	9.278f	0	22456	N.D.	0.026 #
19)	B Endosulfa...	0.000	9.498	0	100106	N.D.	0.096 #
21)	B Endrin ke...	0.000	9.972f	0	136933	N.D.	0.121 #
25)	Chlordane-3	0.000	8.234	0	307807	N.D.	1.508 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
Data File : PL071900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 13:39
Operator : AR\AJ
Sample : N1054-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:30:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

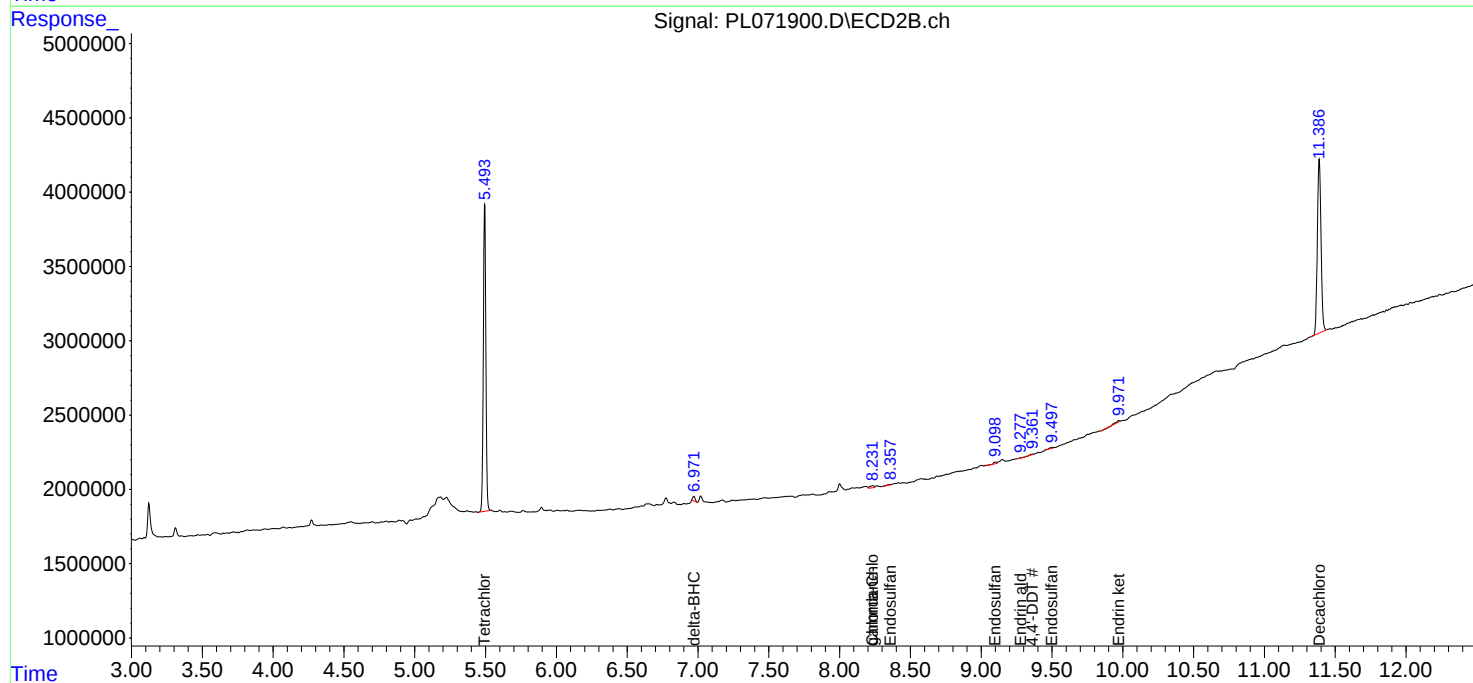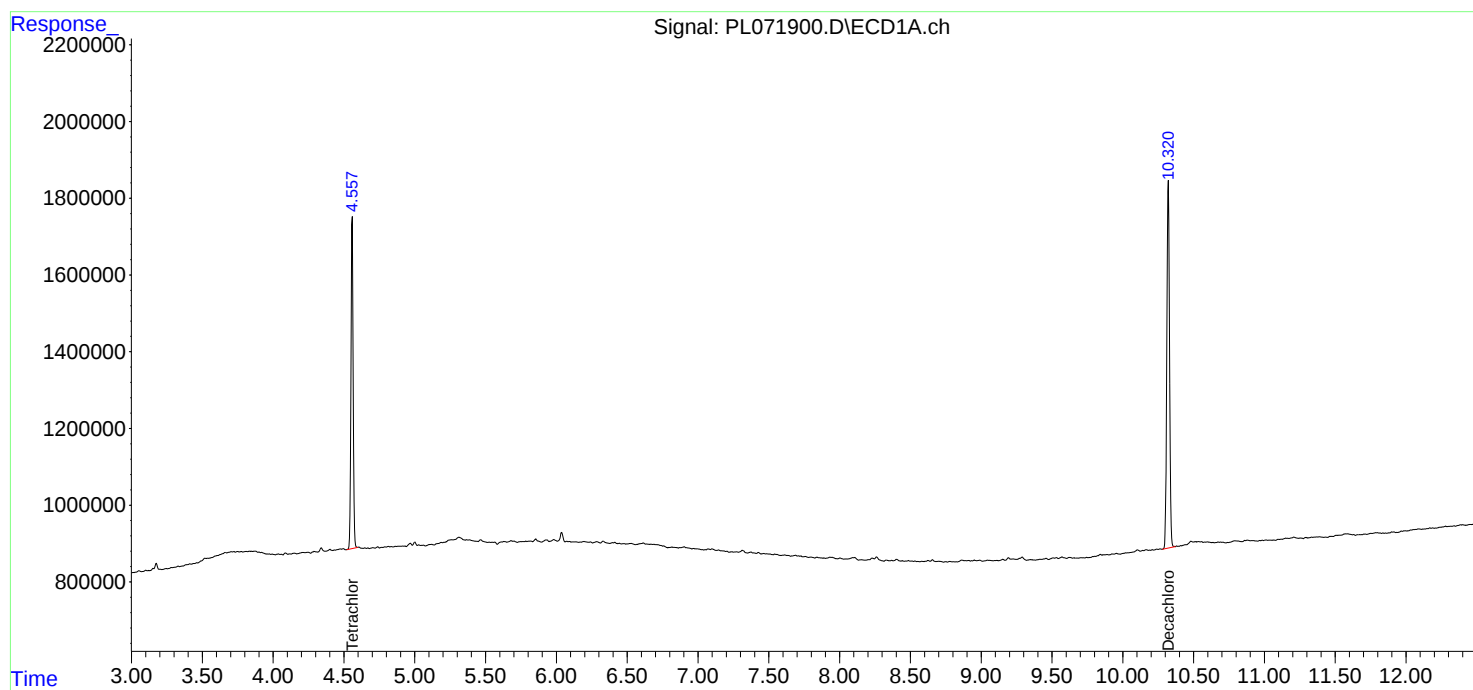


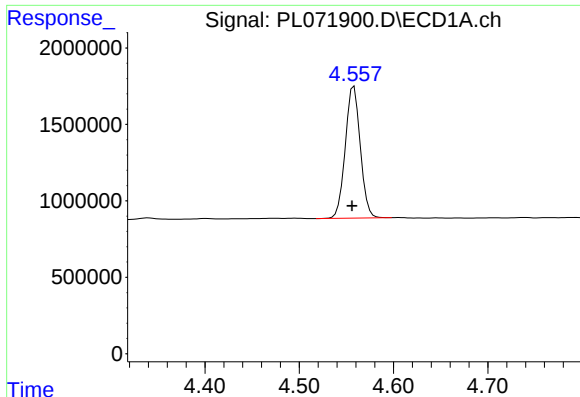

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9540948
Conc: 20.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

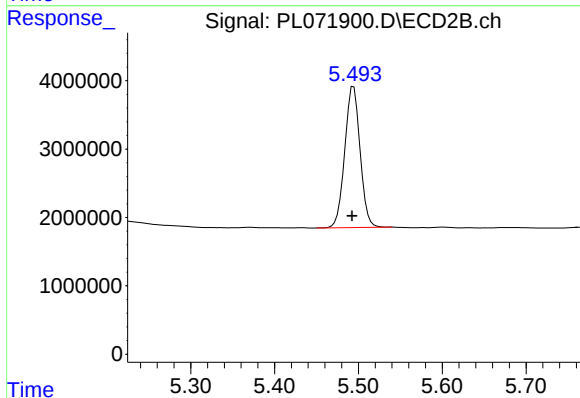


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 26293500
Conc: 21.40 ng/ml

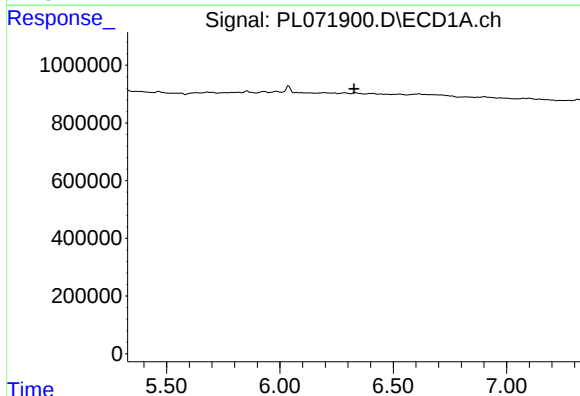


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

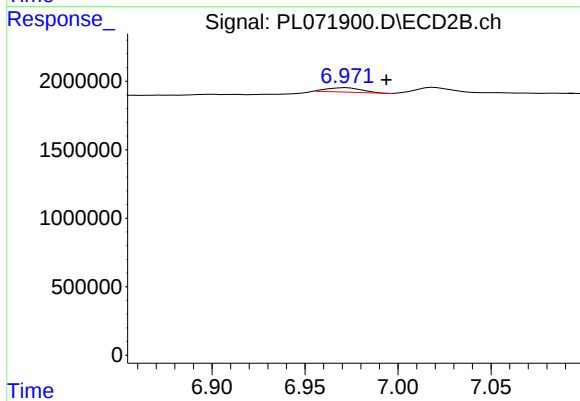

#7 delta-BHC


R.T.: 6.972 min
Delta R.T.: -0.022 min
Response: 407105
Conc: 0.27 ng/ml

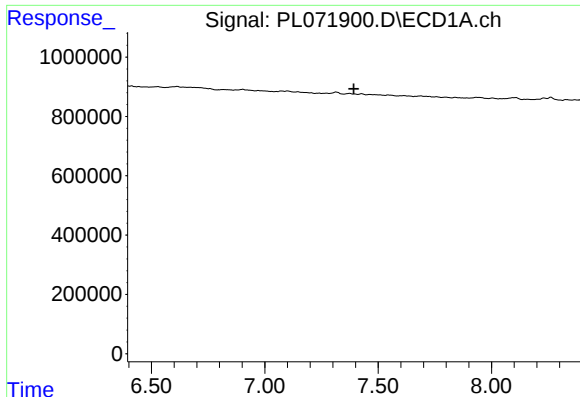

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

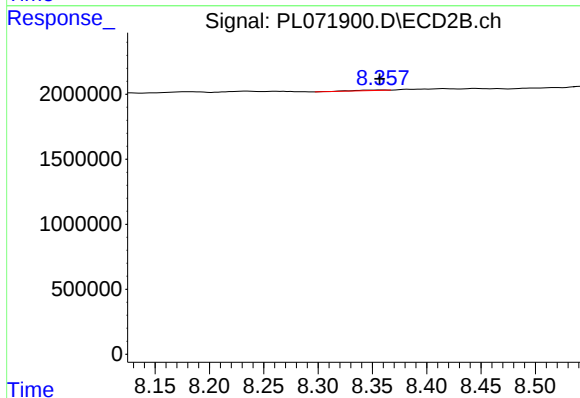


#9 Endosulfan I

R.T.: 8.358 min
Delta R.T.: 0.001 min
Response: 95432
Conc: 0.08 ng/ml

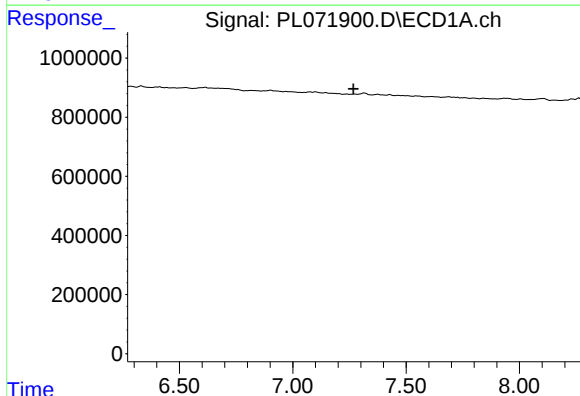


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

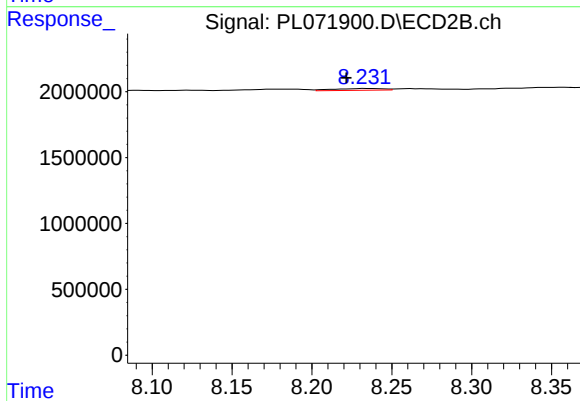

#10 gamma-Chlordane


R.T.: 8.234 min
Delta R.T.: 0.012 min
Response: 307807
Conc: 0.23 ng/ml

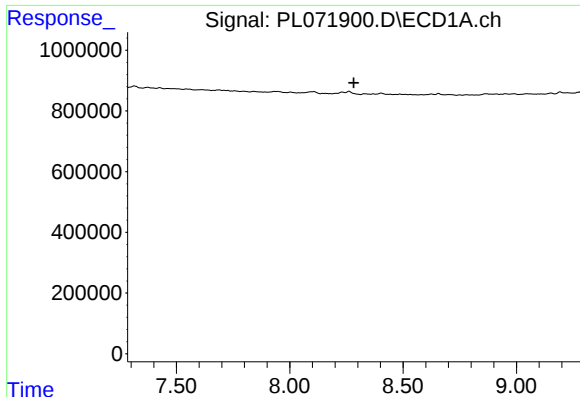

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

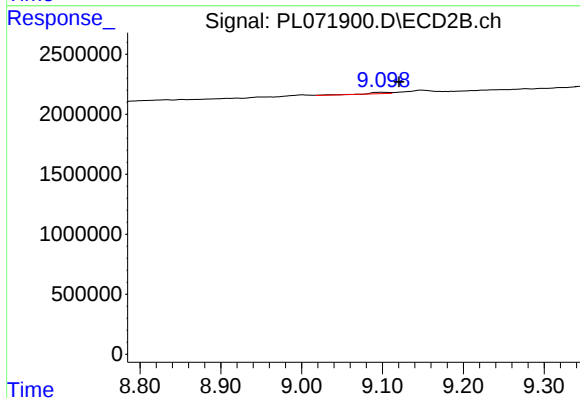


#15 Endosulfan II

R.T.: 9.100 min
Delta R.T.: -0.021 min
Response: 203584
Conc: 0.18 ng/ml

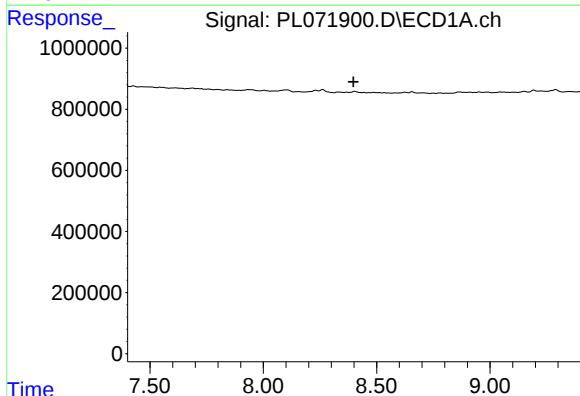


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

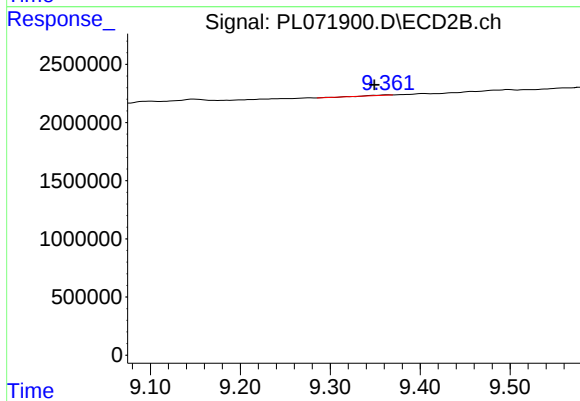

#17 4,4'-DDT


R.T.: 9.363 min
Delta R.T.: 0.014 min
Response: 36559
Conc: 0.04 ng/ml

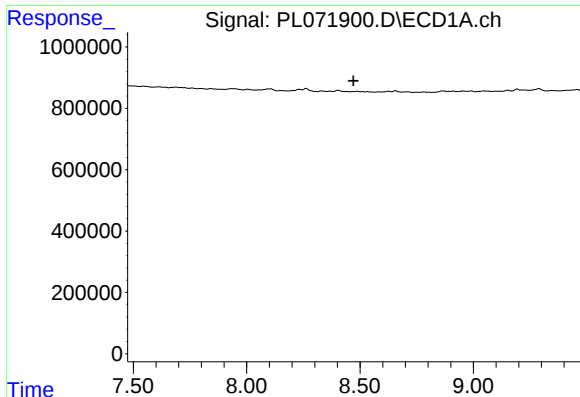

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

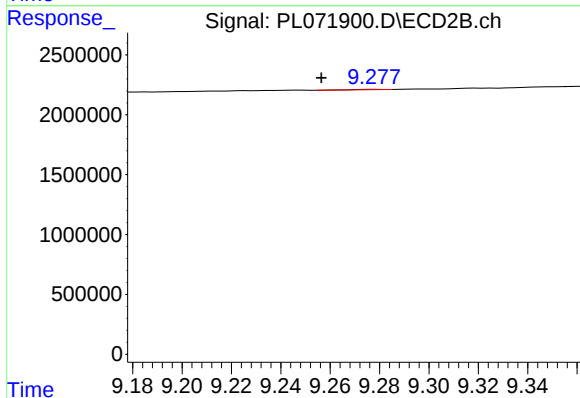


#18 Endrin aldehyde

R.T.: 9.278 min
Delta R.T.: 0.022 min
Response: 22456
Conc: 0.03 ng/ml

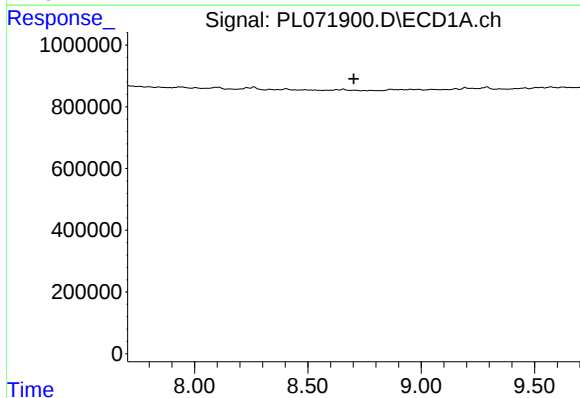


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.703 min
Response: 0
Conc: N.D.

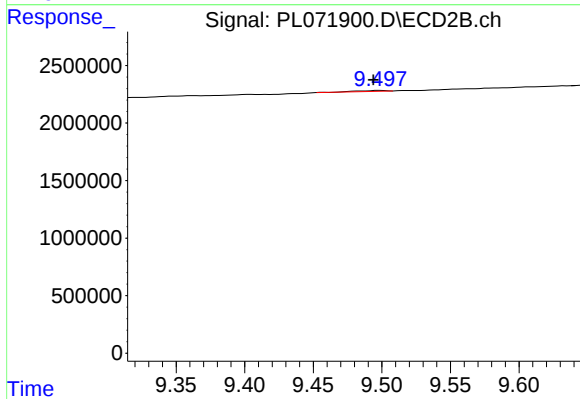

#19 Endosulfan Sulfate


R.T.: 9.498 min
Delta R.T.: 0.005 min
Response: 100106
Conc: 0.10 ng/ml

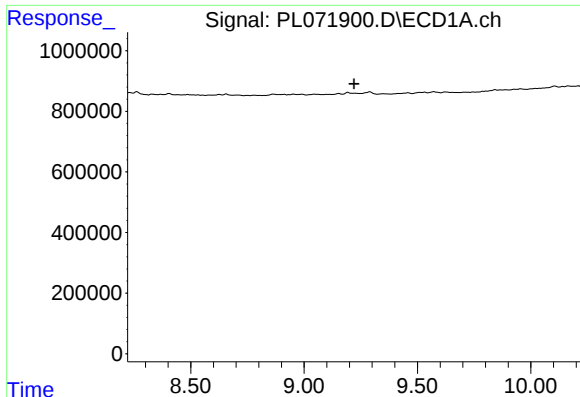

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

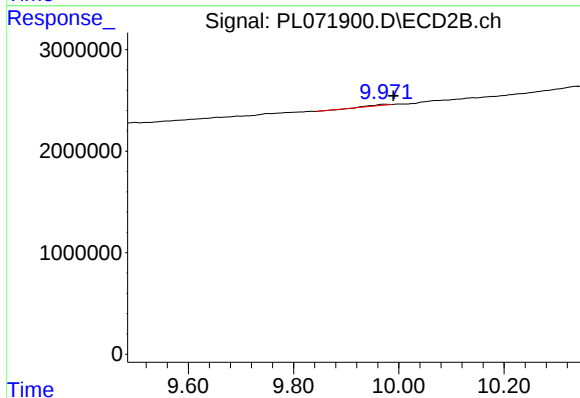


#21 Endrin ketone

R.T.: 9.972 min
Delta R.T.: -0.018 min
Response: 136933
Conc: 0.12 ng/ml

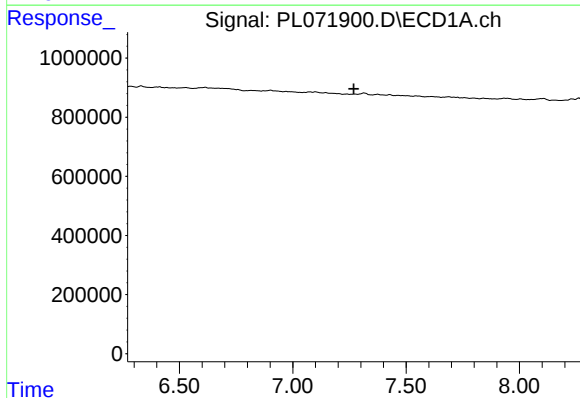


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

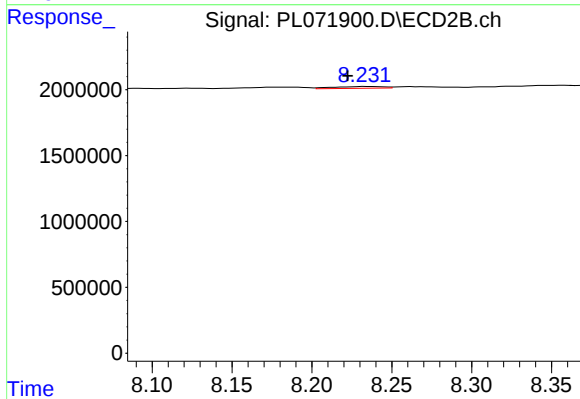

#25 Chlordane-3


R.T.: 8.234 min
Delta R.T.: 0.011 min
Response: 307807
Conc: 1.51 ng/ml

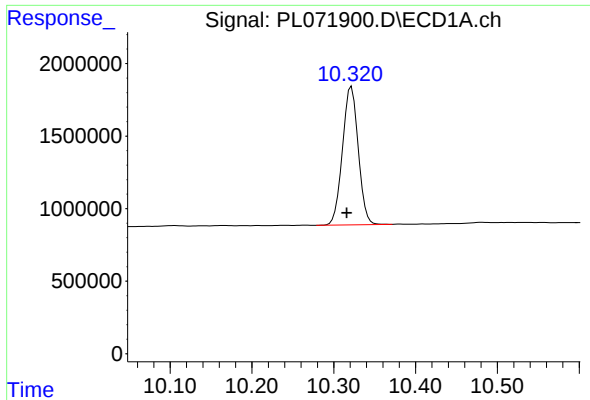

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.006 min
Response: 12688282
Conc: 17.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

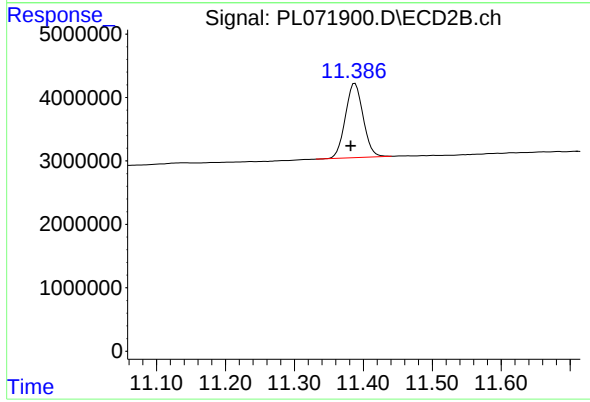

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.006 min
Response: 20948107
Conc: 17.68 ng/ml