

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
 Data File : PL071901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 13:56
 Operator : AR\AJ
 Sample : N1054-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:31:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	7780676	21423332	16.843	17.437
28)	SA Decachlor...	10.322	11.388	8085675	12863523	11.183	10.855
Target Compounds							
7)	B delta-BHC	0.000	6.972f	0	364993	N.D.	0.238 #
10)	B gamma-Chl...	0.000	8.239f	0	152923	N.D.	0.112 #
11)	B alpha-Chl...	0.000	8.308	0	6426	N.D.	0.005 #
15)	B Endosulfa...	0.000	9.150f	0	574959	N.D.	0.512 #
16)	A 4,4'-DDD	0.000	9.037	0	41558	N.D.	0.043 #
17)	MA 4,4'-DDT	0.000	9.360	0	19683	N.D.	0.021 #
20)	A Methoxychlor	0.000	9.847	0	21683	N.D.	0.044 #
21)	B Endrin ke...	0.000	9.976	0	391473	N.D.	0.347 #
22)	Mirex	0.000	10.439	0	152110	N.D.	0.177 #
25)	Chlordane-3	0.000	8.239f	0	152923	N.D.	0.749 #
26)	Chlordane-4	0.000	8.308	0	6426	N.D.	0.026 #
27)	Chlordane-5	0.000	9.189	0	11531	N.D.	0.288 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
Data File : PL071901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 13:56
Operator : AR\AJ
Sample : N1054-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:31:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

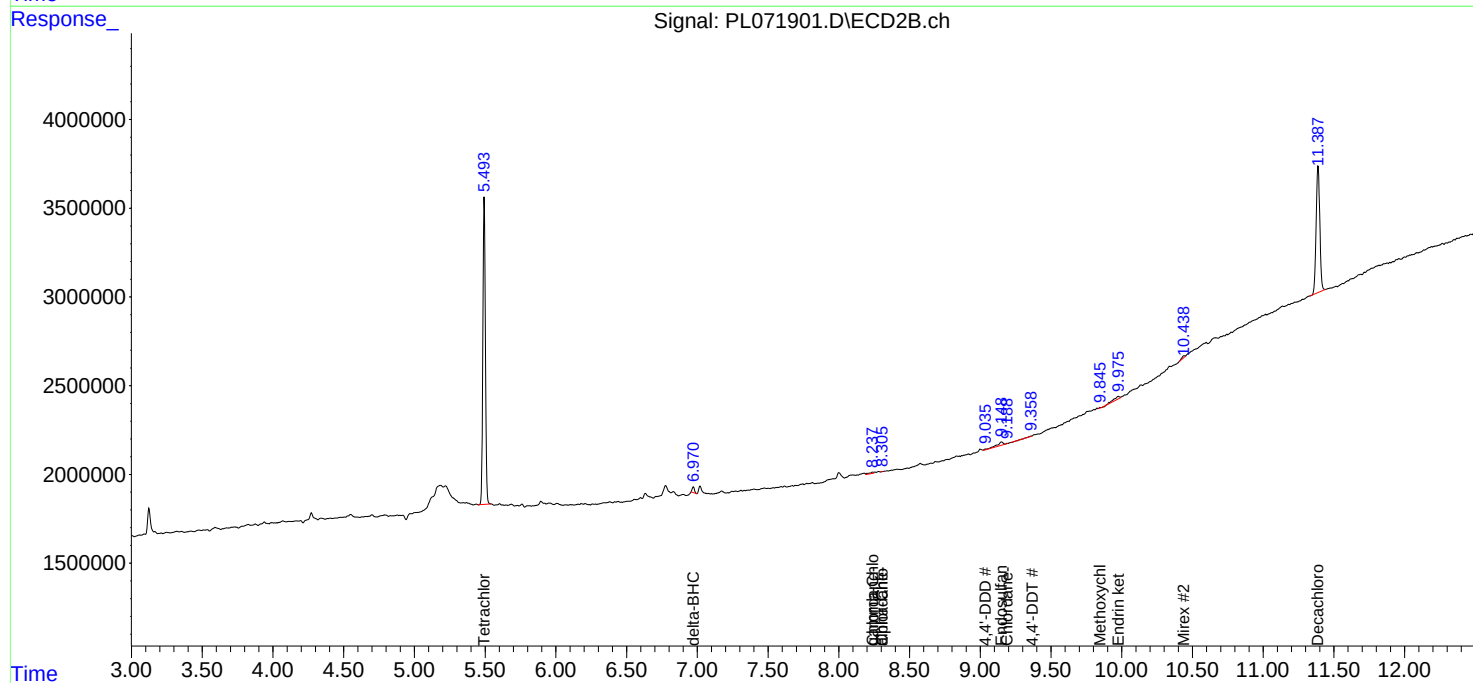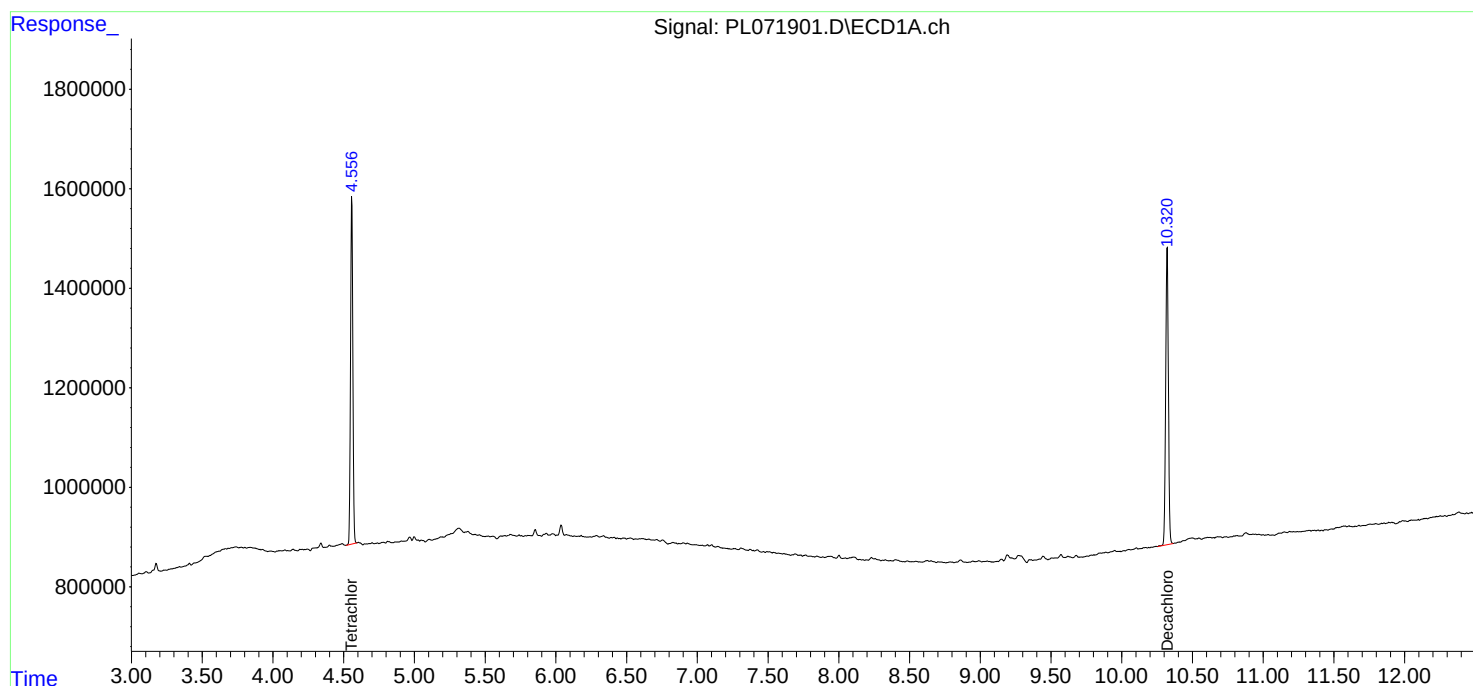


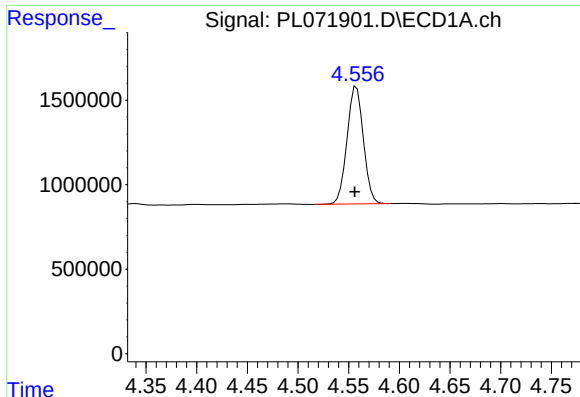

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 7780676
Conc: 16.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

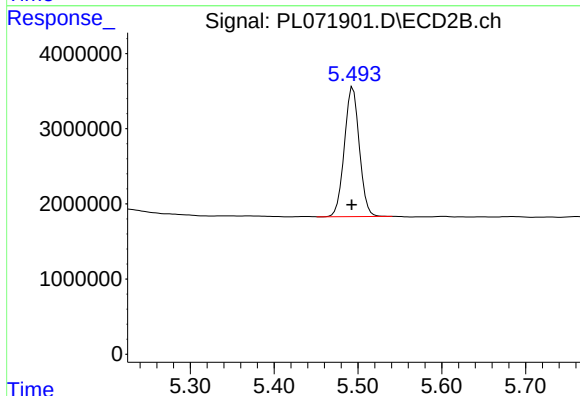


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 21423332
Conc: 17.44 ng/ml

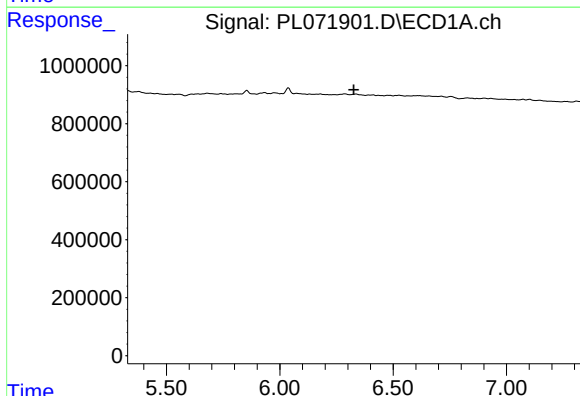


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

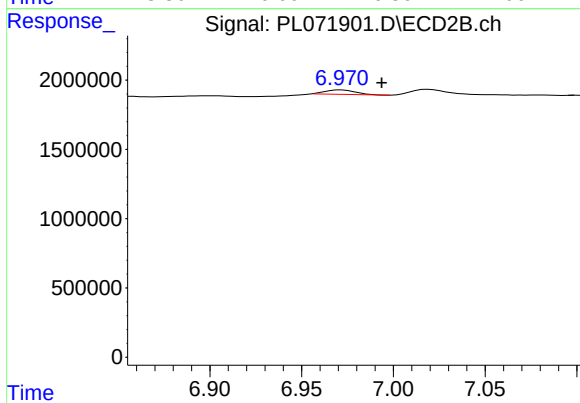

#7 delta-BHC


R.T.: 6.972 min
Delta R.T.: -0.022 min
Response: 364993
Conc: 0.24 ng/ml

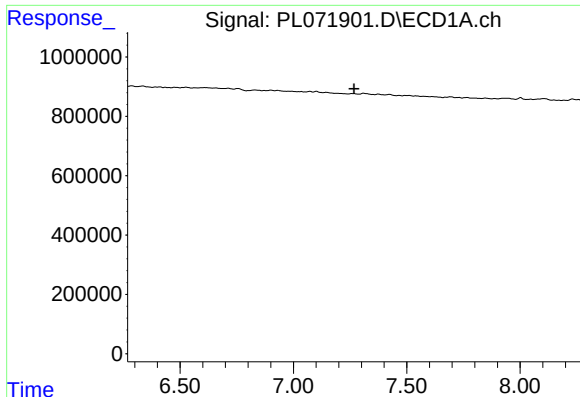

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

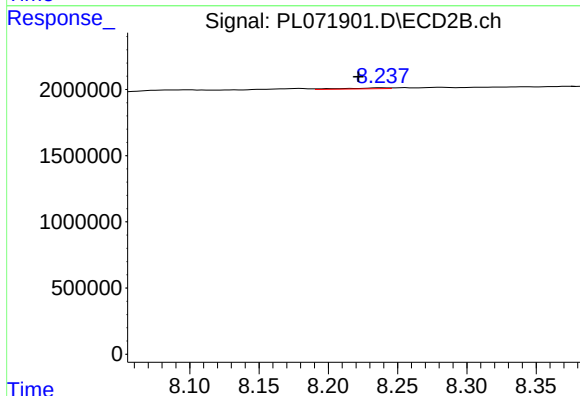


#10 gamma-Chlordane

R.T.: 8.239 min
Delta R.T.: 0.017 min
Response: 152923
Conc: 0.11 ng/ml

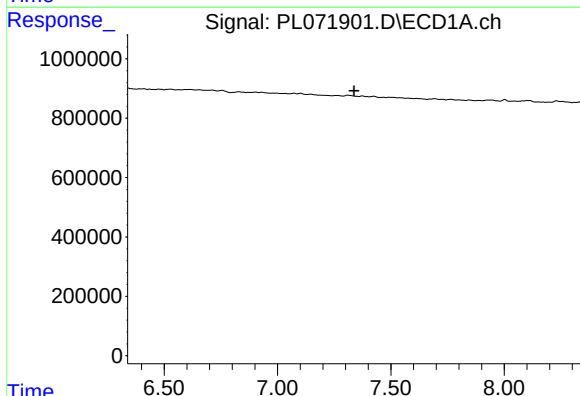


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

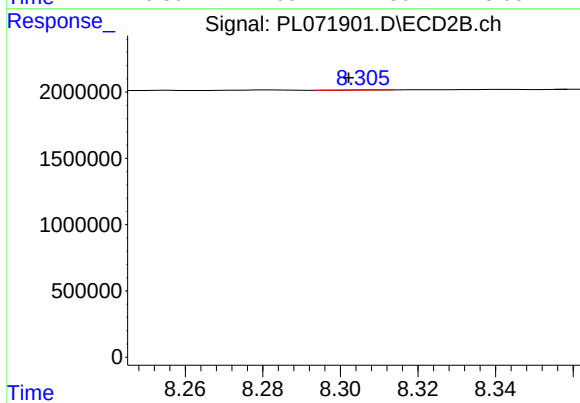

#11 alpha-Chlordane


R.T.: 8.308 min
Delta R.T.: 0.006 min
Response: 6426
Conc: 0.00 ng/ml

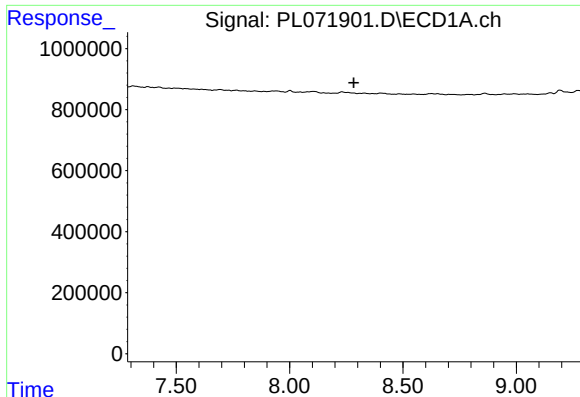

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

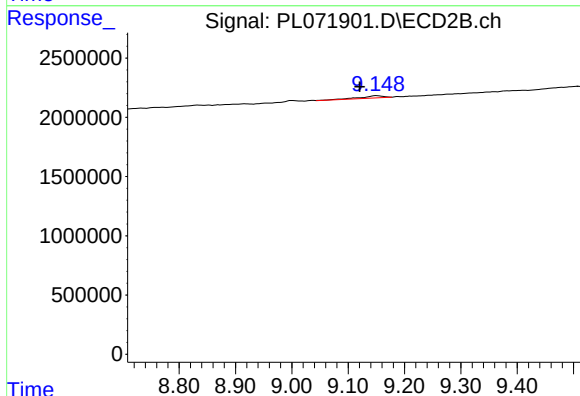


#15 Endosulfan II

R.T.: 9.150 min
Delta R.T.: 0.029 min
Response: 574959
Conc: 0.51 ng/ml

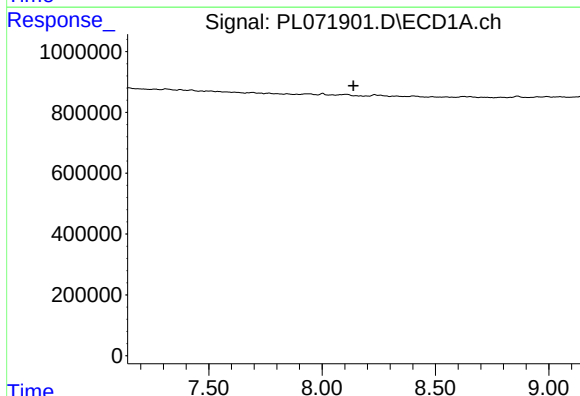


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

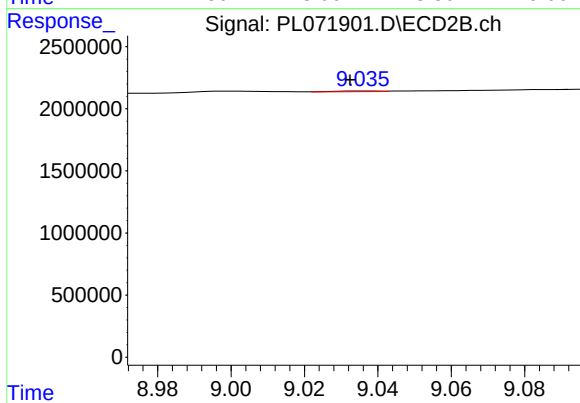

#16 4,4'-DDD


R.T.: 9.037 min
Delta R.T.: 0.004 min
Response: 41558
Conc: 0.04 ng/ml

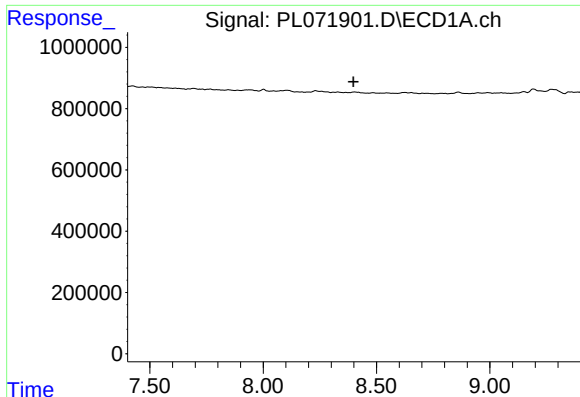

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

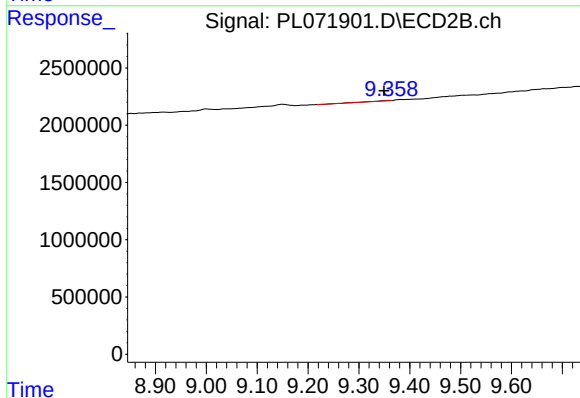


#17 4,4'-DDT

R.T.: 9.360 min
Delta R.T.: 0.010 min
Response: 19683
Conc: 0.02 ng/ml

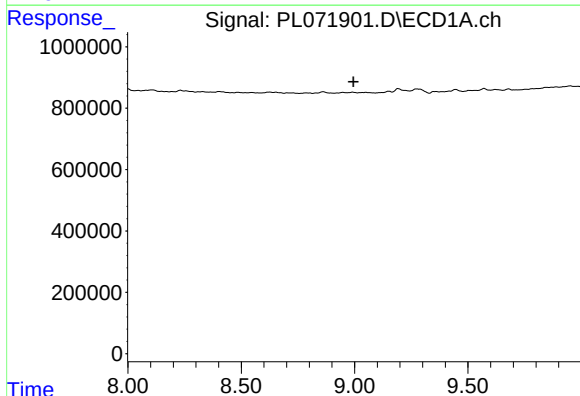


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 8.995 min
Response: 0
Conc: N.D.

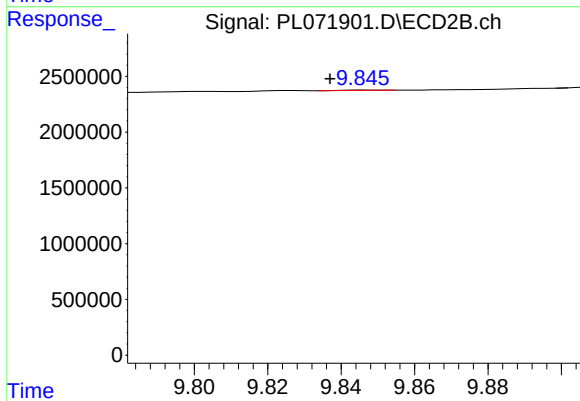

#20 Methoxychlor


R.T.: 9.847 min
Delta R.T.: 0.010 min
Response: 21683
Conc: 0.04 ng/ml

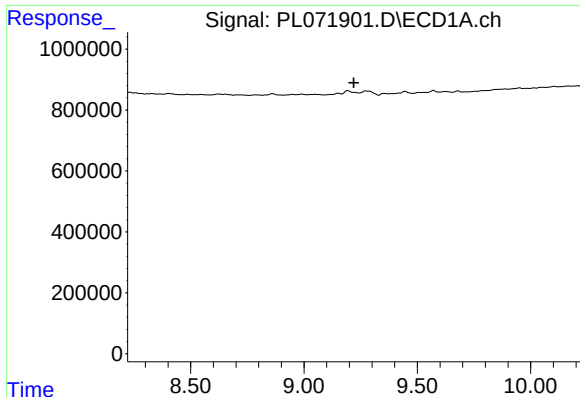

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

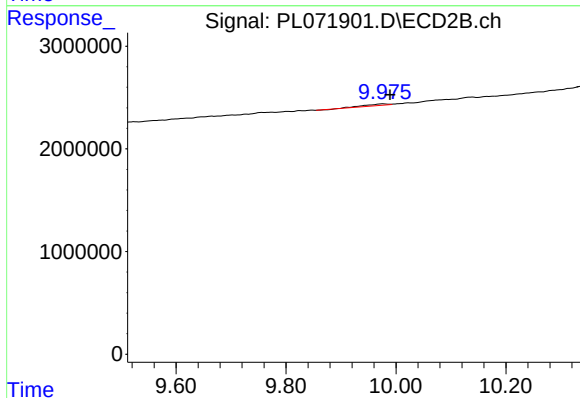


#21 Endrin ketone

R.T.: 9.976 min
Delta R.T.: -0.013 min
Response: 391473
Conc: 0.35 ng/ml

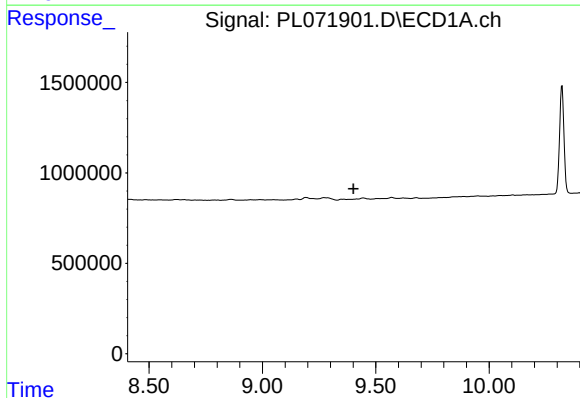


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.402 min
Response: 0
Conc: N.D.

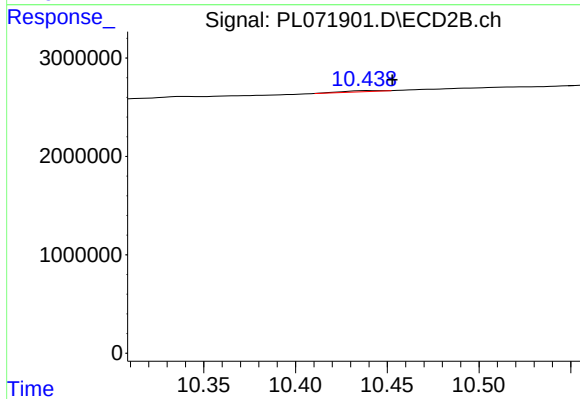

#22 Mirex


R.T.: 10.439 min
Delta R.T.: -0.013 min
Response: 152110
Conc: 0.18 ng/ml

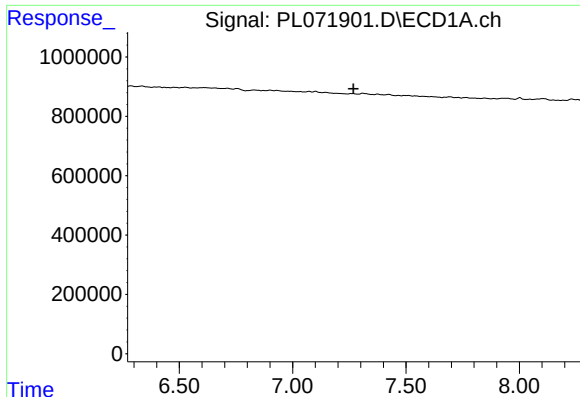

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

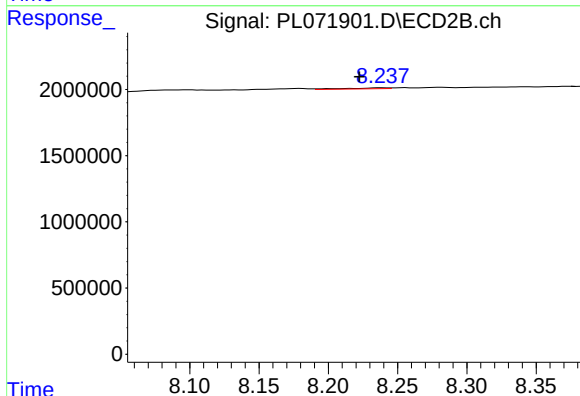


#25 Chlordane-3

R.T.: 8.239 min
Delta R.T.: 0.016 min
Response: 152923
Conc: 0.75 ng/ml

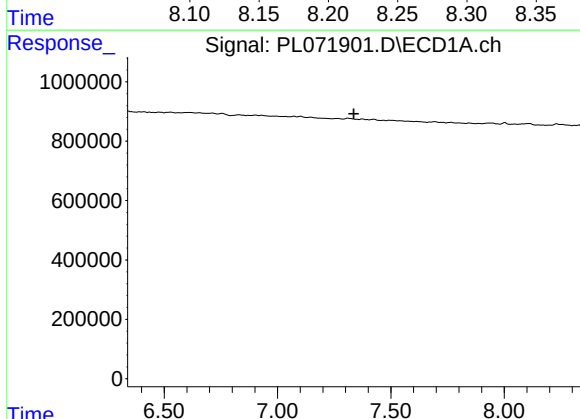


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

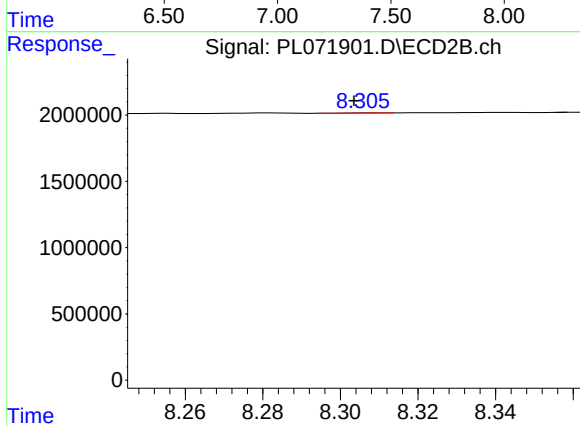

#26 Chlordane-4


R.T.: 8.308 min
Delta R.T.: 0.005 min
Response: 6426
Conc: 0.03 ng/ml

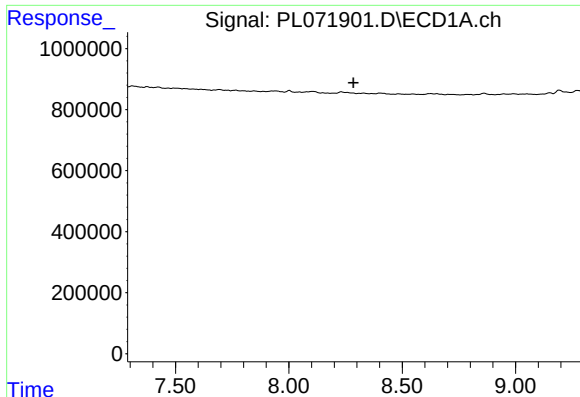

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

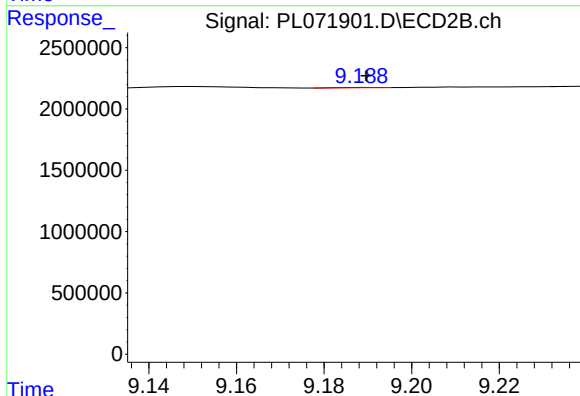


#27 Chlordane-5

R.T.: 9.189 min
Delta R.T.: 0.000 min
Response: 11531
Conc: 0.29 ng/ml

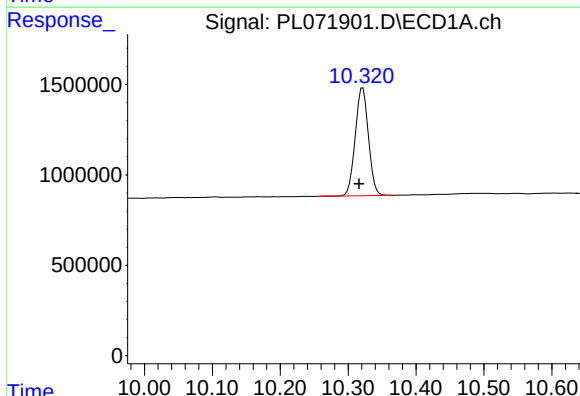

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.006 min
Response: 8085675
Conc: 11.18 ng/ml

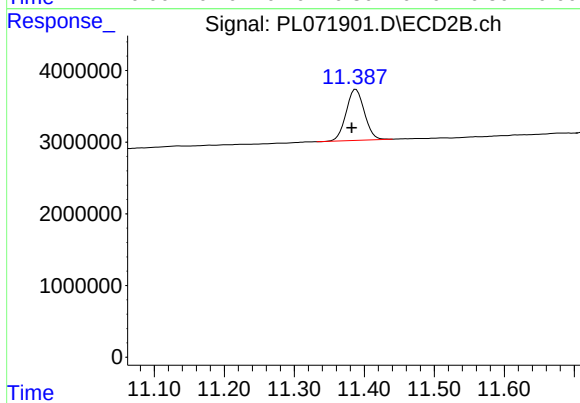

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.006 min
Response: 12863523
Conc: 10.86 ng/ml