

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
 Data File : PL071906.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 15:17
 Operator : AR\AJ
 Sample : N1054-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:32:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	9773107	26500418	21.156	21.569
28)	SA Decachlor...	10.321	11.388	12148427	20060253	16.802	16.928
Target Compounds							
7)	B delta-BHC	0.000	6.973f	0	339351	N.D.	0.221 #
8)	B Heptachlo...	0.000	7.965	0	241360	N.D.	0.173 #
9)	A Endosulfan I	0.000	8.345	0	75662	N.D.	0.061 #
11)	B alpha-Chl...	0.000	8.303	0	49047	N.D.	0.037 #
15)	B Endosulfa...	0.000	9.150f	0	460384	N.D.	0.410 #
16)	A 4,4'-DDD	0.000	9.033	0	130740	N.D.	0.136 #
17)	MA 4,4'-DDT	0.000	9.363	0	115024	N.D.	0.122 #
18)	B Endrin al...	0.000	9.273f	0	119800	N.D.	0.141 #
21)	B Endrin ke...	0.000	9.975	0	31161	N.D.	0.028 #
22)	Mirex	0.000	10.443	0	140243	N.D.	0.163 #
26)	Chlordane-4	0.000	8.303	0	49047	N.D.	0.201 #
27)	Chlordane-5	0.000	9.178	0	40925	N.D.	1.022 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
Data File : PL071906.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 15:17
Operator : AR\AJ
Sample : N1054-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:32:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

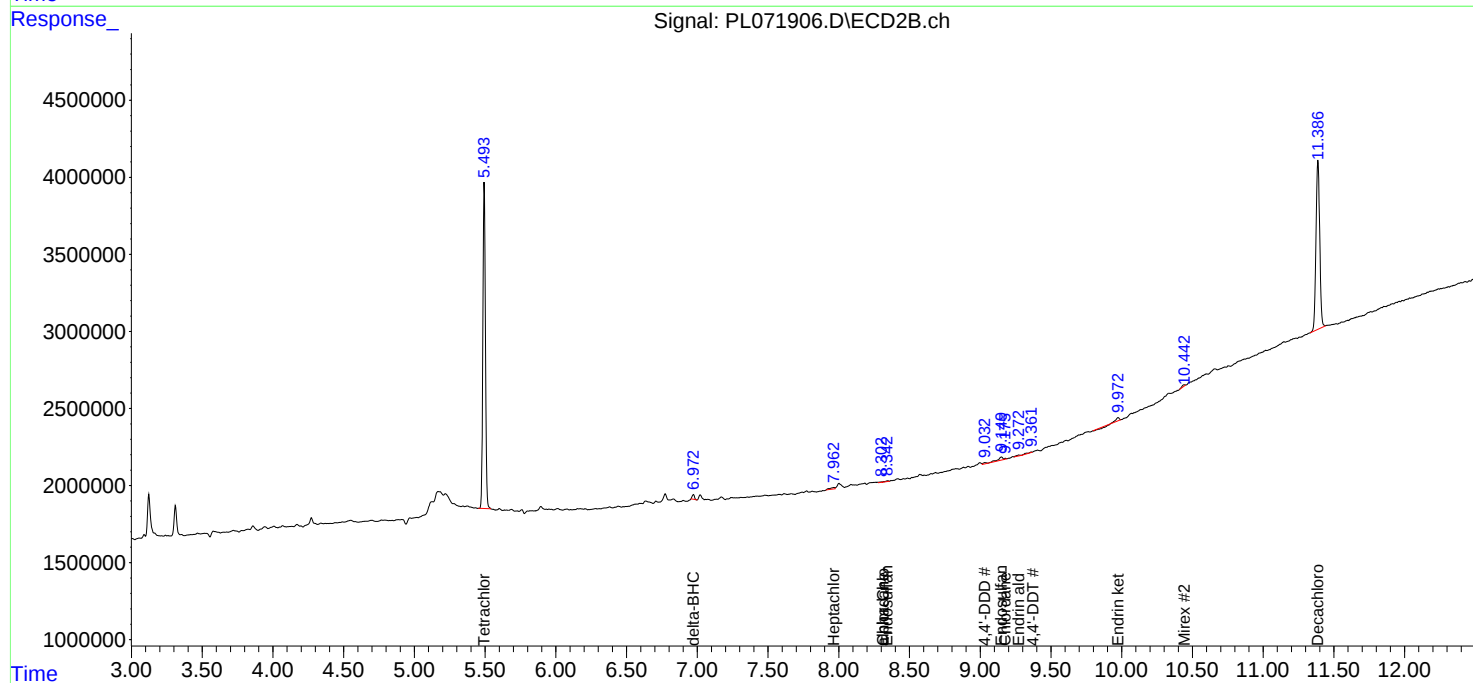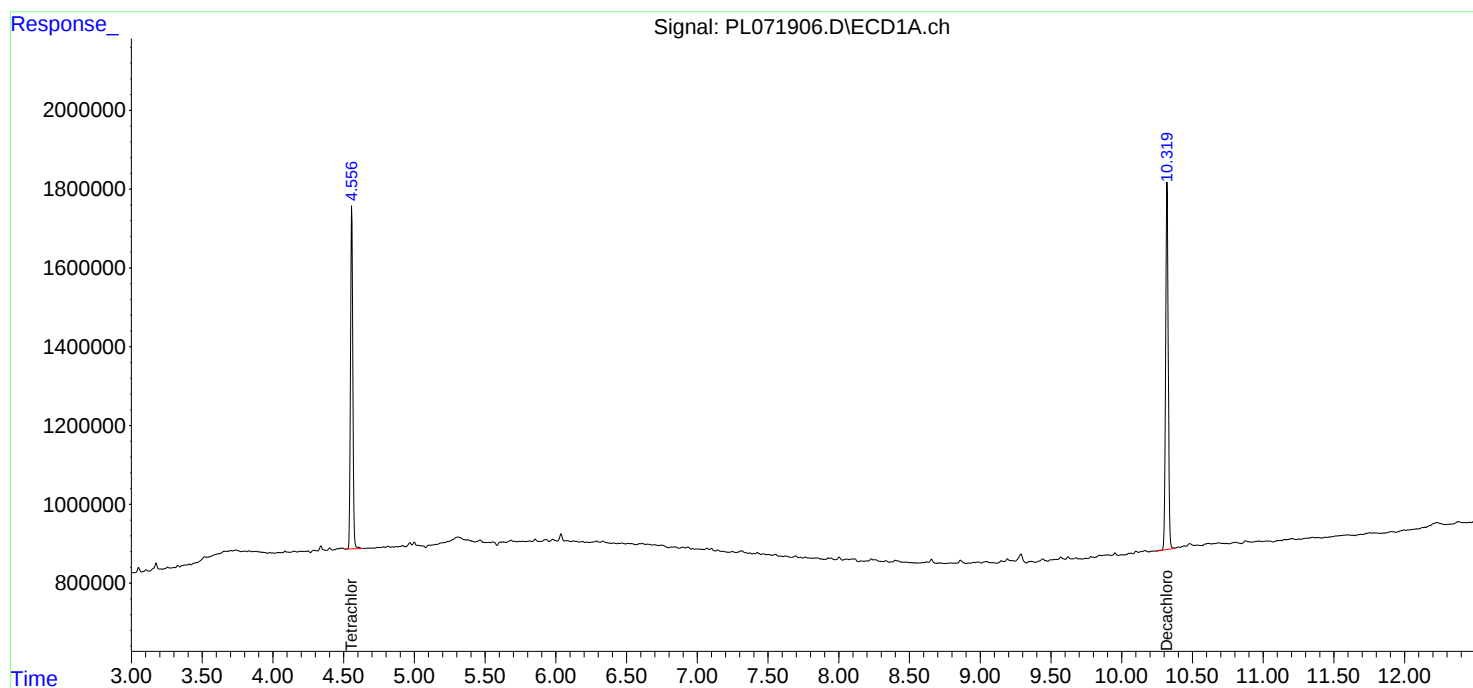


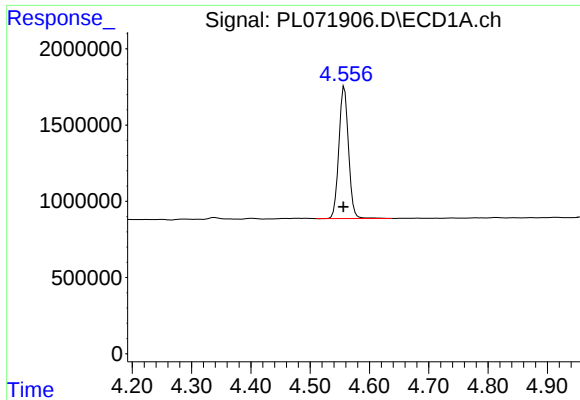

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9773107
Conc: 21.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

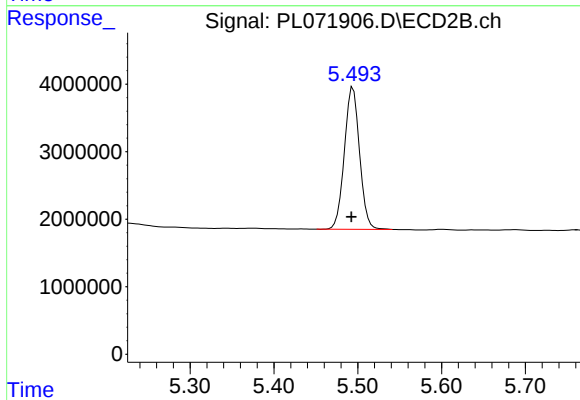


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 26500418
Conc: 21.57 ng/ml

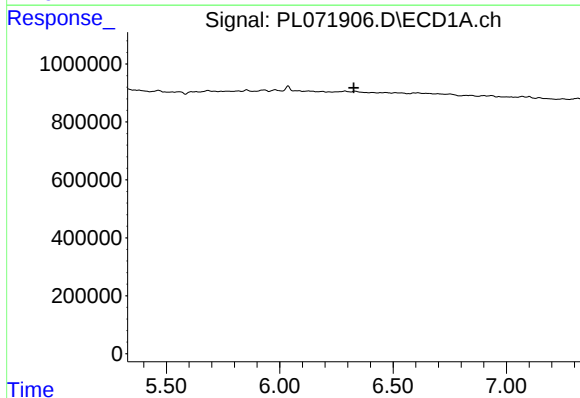


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

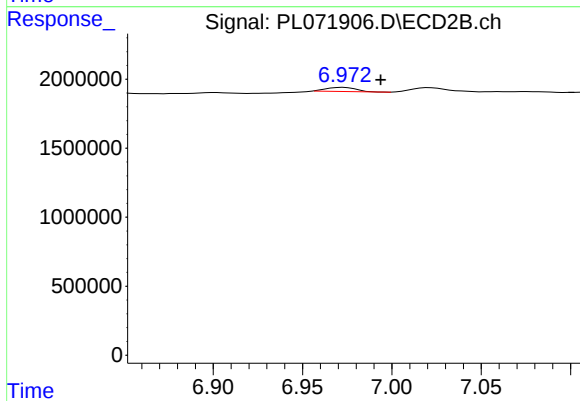

#7 delta-BHC

R.T.: 6.973 min
Delta R.T.: -0.021 min
Response: 339351
Conc: 0.22 ng/ml

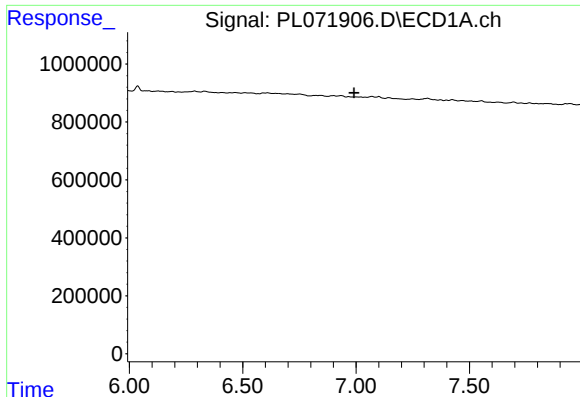

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#8 Heptachlor epoxide


R.T.: 7.965 min
Delta R.T.: 0.012 min
Response: 241360
Conc: 0.17 ng/ml

#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

#9 Endosulfan I


R.T.: 8.345 min
Delta R.T.: -0.012 min
Response: 75662
Conc: 0.06 ng/ml

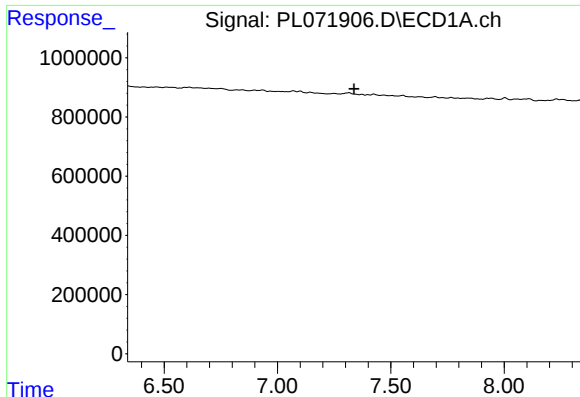

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

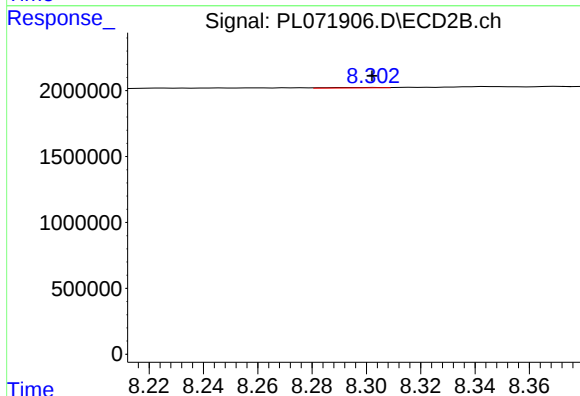


#11 alpha-Chlordane

R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 49047
Conc: 0.04 ng/ml

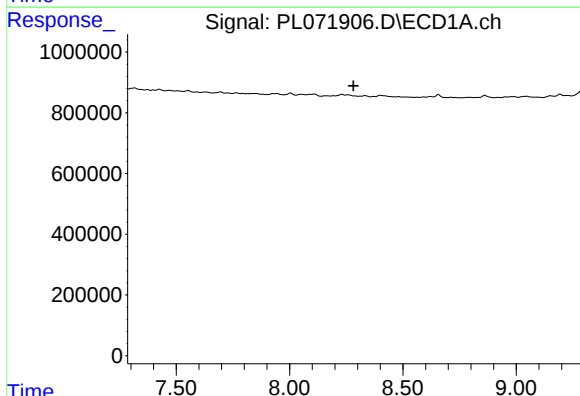


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

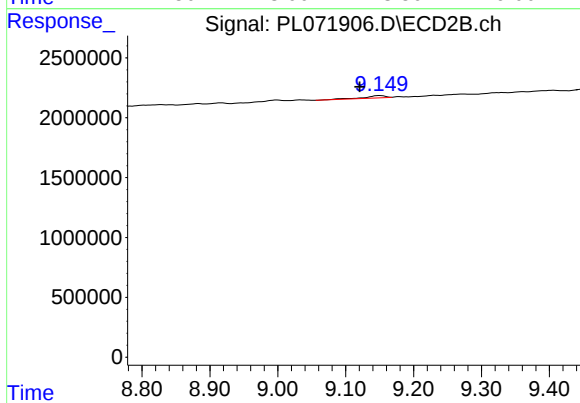

#15 Endosulfan II


R.T.: 9.150 min
Delta R.T.: 0.030 min
Response: 460384
Conc: 0.41 ng/ml

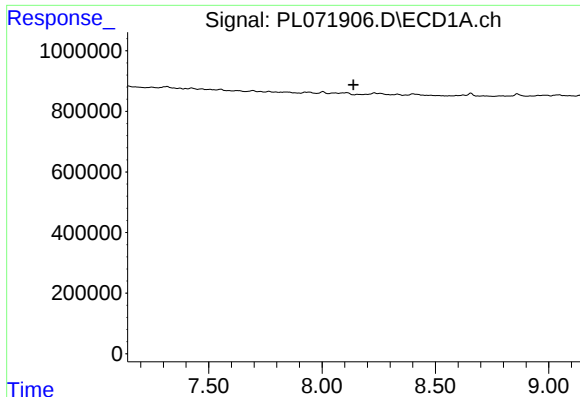

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

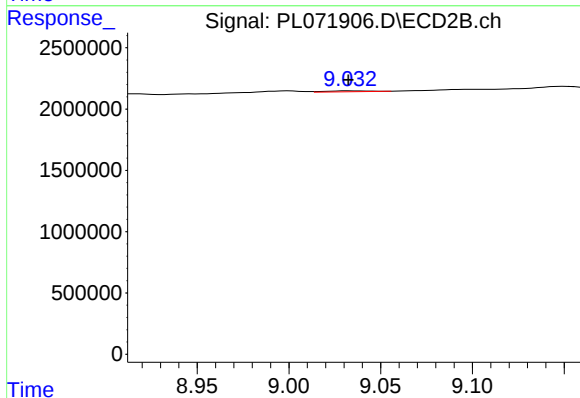


#16 4,4'-DDD

R.T.: 9.033 min
Delta R.T.: 0.000 min
Response: 130740
Conc: 0.14 ng/ml

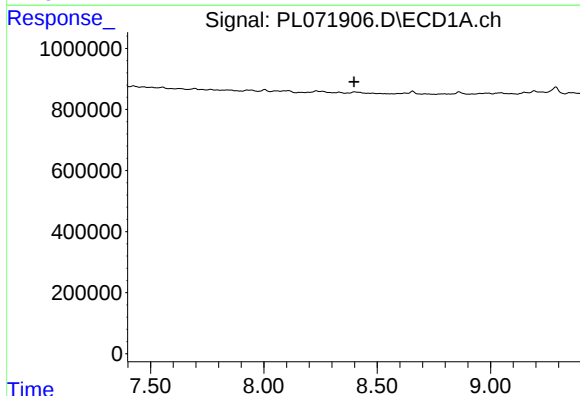


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

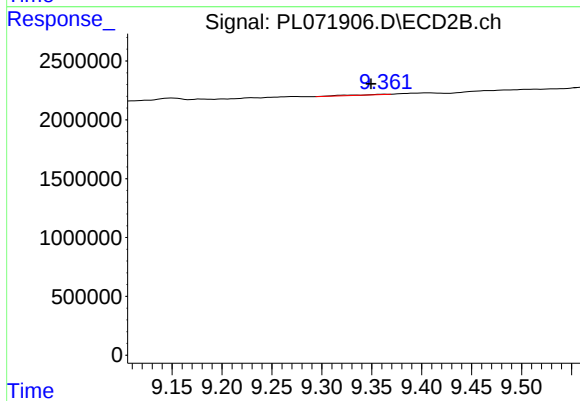

#17 4,4'-DDT


R.T.: 9.363 min
Delta R.T.: 0.014 min
Response: 115024
Conc: 0.12 ng/ml

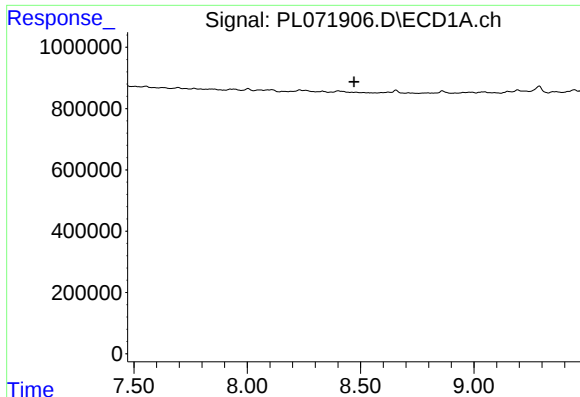

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

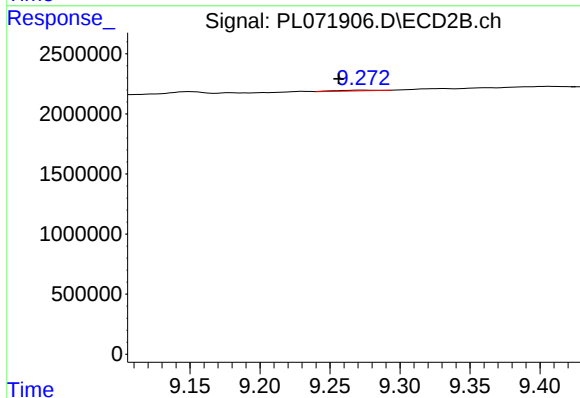


#18 Endrin aldehyde

R.T.: 9.273 min
Delta R.T.: 0.017 min
Response: 119800
Conc: 0.14 ng/ml

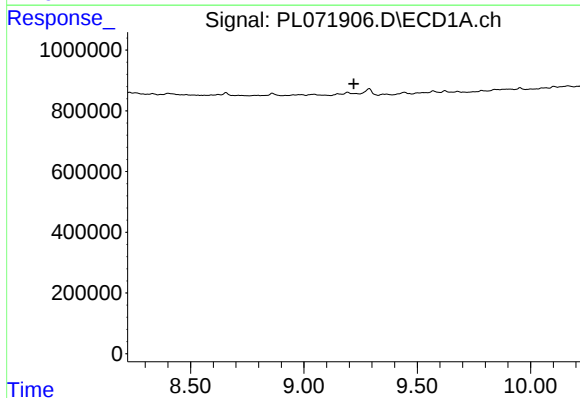


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

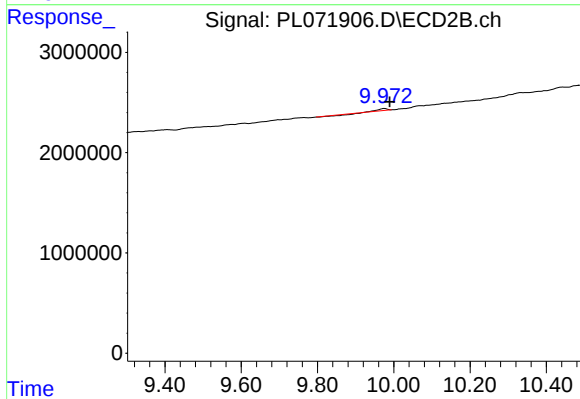

#21 Endrin ketone


R.T.: 9.975 min
Delta R.T.: -0.015 min
Response: 31161
Conc: 0.03 ng/ml

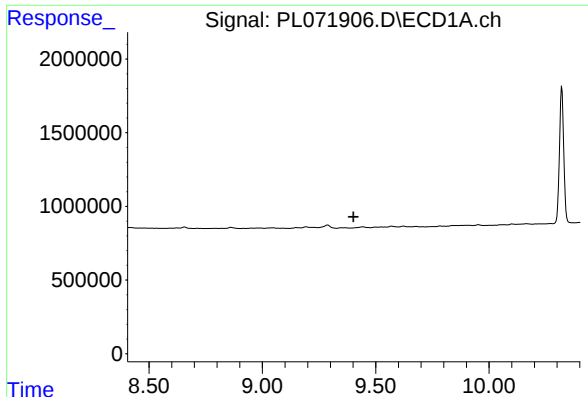

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

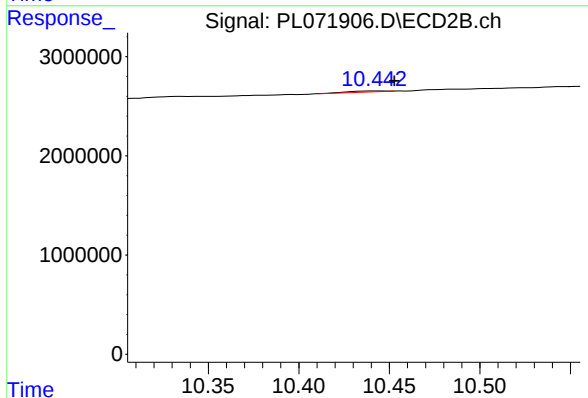


#22 Mirex

R.T.: 10.443 min
Delta R.T.: -0.009 min
Response: 140243
Conc: 0.16 ng/ml

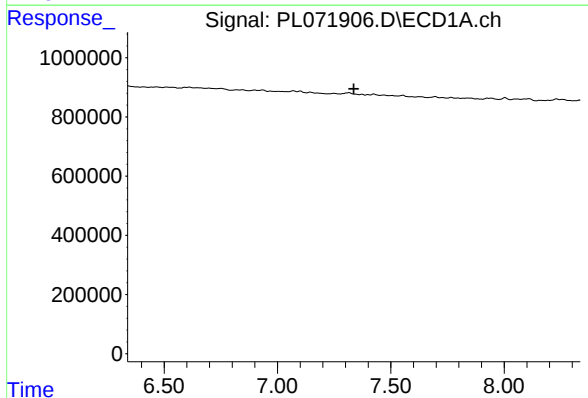


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

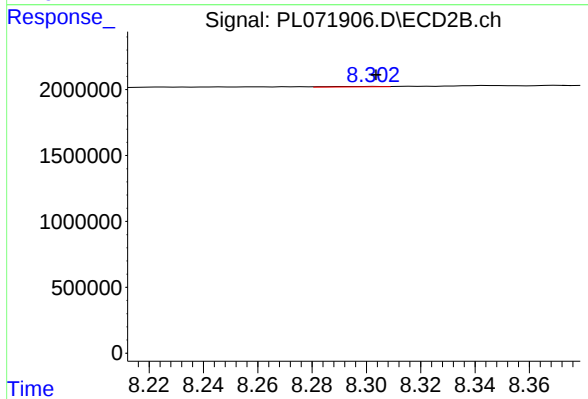

#26 Chlordane-4


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 49047
Conc: 0.20 ng/ml

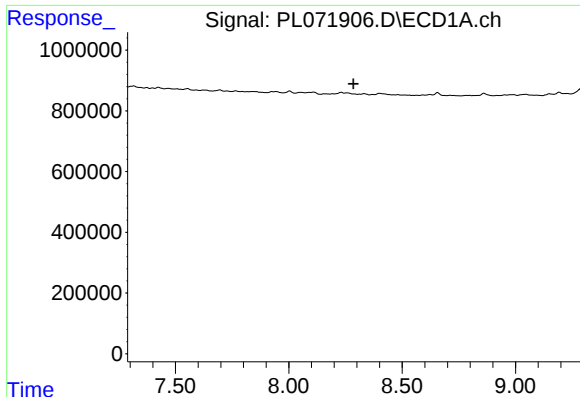

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

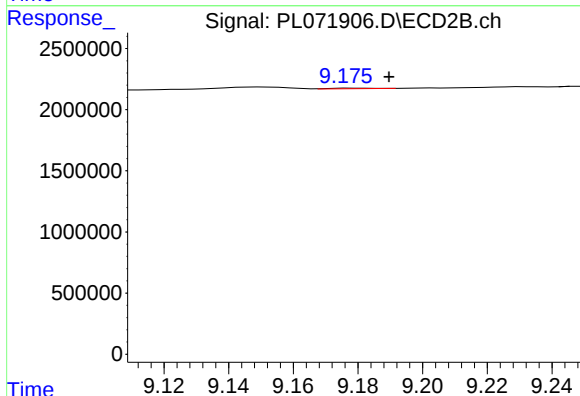


#27 Chlorodane-5

R.T.: 9.178 min
Delta R.T.: -0.011 min
Response: 40925
Conc: 1.02 ng/ml

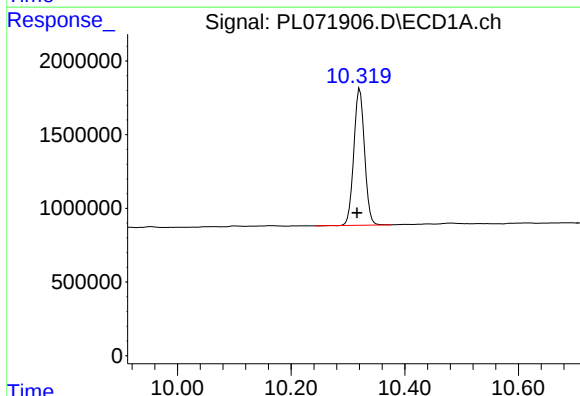

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: 0.005 min
Response: 12148427
Conc: 16.80 ng/ml

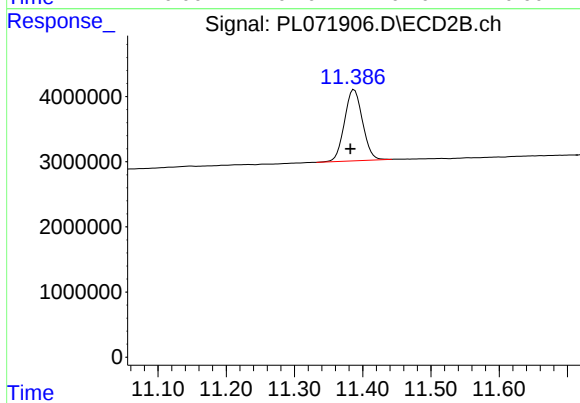

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.006 min
Response: 20060253
Conc: 16.93 ng/ml