

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
 Data File : PL071918.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 19:00
 Operator : AR\AJ
 Sample : N1054-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:37:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	8532820	23556972	18.471	19.173
28)	SA Decachlor...	10.320	11.388	6835833	11337413	9.454	9.567
Target Compounds							
7)	B delta-BHC	0.000	7.018f	0	1129873	N.D.	0.736 #
9)	A Endosulfan I	0.000	8.346	0	184144	N.D.	0.149 #
10)	B gamma-Chl...	0.000	8.220	0	169449	N.D.	0.124 #
15)	B Endosulfa...	0.000	9.147f	0	1051686	N.D.	0.937 #
16)	A 4,4'-DDD	0.000	9.033	0	291894	N.D.	0.304 #
19)	B Endosulfa...	0.000	9.510f	0	17370	N.D.	0.017 #
20)	A Methoxychlor	0.000	9.863f	0	137466	N.D.	0.279 #
21)	B Endrin ke...	0.000	10.001	0	58484	N.D.	0.052 #
25)	Chlordane-3	0.000	8.220	0	169449	N.D.	0.830 #
27)	Chlordane-5	0.000	9.213f	0	241302	N.D.	6.026 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
Data File : PL071918.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 19:00
Operator : AR\AJ
Sample : N1054-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:37:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

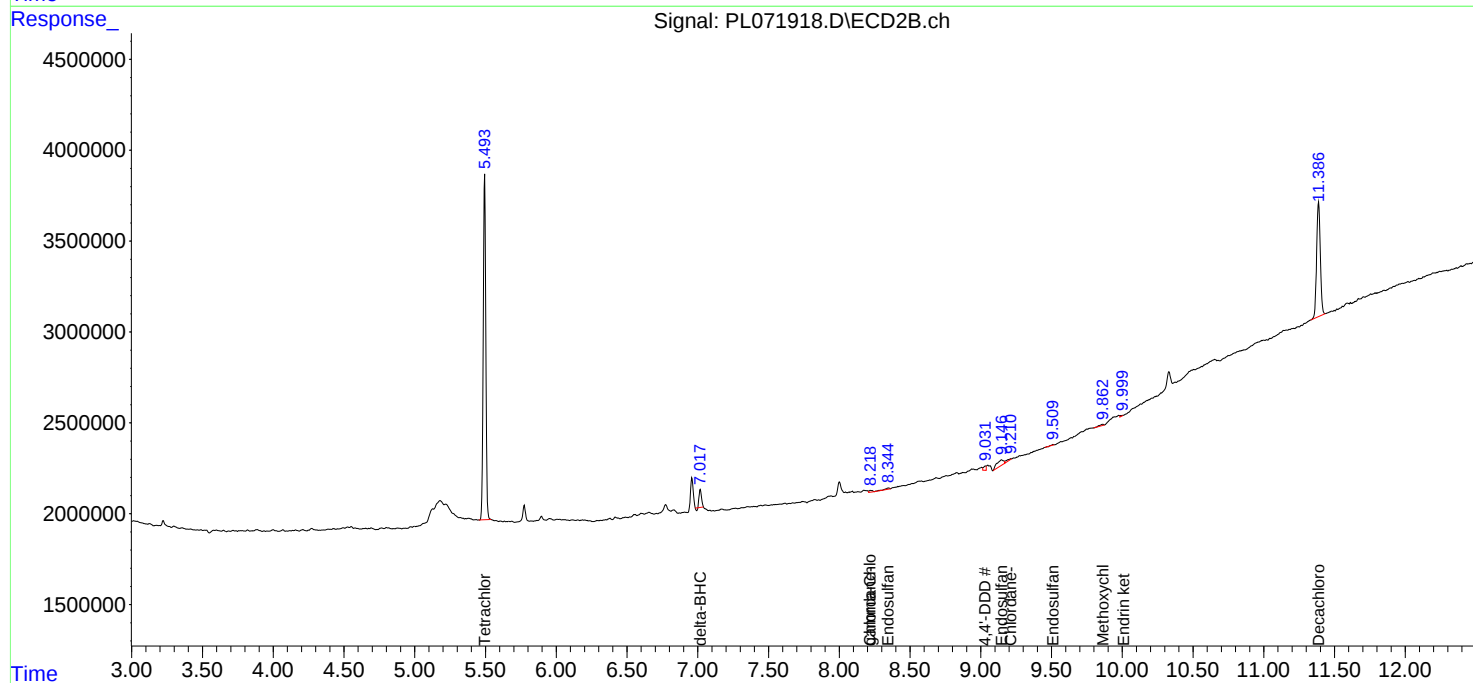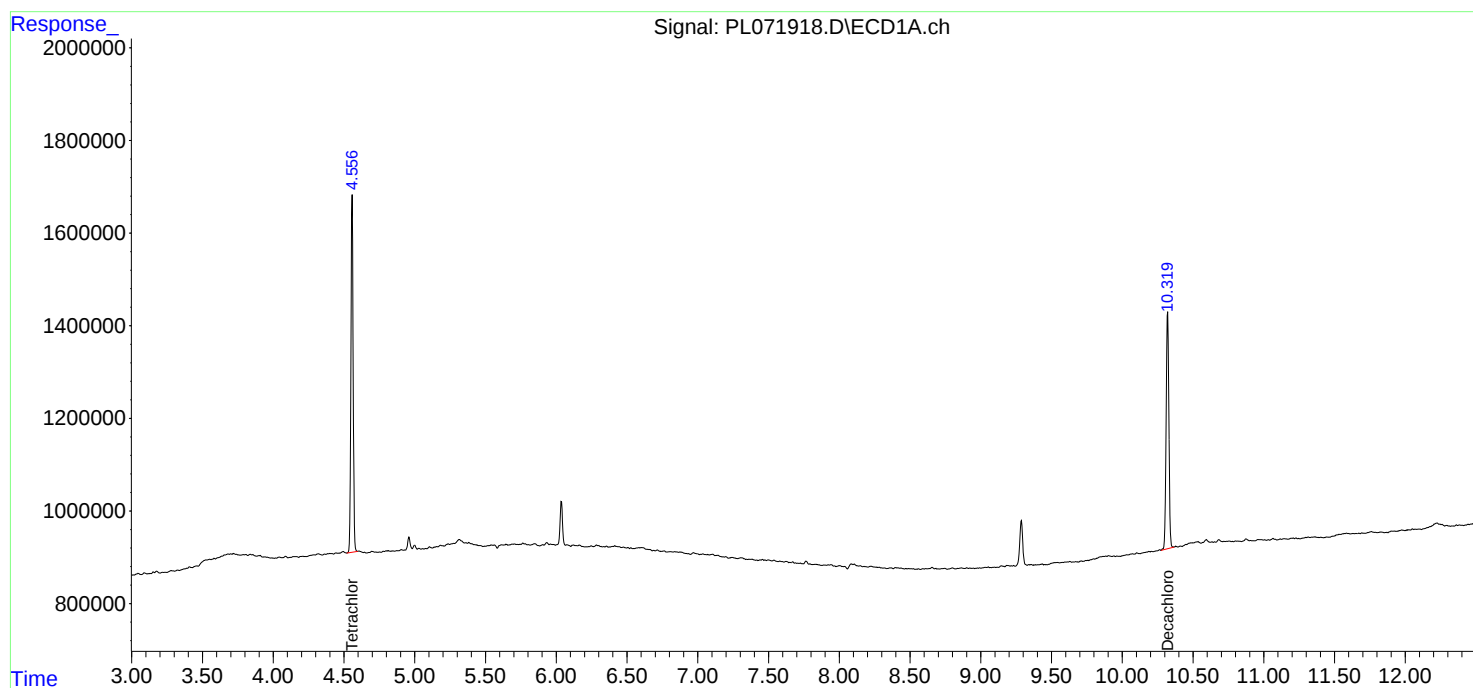


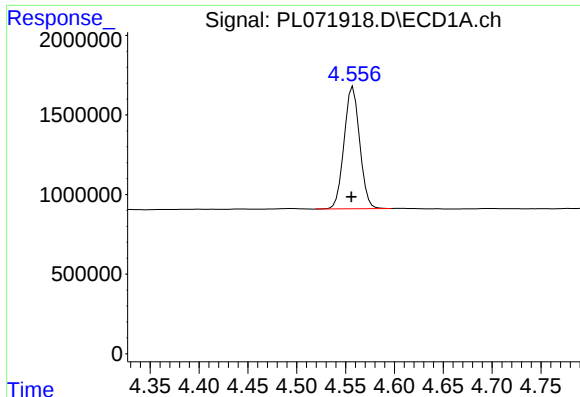

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 8532820
Conc: 18.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

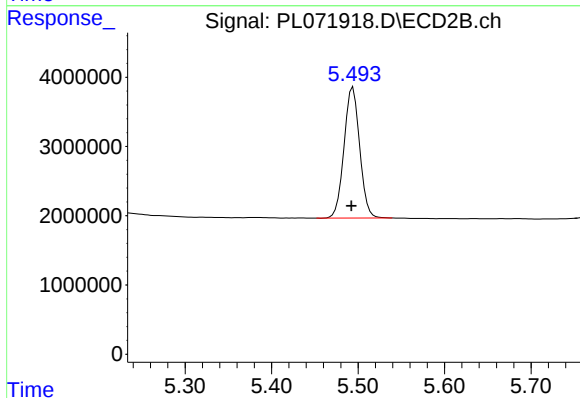


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 23556972
Conc: 19.17 ng/ml

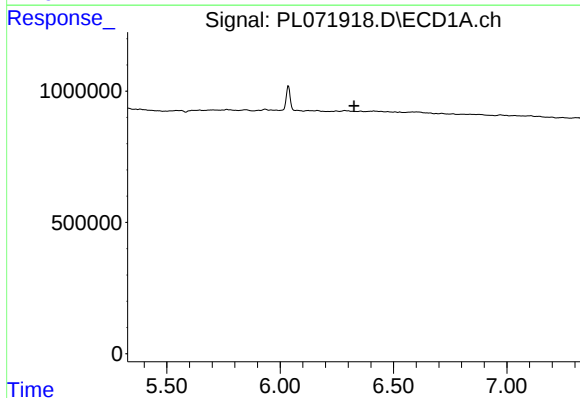


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

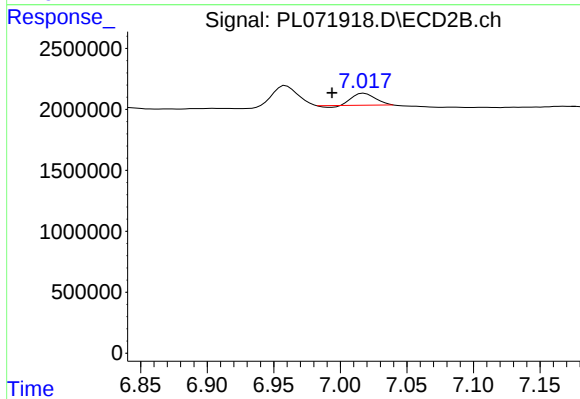

#7 delta-BHC


R.T.: 7.018 min
Delta R.T.: 0.024 min
Response: 1129873
Conc: 0.74 ng/ml

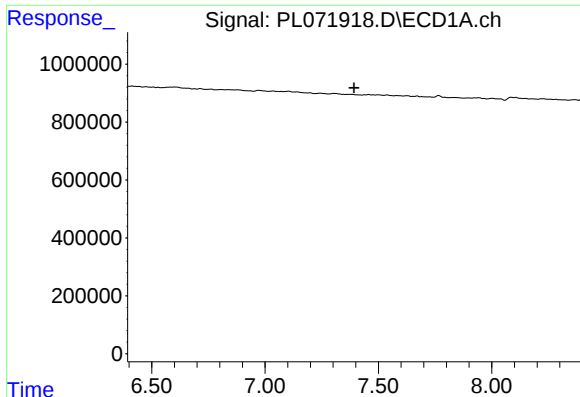

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

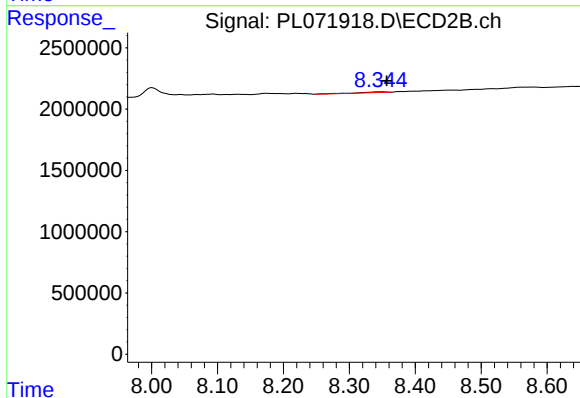


#9 Endosulfan I

R.T.: 8.346 min
Delta R.T.: -0.011 min
Response: 184144
Conc: 0.15 ng/ml

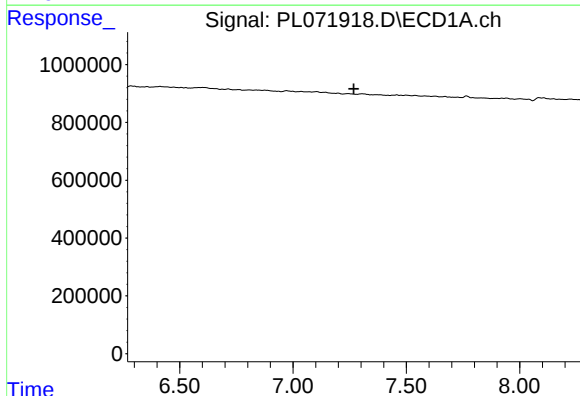


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

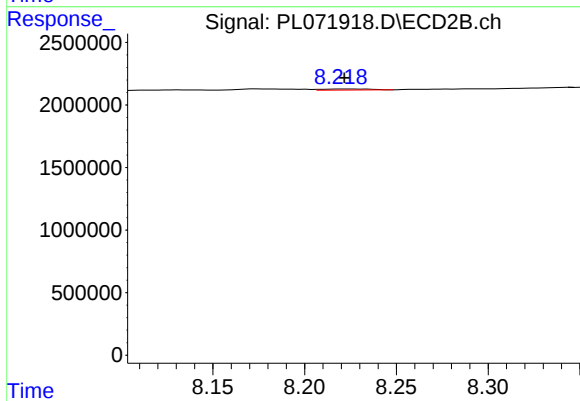

#10 gamma-Chlordane


R.T.: 8.220 min
Delta R.T.: -0.002 min
Response: 169449
Conc: 0.12 ng/ml

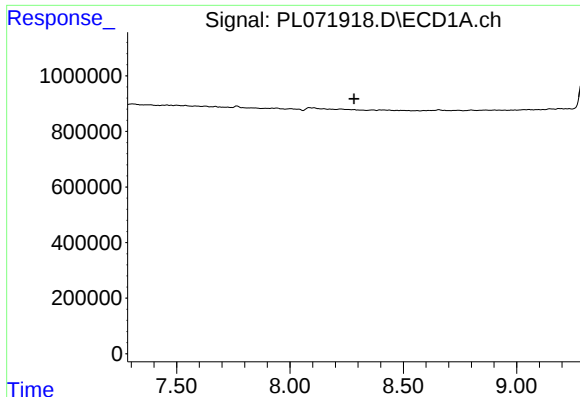

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

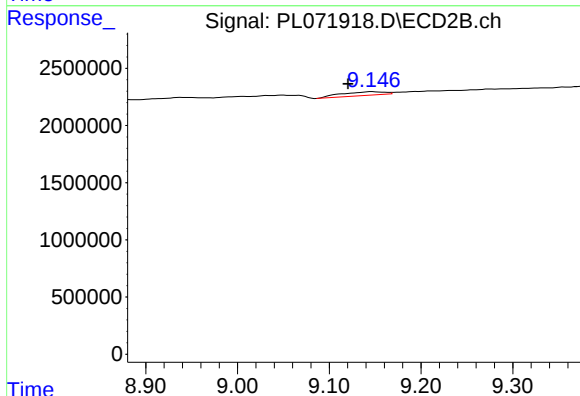


#15 Endosulfan II

R.T.: 9.147 min
Delta R.T.: 0.027 min
Response: 1051686
Conc: 0.94 ng/ml

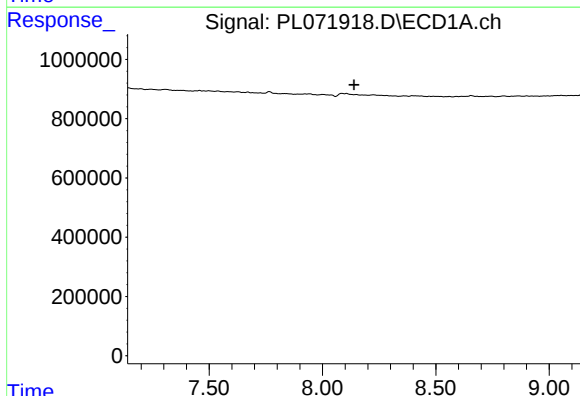


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

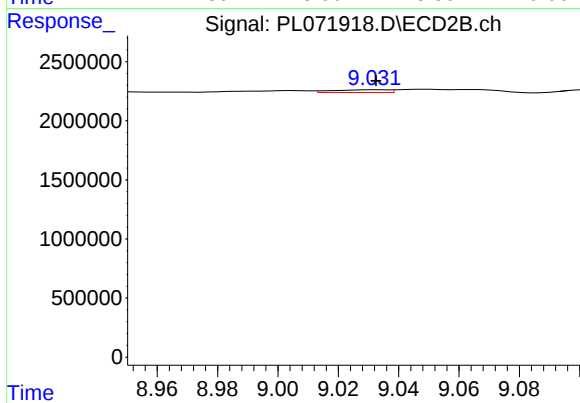

#16 4,4'-DDD


R.T.: 9.033 min
Delta R.T.: 0.000 min
Response: 291894
Conc: 0.30 ng/ml

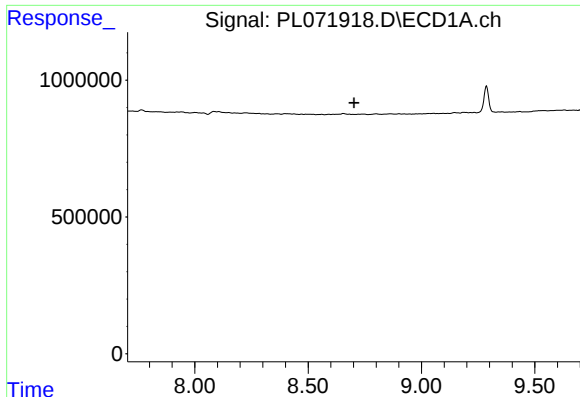

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

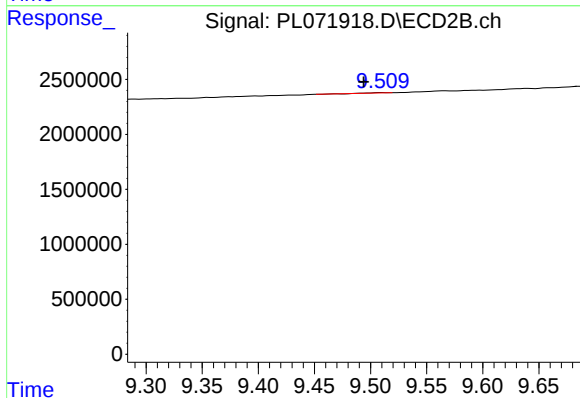


#19 Endosulfan Sulfate

R.T.: 9.510 min
Delta R.T.: 0.016 min
Response: 17370
Conc: 0.02 ng/ml

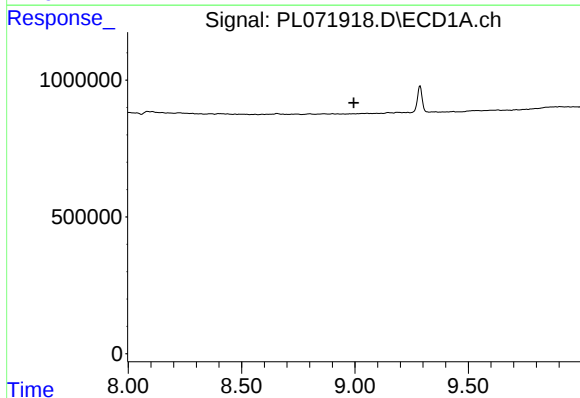


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 8.995 min
Response: 0
Conc: N.D.

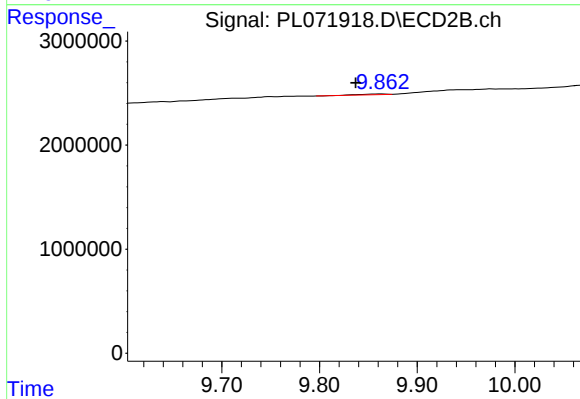

#20 Methoxychlor


R.T.: 9.863 min
Delta R.T.: 0.026 min
Response: 137466
Conc: 0.28 ng/ml

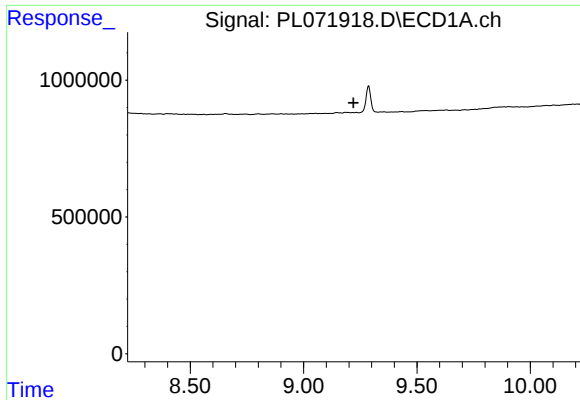

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

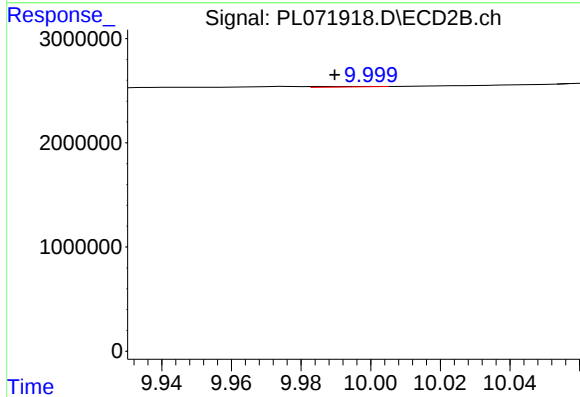


#21 Endrin ketone

R.T.: 10.001 min
Delta R.T.: 0.011 min
Response: 58484
Conc: 0.05 ng/ml

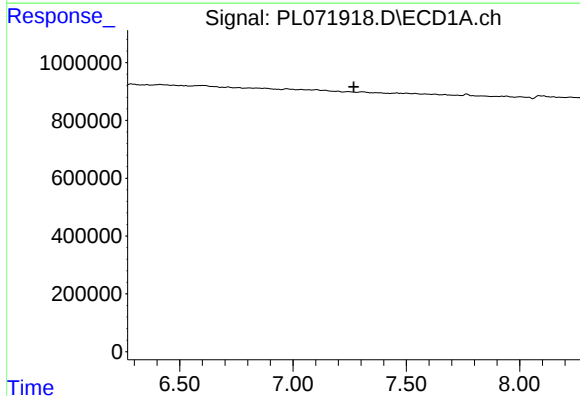


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

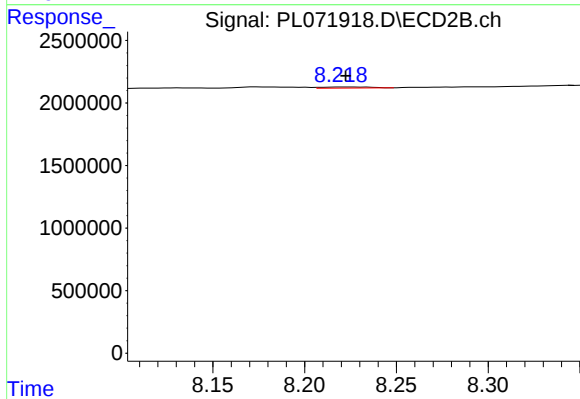

#25 Chlordane-3


R.T.: 8.220 min
Delta R.T.: -0.003 min
Response: 169449
Conc: 0.83 ng/ml

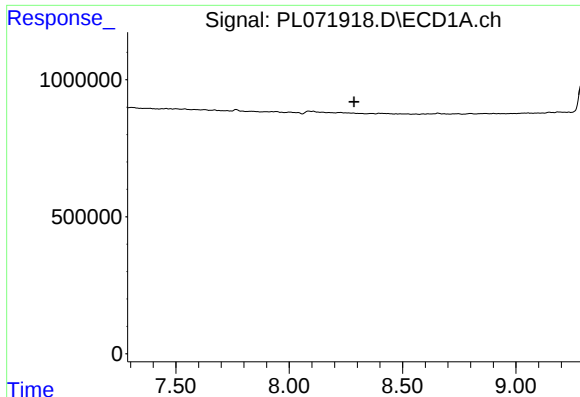

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

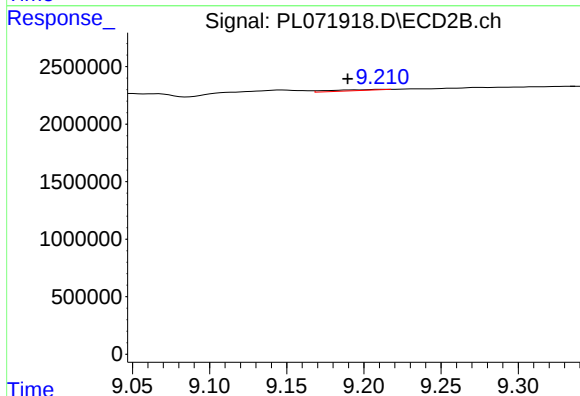


#27 Chlordane-5

R.T.: 9.213 min
Delta R.T.: 0.023 min
Response: 241302
Conc: 6.03 ng/ml

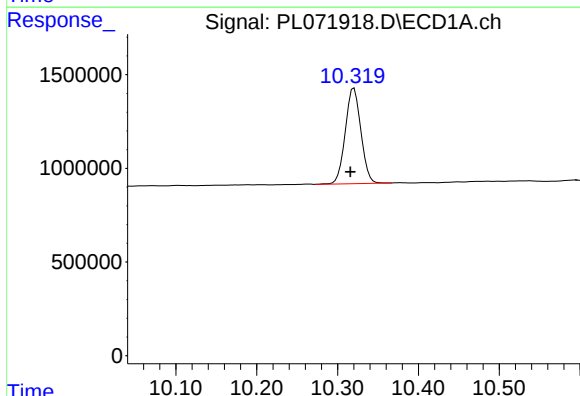

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: 0.004 min
Response: 6835833
Conc: 9.45 ng/ml

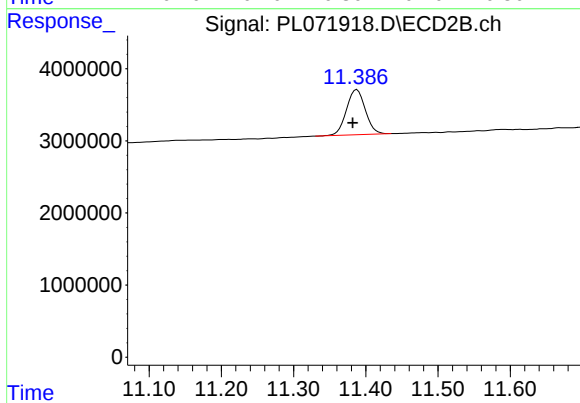

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.006 min
Response: 11337413
Conc: 9.57 ng/ml