

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
 Data File : PL071927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 21:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:40:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	9515751	25668452	20.599	20.892
28)	SA Decachlor...	10.321	11.388	15185096	26015526	21.002	21.954
Target Compounds							
7)	B delta-BHC	0.000	6.974f	0	560616	N.D.	0.365 #
8)	B Heptachlo...	0.000	7.966	0	338485	N.D.	0.242 #
9)	A Endosulfan I	0.000	8.352	0	45072	N.D.	0.036 #
10)	B gamma-Chl...	0.000	8.228	0	193291	N.D.	0.141 #
11)	B alpha-Chl...	0.000	8.306	0	122255	N.D.	0.092 #
13)	MA Dieldrin	0.000	8.666f	0	40308	N.D.	0.031 #
15)	B Endosulfa...	0.000	9.150f	0	430380	N.D.	0.383 #
17)	MA 4,4'-DDT	0.000	9.339	0	34515	N.D.	0.037 #
19)	B Endosulfa...	0.000	9.506	0	45449	N.D.	0.044 #
21)	B Endrin ke...	0.000	9.964f	0	49271	N.D.	0.044 #
25)	Chlordane-3	0.000	8.228	0	193291	N.D.	0.947 #
26)	Chlordane-4	0.000	8.306	0	122255	N.D.	0.502 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
Data File : PL071927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 21:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:40:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

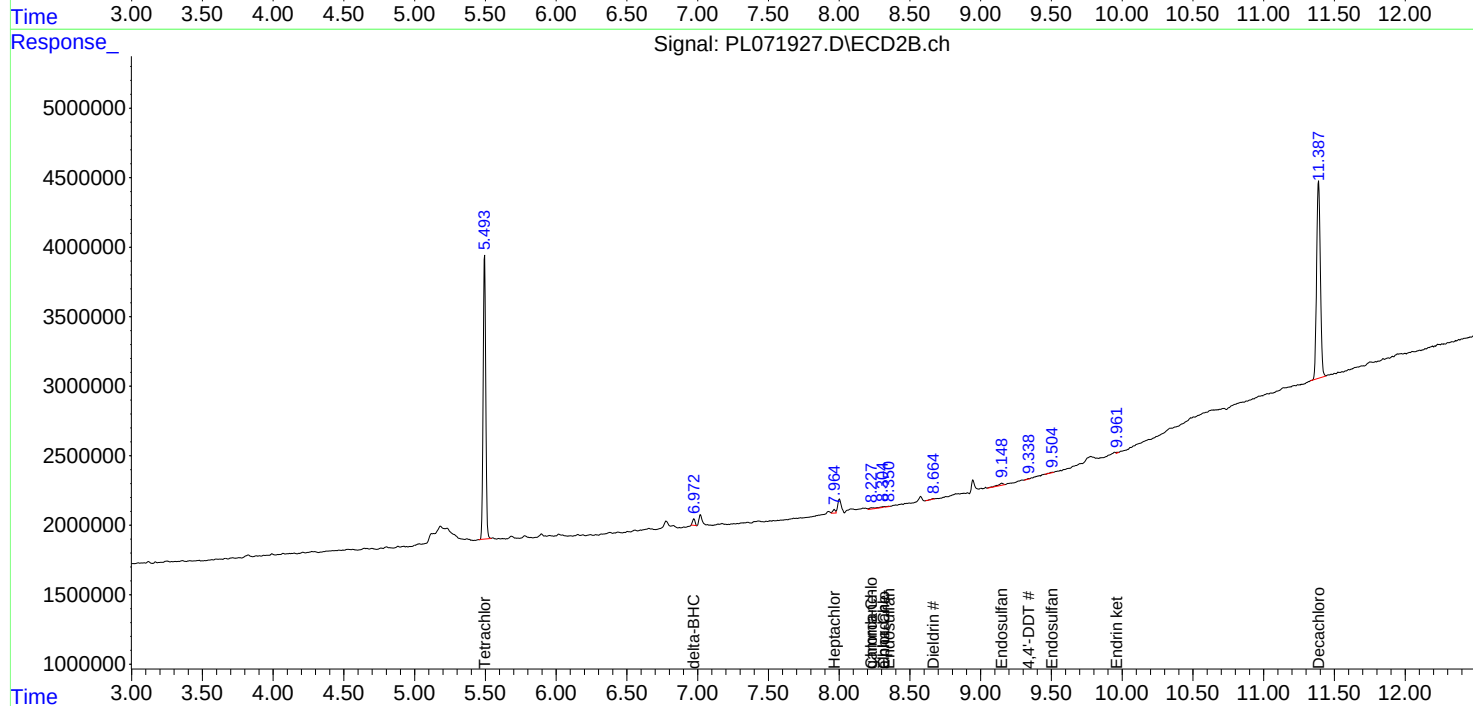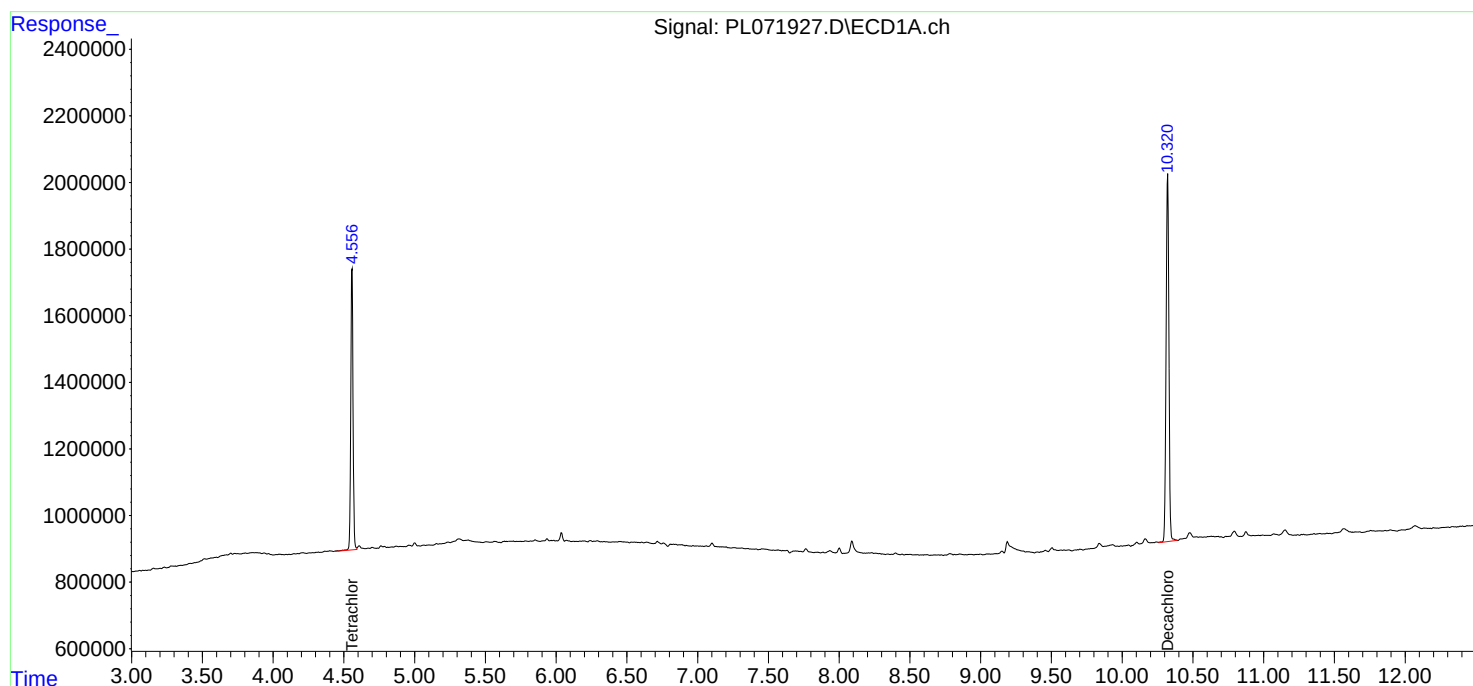


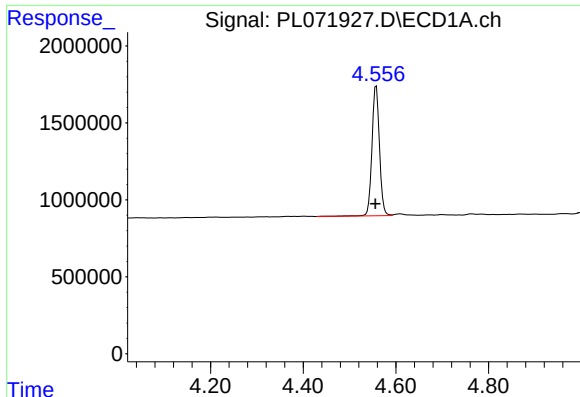

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9515751
Conc: 20.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

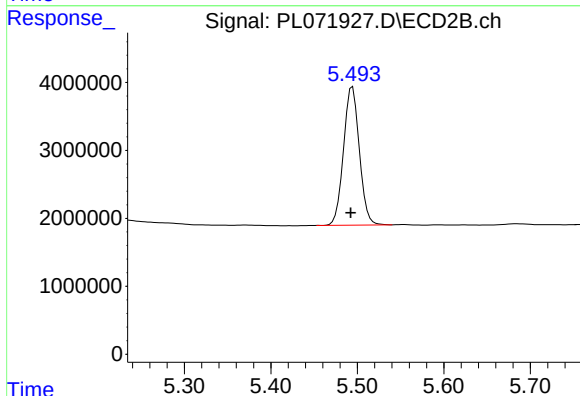


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 25668452
Conc: 20.89 ng/ml

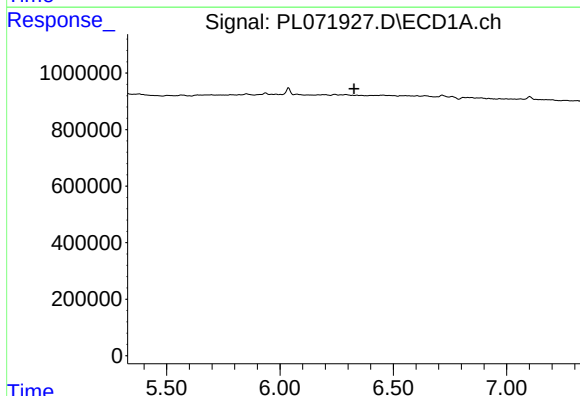


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

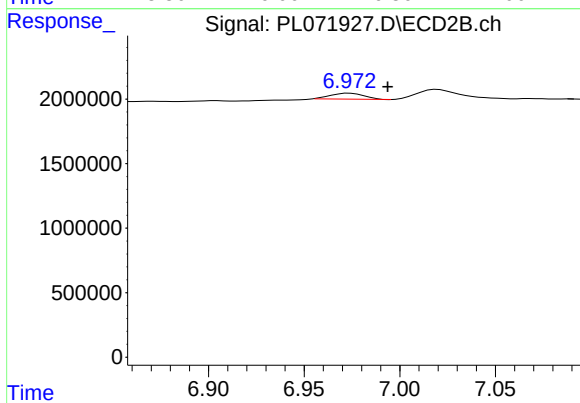

#7 delta-BHC


R.T.: 6.974 min
Delta R.T.: -0.020 min
Response: 560616
Conc: 0.37 ng/ml

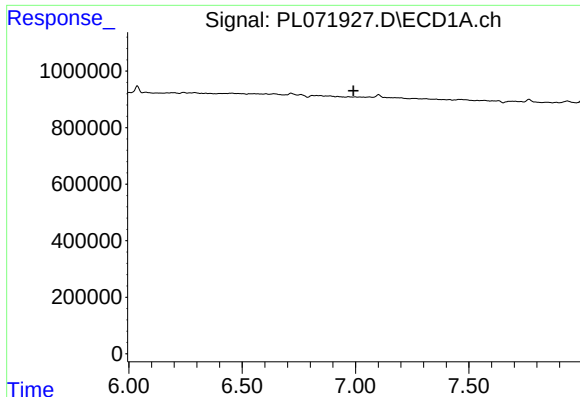

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

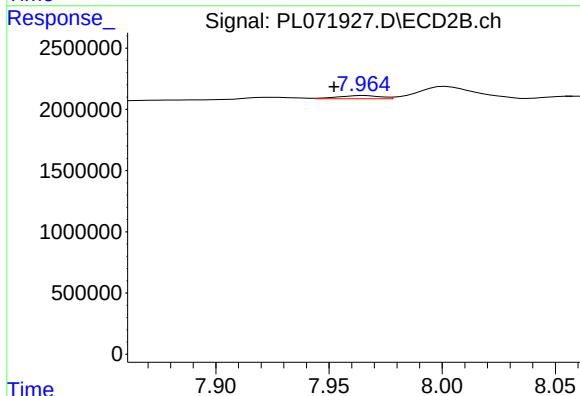


#8 Heptachlor epoxide

R.T.: 7.966 min
Delta R.T.: 0.013 min
Response: 338485
Conc: 0.24 ng/ml

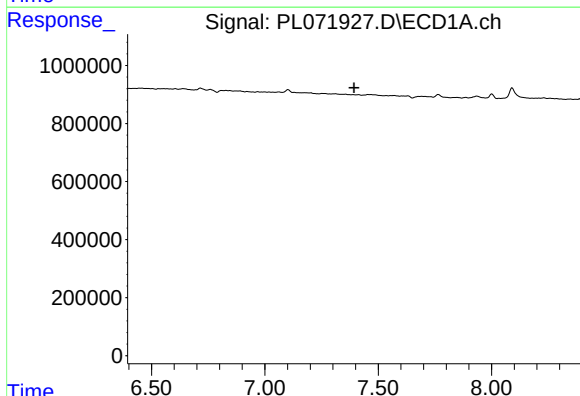


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

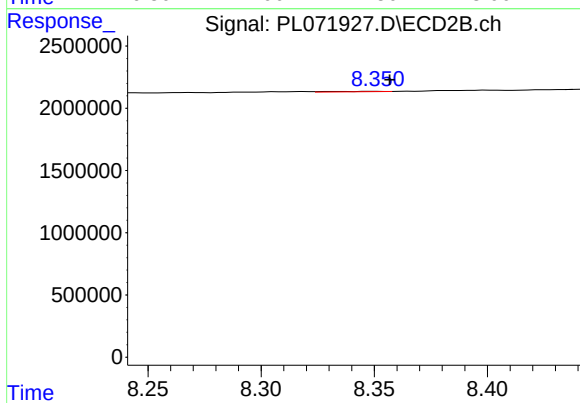

#9 Endosulfan I


R.T.: 8.352 min
Delta R.T.: -0.005 min
Response: 45072
Conc: 0.04 ng/ml

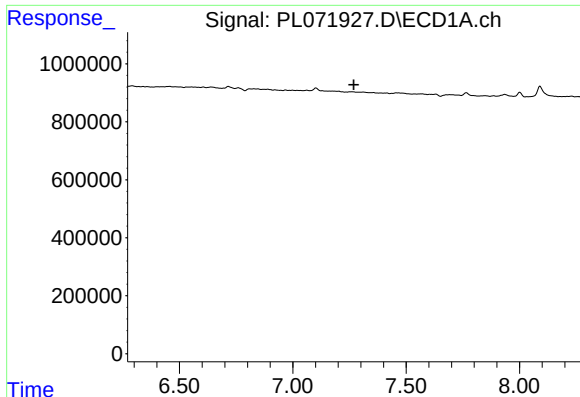

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

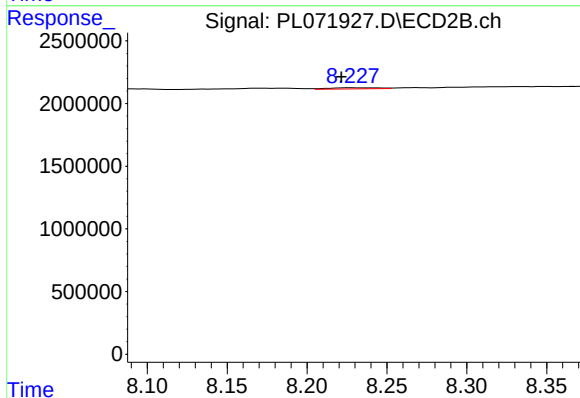


#10 gamma-Chlordane

R.T.: 8.228 min
Delta R.T.: 0.007 min
Response: 193291
Conc: 0.14 ng/ml

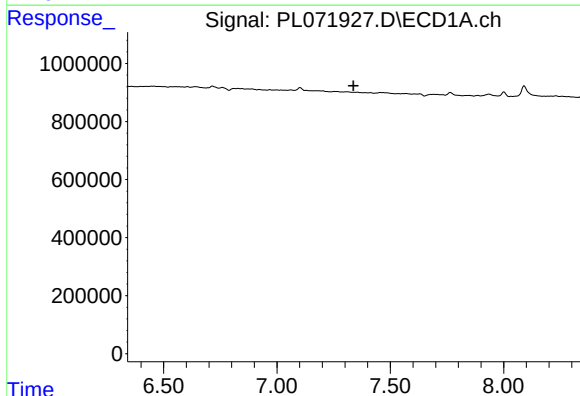


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

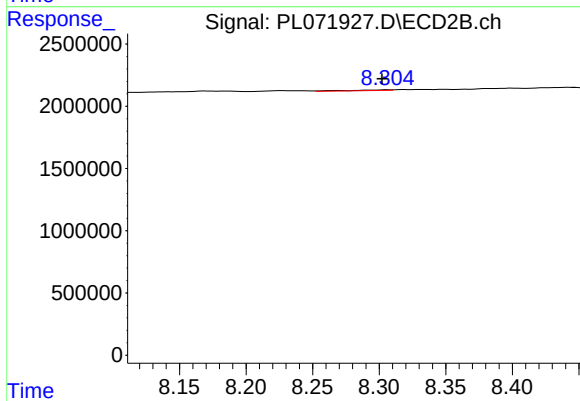

#11 alpha-Chlordane


R.T.: 8.306 min
Delta R.T.: 0.004 min
Response: 122255
Conc: 0.09 ng/ml

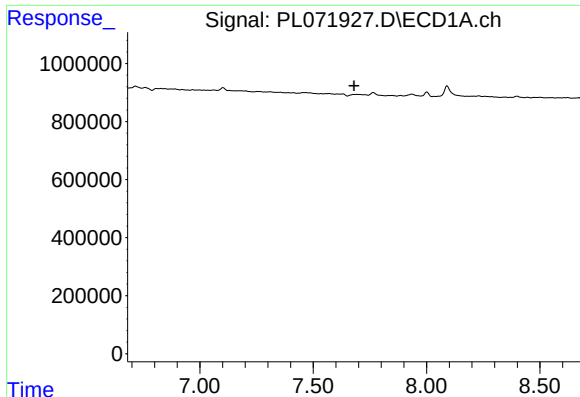

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

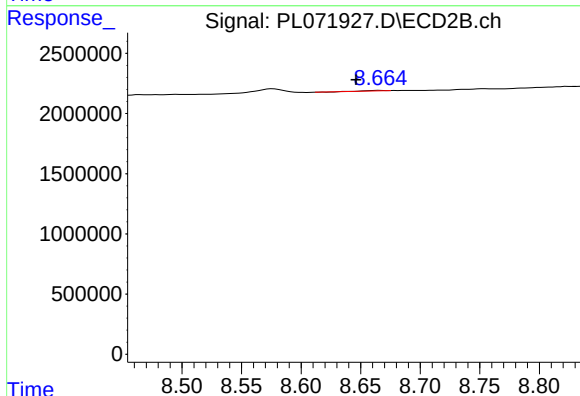


#13 Dieldrin

R.T.: 8.666 min
Delta R.T.: 0.020 min
Response: 40308
Conc: 0.03 ng/ml

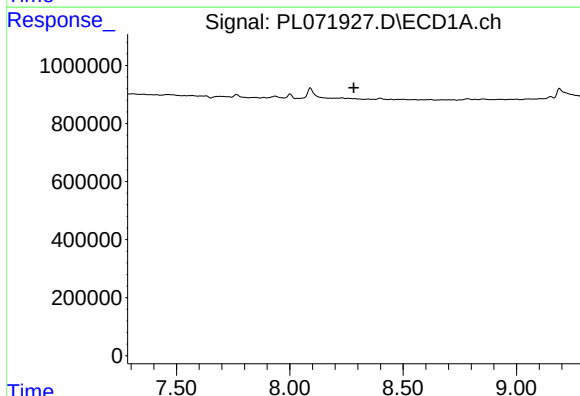


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

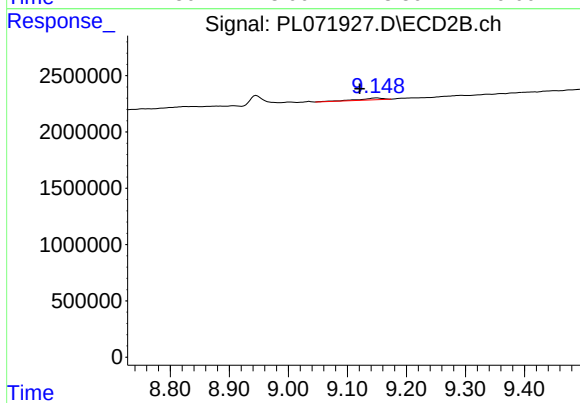

#15 Endosulfan II


R.T.: 9.150 min
Delta R.T.: 0.029 min
Response: 430380
Conc: 0.38 ng/ml

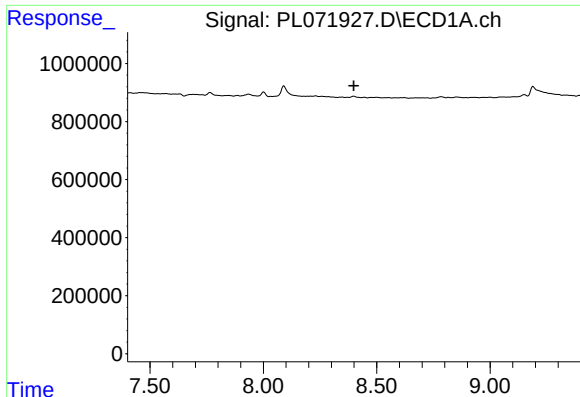

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

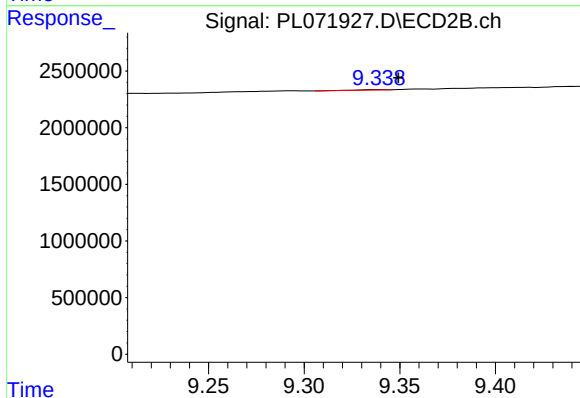


#17 4,4'-DDT

R.T.: 9.339 min
Delta R.T.: -0.010 min
Response: 34515
Conc: 0.04 ng/ml

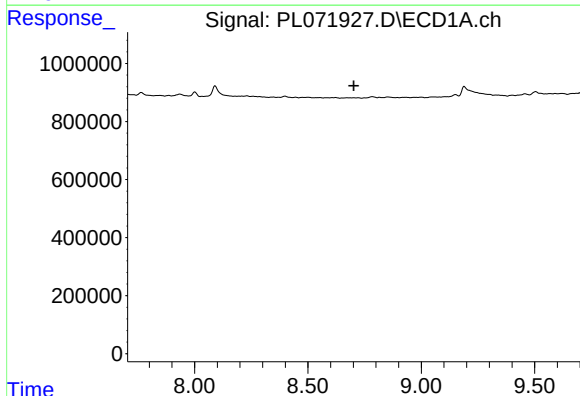


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

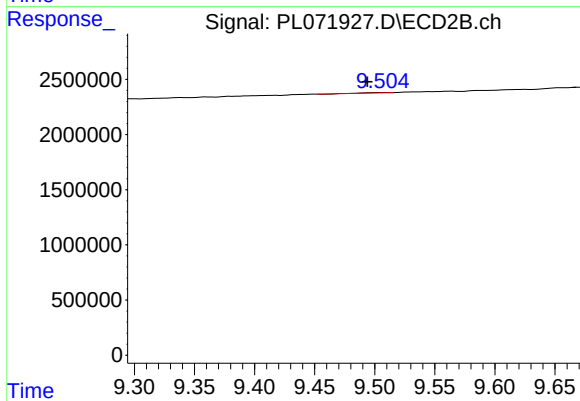

#19 Endosulfan Sulfate


R.T.: 9.506 min
Delta R.T.: 0.012 min
Response: 45449
Conc: 0.04 ng/ml

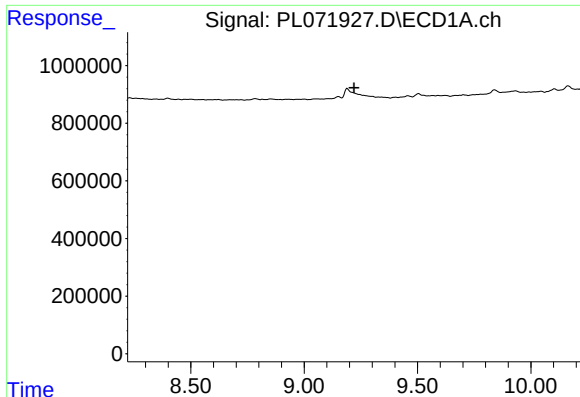

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

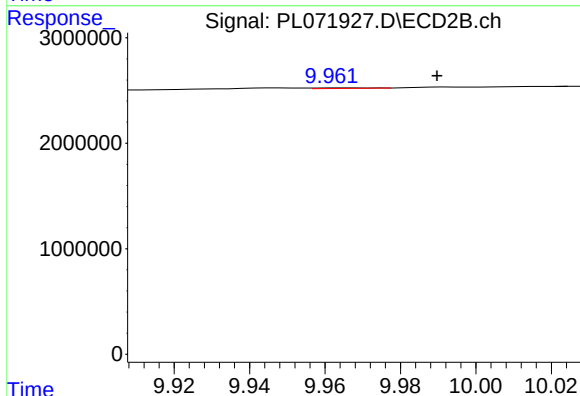


#21 Endrin ketone

R.T.: 9.964 min
Delta R.T.: -0.026 min
Response: 49271
Conc: 0.04 ng/ml

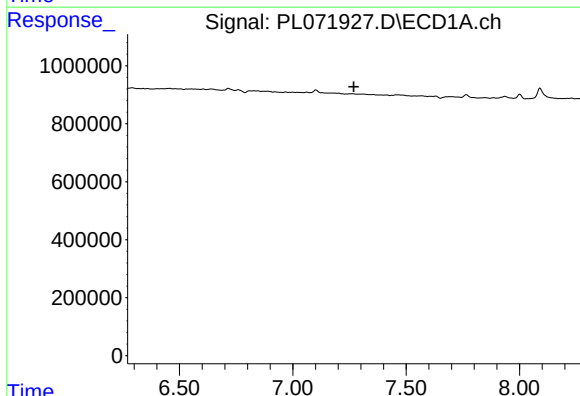


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

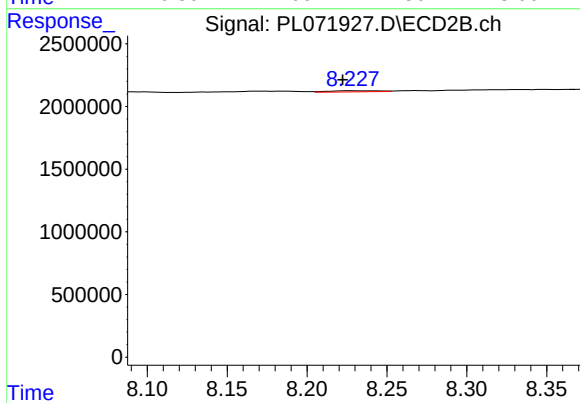

#25 Chlordane-3


R.T.: 8.228 min
Delta R.T.: 0.006 min
Response: 193291
Conc: 0.95 ng/ml

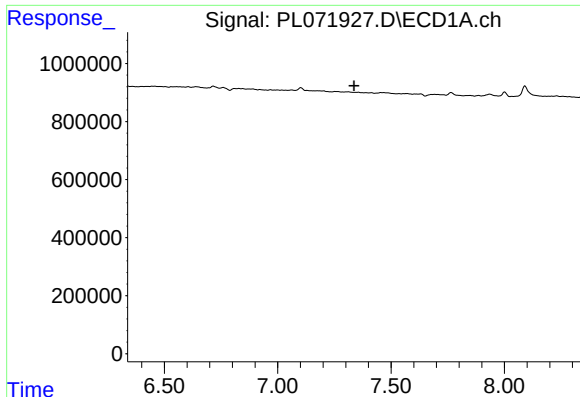

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

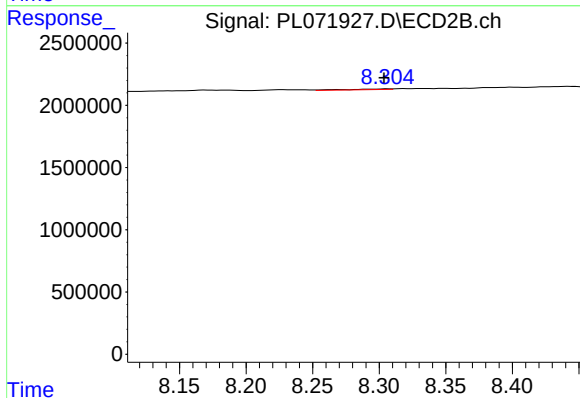


#26 Chlordane-4

R.T.: 8.306 min
Delta R.T.: 0.003 min
Response: 122255
Conc: 0.50 ng/ml

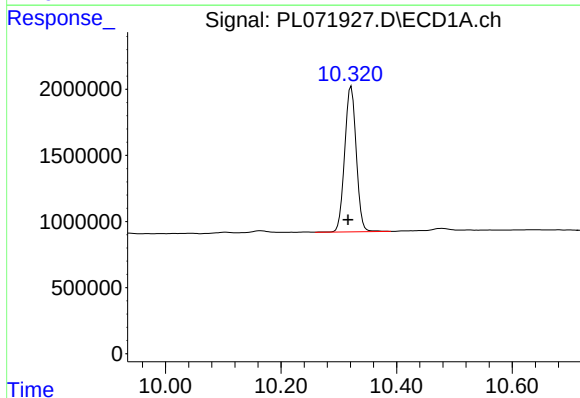

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: 0.006 min
Response: 15185096
Conc: 21.00 ng/ml

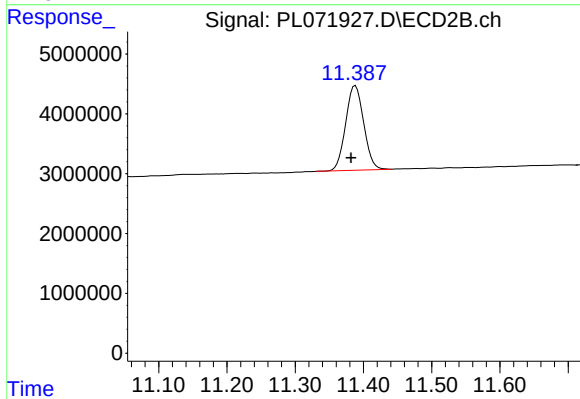

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.006 min
Response: 26015526
Conc: 21.95 ng/ml