

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
 Data File : PL071903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 14:28
 Operator : AR\AJ
 Sample : N1054-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20211303-CAPE-5-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/11/2022
 Supervised By :mohammad ahmed 01/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:31:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.558	5.494	9218509	24988986	19.956	20.339
28) SA Decachlor...	10.319	11.387	9848010	16018133	13.621m	13.517

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
Data File : PL071903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 14:28
Operator : AR\AJ
Sample : N1054-05
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20211303-CAPE-5-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/11/2022
Supervised By : mohammad ahmed 01/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:31:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

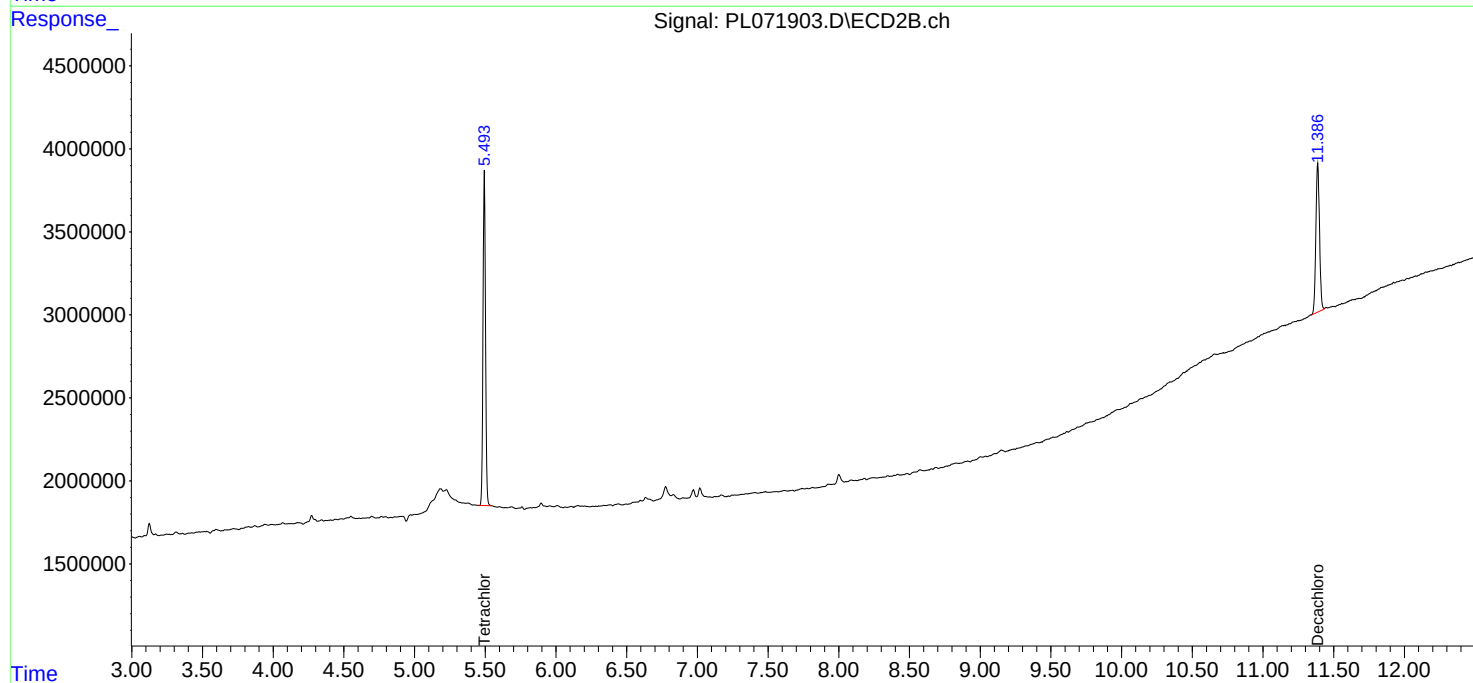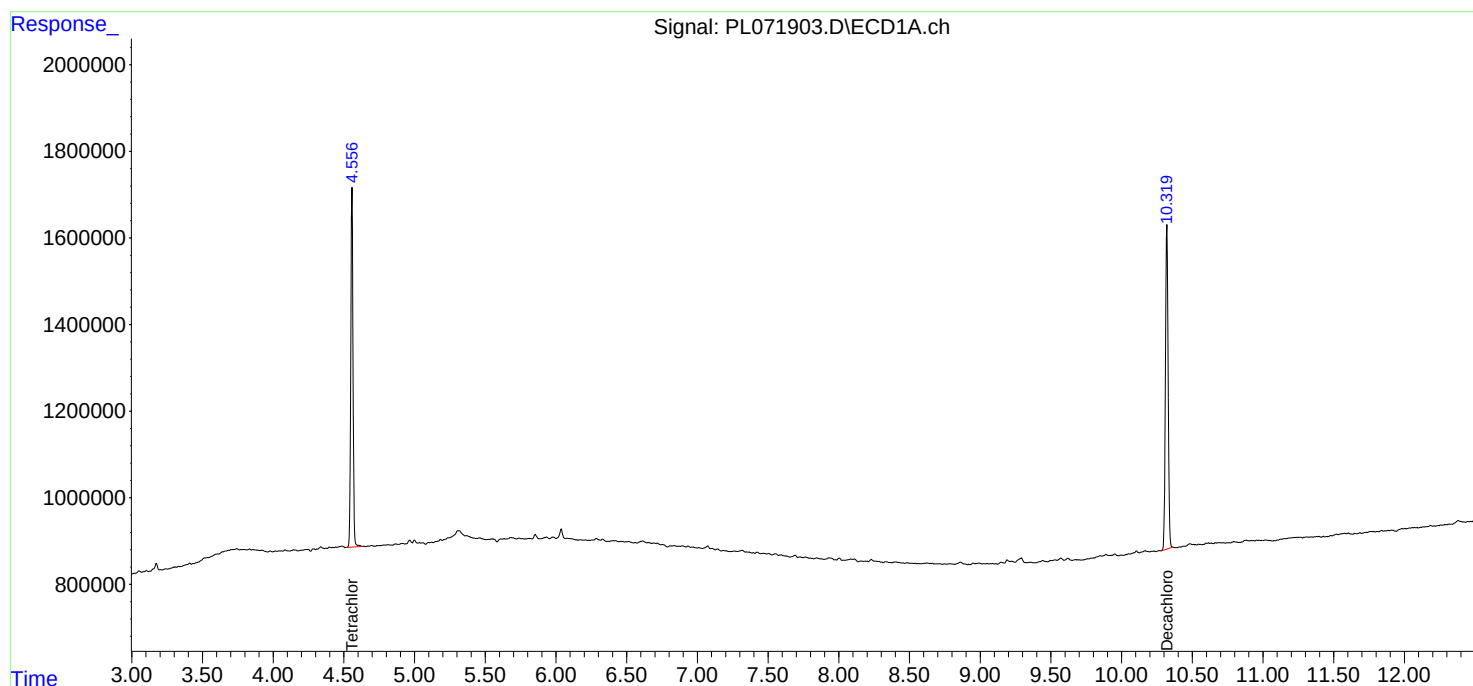

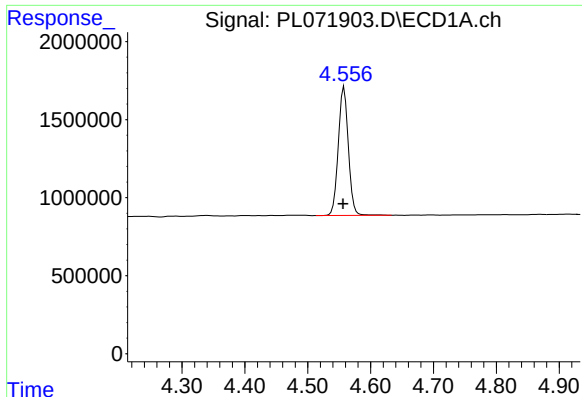


#1 Tetrachloro-m-xylene

R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9218509
Conc: 19.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
20211303-CAPE-5-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2022
Supervised By :mohammad ahmed 01/12/2022

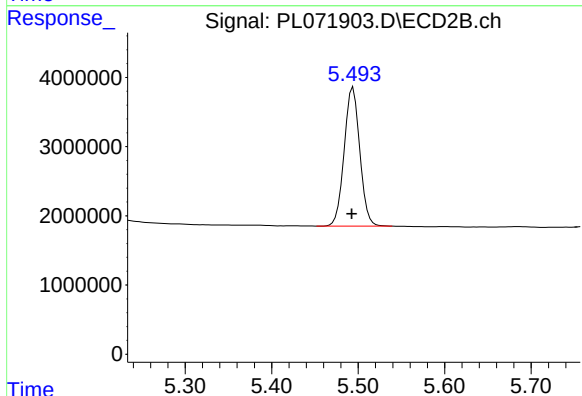


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 24988986
Conc: 20.34 ng/ml

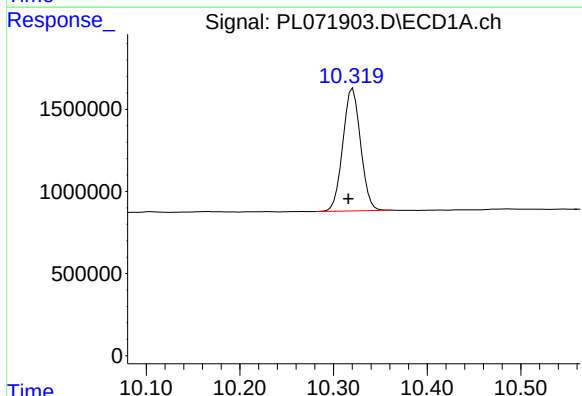

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: 0.003 min
Response: 9848010
Conc: 13.62 ng/ml m

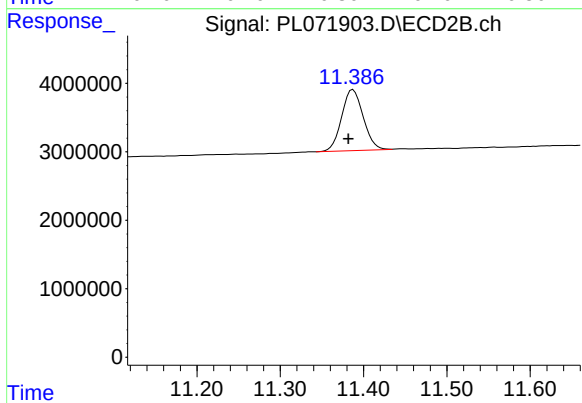

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: 0.005 min
Response: 16018133
Conc: 13.52 ng/ml