

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
 Data File : PL071910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 16:49
 Operator : AR\AJ
 Sample : PB141941BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB141941BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/11/2022
 Supervised By : mohammad ahmed 01/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:34:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.494	10068169	26902966	21.795m	21.896
28)	SA Decachlor...	10.325	11.391	15970846	26759550	22.089m	22.582

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011022\
Data File : PL071910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 16:49
Operator : AR\AJ
Sample : PB141941BL
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB141941BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/11/2022
Supervised By : mohammad ahmed 01/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:34:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

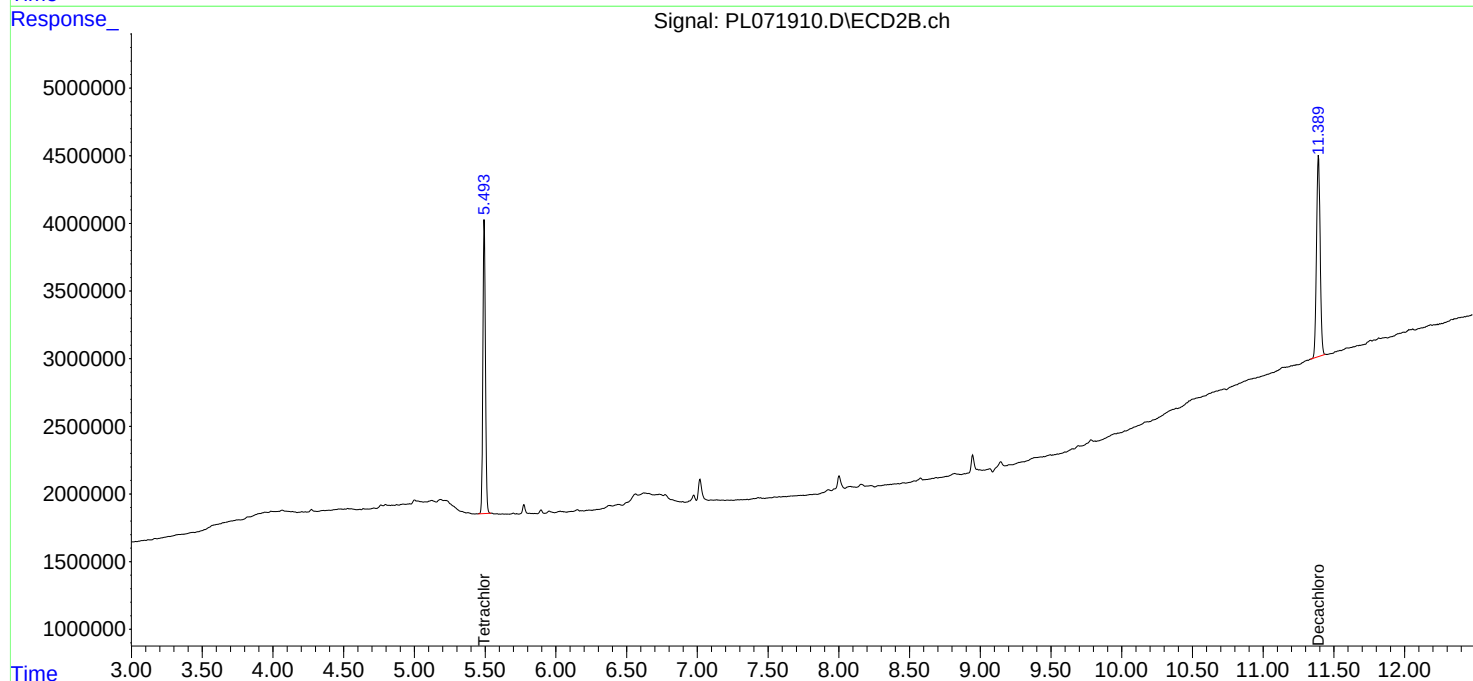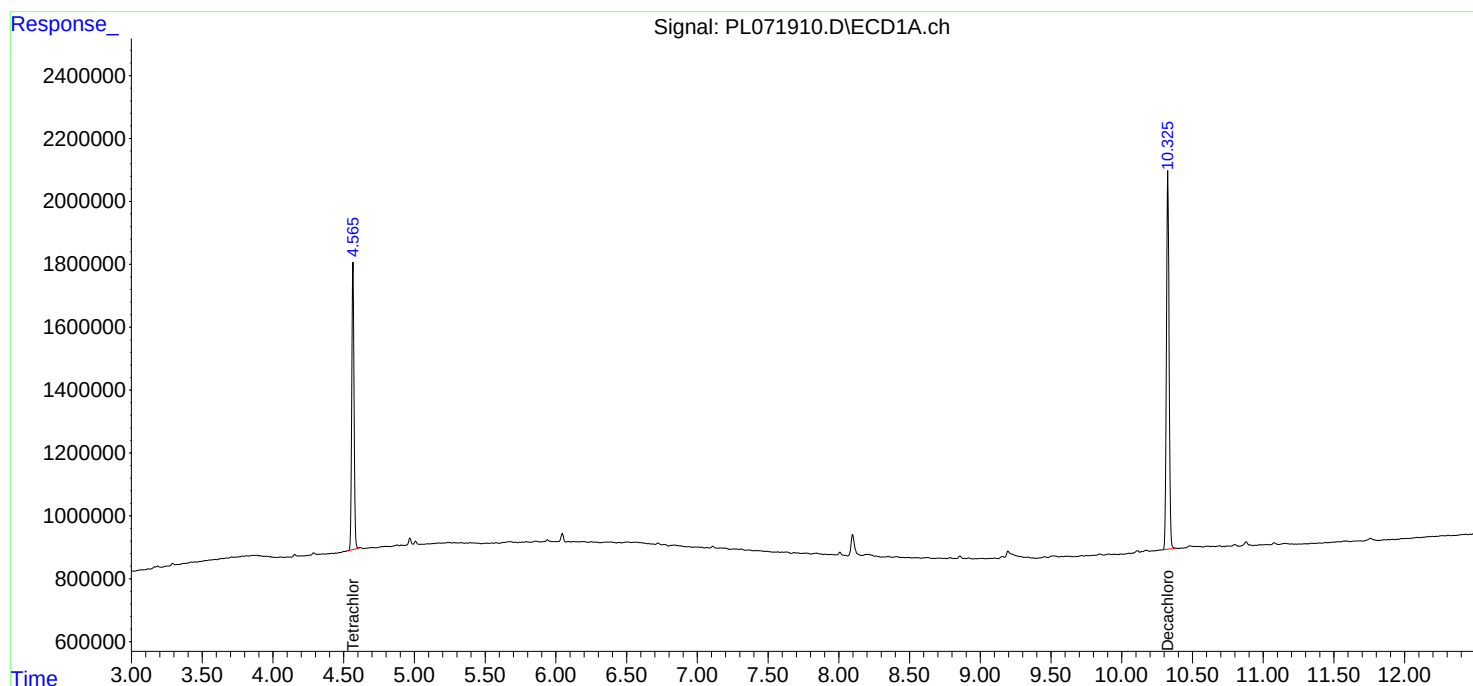

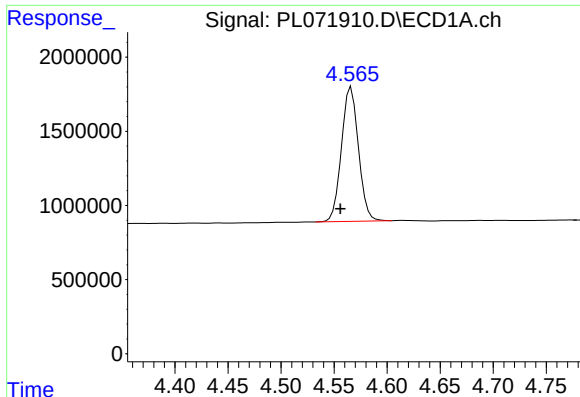


#1 Tetrachloro-m-xylene

R.T.: 4.565 min
Delta R.T.: 0.009 min
Response: 10068169
Conc: 21.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB141941BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2022
Supervised By :mohammad ahmed 01/12/2022

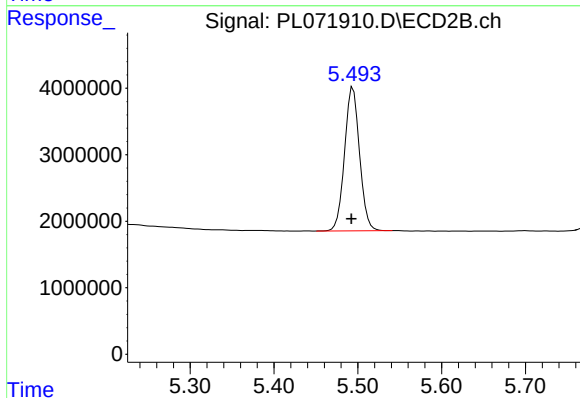


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 26902966
Conc: 21.90 ng/ml

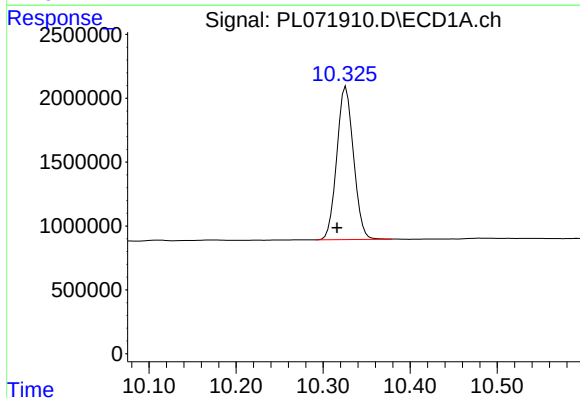

#28 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: 0.009 min
Response: 15970846
Conc: 22.09 ng/ml m

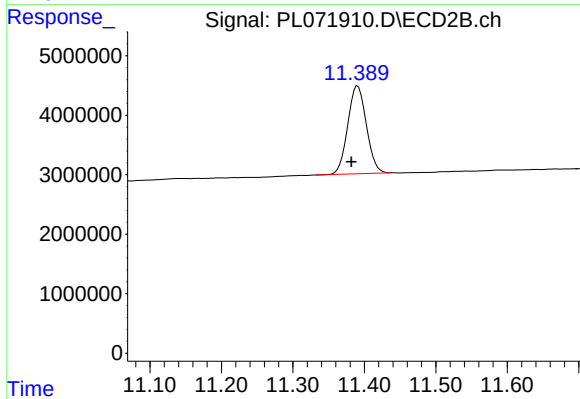

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: 0.009 min
Response: 26759550
Conc: 22.58 ng/ml