

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011024\
 Data File : PL087723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2024 22:00
 Operator : AR\AJ
 Sample : P1056-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MR-311P-30-32

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/11/2024
 Supervised By : Ankita Jodhani 01/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 23:43:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.418	2.674	58390621	24866203	19.504m	20.528
2) SA Decachlor...	8.983	7.864	52433632	24541239	18.411	19.372

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011024\
Data File : PL087723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2024 22:00
Operator : AR\AJ
Sample : P1056-04
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MR-311P-30-32


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/11/2024
Supervised By : Ankita Jodhani 01/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 23:43:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

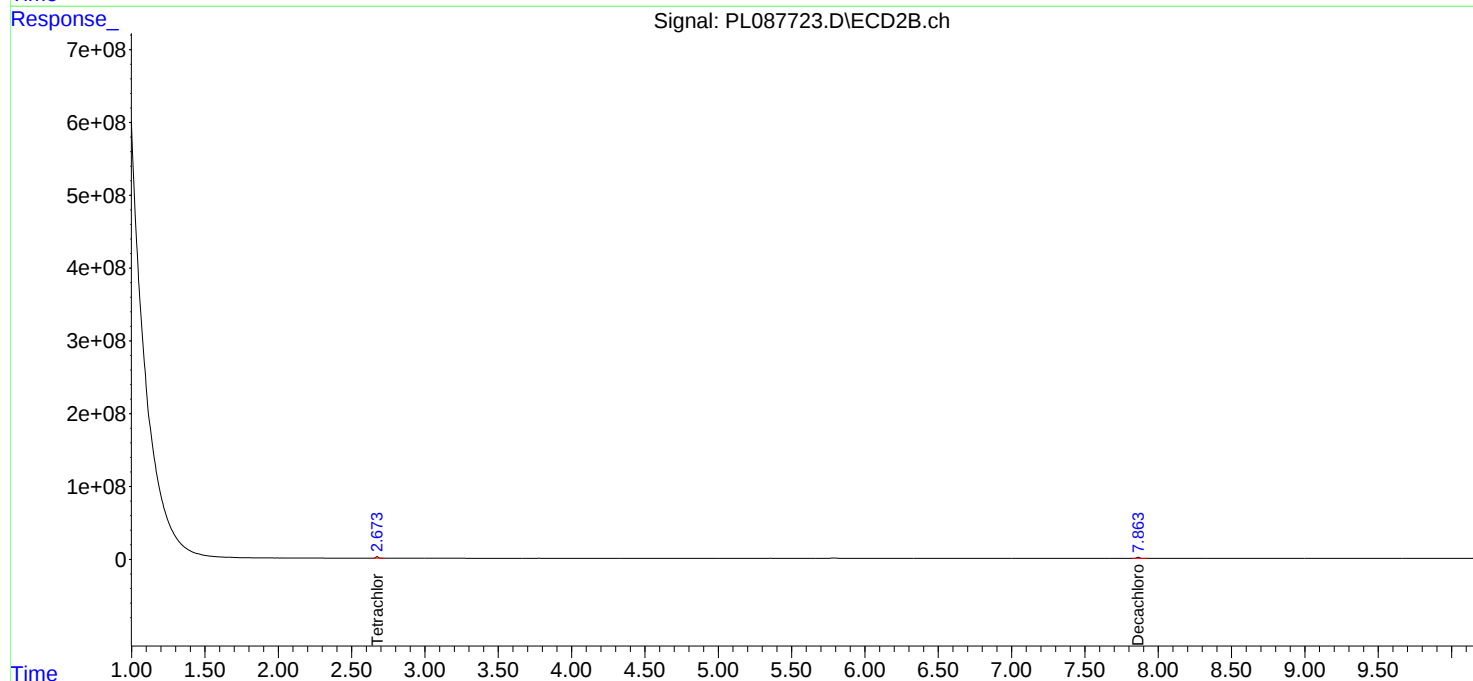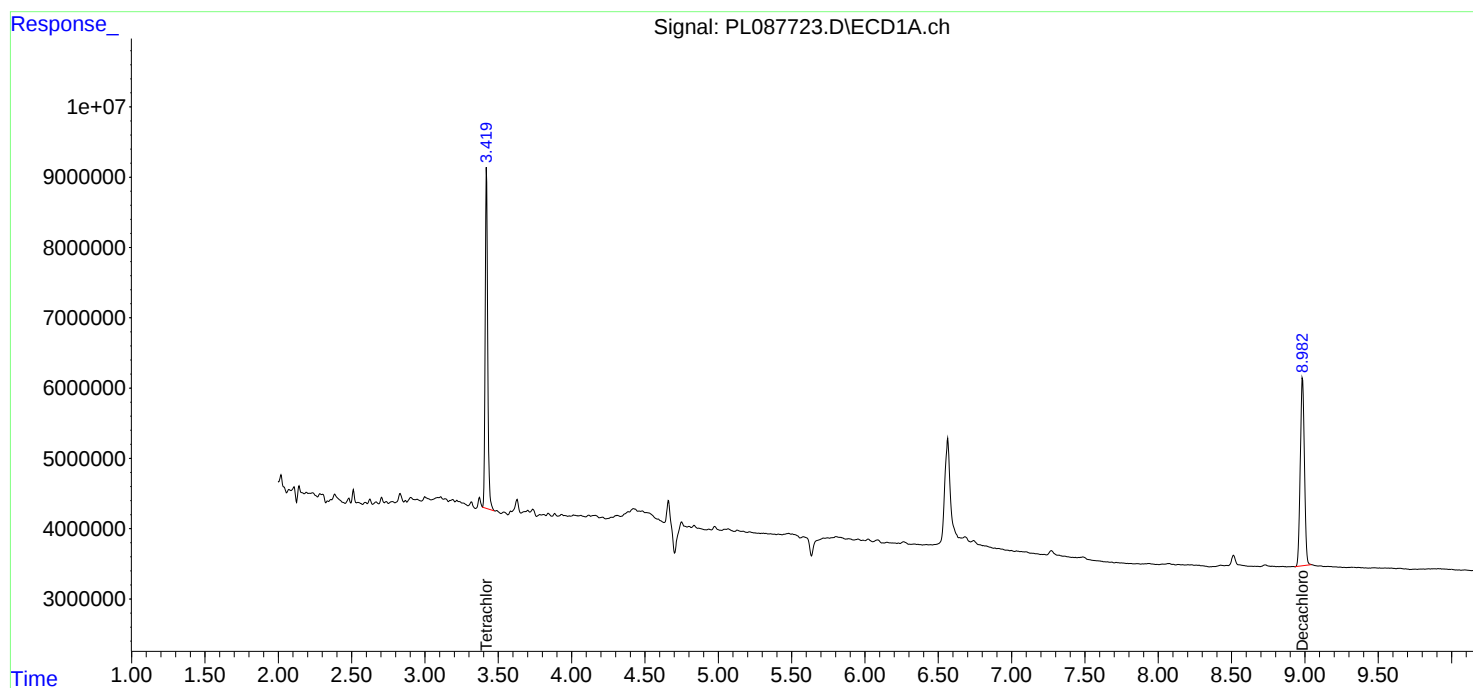

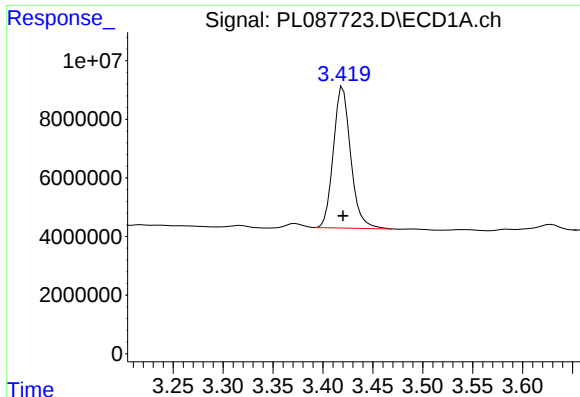


#1 Tetrachloro-m-xylene

R.T.: 3.418 min
Delta R.T.: -0.002 min
Response: 58390621
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-311P-30-32


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2024
Supervised By :Ankita Jodhani 01/11/2024

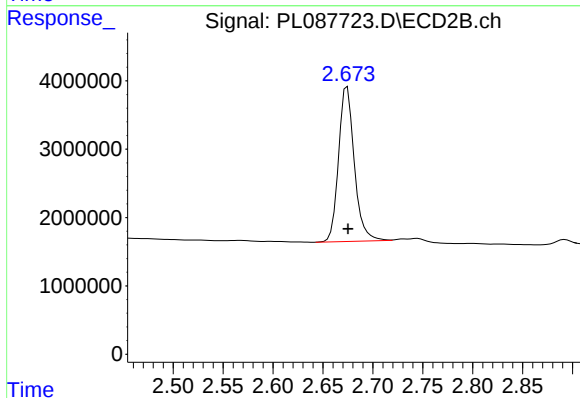


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: 0.000 min
Response: 24866203
Conc: 20.53 ng/ml

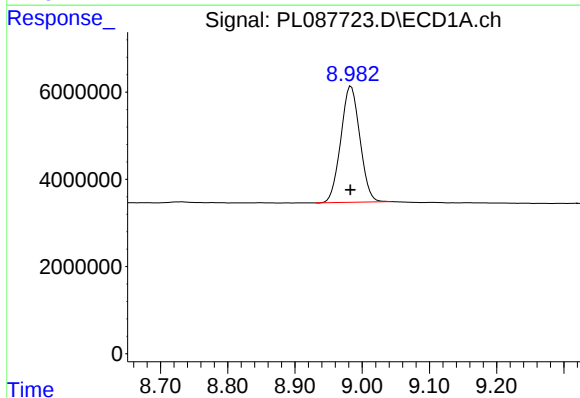

#28 Decachlorobiphenyl

R.T.: 8.983 min
Delta R.T.: 0.000 min
Response: 52433632
Conc: 18.41 ng/ml

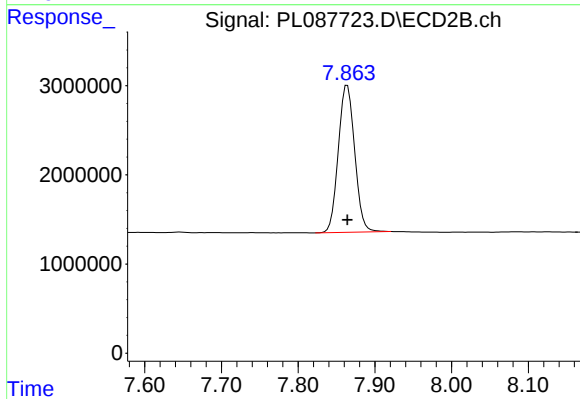

#28 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 24541239
Conc: 19.37 ng/ml