

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011119\
 Data File : PL043796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2019 14:23
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 01:22:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:21:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	4.008	265.8E6	95109298	50.000	50.000
28)	SA Decachlor...	8.249	9.080	278.4E6	77435145	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.391	5.005	111.8E6	44859429	500.000	500.000
24)	Chlordane-2	4.891	5.473	121.6E6	46424975	500.000	500.000
25)	Chlordane-3	5.457	6.119	363.1E6	153.2E6	500.000	500.000
26)	Chlordane-4	5.514	6.194	318.6E6	182.8E6	500.000	500.000
27)	Chlordane-5	6.348	6.998	99628741	34766646	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011119\
Data File : PL043796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2019 14:23
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 01:22:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:21:47 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

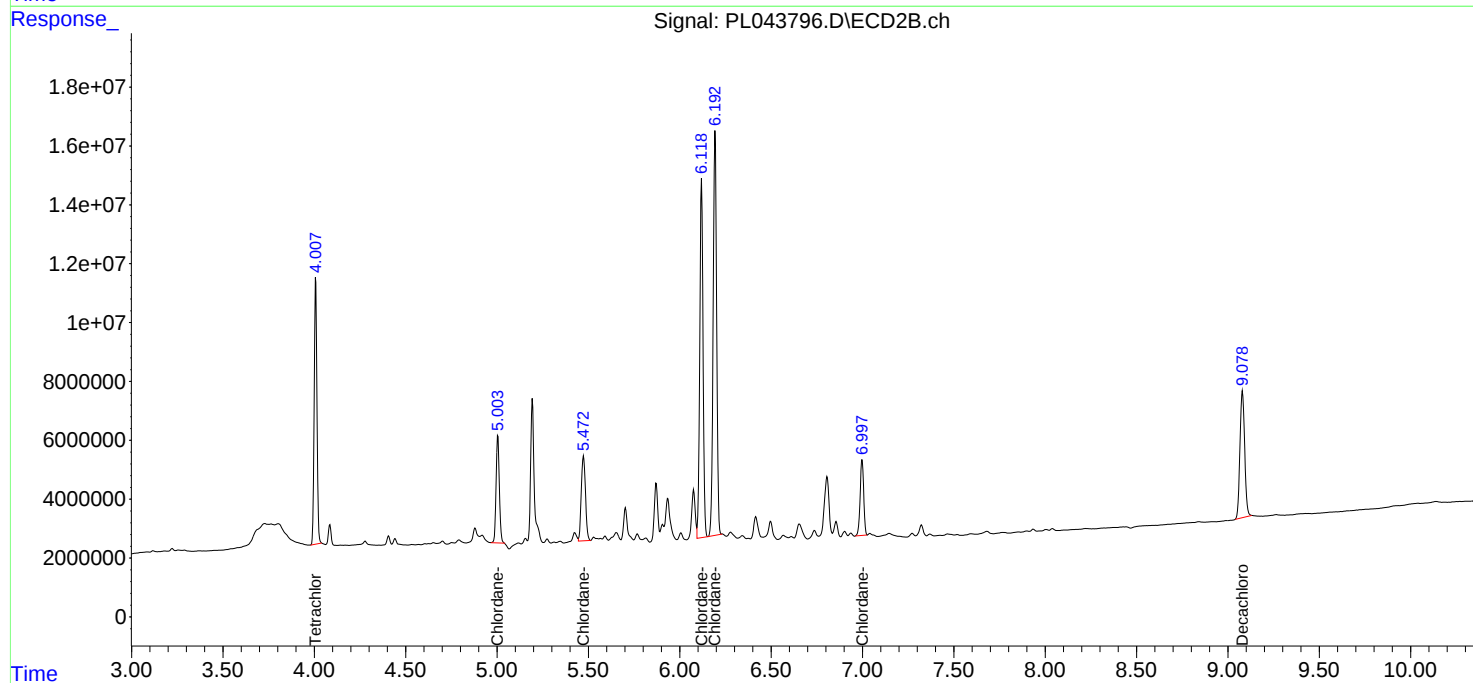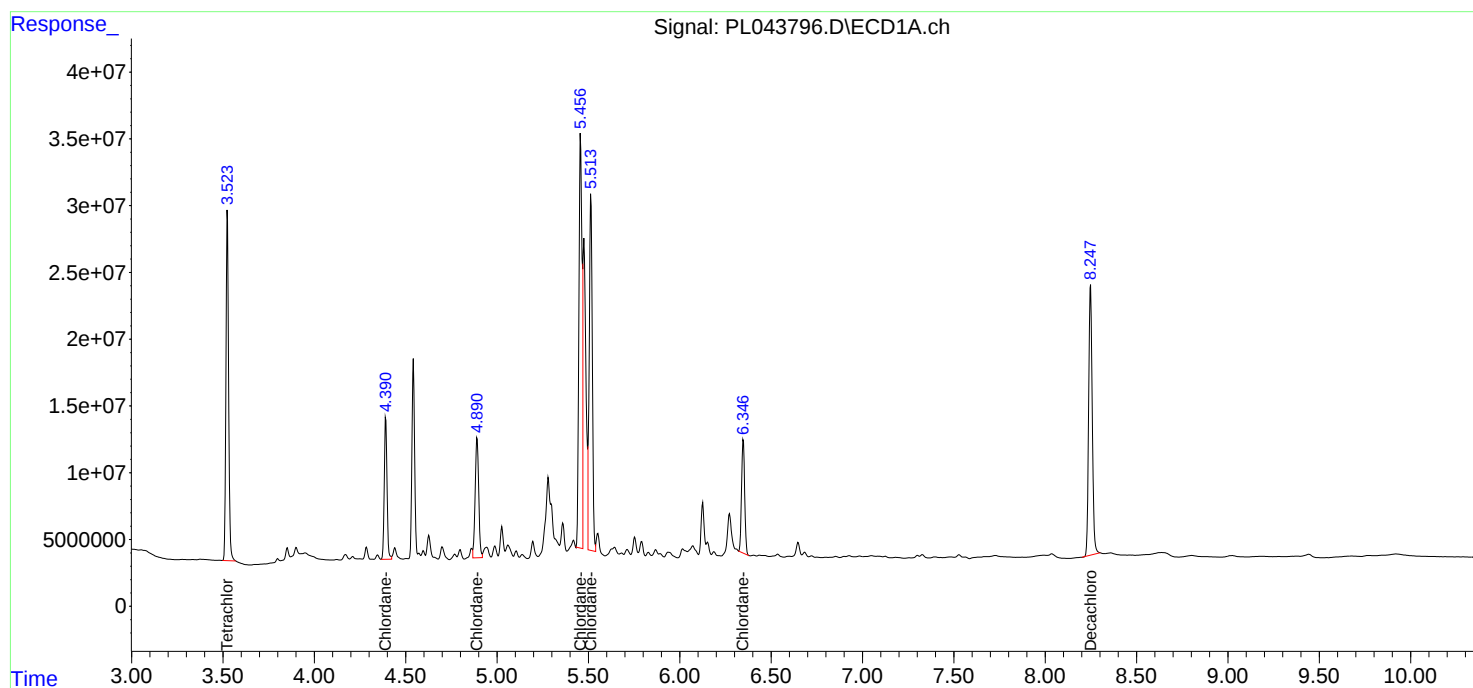


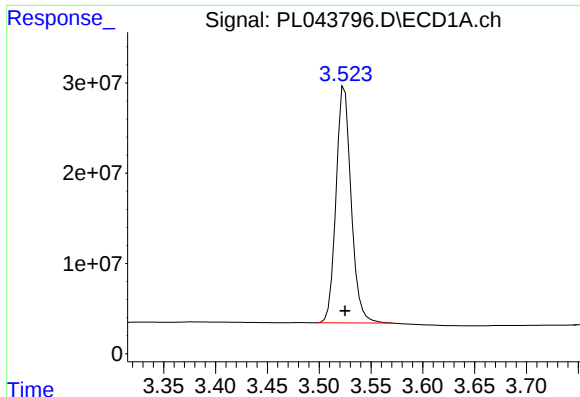

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 265765730
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

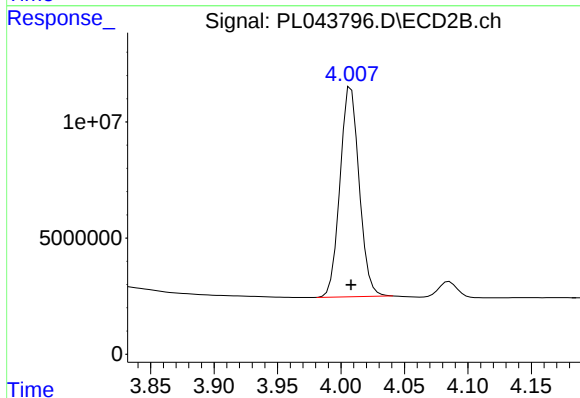


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 95109298
Conc: 50.00 ng/ml

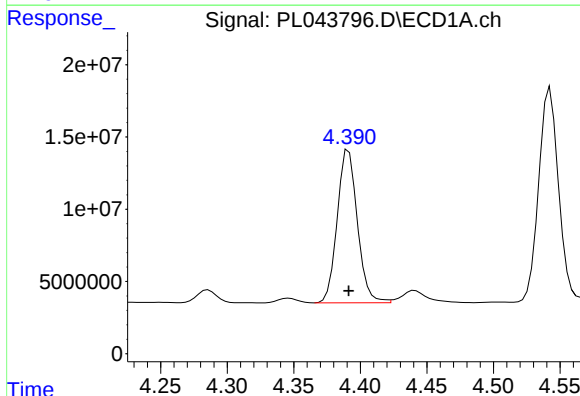


#23 Chlordane-1

R.T.: 4.391 min
Delta R.T.: 0.000 min
Response: 111842843
Conc: 500.00 ng/ml

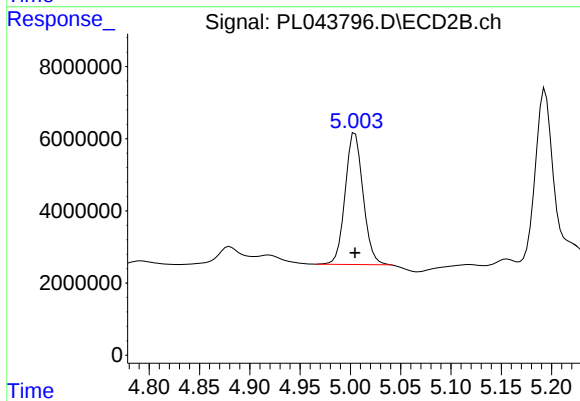

#23 Chlordane-1


R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 44859429
Conc: 500.00 ng/ml

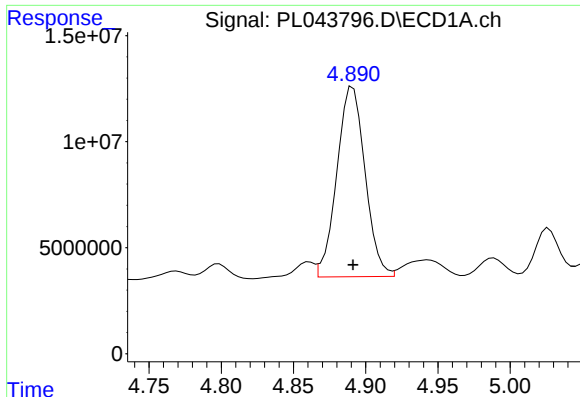

#24 Chlordane-2


R.T.: 4.891 min
Delta R.T.: 0.000 min
Response: 121633411
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

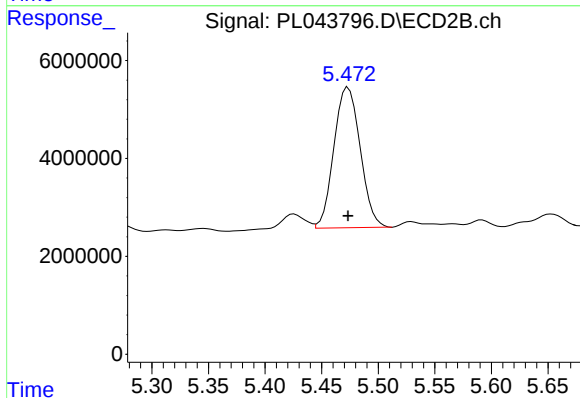


#24 Chlordane-2

R.T.: 5.473 min
Delta R.T.: 0.000 min
Response: 46424975
Conc: 500.00 ng/ml

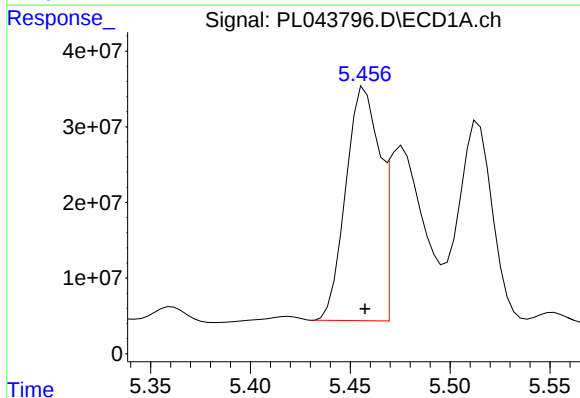


#25 Chlordane-3

R.T.: 5.457 min
Delta R.T.: 0.000 min
Response: 363076012
Conc: 500.00 ng/ml

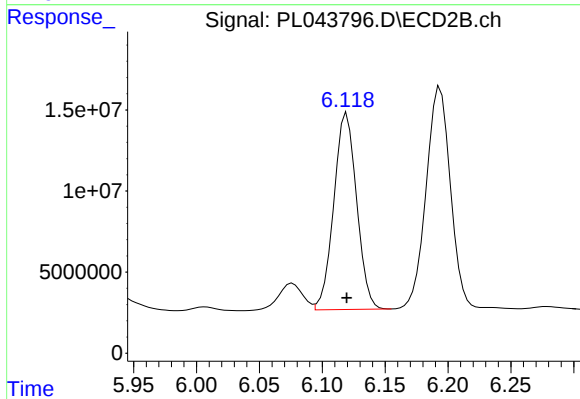

#25 Chlordane-3


R.T.: 6.119 min
Delta R.T.: 0.000 min
Response: 153169054
Conc: 500.00 ng/ml

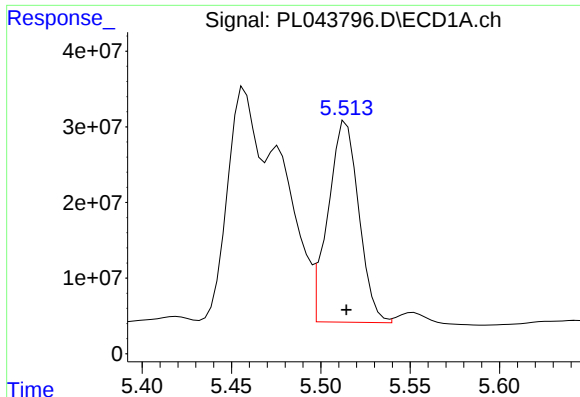

#26 Chlordane-4


R.T.: 5.514 min
Delta R.T.: 0.000 min
Response: 318636276
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

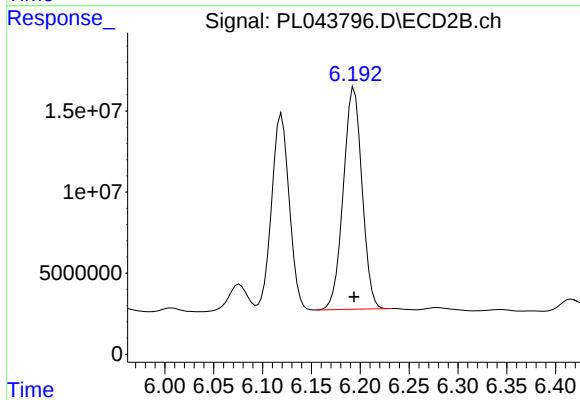


#26 Chlordane-4

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 182788965
Conc: 500.00 ng/ml

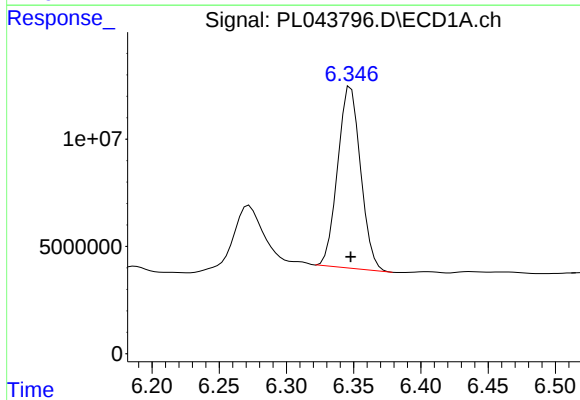


#27 Chlordane-5

R.T.: 6.348 min
Delta R.T.: 0.000 min
Response: 99628741
Conc: 500.00 ng/ml

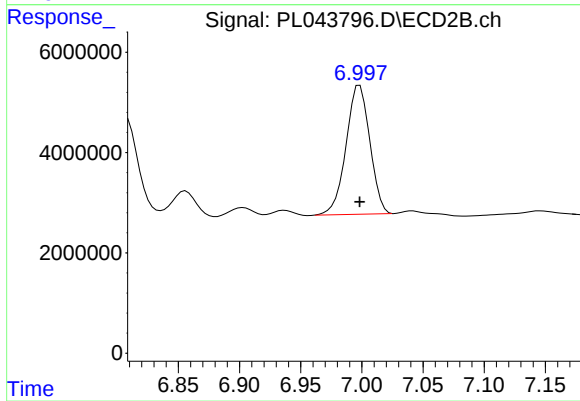

#27 Chlordane-5


R.T.: 6.998 min
Delta R.T.: 0.000 min
Response: 34766646
Conc: 500.00 ng/ml

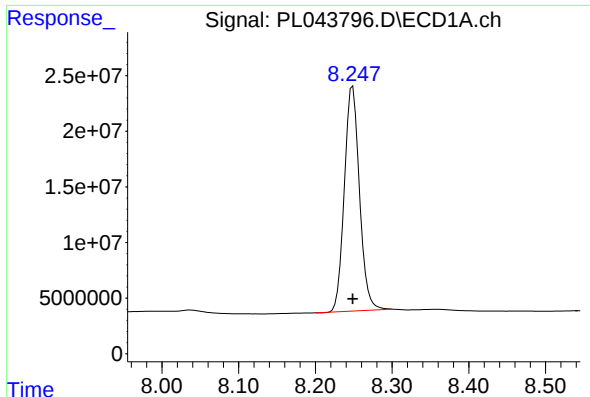

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 278350319
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

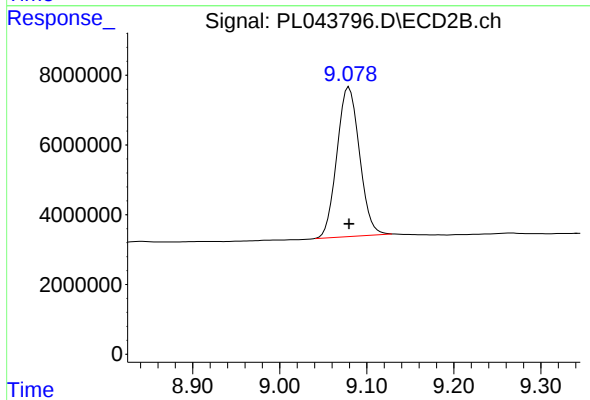

#28 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: 0.000 min
Response: 77435145
Conc: 50.00 ng/ml