

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011119\
 Data File : PL043846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2019 02:21
 Operator : AJ\SJ
 Sample : K1100-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 04:00:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	4.007	58295936	22772951	11.876	11.685
28)	SA Decachlor...	8.247	9.076	25726829	7583806	4.552	4.774
Target Compounds							
6)	B beta-BHC	4.453f	0.000	7534016	0	2.531	N.D. #
13)	MA Dieldrin	5.809	0.000	7477297	0	1.200	N.D. #
15)	B Endosulfa...	6.271f	0.000	26349339	0	5.065	N.D. #
16)	A 4,4'-DDD	0.000	6.797f	0	9087924	N.D.	6.014 #
23)	Chlordane-1	4.453	0.000	7534016	0	33.681	N.D. #
24)	Chlordane-2	4.854	0.000	4604543	0	18.928	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011119\
Data File : PL043846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2019 02:21
Operator : AJ\SJ
Sample : K1100-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 04:00:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

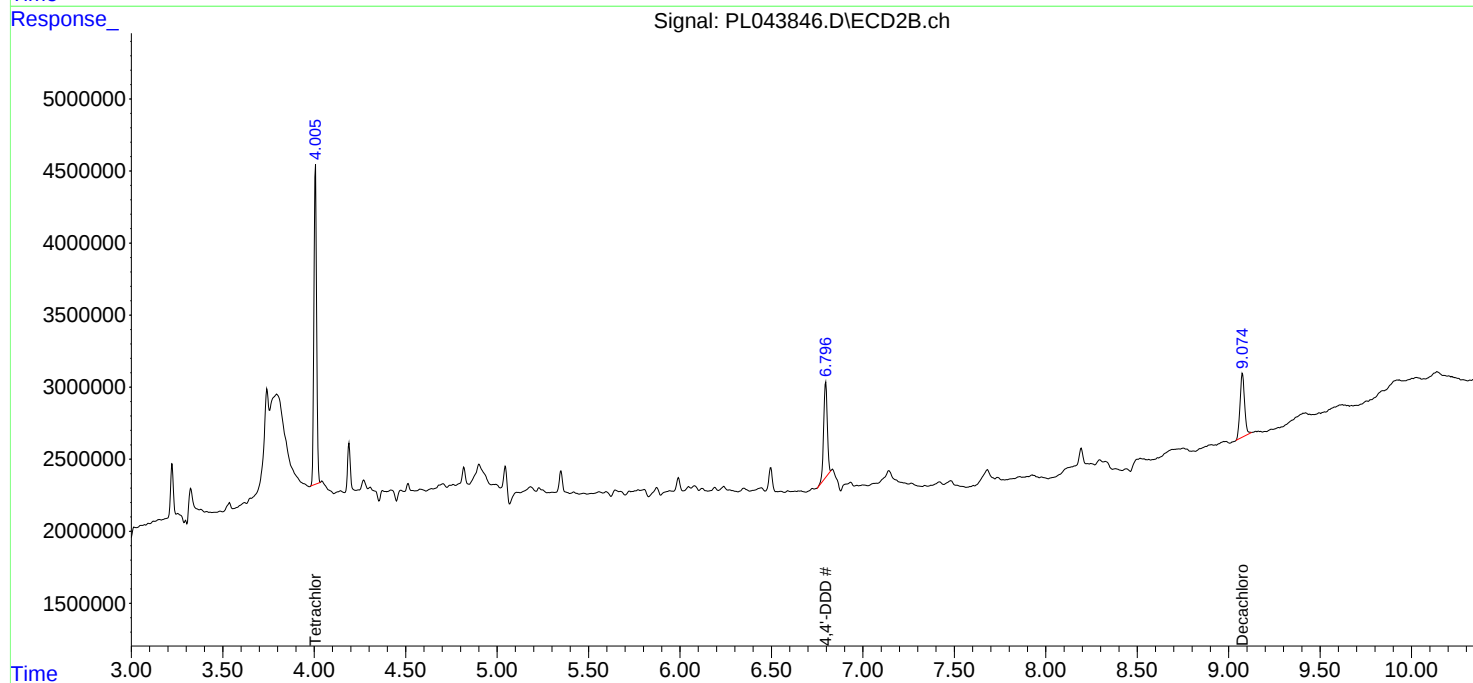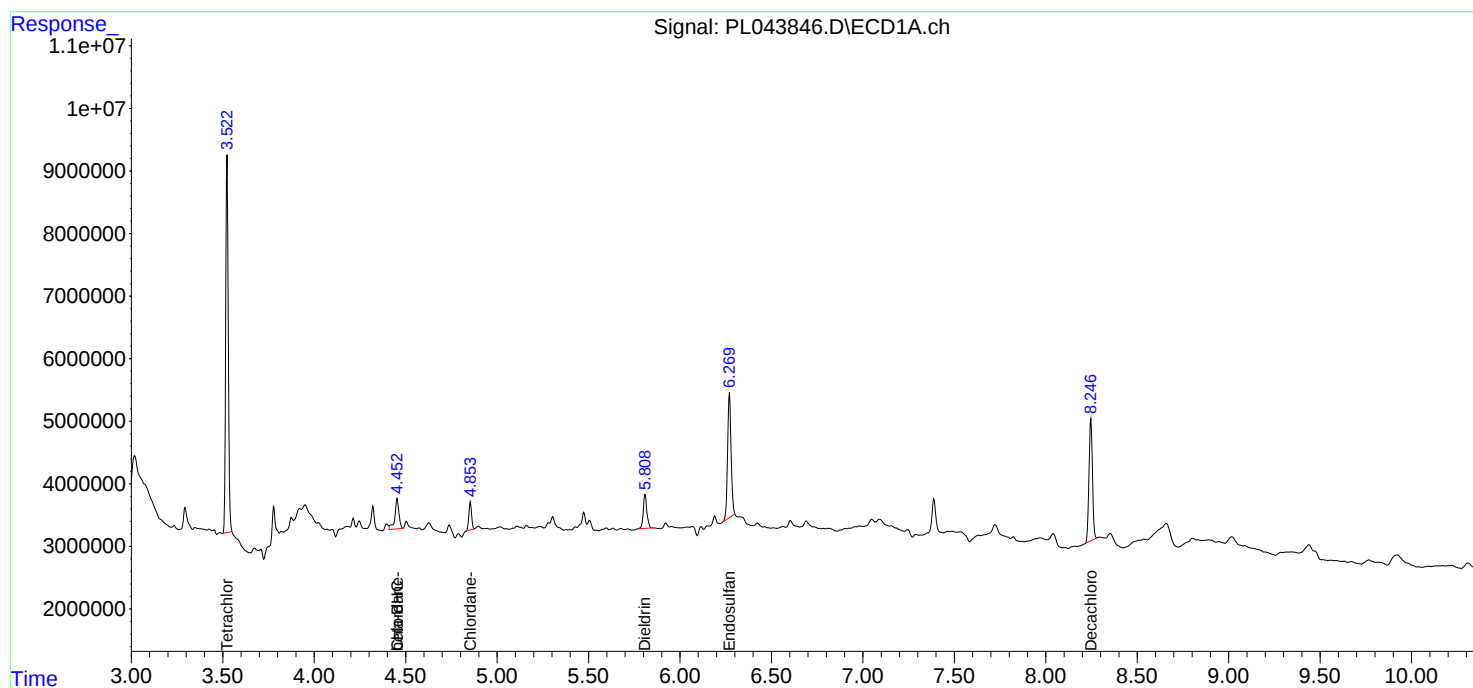


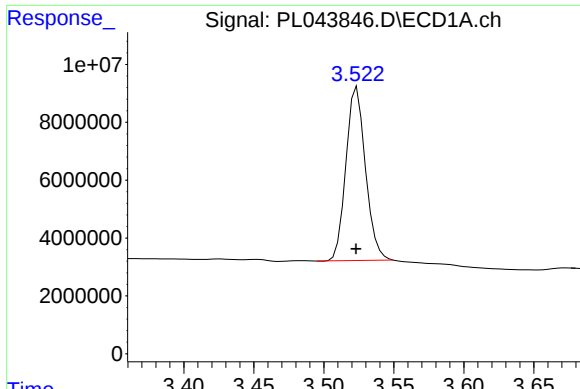

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 58295936
Conc: 11.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

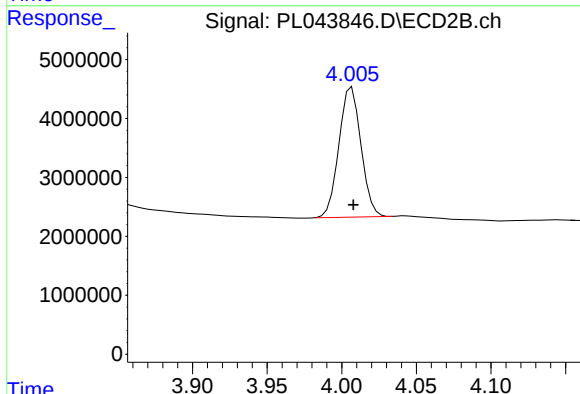


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 22772951
Conc: 11.69 ng/ml

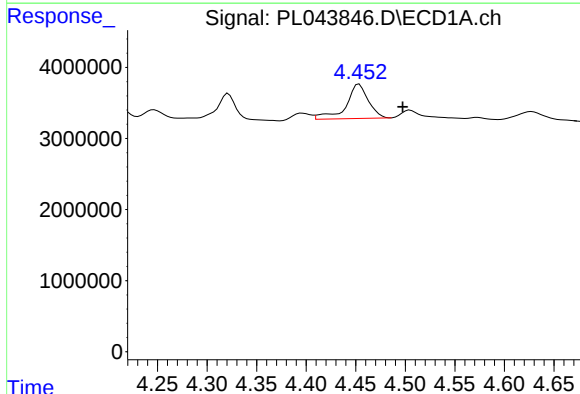


#6 beta-BHC

R.T.: 4.453 min
Delta R.T.: -0.044 min
Response: 7534016
Conc: 2.53 ng/ml

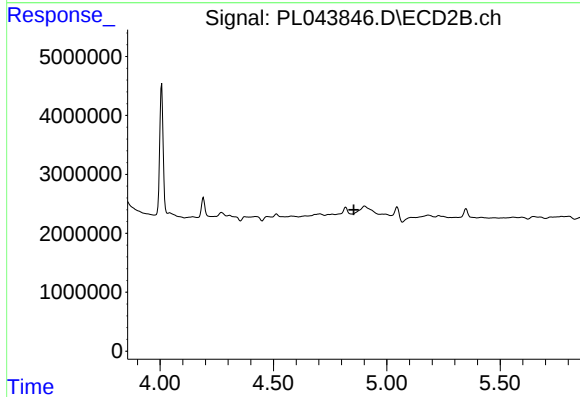

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

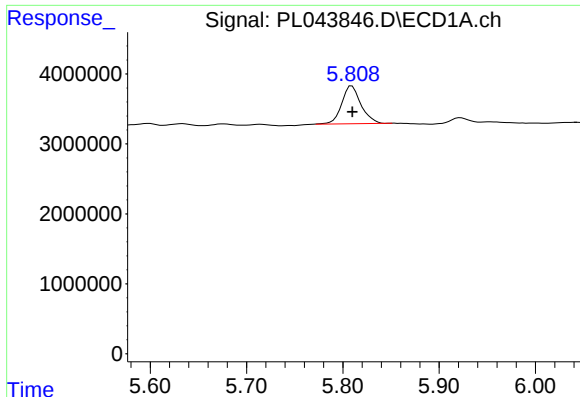

#13 Dieldrin


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 7477297
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

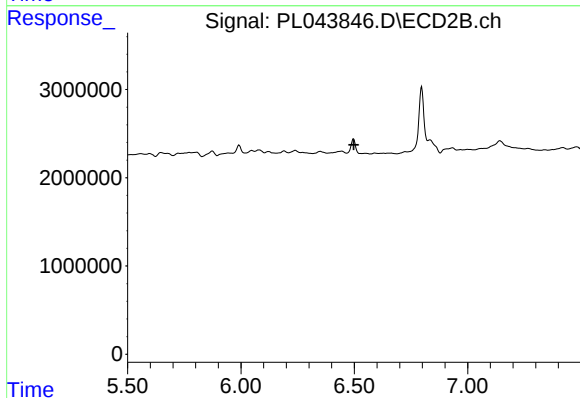


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.498 min
Response: 0
Conc: N.D.

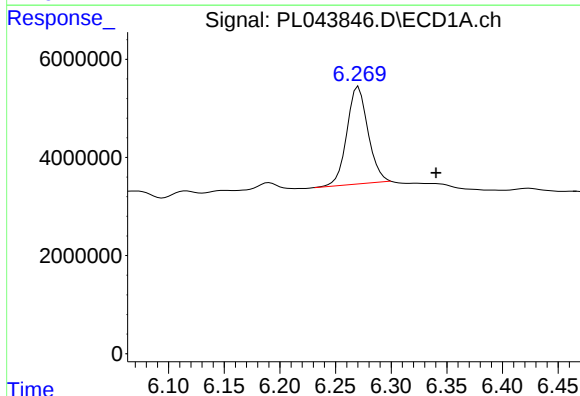


#15 Endosulfan II

R.T.: 6.271 min
Delta R.T.: -0.070 min
Response: 26349339
Conc: 5.06 ng/ml

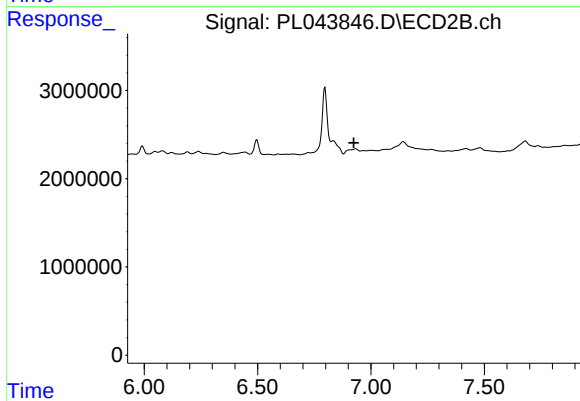

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

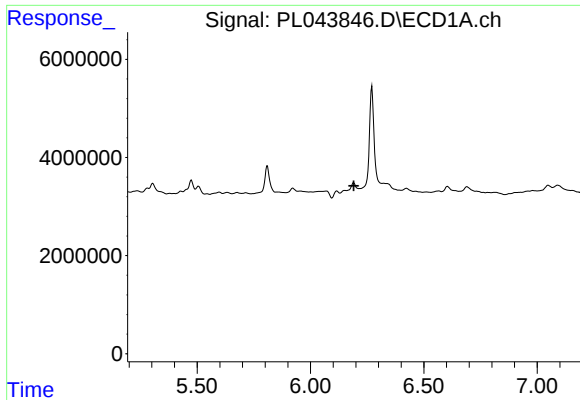

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

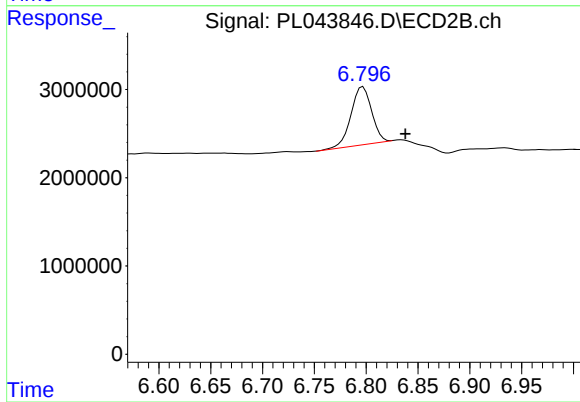


#16 4,4'-DDD

R.T.: 6.797 min
Delta R.T.: -0.041 min
Response: 9087924
Conc: 6.01 ng/ml

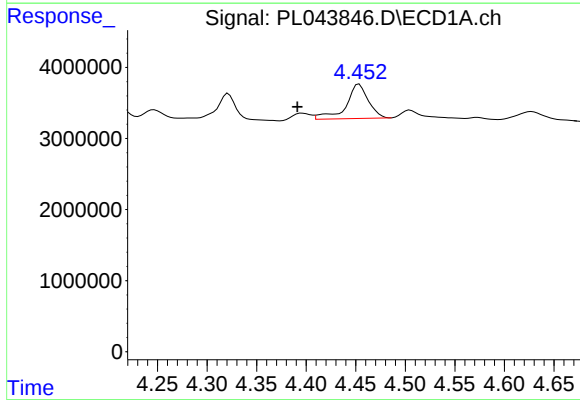


#23 Chlordane-1

R.T.: 4.453 min
Delta R.T.: 0.062 min
Response: 7534016
Conc: 33.68 ng/ml

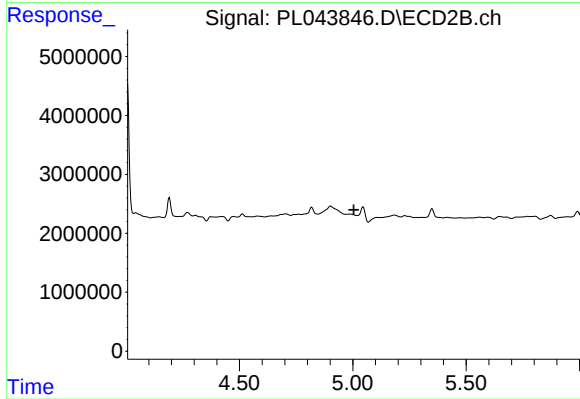

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.005 min
Response: 0
Conc: N.D.

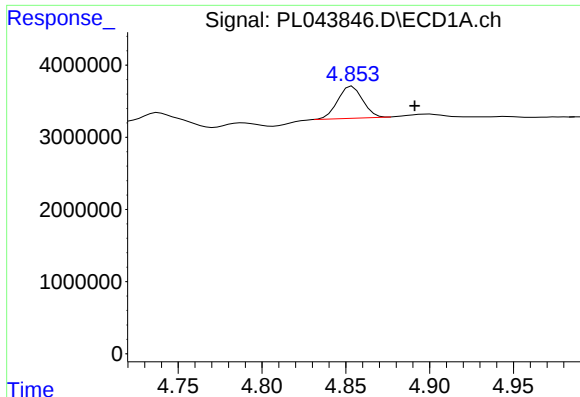

#24 Chlordane-2


R.T.: 4.854 min
Delta R.T.: -0.037 min
Response: 4604543
Conc: 18.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

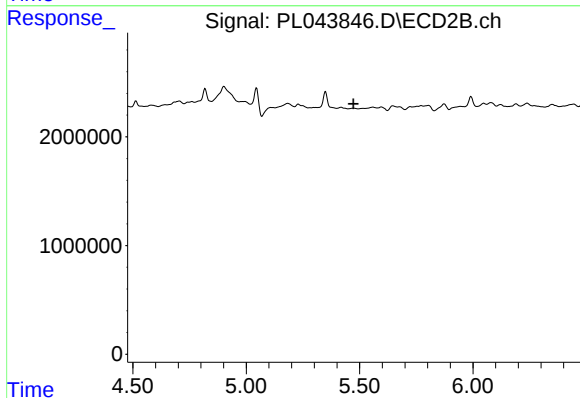


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.473 min
Response: 0
Conc: N.D.

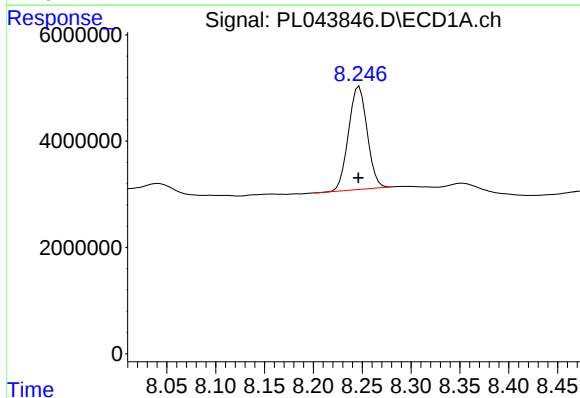

#28 Decachlorobiphenyl

R.T.: 8.247 min
Delta R.T.: 0.000 min
Response: 25726829
Conc: 4.55 ng/ml

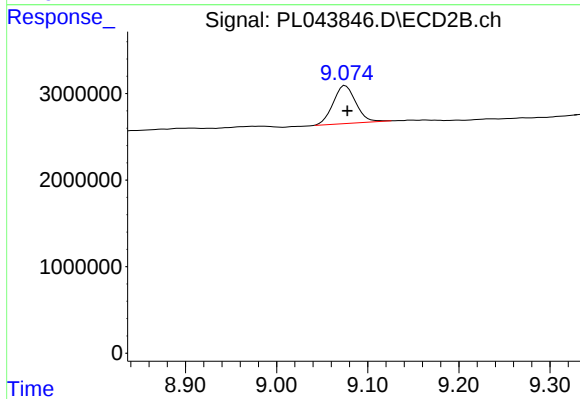

#28 Decachlorobiphenyl

R.T.: 9.076 min
Delta R.T.: -0.002 min
Response: 7583806
Conc: 4.77 ng/ml