

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011119\
 Data File : PL043851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2019 03:31
 Operator : AJ\SJ
 Sample : K1119-01
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 05:29:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	4.007	46725827	18774341	9.519	9.634
28)	SA Decachlor...	8.246	9.076	71634178	19772964	12.676	12.447
Target Compounds							
6)	B beta-BHC	4.451f	0.000	6410197	0	2.153	N.D. #
8)	B Heptachlo...	5.282f	0.000	5421521	0	0.853	N.D. #
12)	B 4,4'-DDE	5.676	0.000	3824027	0	0.706	N.D. #
13)	MA Dieldrin	5.802	0.000	10806949	0	1.735	N.D. #
14)	MA Endrin	6.026f	0.000	2201327	0	0.406	N.D. #
16)	A 4,4'-DDD	0.000	6.797f	0	8671713	N.D.	5.739 #
17)	MA 4,4'-DDT	6.424	0.000	23458876	0	5.143	N.D. #
23)	Chlordane-1	4.451	0.000	6410197	0	28.657	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011119\
Data File : PL043851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2019 03:31
Operator : AJ\SJ
Sample : K1119-01
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 05:29:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

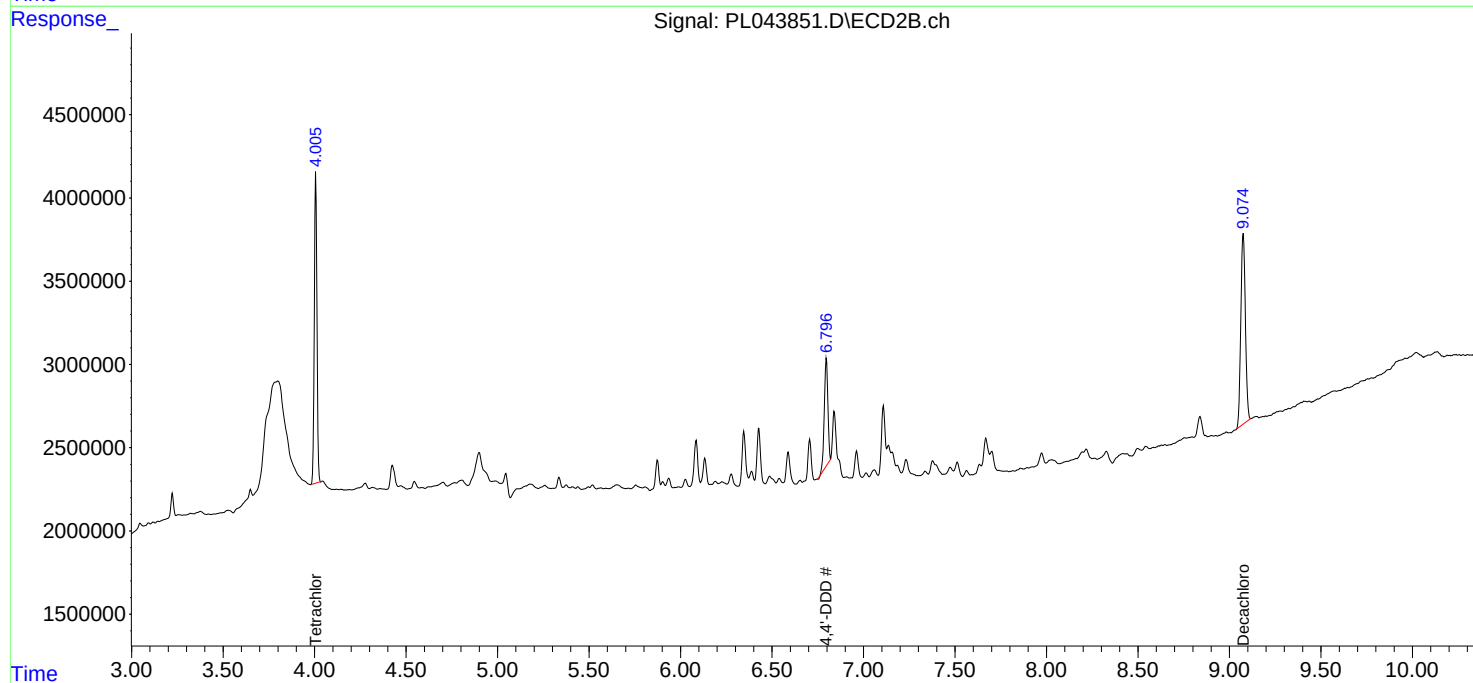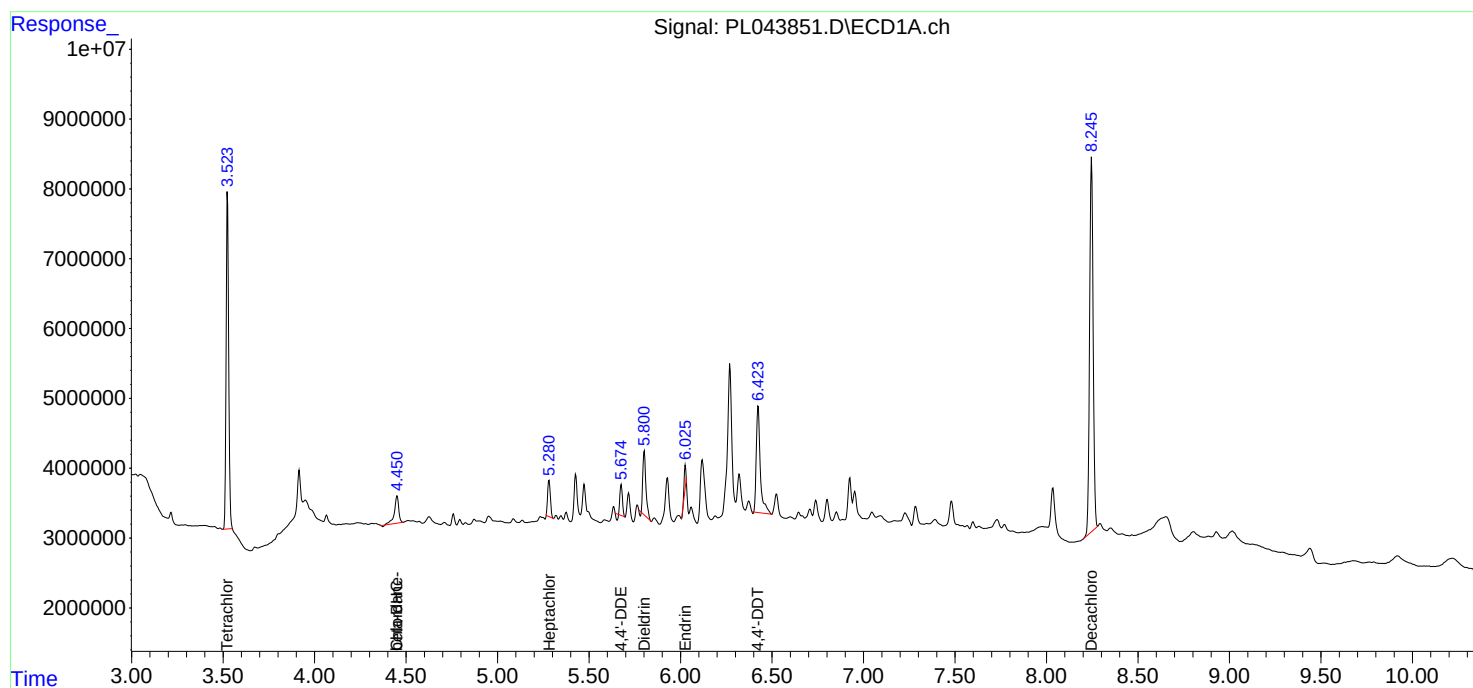


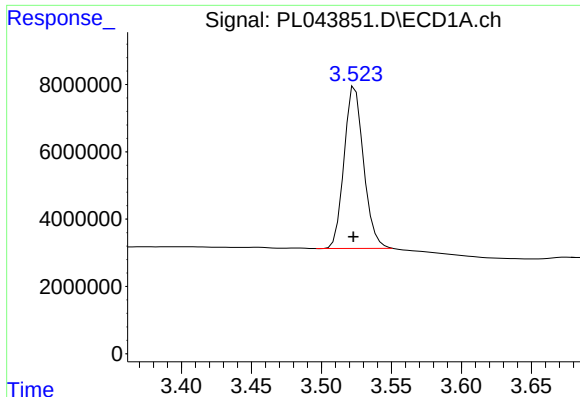

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.001 min
Response: 46725827
Conc: 9.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

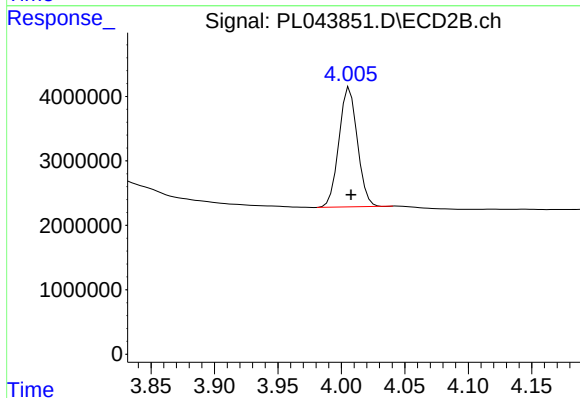


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.001 min
Response: 18774341
Conc: 9.63 ng/ml

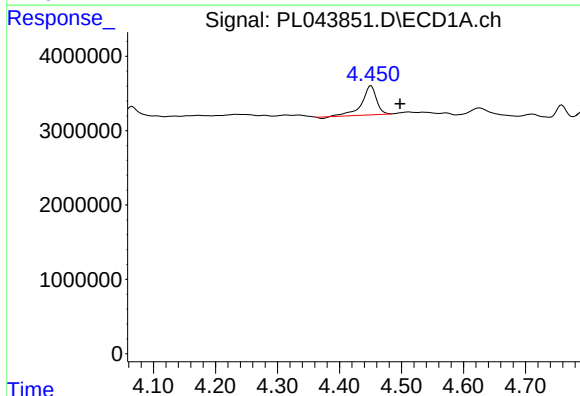


#6 beta-BHC

R.T.: 4.451 min
Delta R.T.: -0.046 min
Response: 6410197
Conc: 2.15 ng/ml

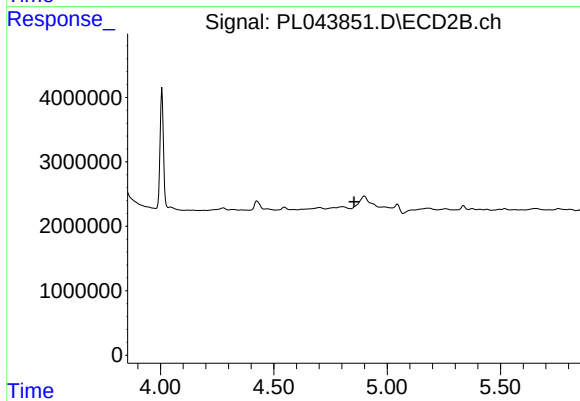

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.855 min
Response: 0
Conc: N.D.

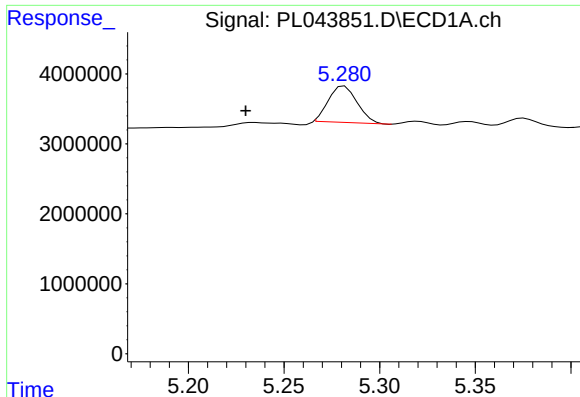

#8 Heptachlor epoxide


R.T.: 5.282 min
Delta R.T.: 0.052 min
Response: 5421521
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

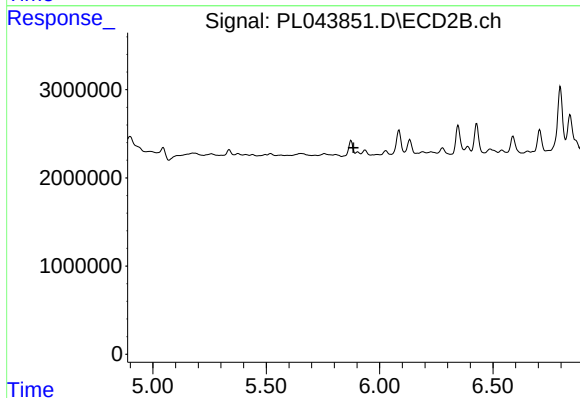


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.885 min
Response: 0
Conc: N.D.

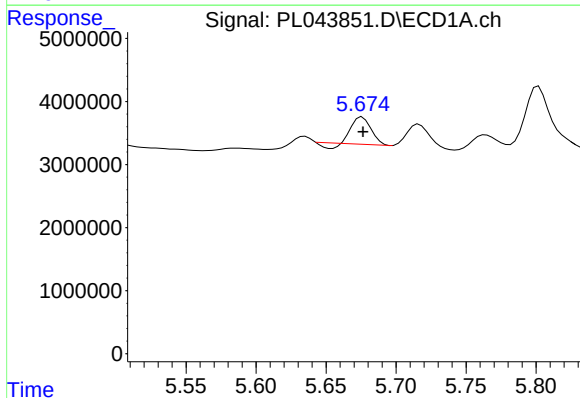


#12 4,4'-DDE

R.T.: 5.676 min
Delta R.T.: 0.000 min
Response: 3824027
Conc: 0.71 ng/ml

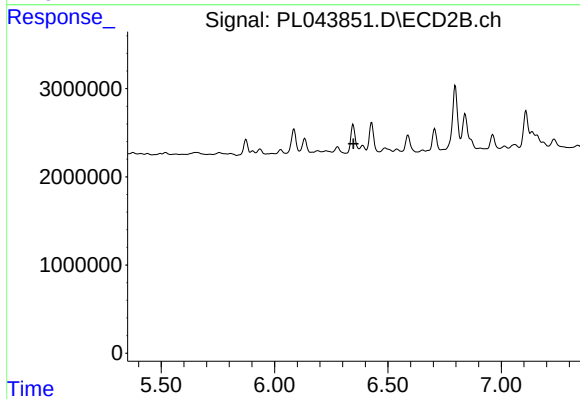

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.348 min
Response: 0
Conc: N.D.

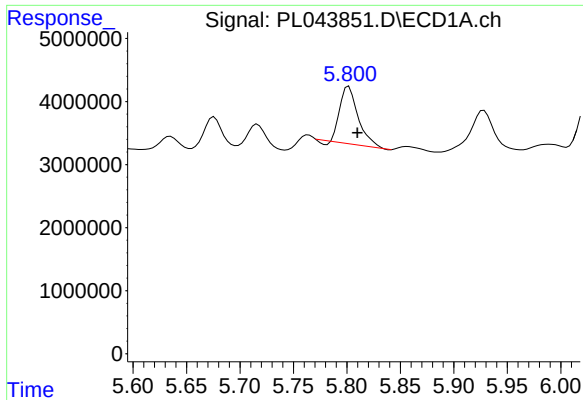

#13 Dieldrin


R.T.: 5.802 min
Delta R.T.: -0.008 min
Response: 10806949
Conc: 1.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

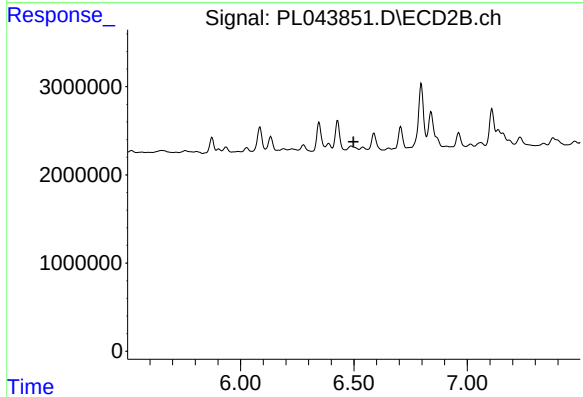


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.498 min
Response: 0
Conc: N.D.

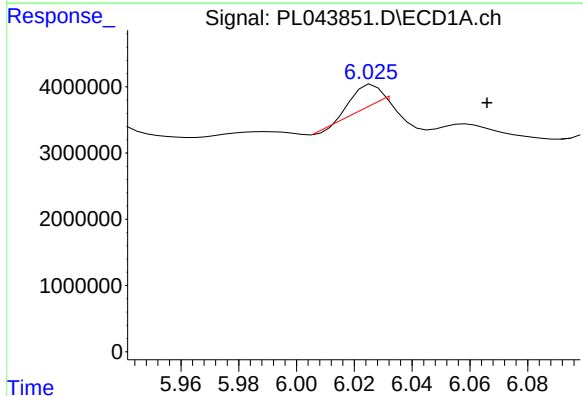


#14 Endrin

R.T.: 6.026 min
Delta R.T.: -0.039 min
Response: 2201327
Conc: 0.41 ng/ml

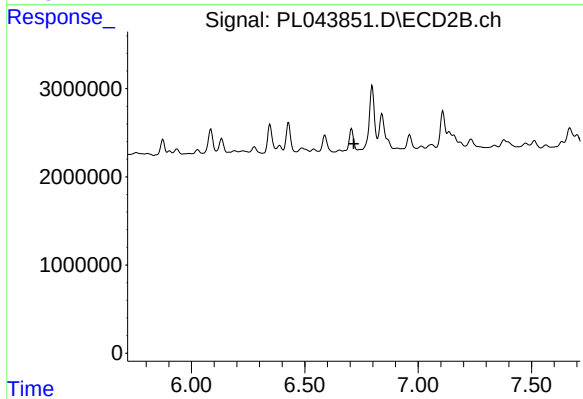

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.716 min
Response: 0
Conc: N.D.

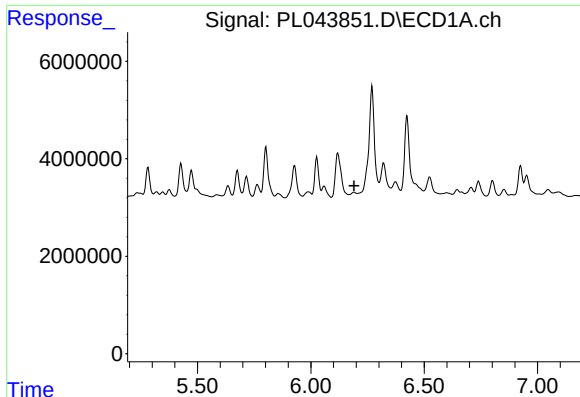

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

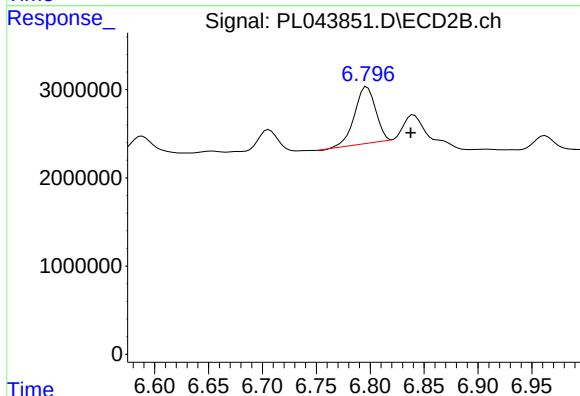


#16 4,4'-DDD

R.T.: 6.797 min
Delta R.T.: -0.041 min
Response: 8671713
Conc: 5.74 ng/ml

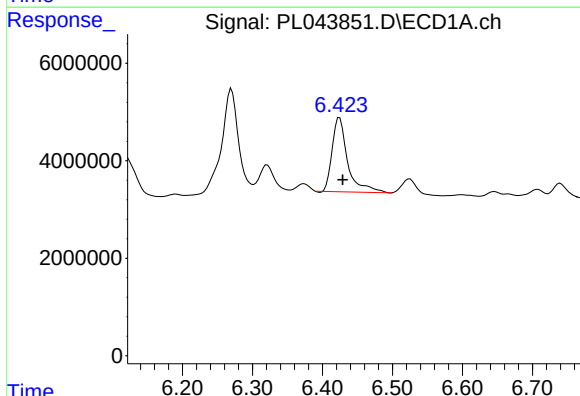


#17 4,4'-DDT

R.T.: 6.424 min
Delta R.T.: -0.005 min
Response: 23458876
Conc: 5.14 ng/ml

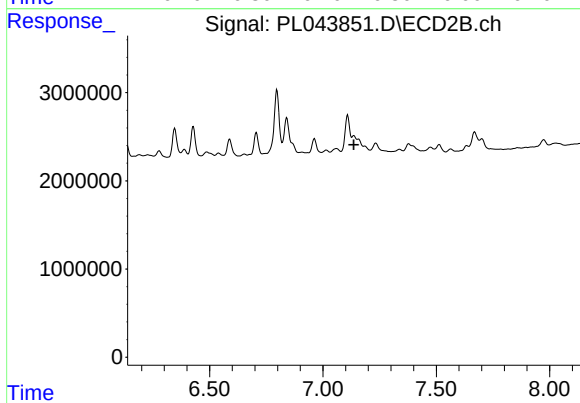

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.136 min
Response: 0
Conc: N.D.

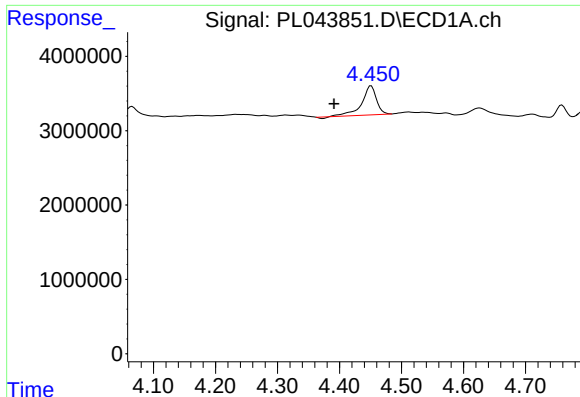

#23 Chlordane-1


R.T.: 4.451 min
Delta R.T.: 0.060 min
Response: 6410197
Conc: 28.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

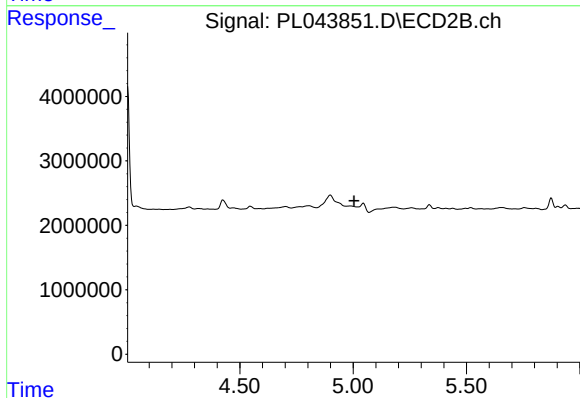


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.005 min
Response: 0
Conc: N.D.

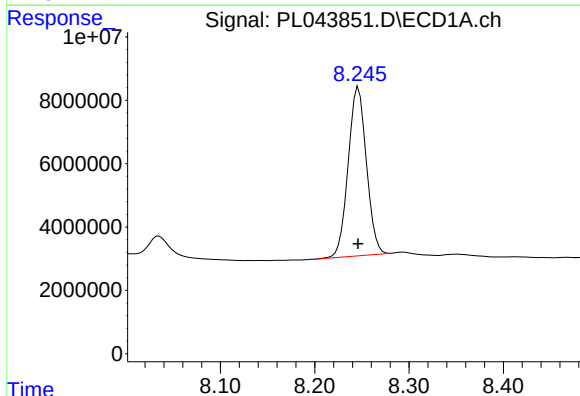

#28 Decachlorobiphenyl

R.T.: 8.246 min
Delta R.T.: 0.000 min
Response: 71634178
Conc: 12.68 ng/ml

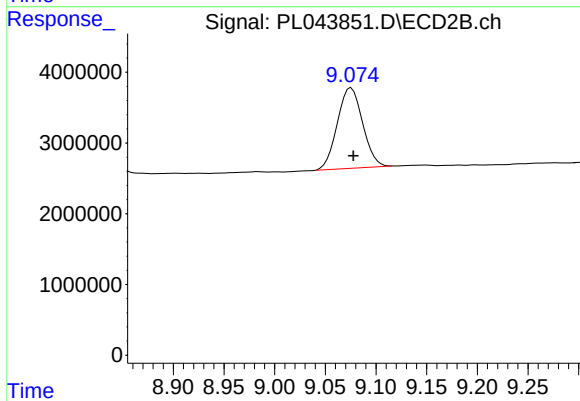

#28 Decachlorobiphenyl

R.T.: 9.076 min
Delta R.T.: -0.002 min
Response: 19772964
Conc: 12.45 ng/ml