

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011119\
 Data File : PL043841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2019 01:10
 Operator : AJ\SJ
 Sample : K1011-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-011019-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 03:59:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 12 01:24:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	4.007	102.9E6	35849666	20.970	18.395
28)	SA Decachlor...	8.246	9.076	103.5E6	31353050	18.307	19.737

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011119\
Data File : PL043841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2019 01:10
Operator : AJ\SJ
Sample : K1011-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-02-011019-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 03:59:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011119.M
Quant Title : GC Extractables
QLast Update : Sat Jan 12 01:24:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

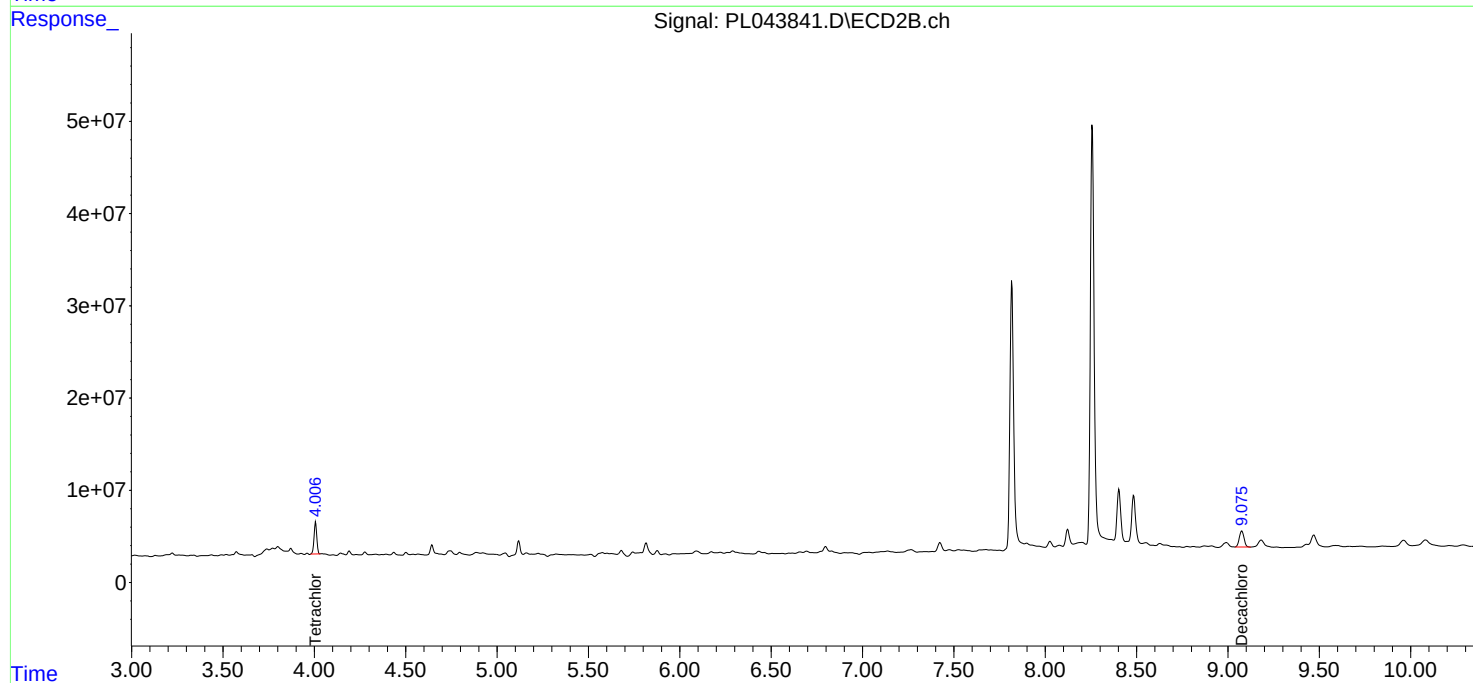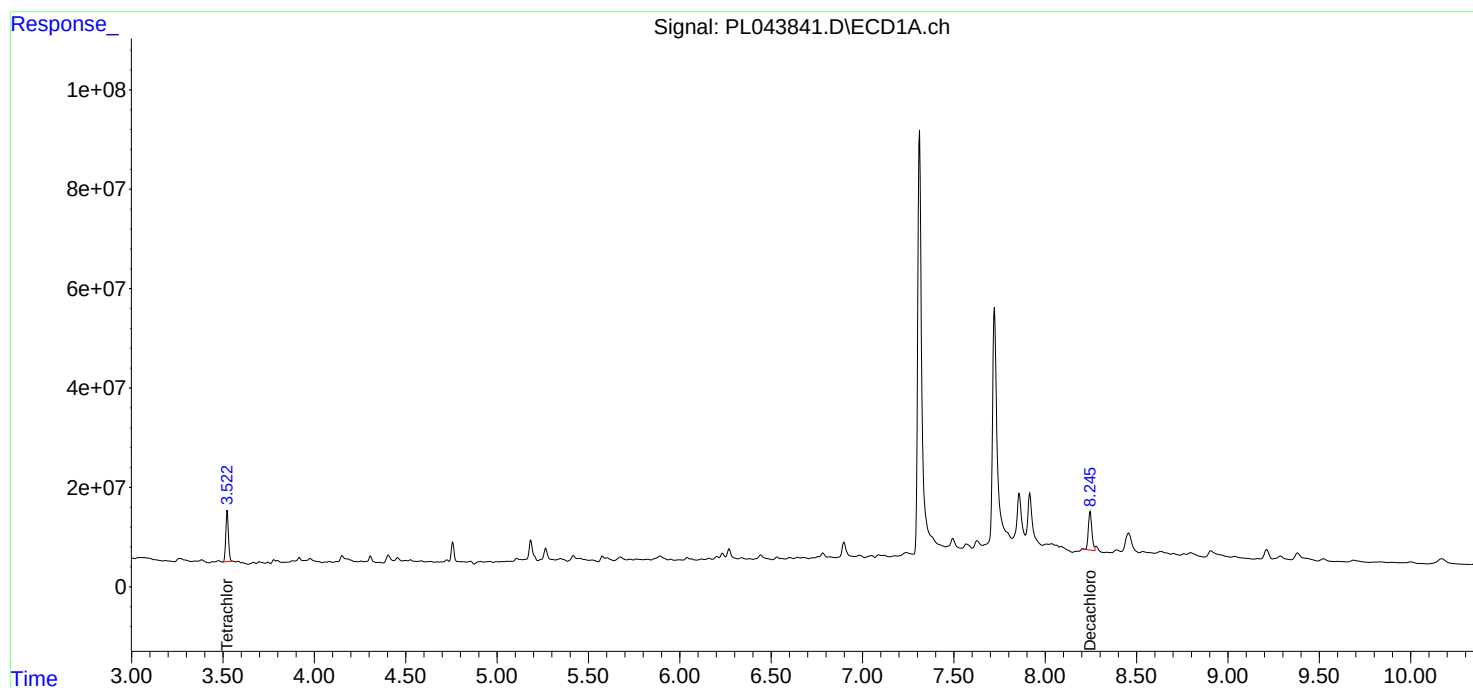


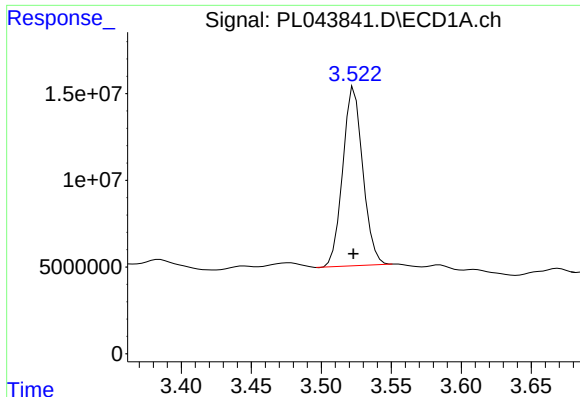

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 102936843
Conc: 20.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-011019-A

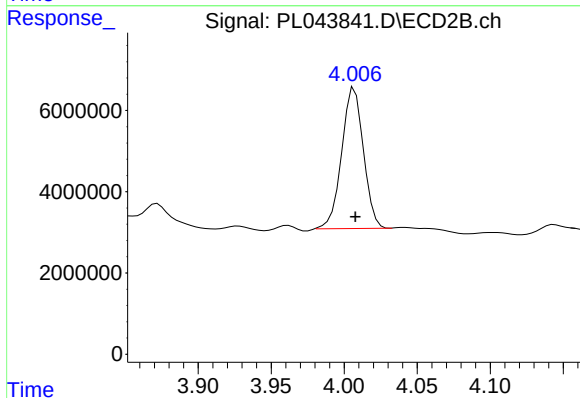


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 35849666
Conc: 18.40 ng/ml

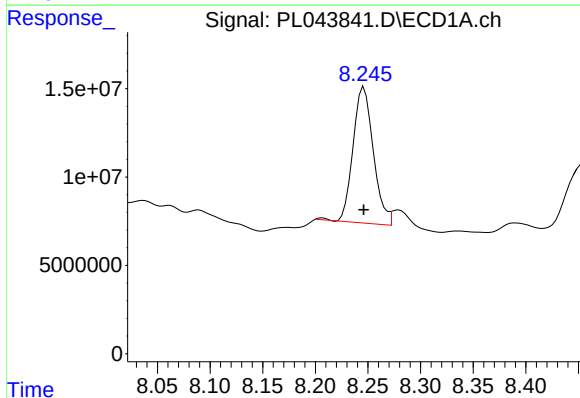

#28 Decachlorobiphenyl

R.T.: 8.246 min
Delta R.T.: 0.000 min
Response: 103454875
Conc: 18.31 ng/ml

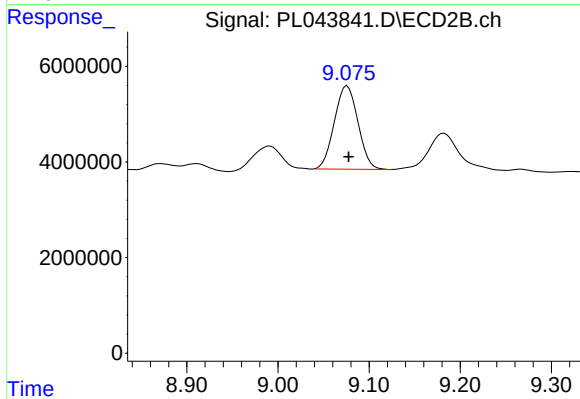

#28 Decachlorobiphenyl

R.T.: 9.076 min
Delta R.T.: -0.002 min
Response: 31353050
Conc: 19.74 ng/ml