

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011120\
 Data File : PL055684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2020 17:44
 Operator : AJ\MA
 Sample : L1065-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 22:01:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	3.968	211.1E6	68798262	22.840	25.970
28)	SA Decachlor...	8.236	8.954	214.6E6	51009922	24.435	24.535
Target Compounds							
4)	MA Heptachlor	4.513	0.000	52047021	0	3.638	N.D. #
5)	MB Aldrin	4.782f	0.000	29198119	0	2.081	N.D. #
7)	B delta-BHC	4.687f	4.988f	2141385	14323484	0.150	4.667 #
11)	B alpha-Chl...	5.464f	0.000	97806165	0	7.449	N.D. #
15)	B Endosulfa...	6.323	0.000	17562552	0	1.628	N.D. #
23)	Chlordane-1	4.358	0.000	37343344	0	107.966	N.D. #
24)	Chlordane-2	4.853	0.000	33784498	0	83.067	N.D. #
26)	Chlordane-4	5.464f	0.000	97806165	0	100.173	N.D. #
27)	Chlordane-5	6.323	0.000	17562552	0	48.788	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011120\
Data File : PL055684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2020 17:44
Operator : AJ\MA
Sample : L1065-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 22:01:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

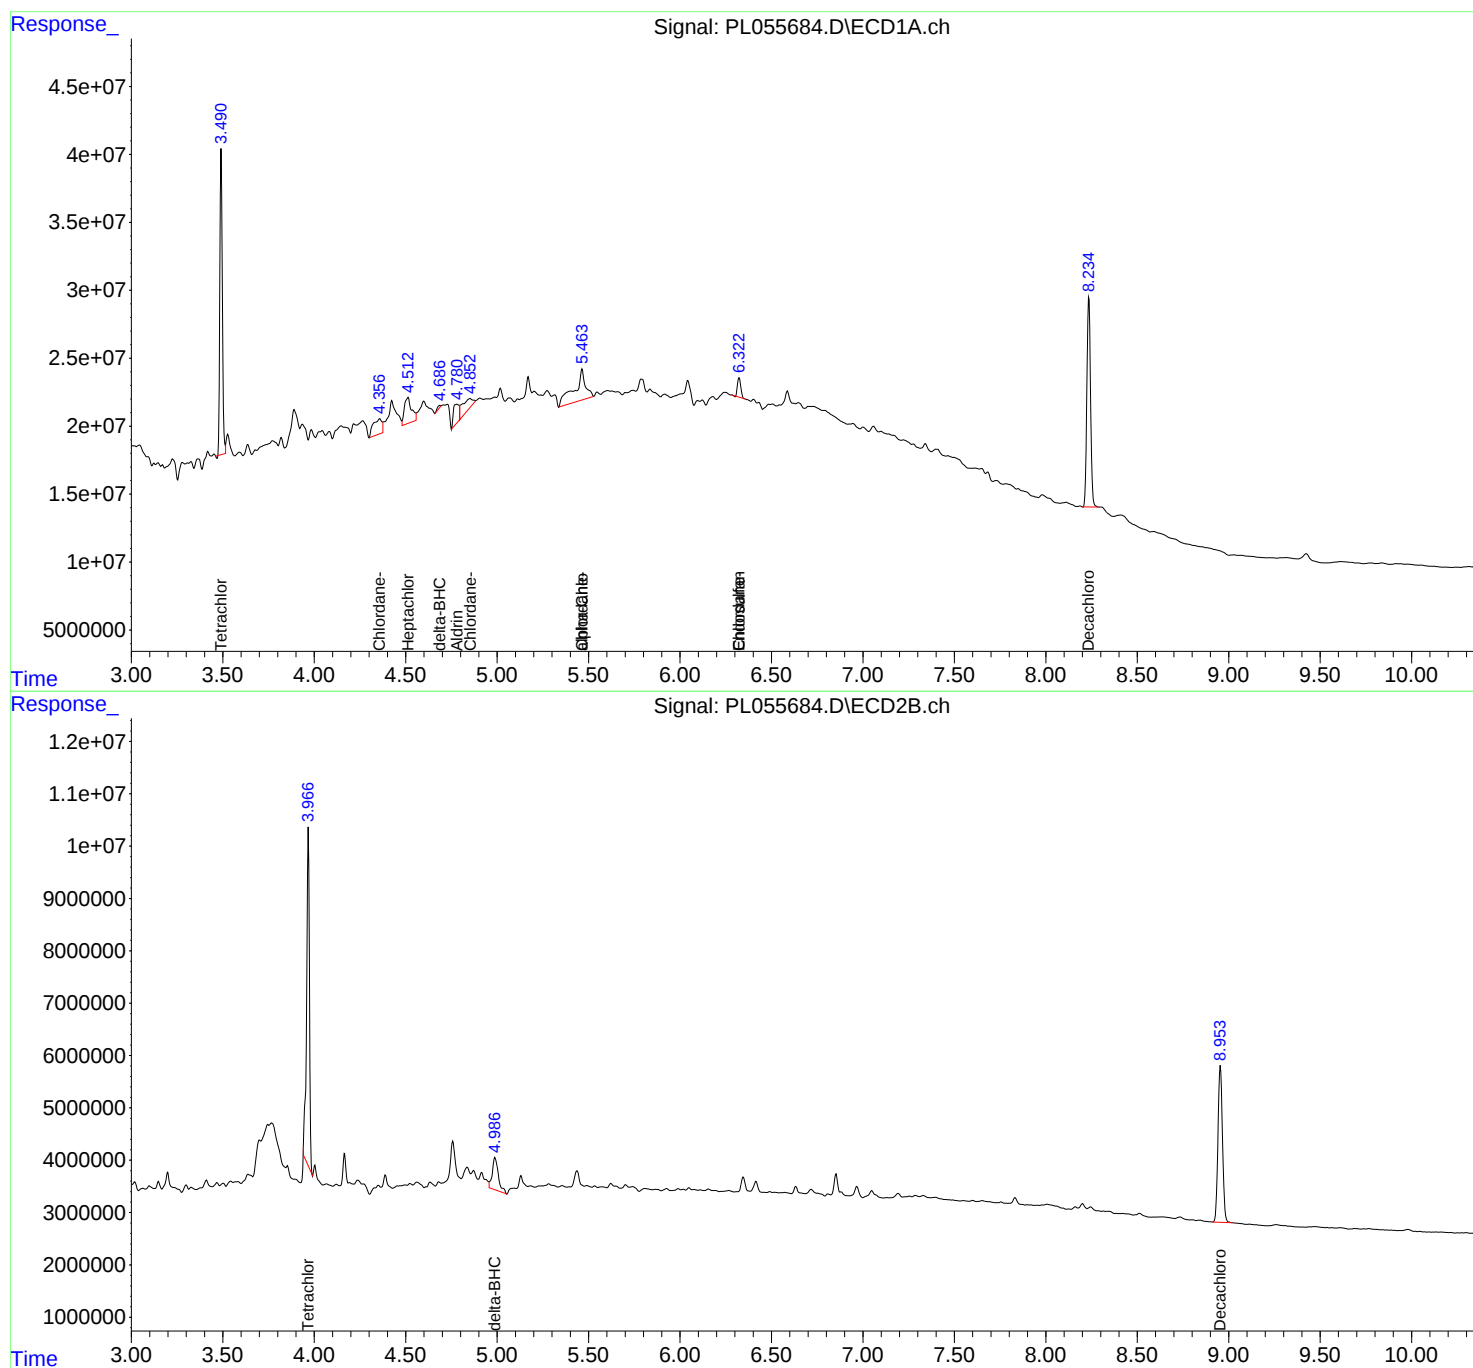


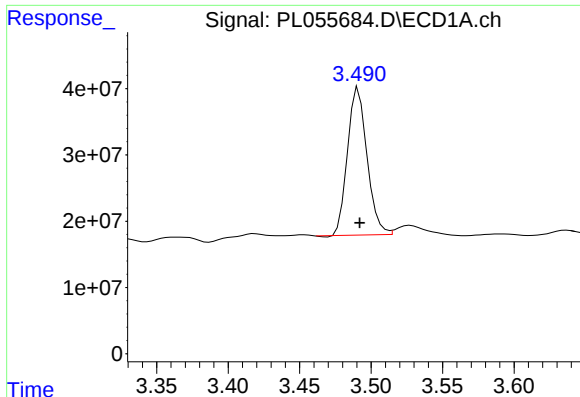

#1 Tetrachloro-m-xylene


R.T.: 3.491 min
Delta R.T.: 0.000 min
Response: 211060922
Conc: 22.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

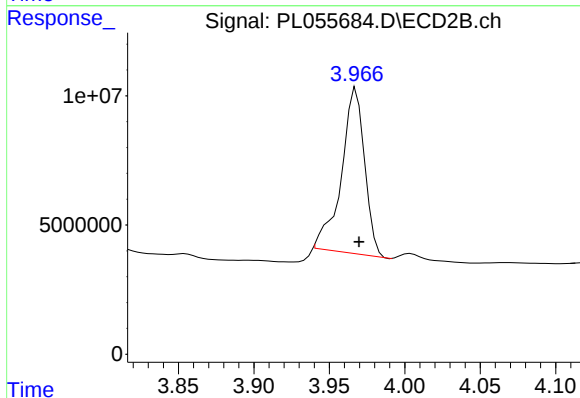


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 68798262
Conc: 25.97 ng/ml

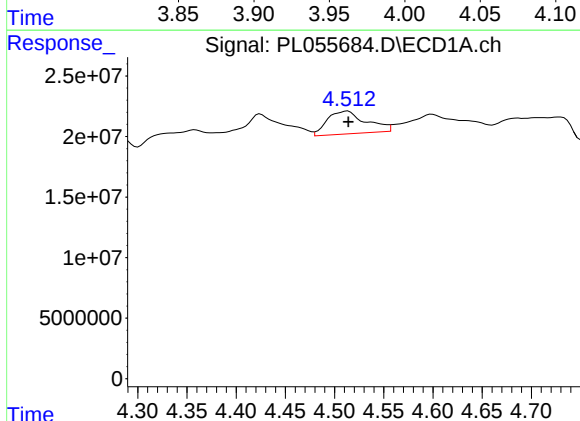


#4 Heptachlor

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 52047021
Conc: 3.64 ng/ml

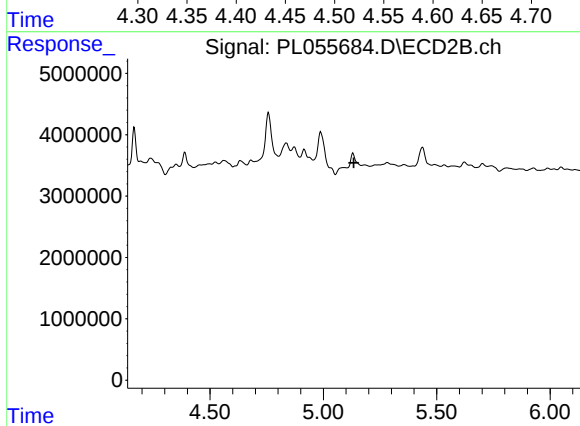

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.134 min
Response: 0
Conc: N.D.

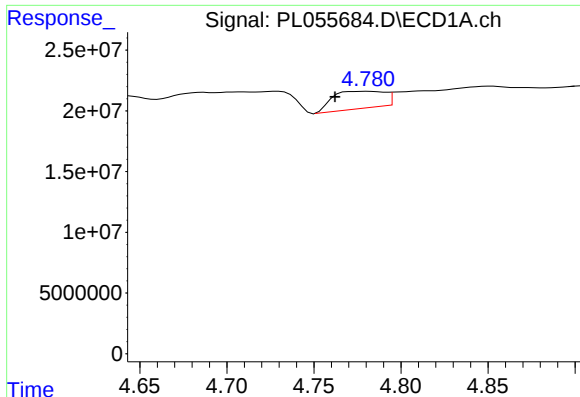

#5 Aldrin


R.T.: 4.782 min
Delta R.T.: 0.019 min
Response: 29198119
Conc: 2.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

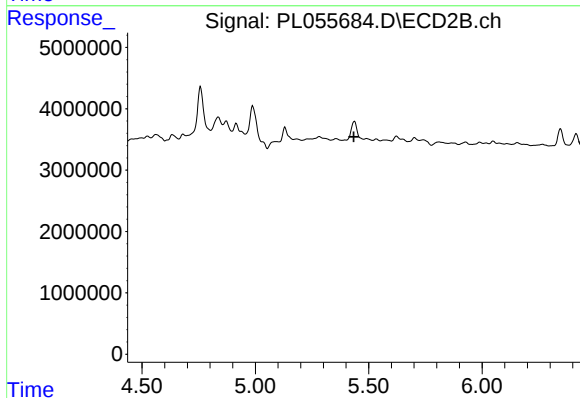


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.435 min
Response: 0
Conc: N.D.

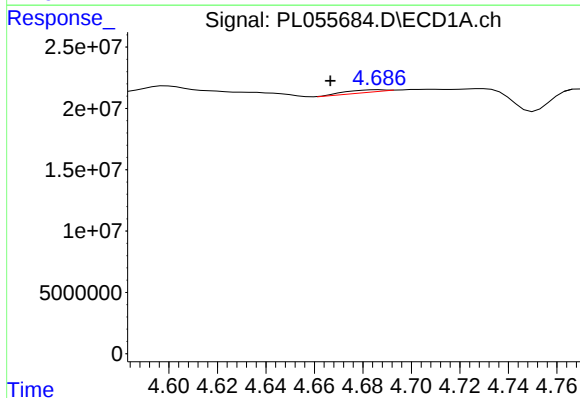


#7 delta-BHC

R.T.: 4.687 min
Delta R.T.: 0.020 min
Response: 2141385
Conc: 0.15 ng/ml

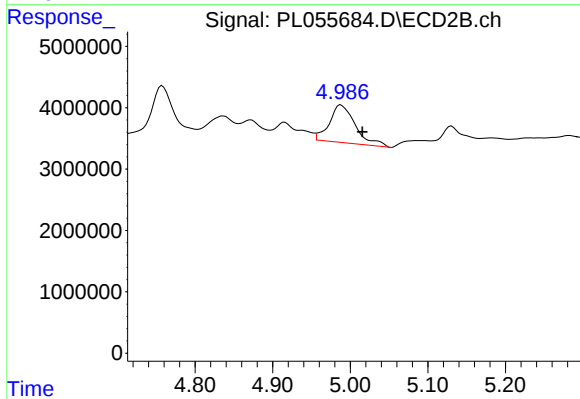

#7 delta-BHC


R.T.: 4.988 min
Delta R.T.: -0.028 min
Response: 14323484
Conc: 4.67 ng/ml

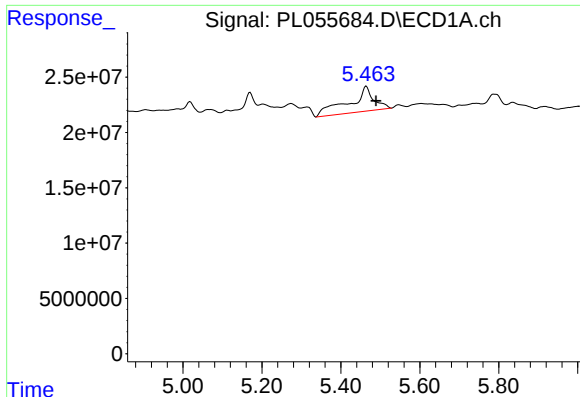

#11 alpha-Chlordane


R.T.: 5.464 min
Delta R.T.: -0.025 min
Response: 97806165
Conc: 7.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

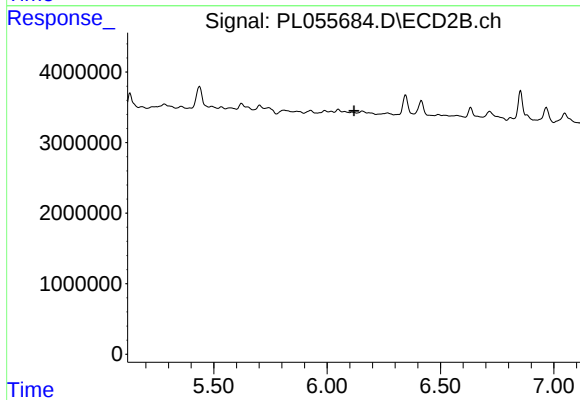


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

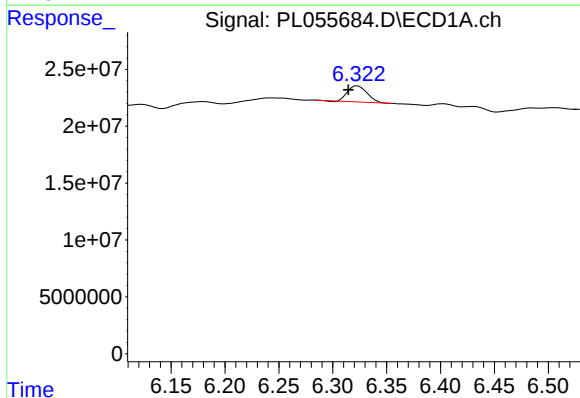


#15 Endosulfan II

R.T.: 6.323 min
Delta R.T.: 0.009 min
Response: 17562552
Conc: 1.63 ng/ml

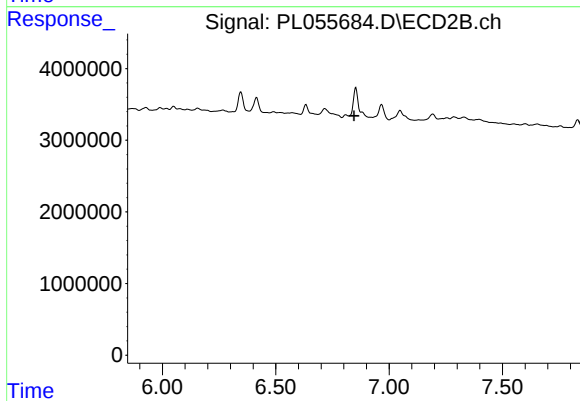

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.845 min
Response: 0
Conc: N.D.

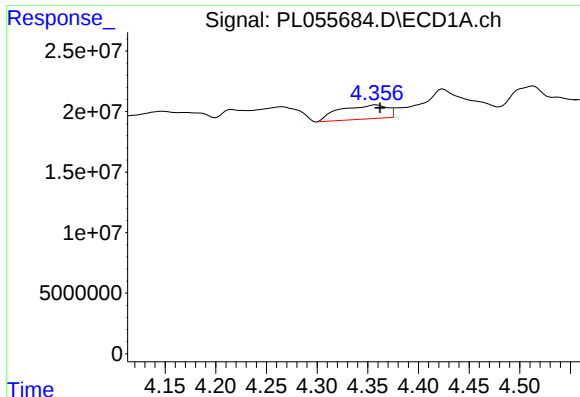

#23 Chlordane-1


R.T.: 4.358 min
Delta R.T.: -0.004 min
Response: 37343344
Conc: 107.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

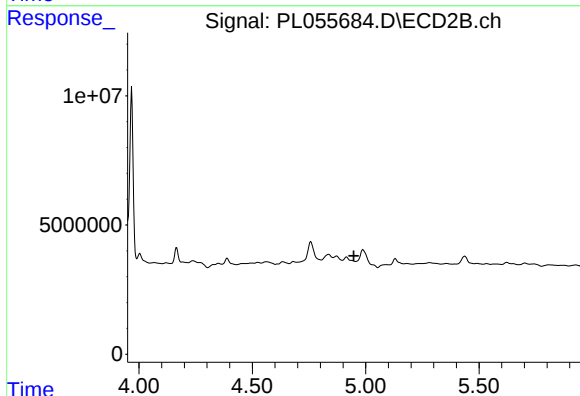


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.947 min
Response: 0
Conc: N.D.

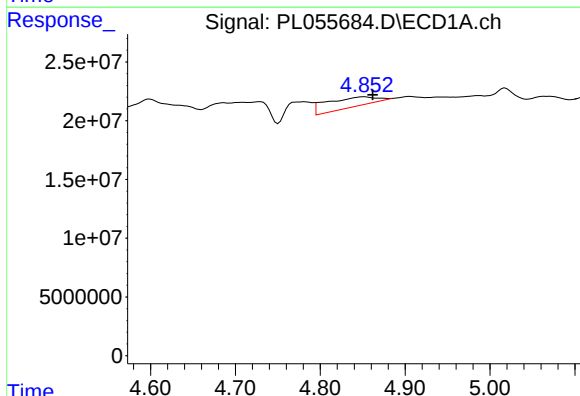


#24 Chlordane-2

R.T.: 4.853 min
Delta R.T.: -0.009 min
Response: 33784498
Conc: 83.07 ng/ml

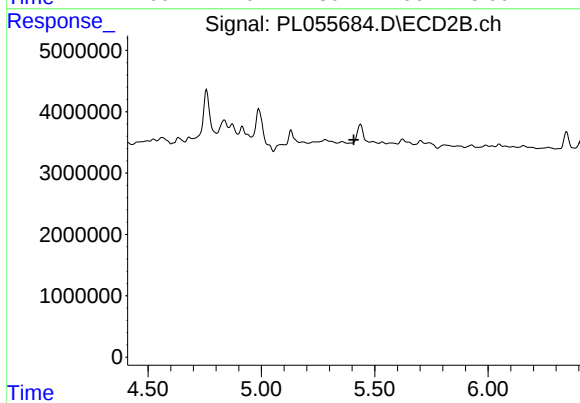

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

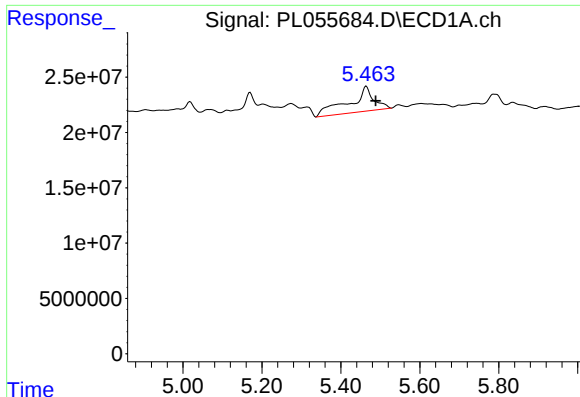

#26 Chlordane-4


R.T.: 5.464 min
Delta R.T.: -0.024 min
Response: 97806165
Conc: 100.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

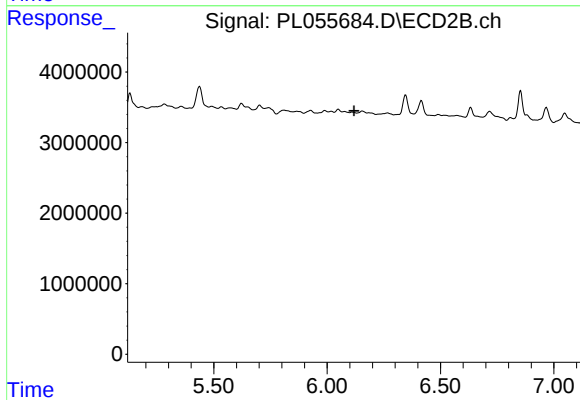


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

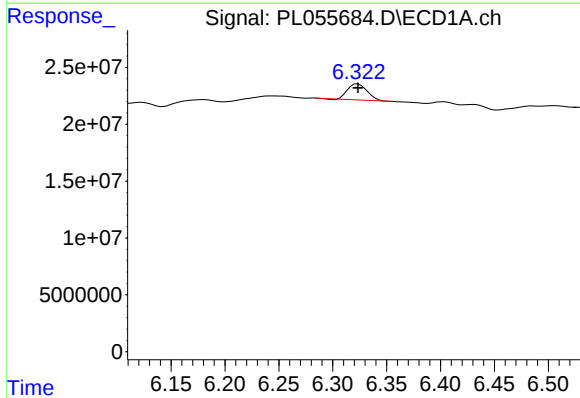


#27 Chlordane-5

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 17562552
Conc: 48.79 ng/ml

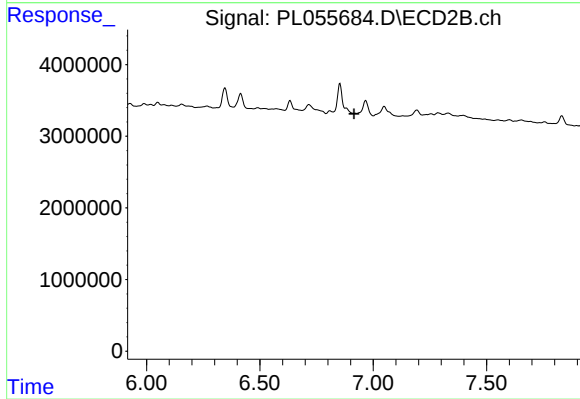

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.915 min
Response: 0
Conc: N.D.

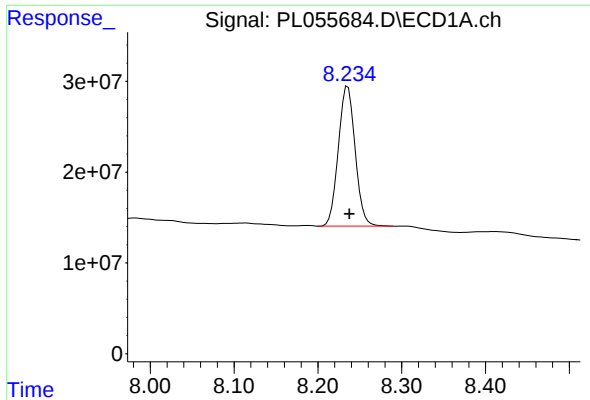

#28 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: -0.002 min
Response: 214579578
Conc: 24.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

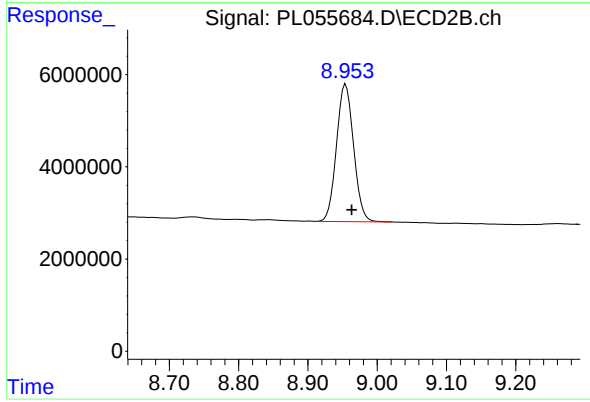

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: -0.009 min
Response: 51009922
Conc: 24.54 ng/ml