

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011121\
 Data File : PL064028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2021 11:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 02:01:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.107	55770221	49166932	18.603	19.258
28)	SA Decachlor...	8.168	9.266	55951363	46955229	20.308	23.816
Target Compounds							
4)	MA Heptachlor	0.000	5.311	0	2341842	N.D.	0.733 #
6)	B beta-BHC	0.000	4.984	0	3734640	N.D.	2.128 #
11)	B alpha-Chl...	0.000	6.349f	0	2887320	N.D.	1.046 #
26)	Chlordane-4	0.000	6.349f	0	2887320	N.D.	7.025 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011121\
Data File : PL064028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2021 11:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 02:01:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

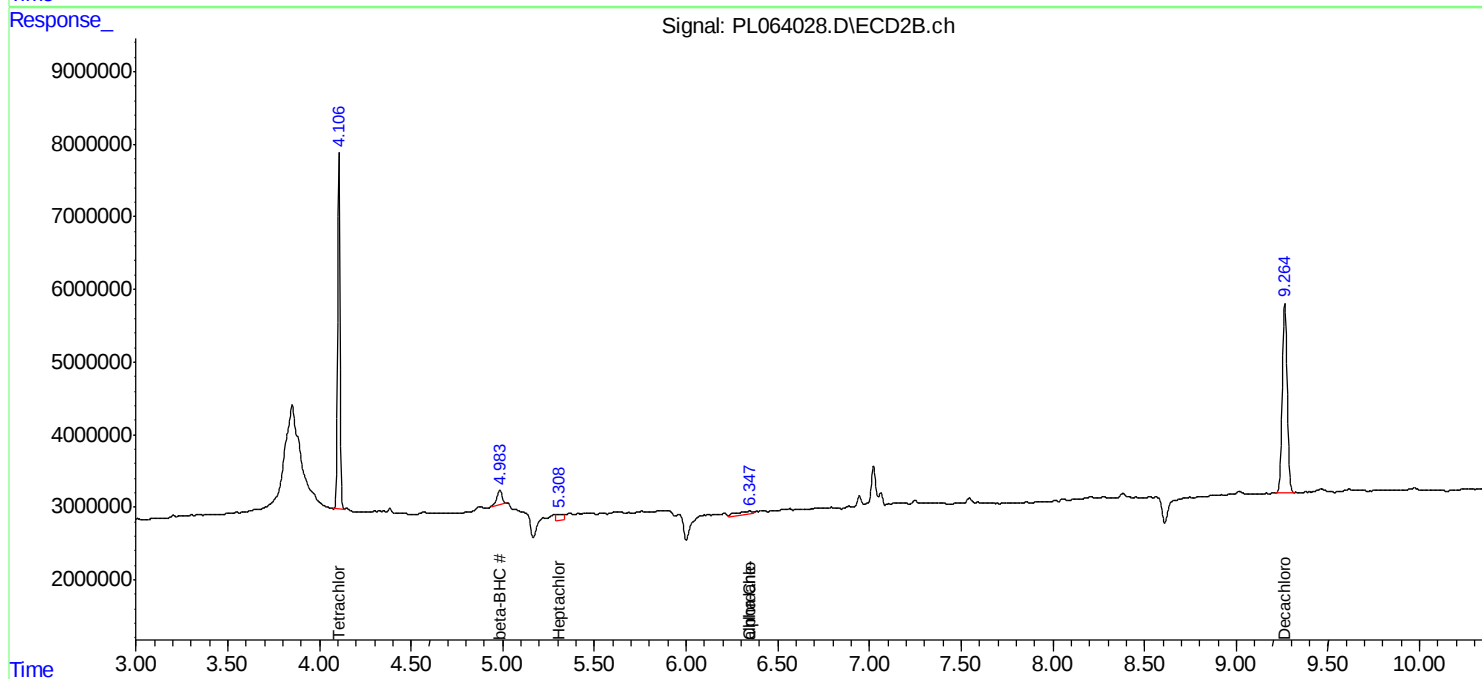


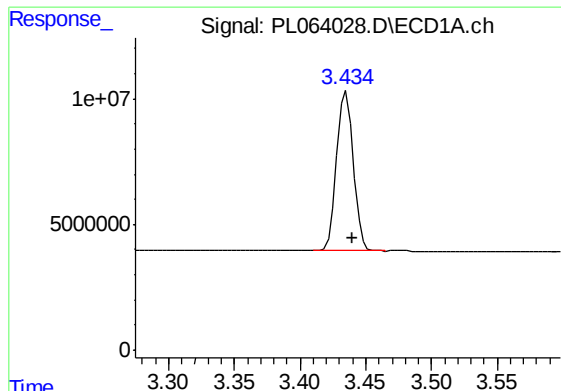

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: -0.005 min
Response: 55770221
Conc: 18.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

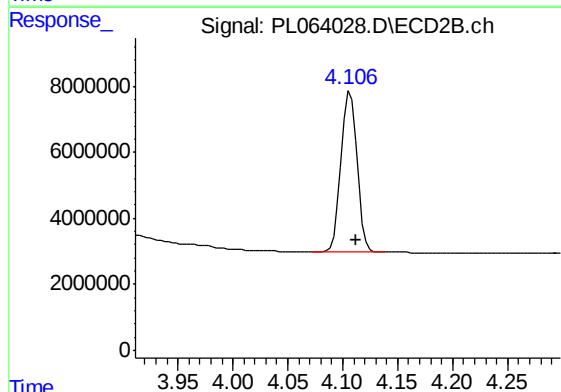


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: -0.006 min
Response: 49166932
Conc: 19.26 ng/ml

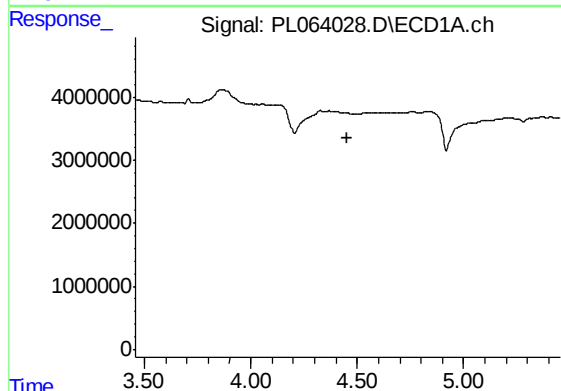


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.456 min
Response: 0
Conc: N.D.

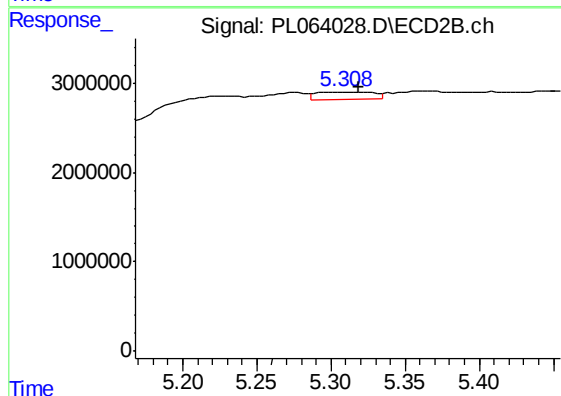

#4 Heptachlor


R.T.: 5.311 min
Delta R.T.: -0.008 min
Response: 2341842
Conc: 0.73 ng/ml

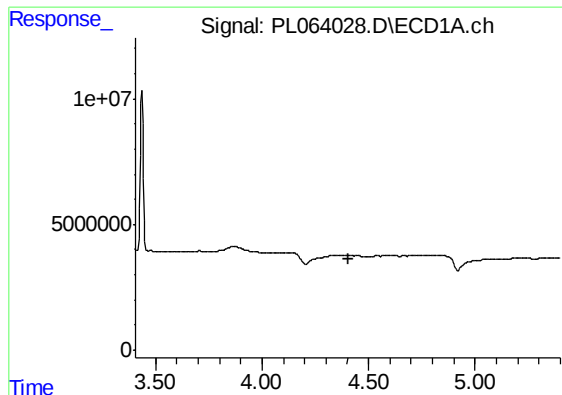

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

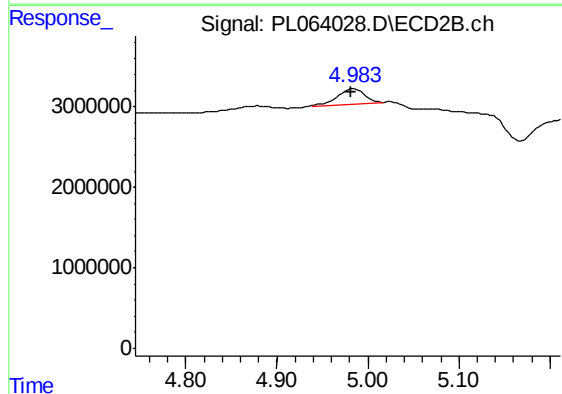


#6 beta-BHC

R.T.: 4.984 min
Delta R.T.: 0.003 min
Response: 3734640
Conc: 2.13 ng/ml

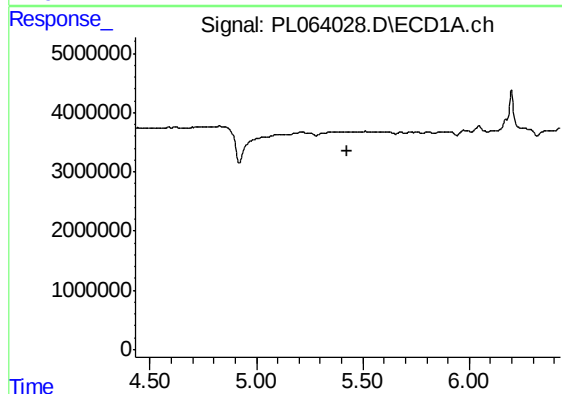


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.428 min
Response: 0
Conc: N.D.

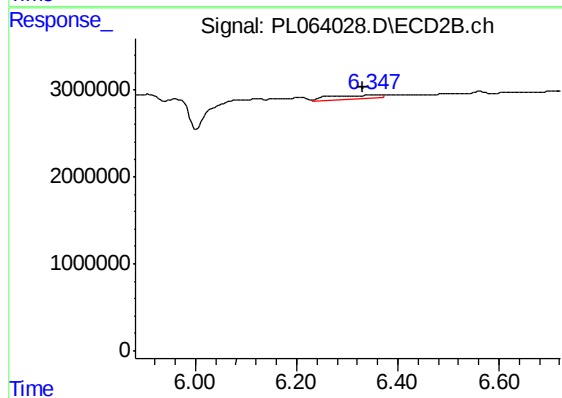

#11 alpha-Chlordane


R.T.: 6.349 min
Delta R.T.: 0.018 min
Response: 2887320
Conc: 1.05 ng/ml

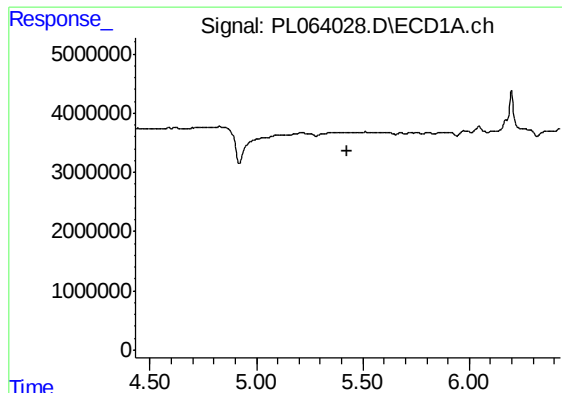

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

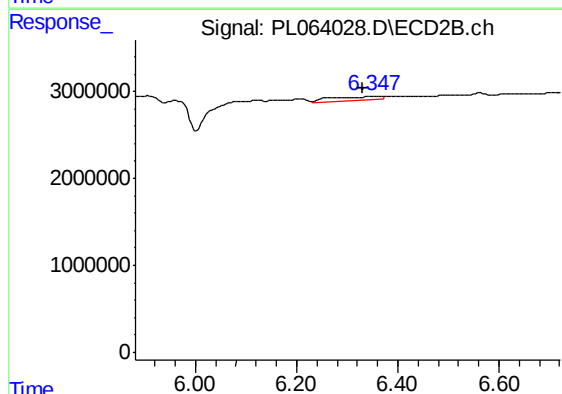


#26 Chlordane-4

R.T.: 6.349 min
Delta R.T.: 0.018 min
Response: 2887320
Conc: 7.02 ng/ml

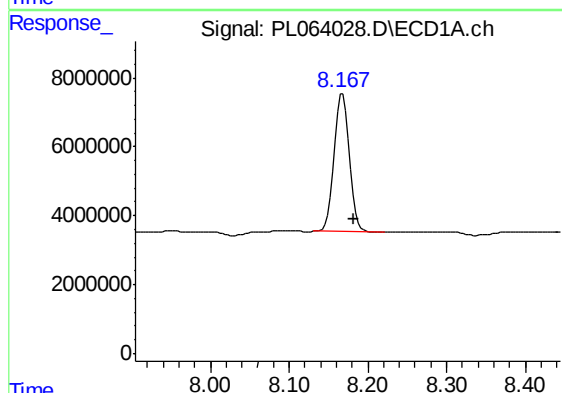

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: -0.014 min
Response: 55951363
Conc: 20.31 ng/ml

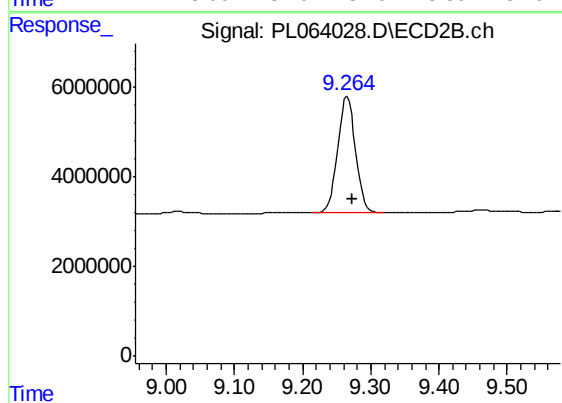

#28 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.006 min
Response: 46955229
Conc: 23.82 ng/ml