

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011121\
 Data File : PL064031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2021 12:29
 Operator : AR\AJ
 Sample : M1044-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-12

Manual Integrations
 APPROVED

Ankita
 1/12/2021 5:37:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 02:02:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.107	34124539	30891424	11.383	12.100
28)	SA Decachlor...	8.174	9.267	43346648	36578101	15.733	18.552
Target Compounds							
4)	MA Heptachlor	4.454	5.311	5370832	4046069	1.275	1.267m
12)	B 4,4'-DDE	5.591	6.482	7345933	7802498	2.137m	3.159 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011121\
Data File : PL064031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2021 12:29
Operator : AR\AJ
Sample : M1044-19
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-12


Manual Integrations
APPROVED

Ankita
1/12/2021 5:37:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 02:02:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

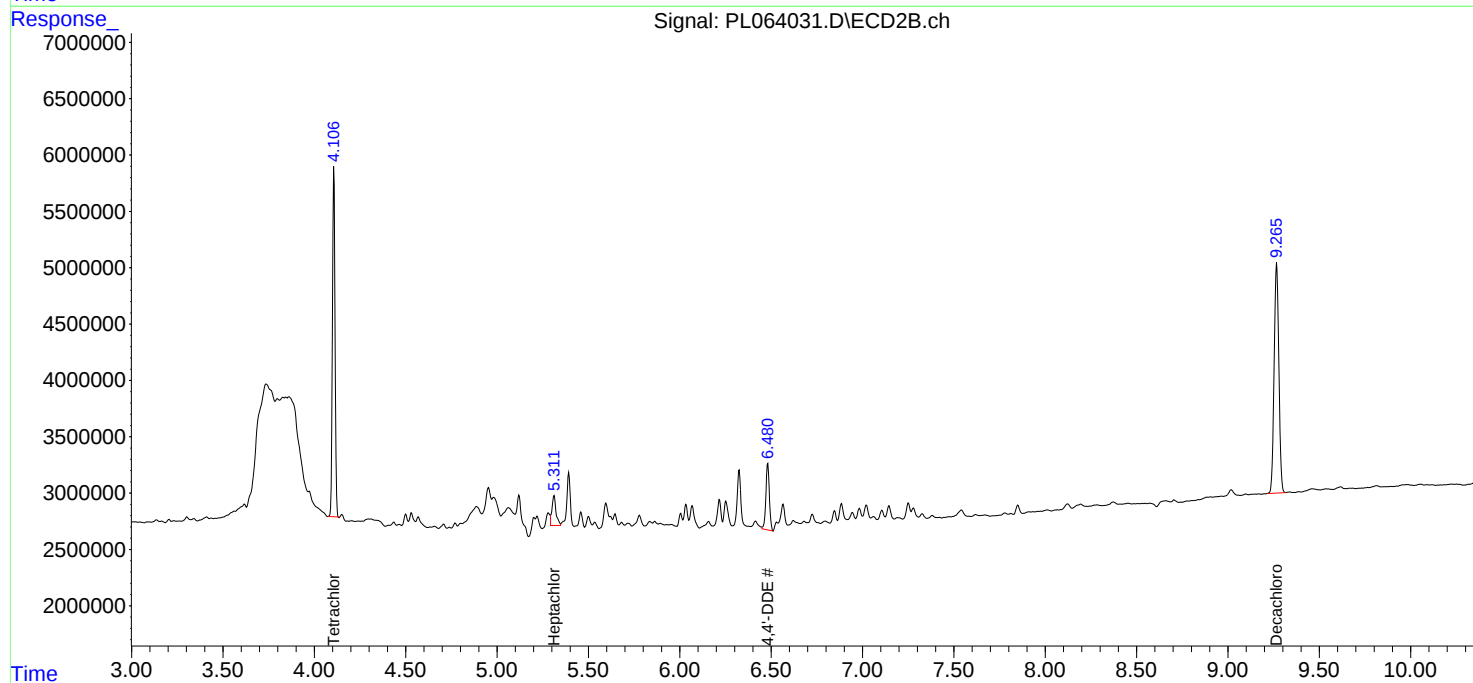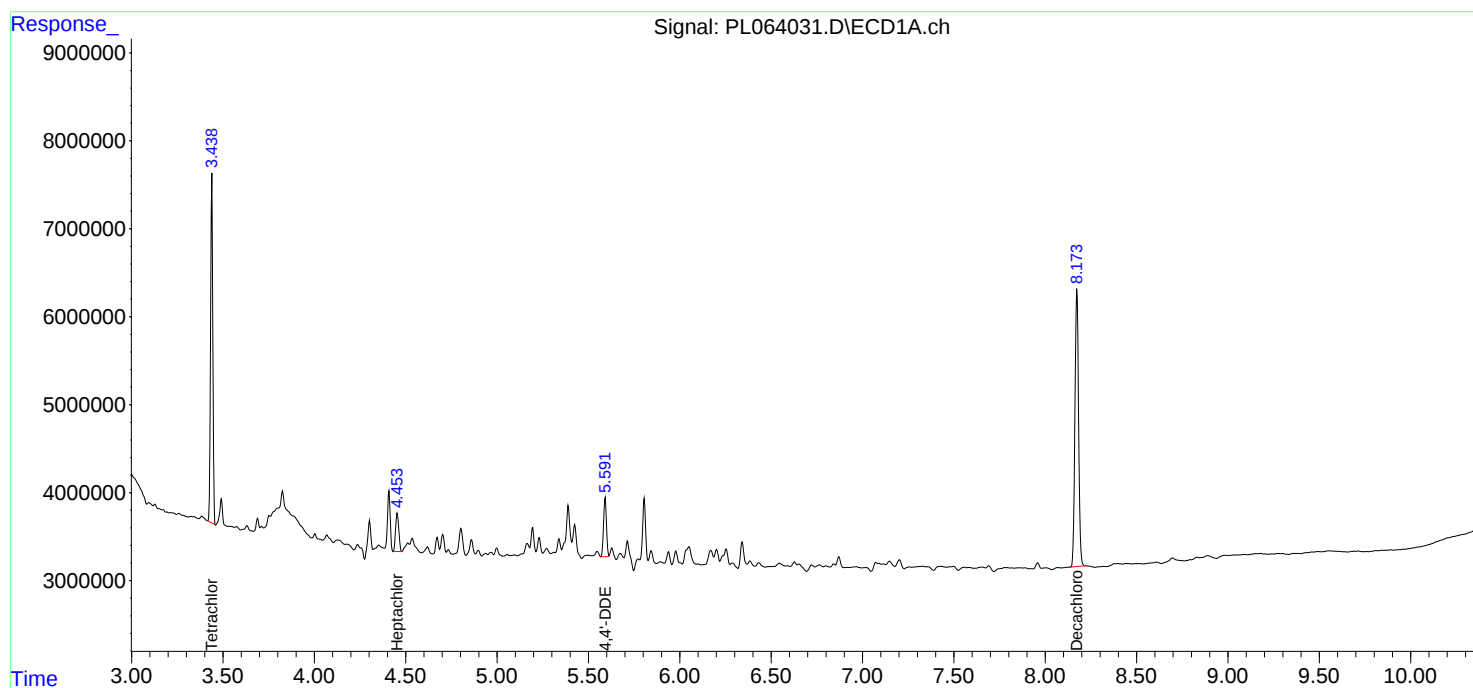

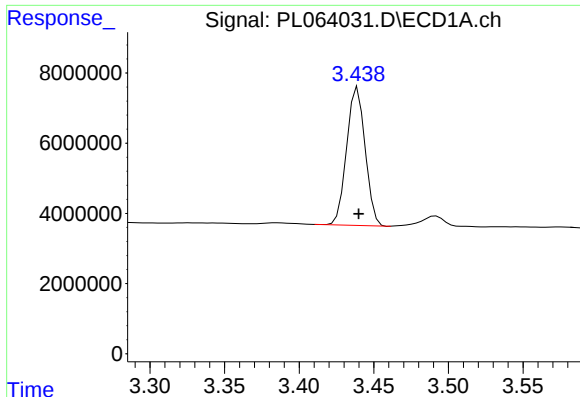


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 34124539
Conc: 11.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12


Manual Integrations
APPROVED

Ankita
1/12/2021 5:37:24 PM

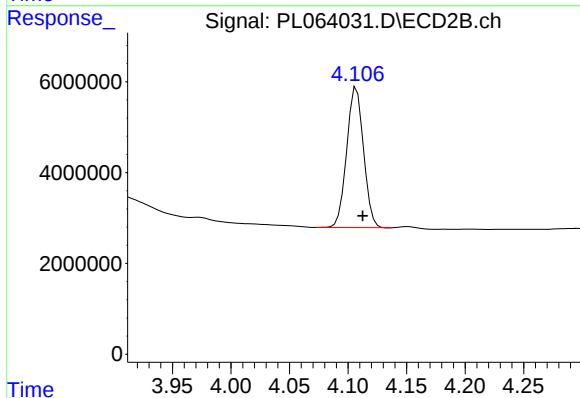


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: -0.005 min
Response: 30891424
Conc: 12.10 ng/ml

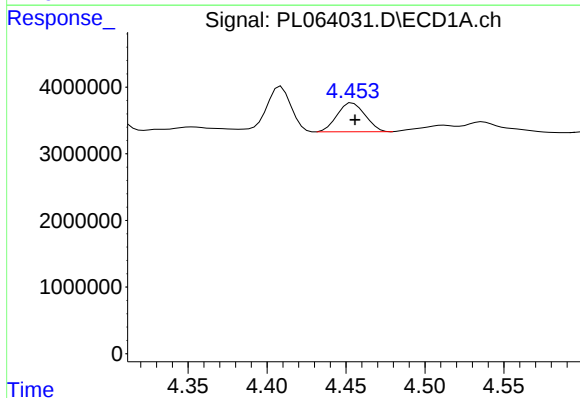


#4 Heptachlor

R.T.: 4.454 min
Delta R.T.: -0.001 min
Response: 5370832
Conc: 1.28 ng/ml

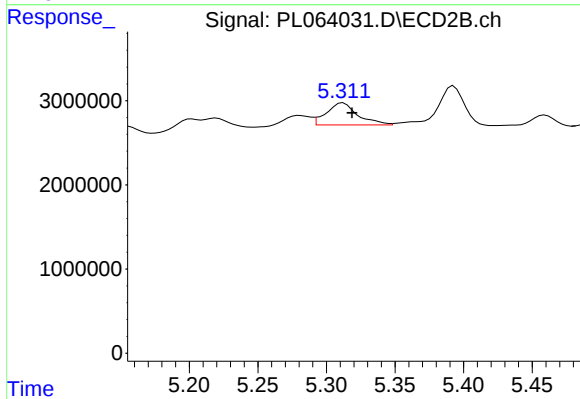

#4 Heptachlor

R.T.: 5.311 min
Delta R.T.: -0.008 min
Response: 4046069
Conc: 1.27 ng/ml m

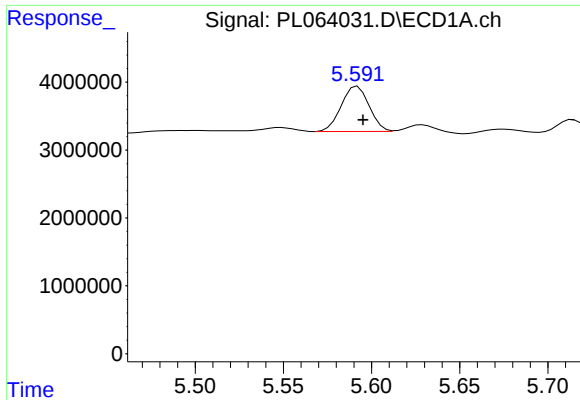


#12 4,4'-DDE

R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 7345933
Conc: 2.14 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-12


Manual Integrations
APPROVED

Ankita
1/12/2021 5:37:24 PM

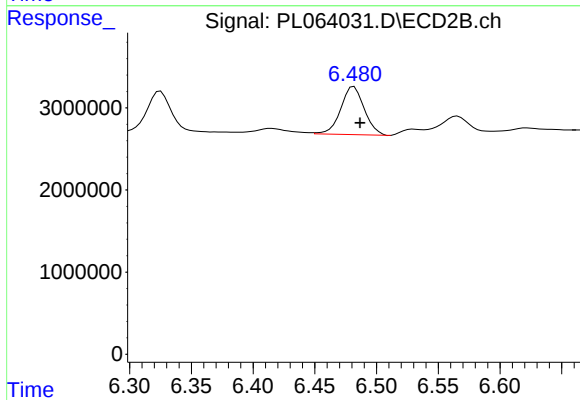


#12 4,4'-DDE

R.T.: 6.482 min
Delta R.T.: -0.005 min
Response: 7802498
Conc: 3.16 ng/ml

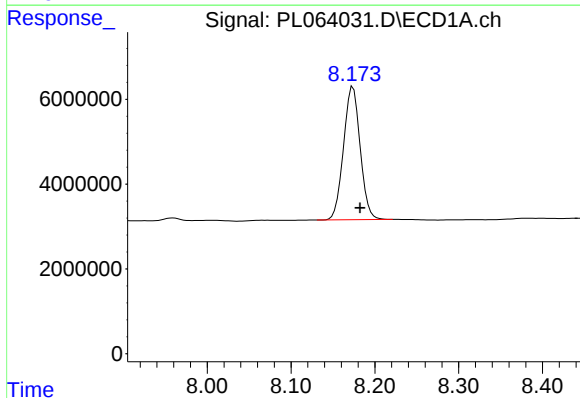

#28 Decachlorobiphenyl

R.T.: 8.174 min
Delta R.T.: -0.008 min
Response: 43346648
Conc: 15.73 ng/ml

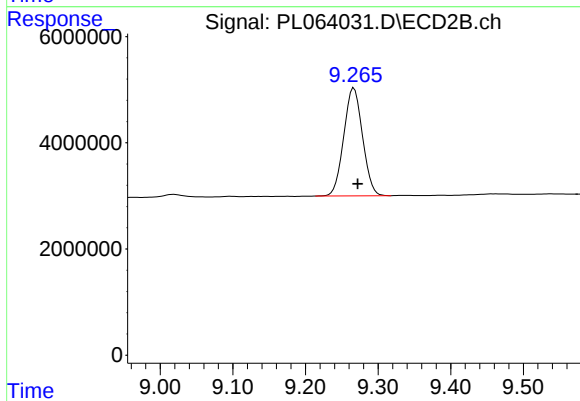

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.005 min
Response: 36578101
Conc: 18.55 ng/ml