

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011121\
 Data File : PL064037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2021 16:47
 Operator : AR\AJ
 Sample : M1056-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-010821

Manual Integrations
 APPROVED

Ankita
 1/12/2021 5:37:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 02:04:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.106	35054664	30991827	11.693	12.139
28)	SA Decachlor...	8.170	9.264	36842774	33206437	13.372	16.842 #
Target Compounds							
12)	B 4,4'-DDE	5.585	6.480	3243194	2400818	0.943m	0.972

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011121\
Data File : PL064037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2021 16:47
Operator : AR\AJ
Sample : M1056-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CL-01-010821


Manual Integrations
APPROVED

Ankita
1/12/2021 5:37:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 02:04:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

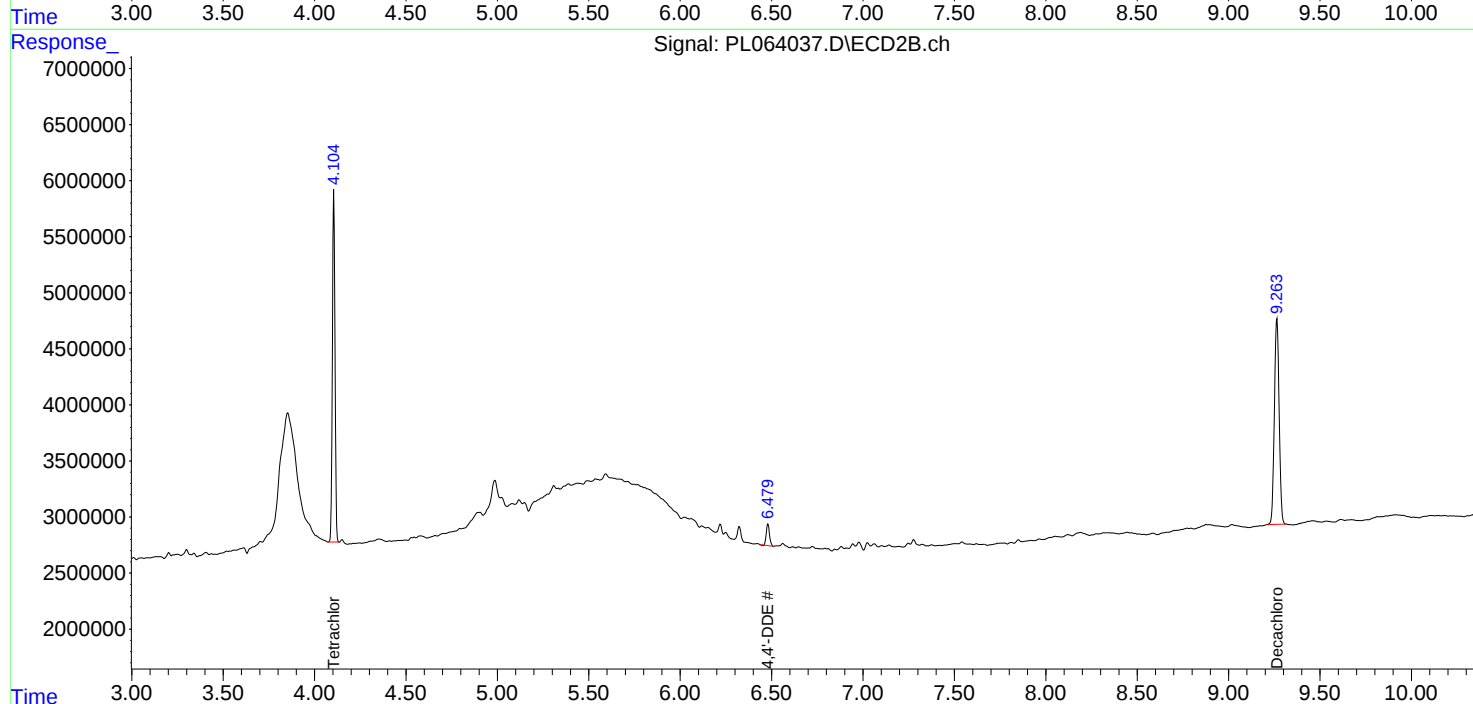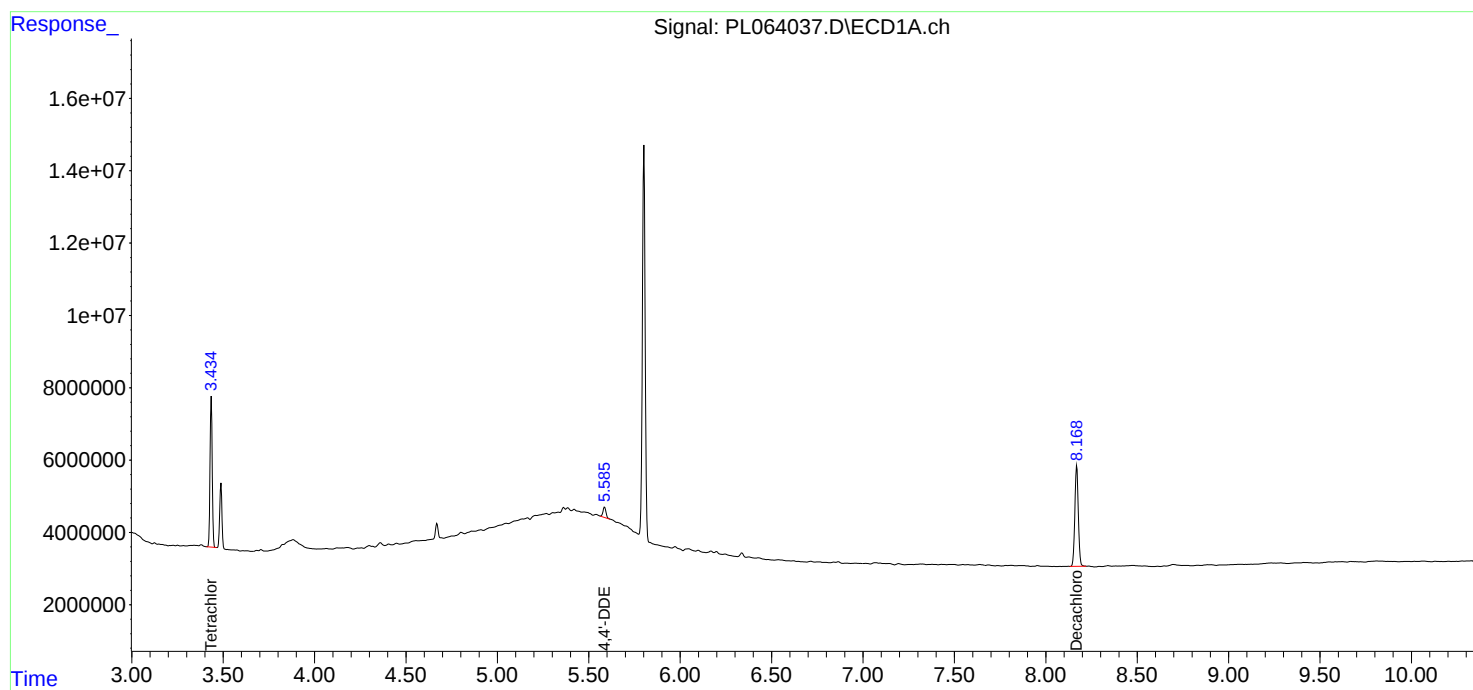

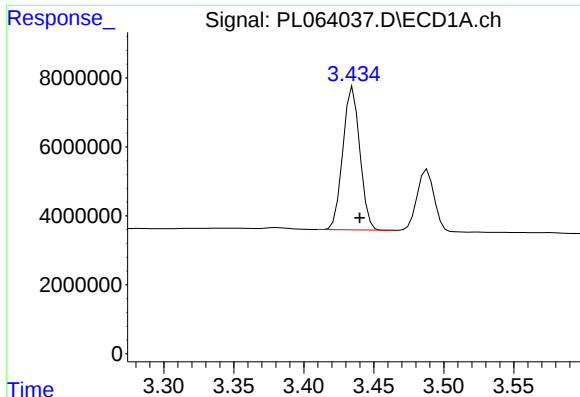


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: -0.005 min
Response: 35054664
Conc: 11.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-010821


Manual Integrations
APPROVED

Ankita
1/12/2021 5:37:27 PM

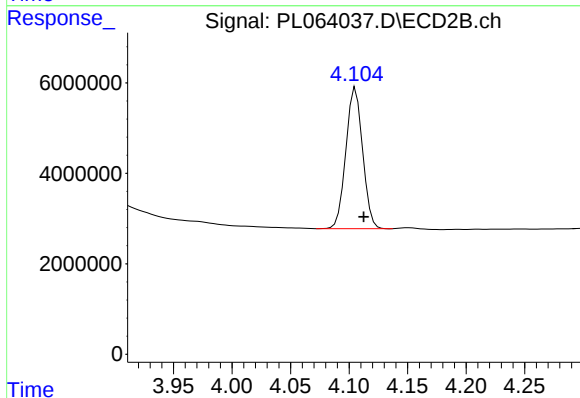


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: -0.007 min
Response: 30991827
Conc: 12.14 ng/ml

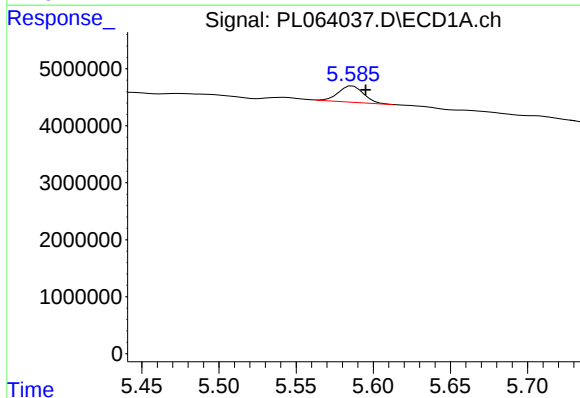


#12 4,4'-DDE

R.T.: 5.585 min
Delta R.T.: -0.010 min
Response: 3243194
Conc: 0.94 ng/ml m

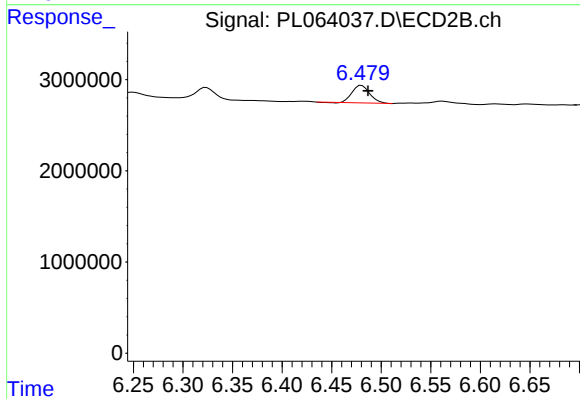

#12 4,4'-DDE

R.T.: 6.480 min
Delta R.T.: -0.006 min
Response: 2400818
Conc: 0.97 ng/ml

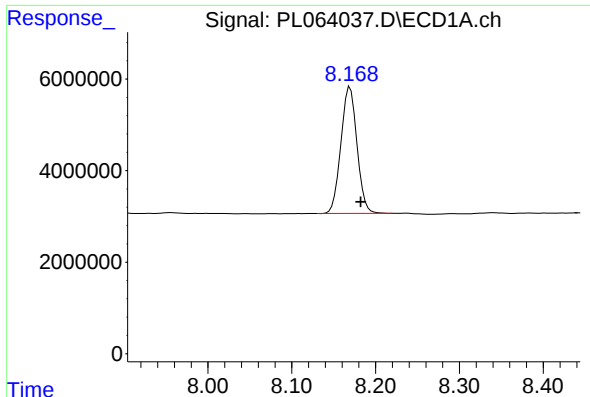


#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: -0.013 min
Response: 36842774
Conc: 13.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-010821

Manual Integrations
APPROVED

Ankita
1/12/2021 5:37:27 PM

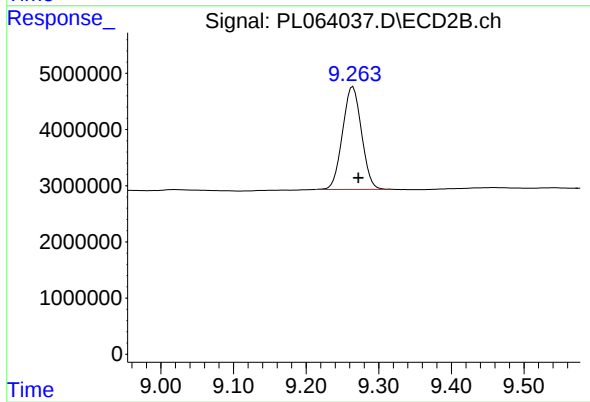

#28 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.008 min
Response: 33206437
Conc: 16.84 ng/ml