

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011122\
 Data File : PL071930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2022 08:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 00:06:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.493	9003694	25195973	19.491	20.507
28)	SA Decachlor...	10.320	11.385	14421089	23646076	19.945	19.954
Target Compounds							
3)	MA gamma-BHC...	0.000	6.457	0	311314	N.D.	0.192 #
7)	B delta-BHC	0.000	6.972f	0	422332	N.D.	0.275 #
9)	A Endosulfan I	0.000	8.363	0	22852	N.D.	0.018 #
10)	B gamma-Chl...	0.000	8.234	0	116704	N.D.	0.085 #
11)	B alpha-Chl...	0.000	8.322f	0	58377	N.D.	0.044 #
15)	B Endosulfa...	8.262f	9.147f	4236243	251130	7.329	0.224 #
17)	MA 4,4'-DDT	0.000	9.334f	0	365421	N.D.	0.387 #
18)	B Endrin al...	0.000	9.237f	0	135910	N.D.	0.160 #
21)	B Endrin ke...	0.000	9.982	0	34928	N.D.	0.031 #
25)	Chlordane-3	0.000	8.234	0	116704	N.D.	0.572 #
26)	Chlordane-4	0.000	8.322f	0	58377	N.D.	0.240 #
27)	Chlordane-5	8.262f	0.000	4236243	0	177.444	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011122\
Data File : PL071930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2022 08:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 00:06:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

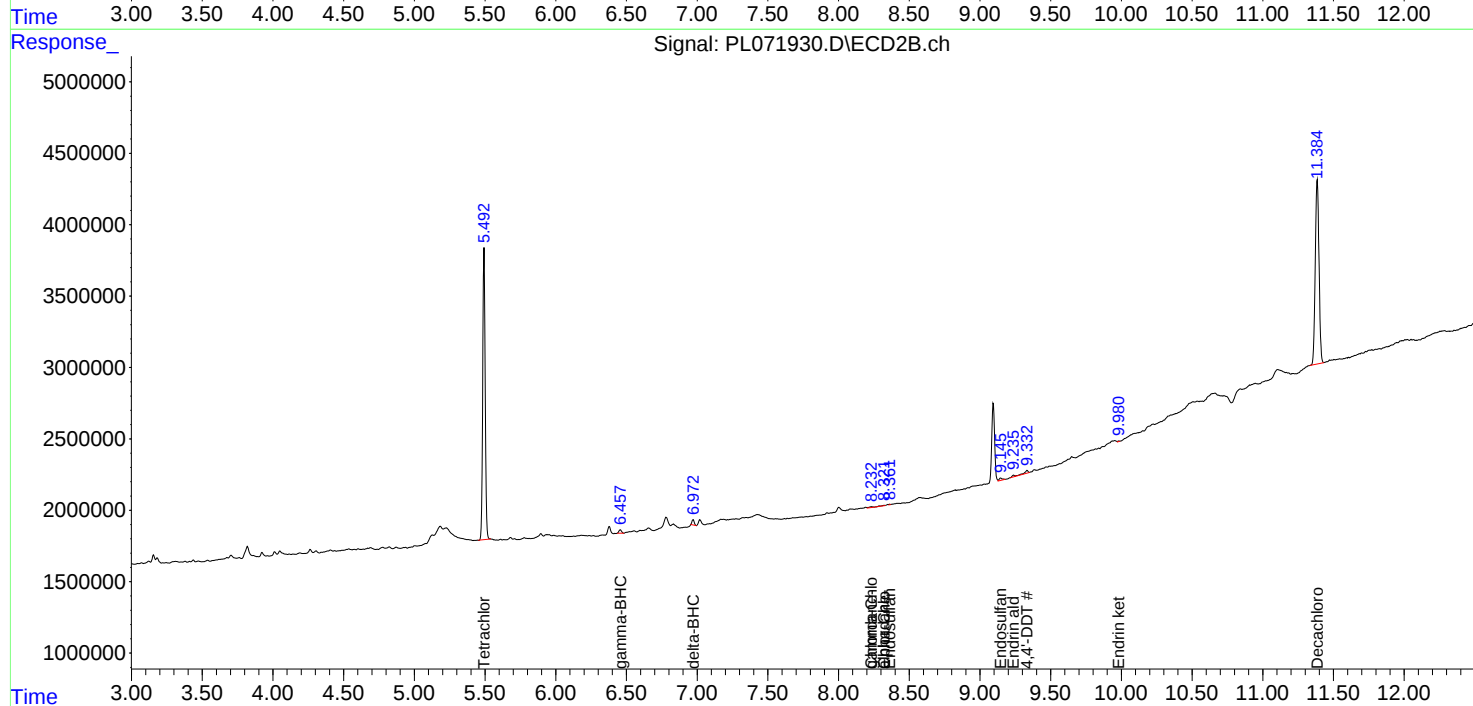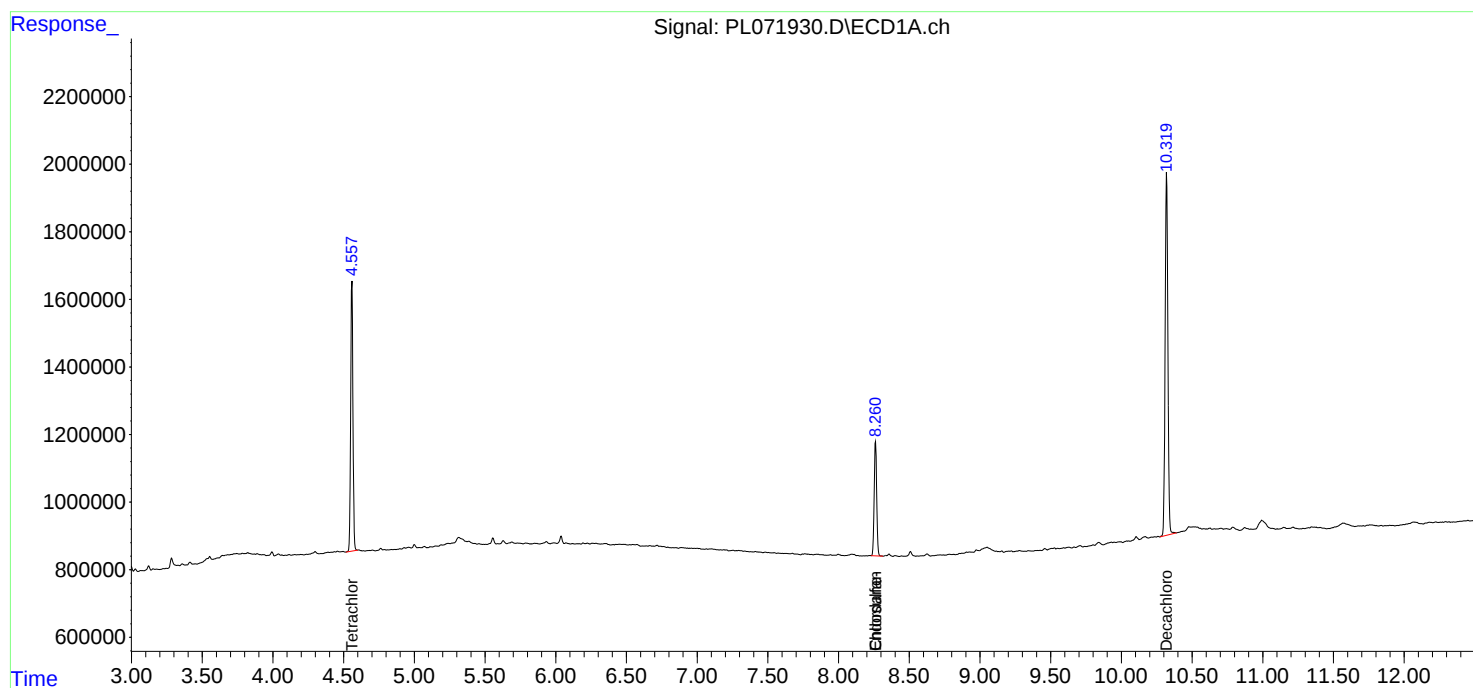


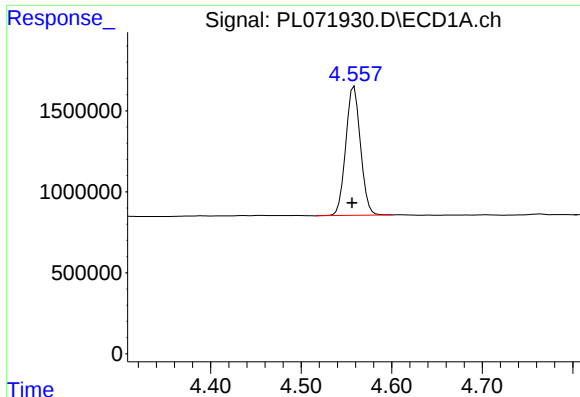

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: 0.003 min
Response: 9003694
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

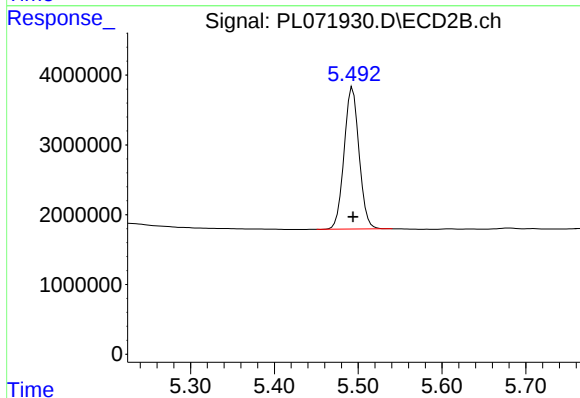


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 25195973
Conc: 20.51 ng/ml

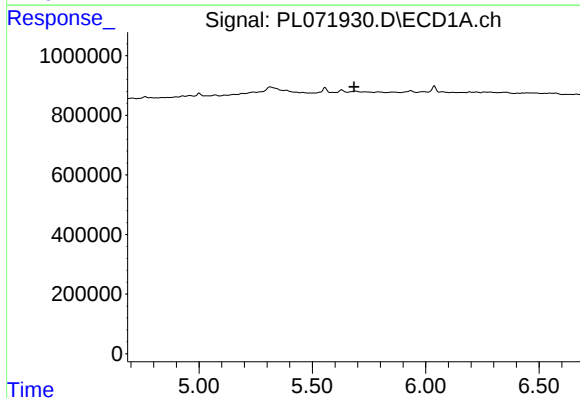


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.684 min
Response: 0
Conc: N.D.

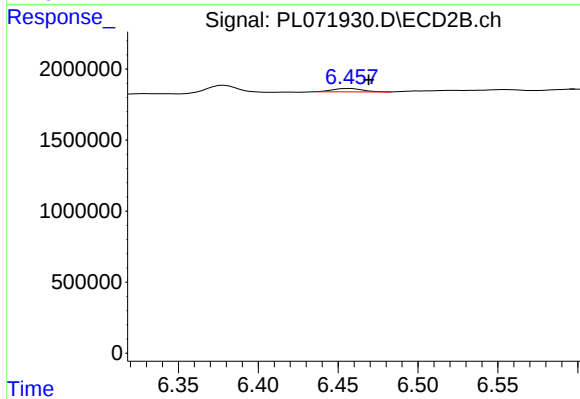

#3 gamma-BHC (Lindane)


R.T.: 6.457 min
Delta R.T.: -0.012 min
Response: 311314
Conc: 0.19 ng/ml

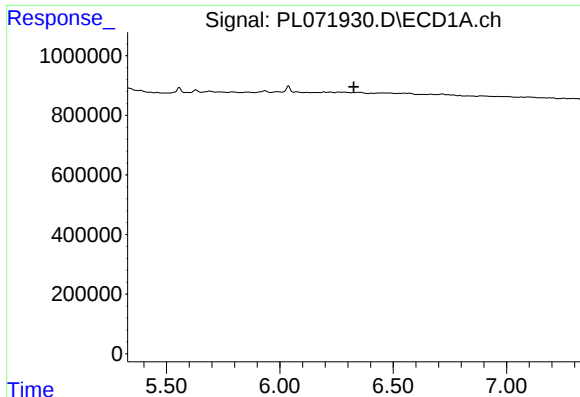

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

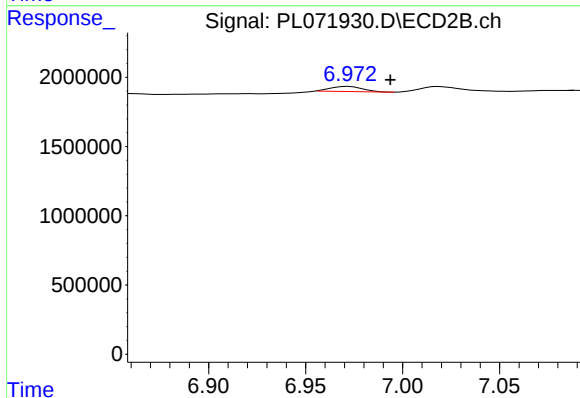


#7 delta-BHC

R.T.: 6.972 min
Delta R.T.: -0.021 min
Response: 422332
Conc: 0.28 ng/ml

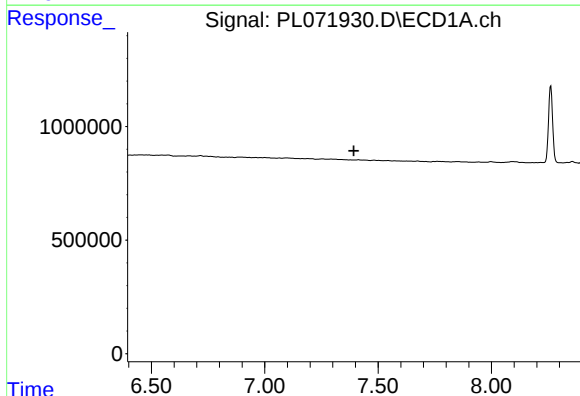


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.393 min
Response: 0
Conc: N.D.

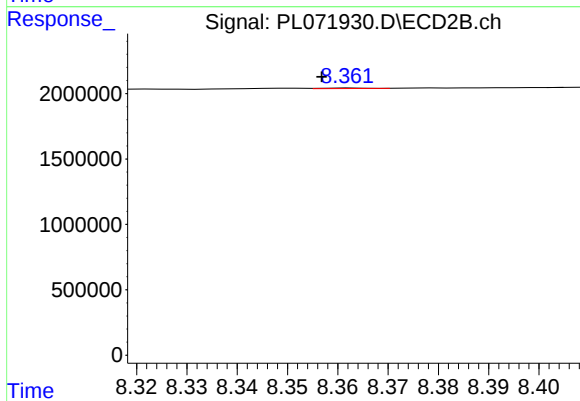

#9 Endosulfan I


R.T.: 8.363 min
Delta R.T.: 0.006 min
Response: 22852
Conc: 0.02 ng/ml

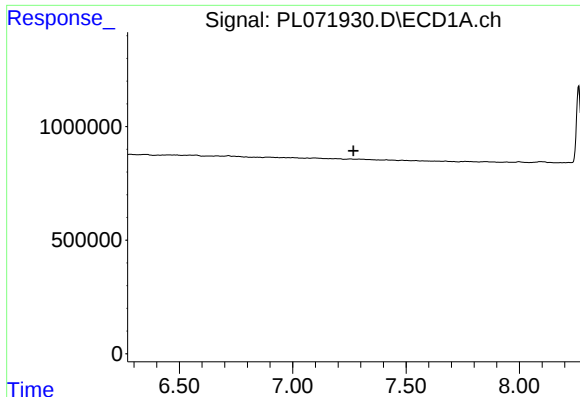

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

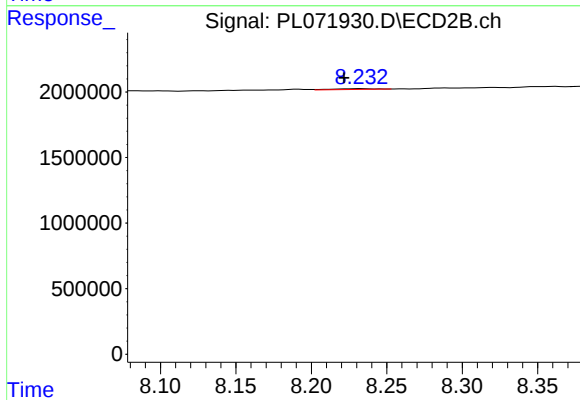


#10 gamma-Chlordane

R.T.: 8.234 min
Delta R.T.: 0.012 min
Response: 116704
Conc: 0.09 ng/ml

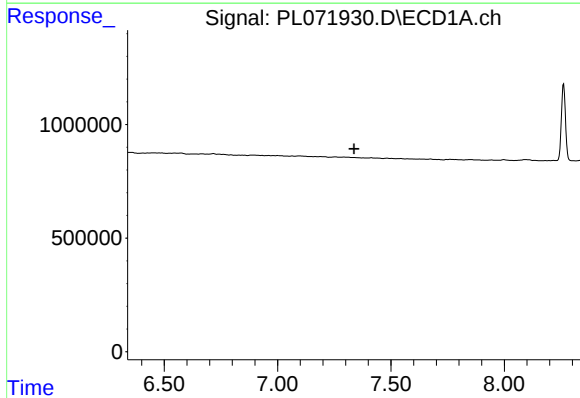


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

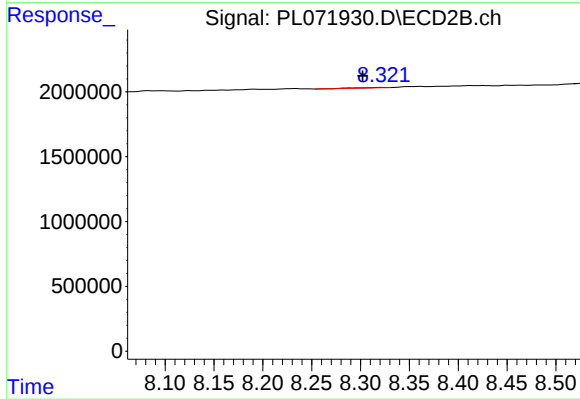

#11 alpha-Chlordane


R.T.: 8.322 min
Delta R.T.: 0.020 min
Response: 58377
Conc: 0.04 ng/ml

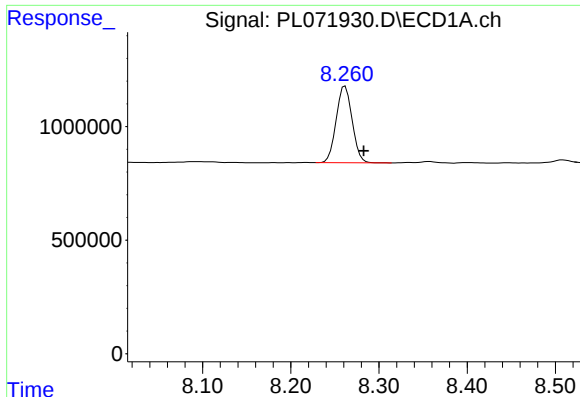

#15 Endosulfan II


R.T.: 8.262 min
Delta R.T.: -0.021 min
Response: 4236243
Conc: 7.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

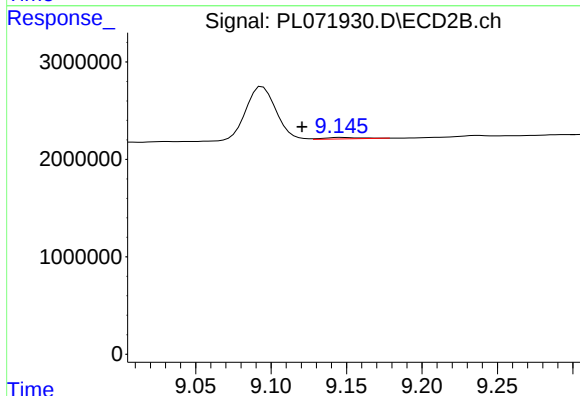


#15 Endosulfan II

R.T.: 9.147 min
Delta R.T.: 0.026 min
Response: 251130
Conc: 0.22 ng/ml

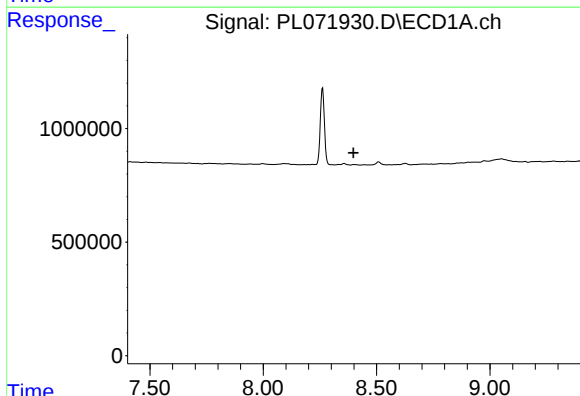


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

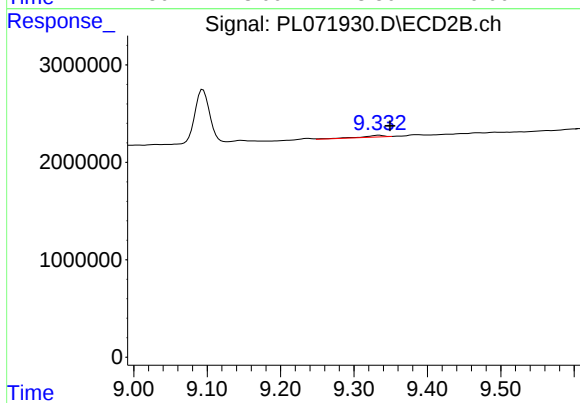

#17 4,4'-DDT


R.T.: 9.334 min
Delta R.T.: -0.015 min
Response: 365421
Conc: 0.39 ng/ml

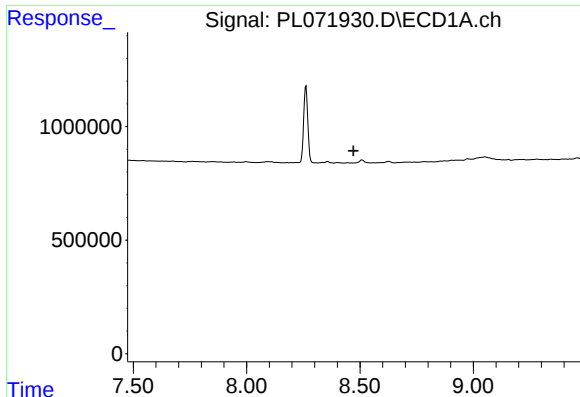

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

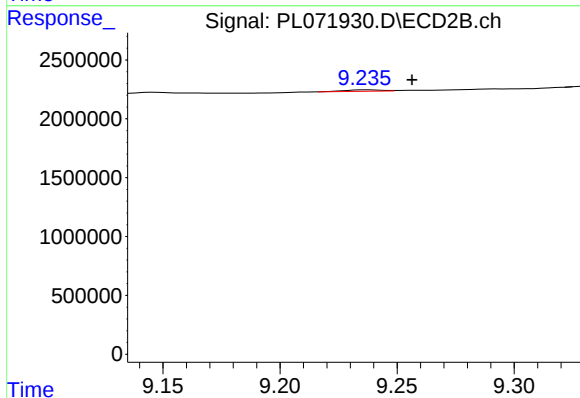


#18 Endrin aldehyde

R.T.: 9.237 min
Delta R.T.: -0.019 min
Response: 135910
Conc: 0.16 ng/ml

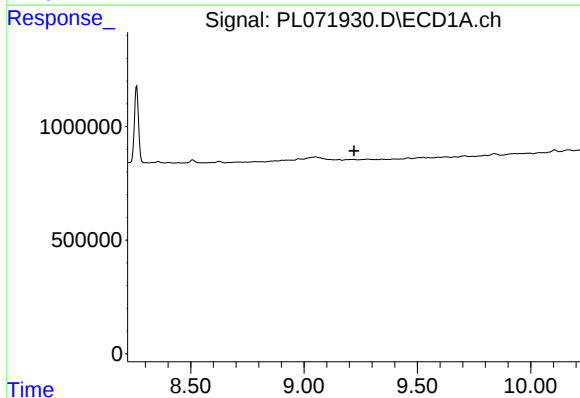


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

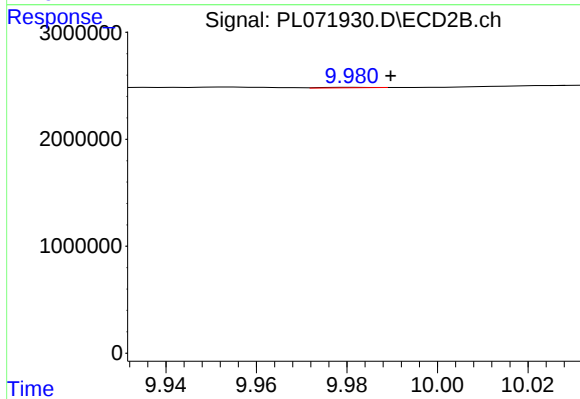

#21 Endrin ketone


R.T.: 9.982 min
Delta R.T.: -0.008 min
Response: 34928
Conc: 0.03 ng/ml

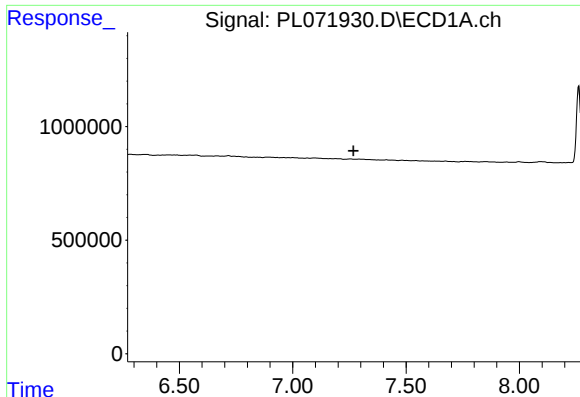

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

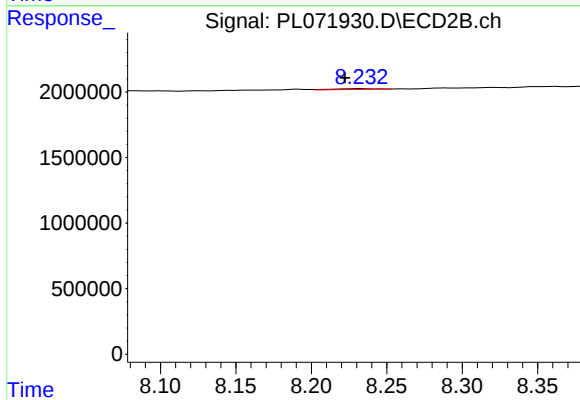


#25 Chlordane-3

R.T.: 8.234 min
Delta R.T.: 0.011 min
Response: 116704
Conc: 0.57 ng/ml

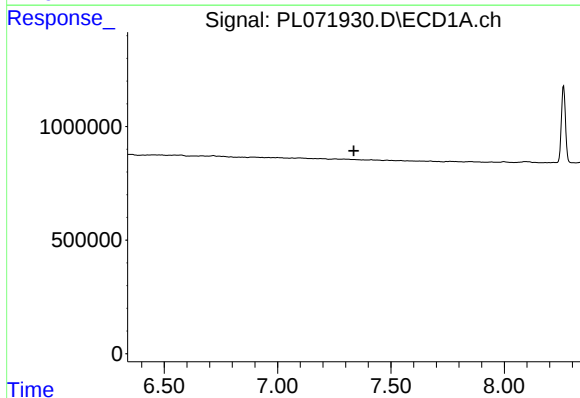


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

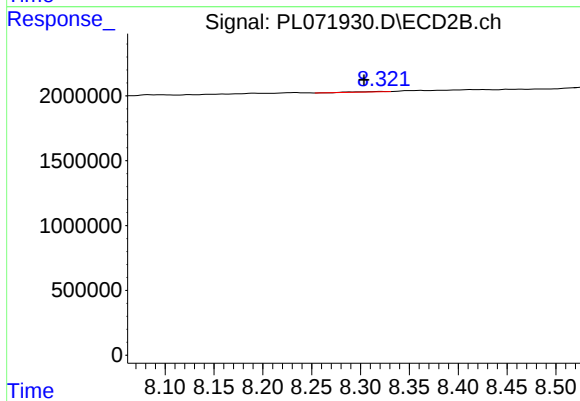

#26 Chlordane-4


R.T.: 8.322 min
Delta R.T.: 0.019 min
Response: 58377
Conc: 0.24 ng/ml

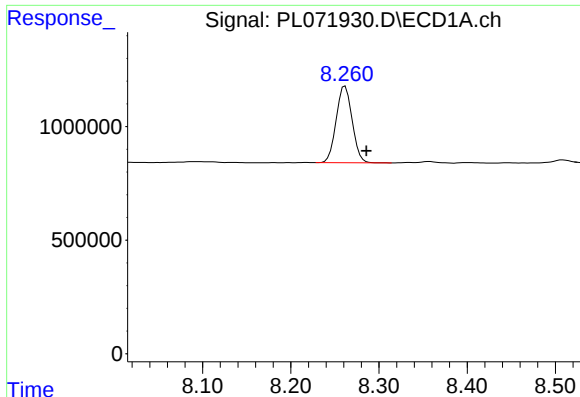

#27 Chlordane-5


R.T.: 8.262 min
Delta R.T.: -0.024 min
Response: 4236243
Conc: 177.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

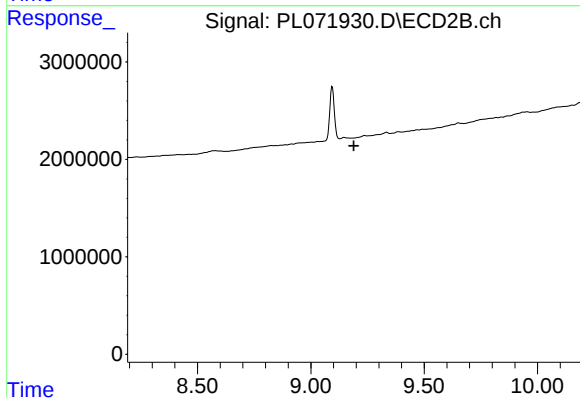


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.190 min
Response: 0
Conc: N.D.

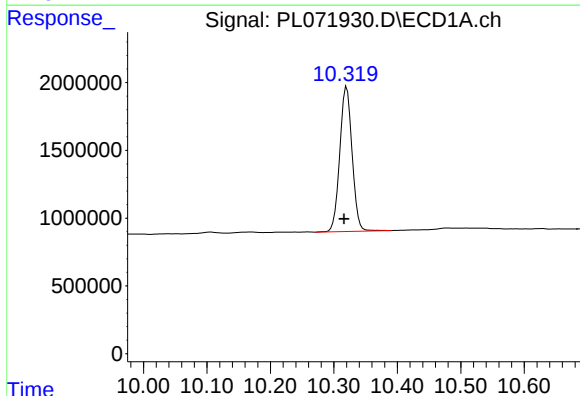

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: 0.004 min
Response: 14421089
Conc: 19.95 ng/ml

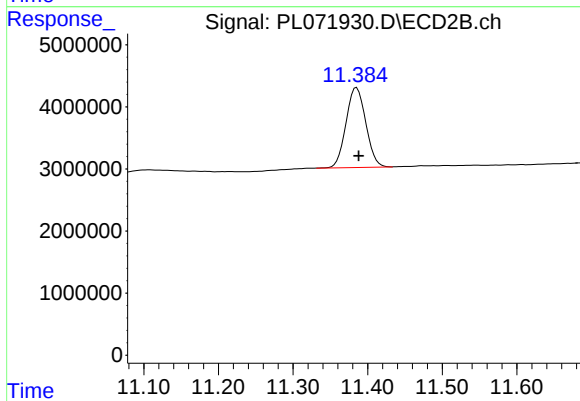

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.003 min
Response: 23646076
Conc: 19.95 ng/ml