

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011221\
 Data File : PL064059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2021 16:16
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 04:47:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:46:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.107	274.6E6	197.5E6	73.271	74.366
28)	SA Decachlor...	8.168	9.267	218.3E6	169.8E6	73.793	72.883
Target Compounds							
23)	Chlordane-1	4.297	5.120	78834607	75637266	737.785	717.782
24)	Chlordane-2	4.796	5.596	93610121	72067923	699.229	718.899
25)	Chlordane-3	5.362	6.251	265.8E6	296.8E6	739.788	748.655
26)	Chlordane-4	5.419	6.325	218.1E6	359.3E6	732.335	741.163
27)	Chlordane-5	6.248	7.145	89516810	61856957	728.535	737.174



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011221\
Data File : PL064059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2021 16:16
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 04:47:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:46:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

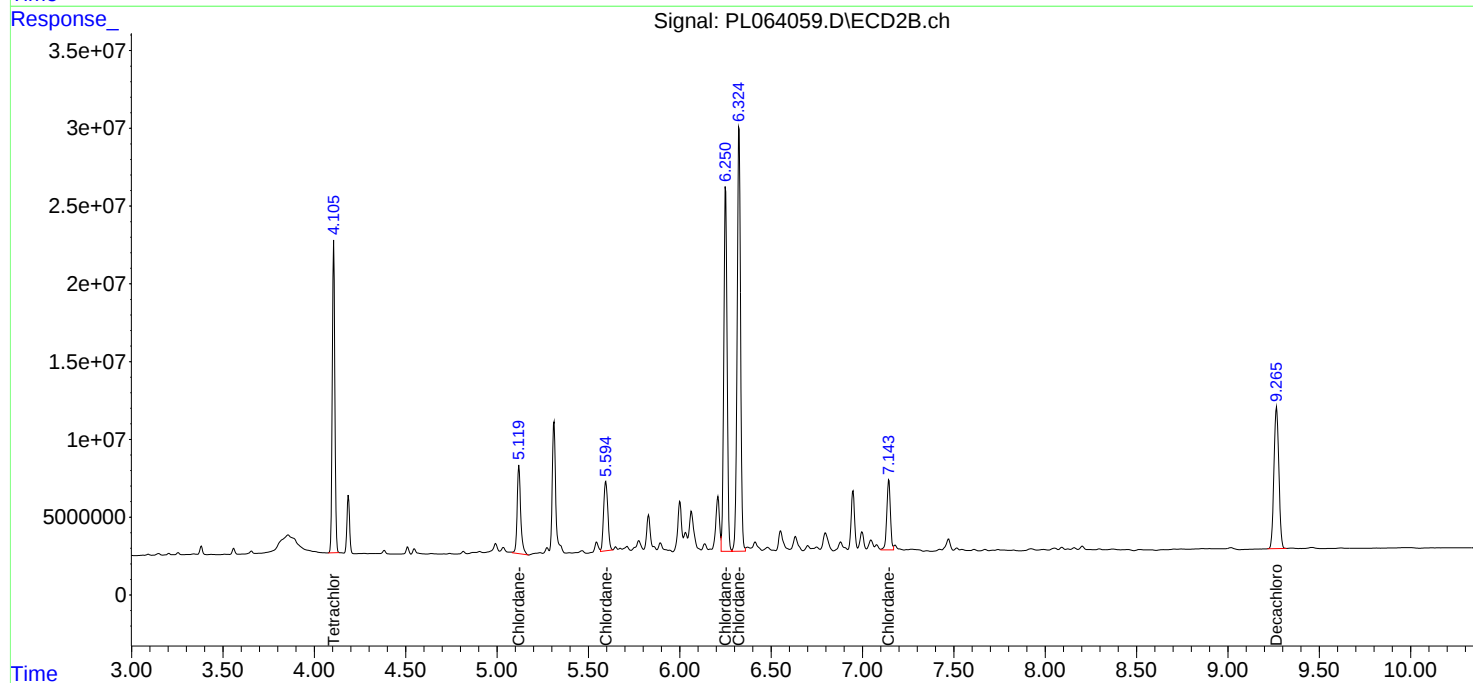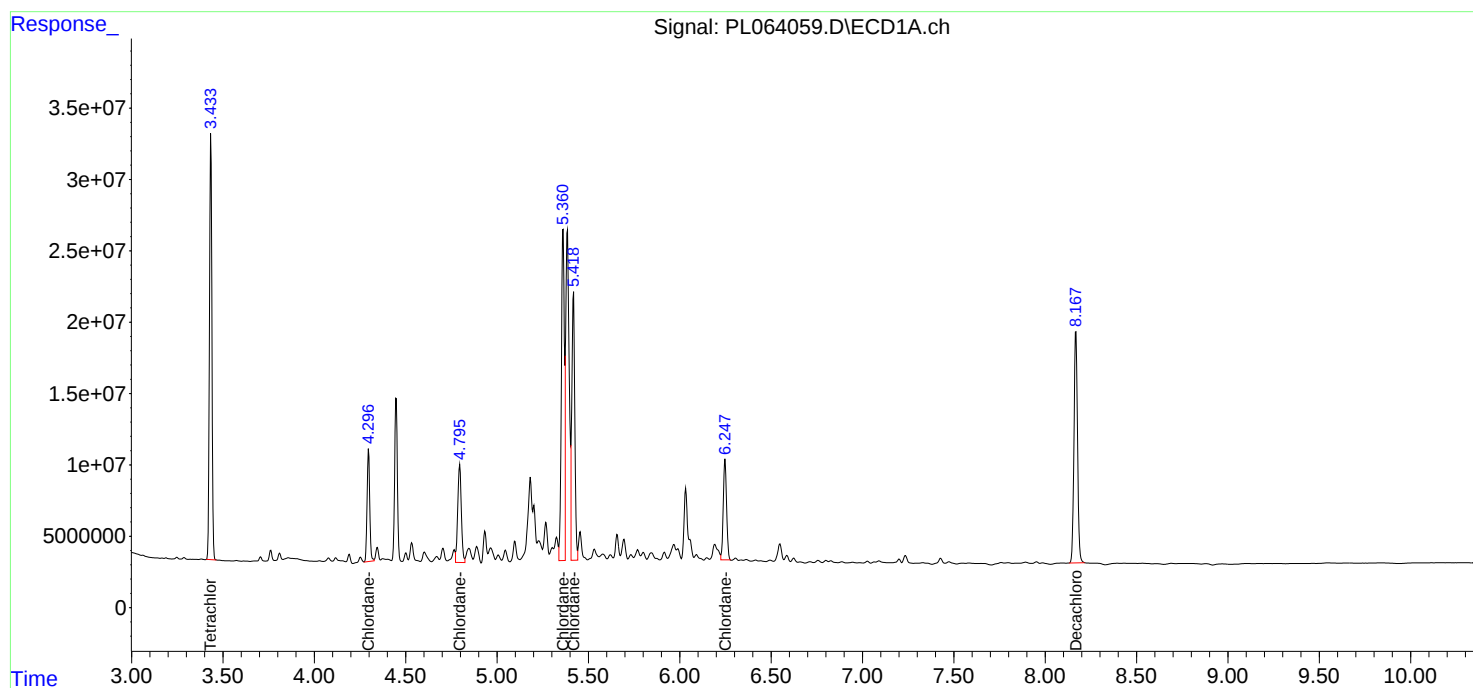


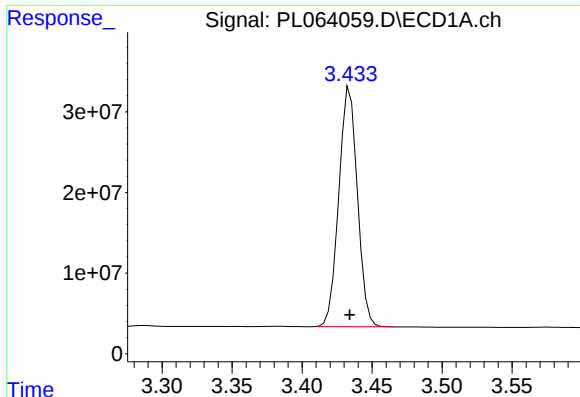

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 274628262
Conc: 73.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

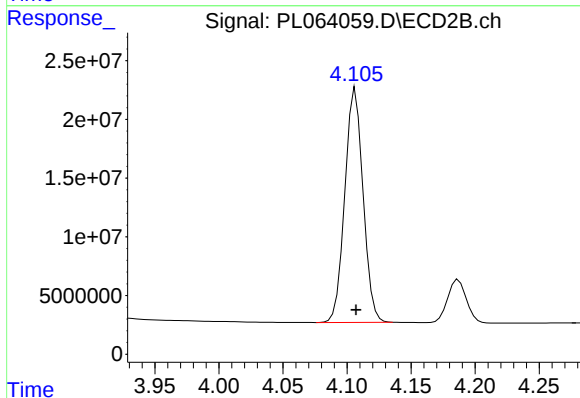


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 197491551
Conc: 74.37 ng/ml

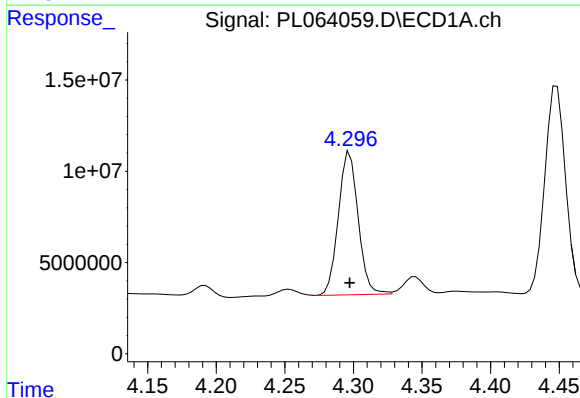


#23 Chlordane-1

R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 78834607
Conc: 737.79 ng/ml

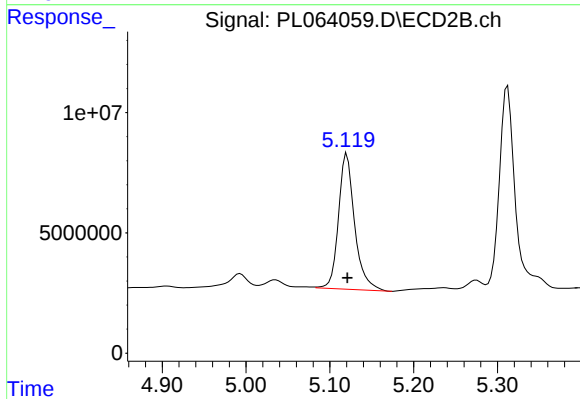

#23 Chlordane-1


R.T.: 5.120 min
Delta R.T.: 0.000 min
Response: 75637266
Conc: 717.78 ng/ml

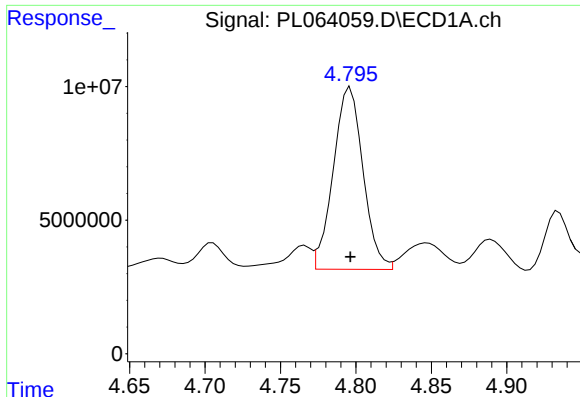

#24 Chlordane-2


R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 93610121
Conc: 699.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

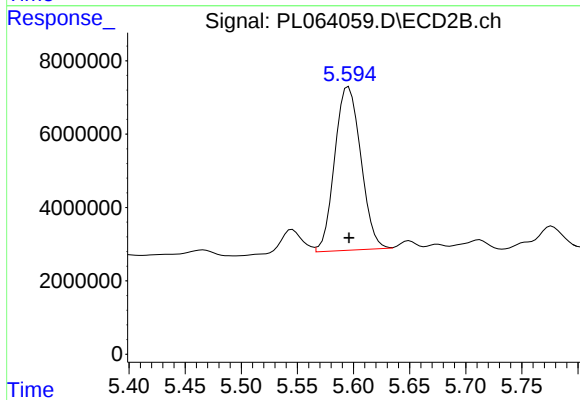


#24 Chlordane-2

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 72067923
Conc: 718.90 ng/ml

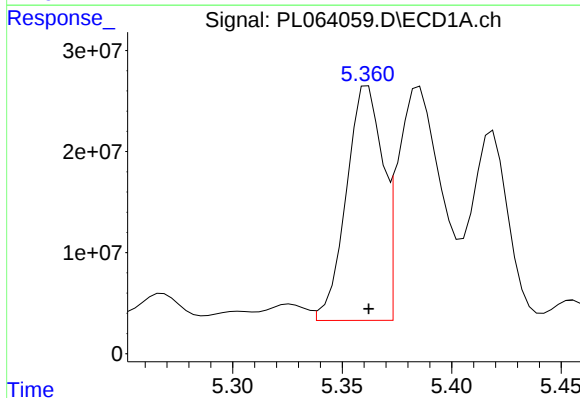


#25 Chlordane-3

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 265778282
Conc: 739.79 ng/ml

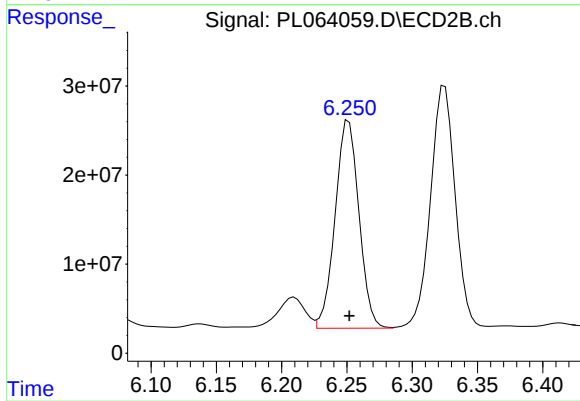

#25 Chlordane-3


R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 296833593
Conc: 748.65 ng/ml

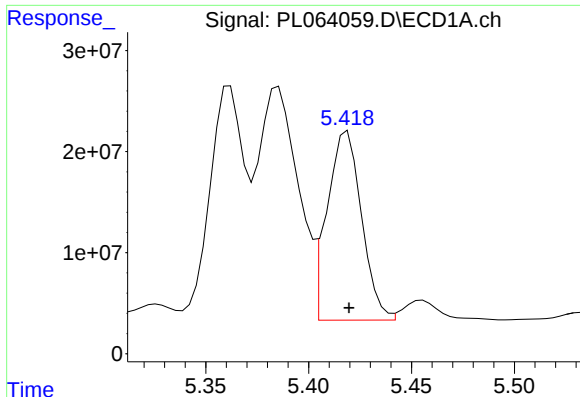

#26 Chlordane-4


R.T.: 5.419 min
Delta R.T.: 0.000 min
Response: 218088811
Conc: 732.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

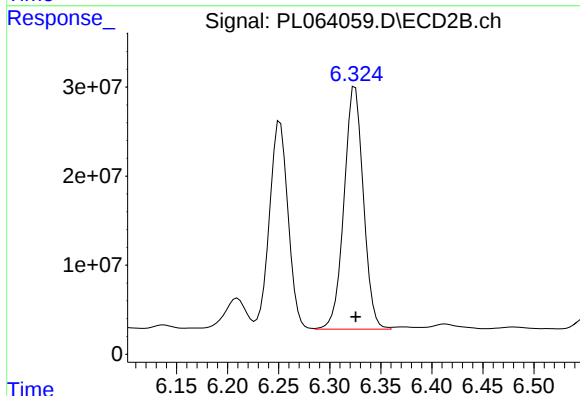


#26 Chlordane-4

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 359328535
Conc: 741.16 ng/ml

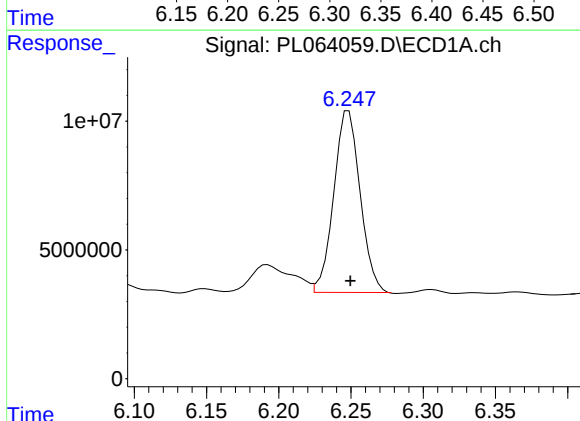


#27 Chlordane-5

R.T.: 6.248 min
Delta R.T.: -0.001 min
Response: 89516810
Conc: 728.53 ng/ml

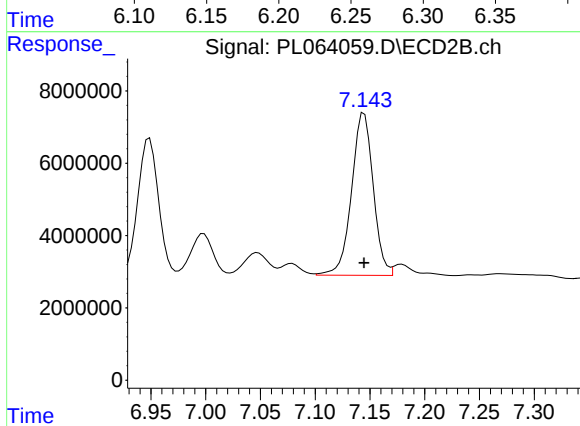

#27 Chlordane-5


R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 61856957
Conc: 737.17 ng/ml

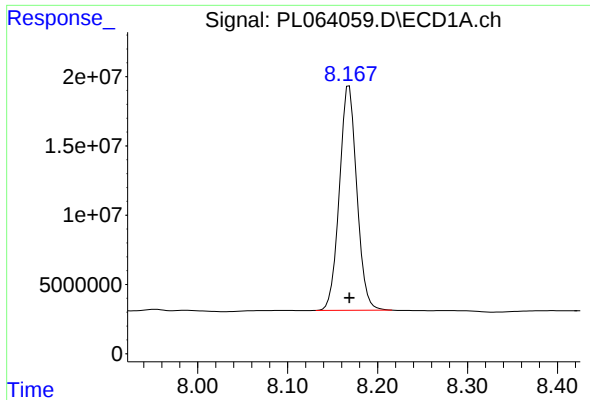

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 218260248
Conc: 73.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

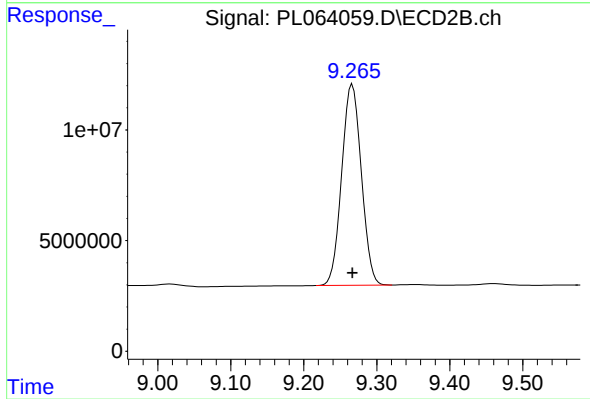

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: 0.000 min
Response: 169818646
Conc: 72.88 ng/ml