

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011221\
 Data File : PL064058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2021 16:02
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 04:47:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:46:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.107	359.5E6	255.5E6	95.922	96.201
28)	SA Decachlor...	8.170	9.267	269.7E6	213.0E6	91.184	91.436
Target Compounds							
23)	Chlordane-1	4.299	5.121	100.3E6	96121555	938.729	912.173
24)	Chlordane-2	4.797	5.597	117.4E6	91195541	876.652	909.703
25)	Chlordane-3	5.363	6.252	341.2E6	386.4E6	949.649	974.585
26)	Chlordane-4	5.420	6.326	280.6E6	463.9E6	942.370	956.849
27)	Chlordane-5	6.249	7.145	113.5E6	79178925	924.015	943.607



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011221\
Data File : PL064058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2021 16:02
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 04:47:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:46:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

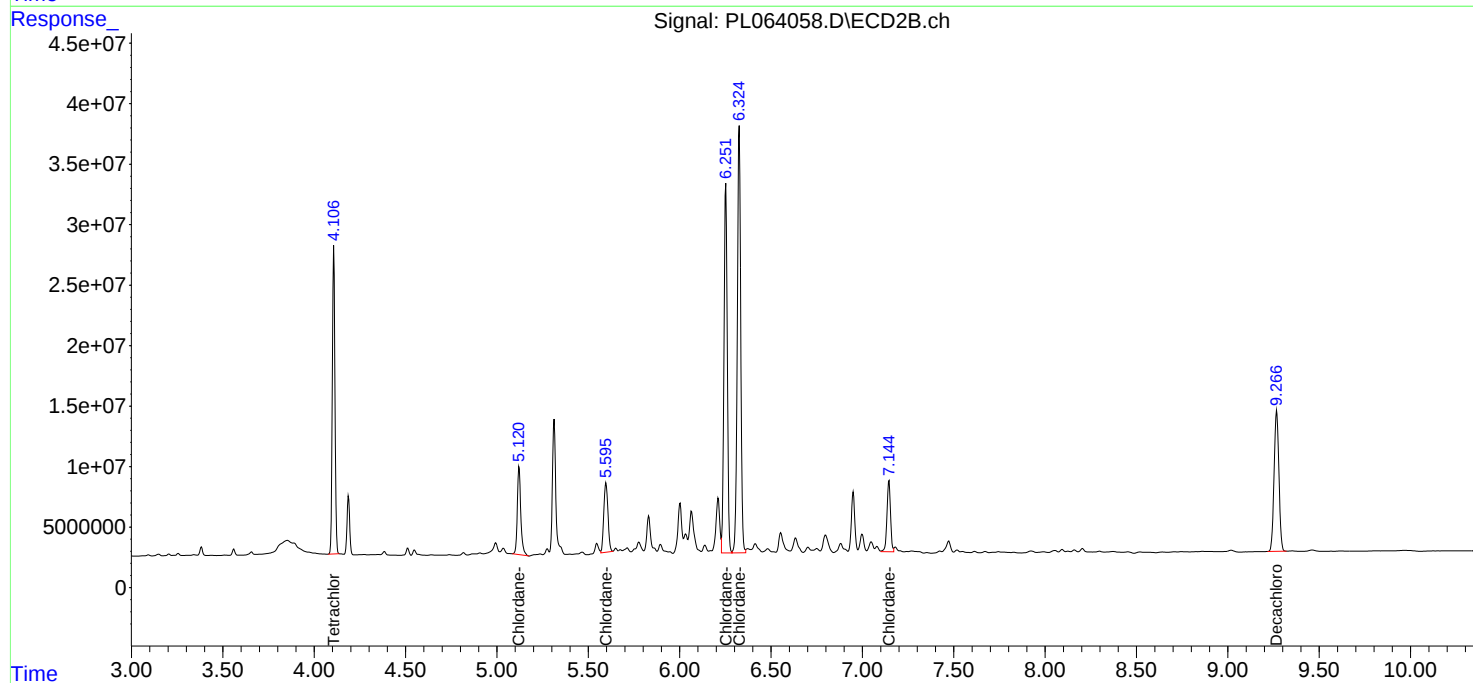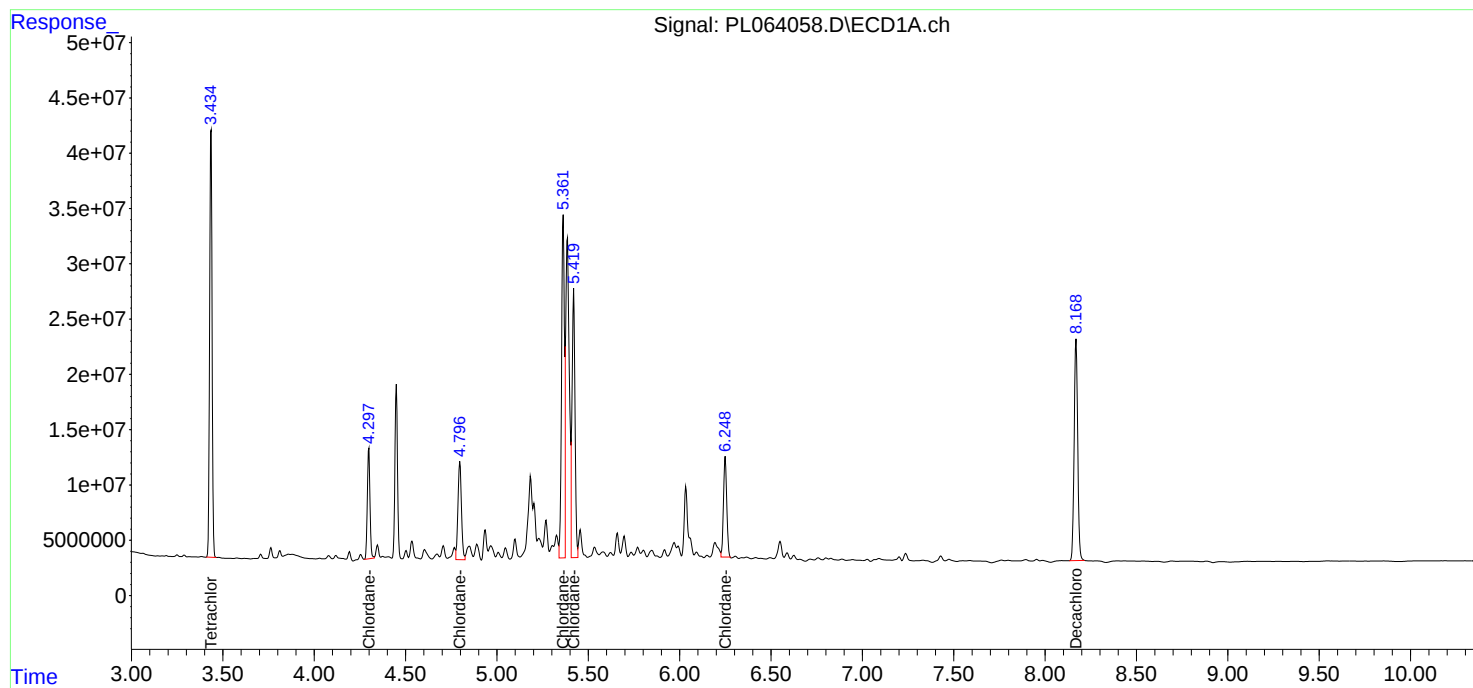


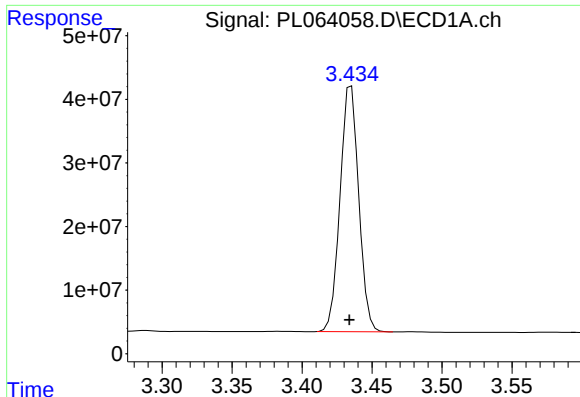

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.001 min
Response: 359529168
Conc: 95.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

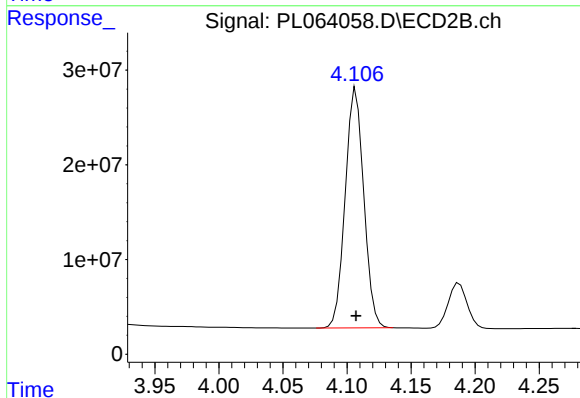


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 255476365
Conc: 96.20 ng/ml

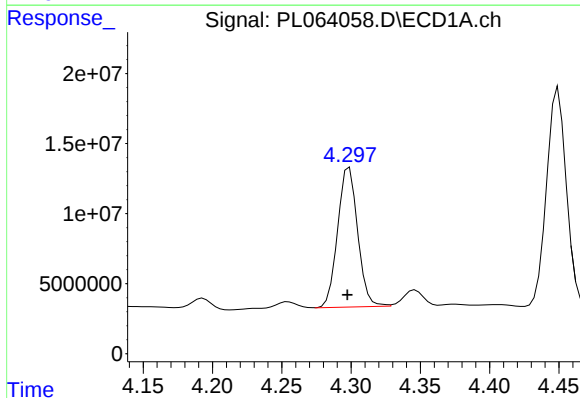


#23 Chlordane-1

R.T.: 4.299 min
Delta R.T.: 0.001 min
Response: 100306063
Conc: 938.73 ng/ml

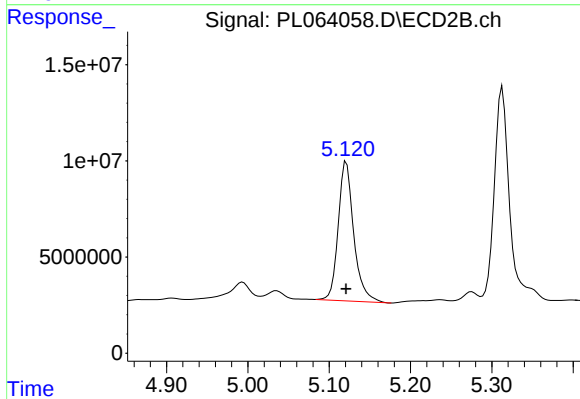

#23 Chlordane-1


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 96121555
Conc: 912.17 ng/ml

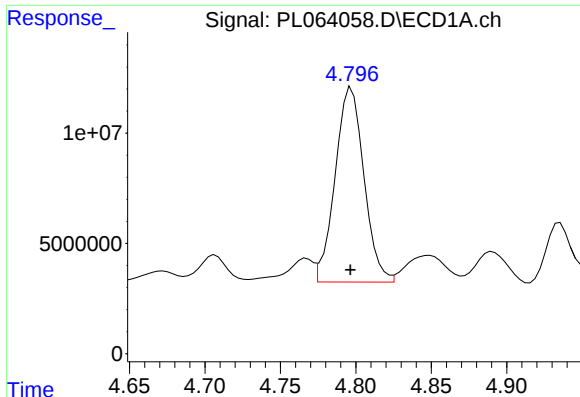

#24 Chlordane-2


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 117362862
Conc: 876.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

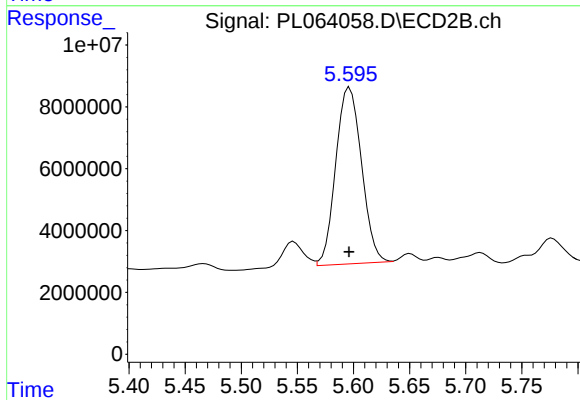


#24 Chlordane-2

R.T.: 5.597 min
Delta R.T.: 0.000 min
Response: 91195541
Conc: 909.70 ng/ml

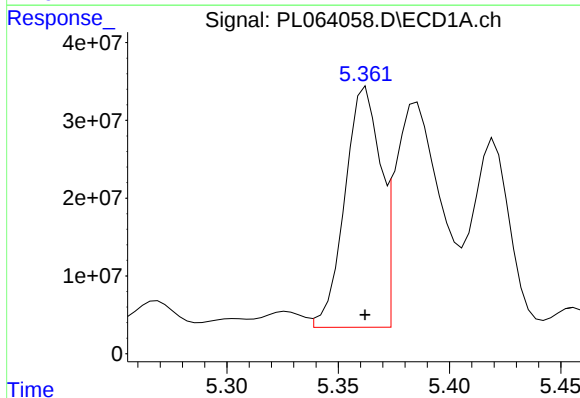


#25 Chlordane-3

R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 341173309
Conc: 949.65 ng/ml

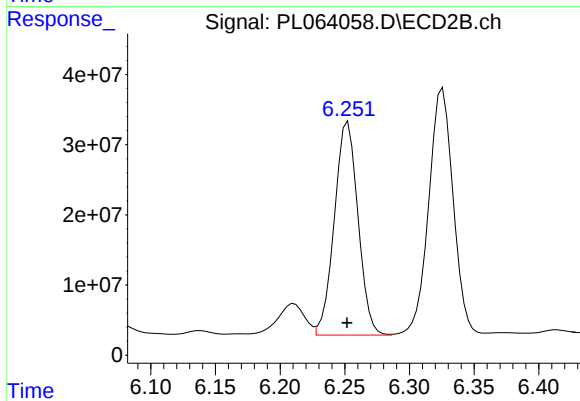

#25 Chlordane-3


R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 386412390
Conc: 974.58 ng/ml

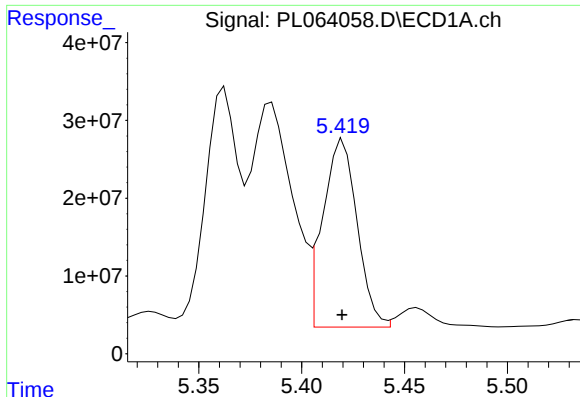

#26 Chlordane-4


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 280637240
Conc: 942.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

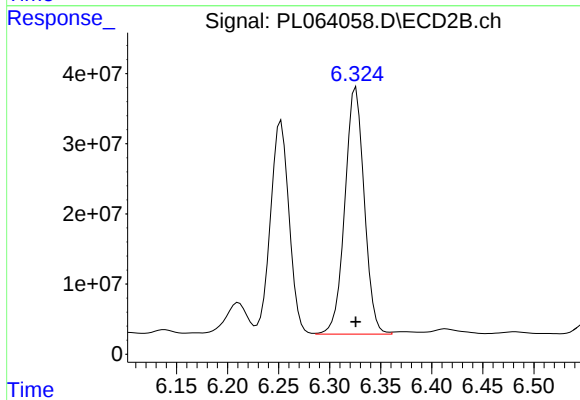


#26 Chlordane-4

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 463897018
Conc: 956.85 ng/ml

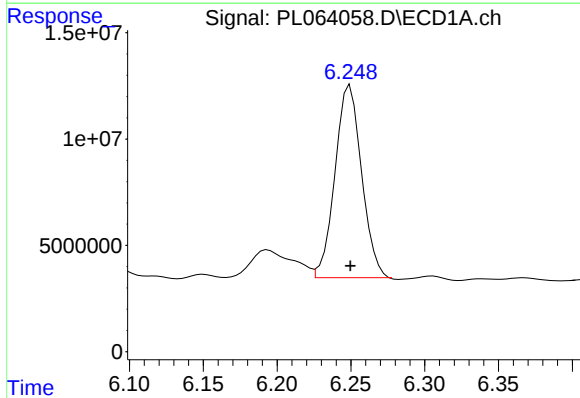


#27 Chlordane-5

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 113535874
Conc: 924.01 ng/ml

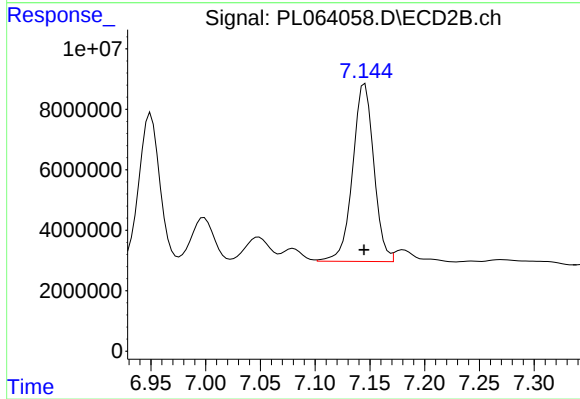

#27 Chlordane-5


R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 79178925
Conc: 943.61 ng/ml

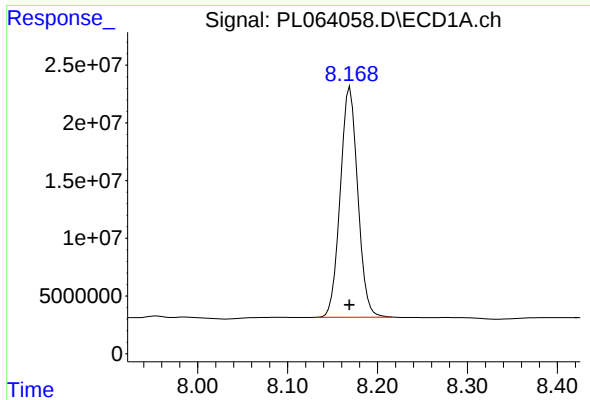

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.000 min
Response: 269700916
Conc: 91.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

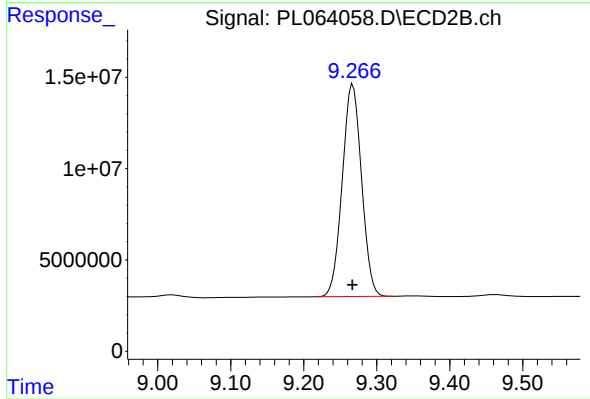

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: 0.000 min
Response: 213047686
Conc: 91.44 ng/ml