

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011221\
 Data File : PL064069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2021 18:39
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL011221

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 05:30:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 13 04:58:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.107	167.6E6	119.7E6	55.888	46.805
28)	SA Decachlor...	8.168	9.267	134.5E6	105.4E6	44.080	44.412
Target Compounds							
23)	Chlordane-1	4.298	5.121	48468941	48193032	453.604	457.342
24)	Chlordane-2	4.796	5.596	57836835	46049329	432.017	459.356
25)	Chlordane-3	5.361	6.252	159.6E6	178.2E6	444.259	449.504
26)	Chlordane-4	5.419	6.325	133.6E6	218.3E6	448.723	450.275
27)	Chlordane-5	6.248	7.145	54986789	37915593	447.511	451.855



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011221\
Data File : PL064069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2021 18:39
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
ICVPL011221

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 05:30:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Wed Jan 13 04:58:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

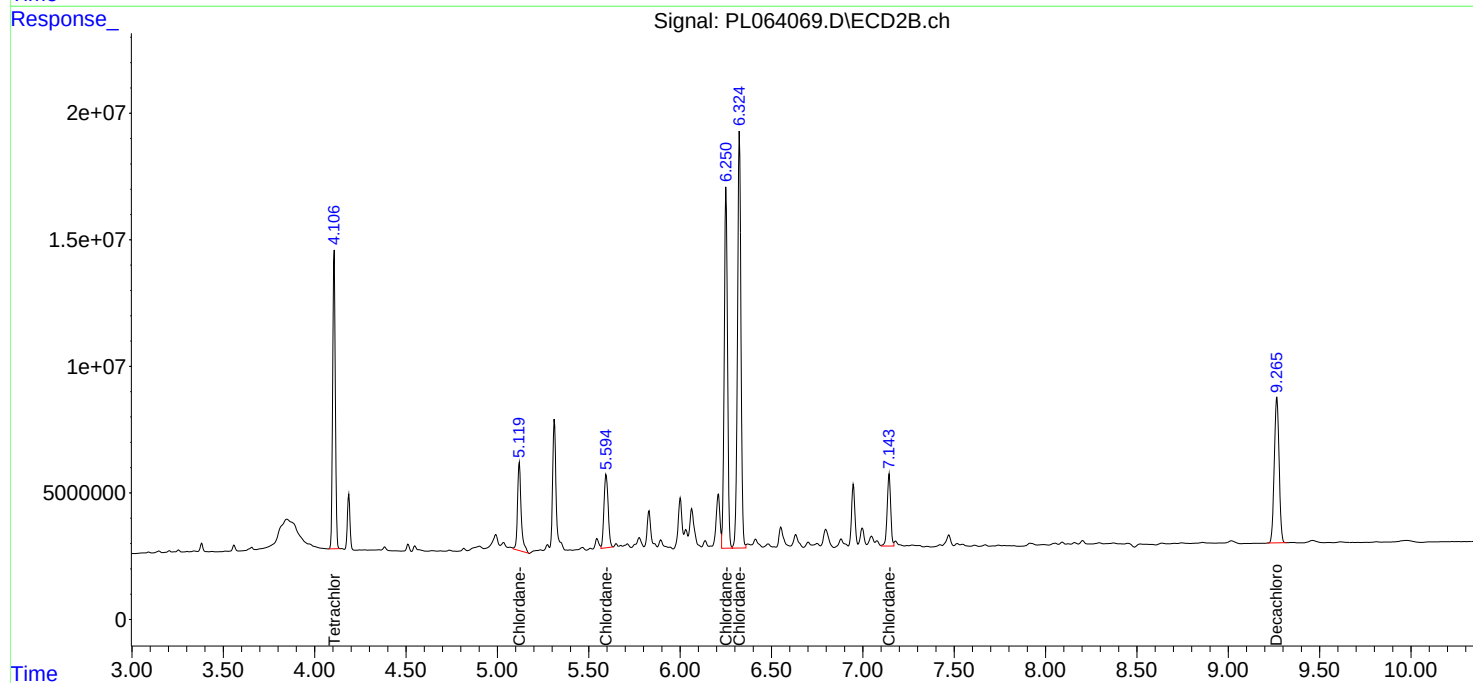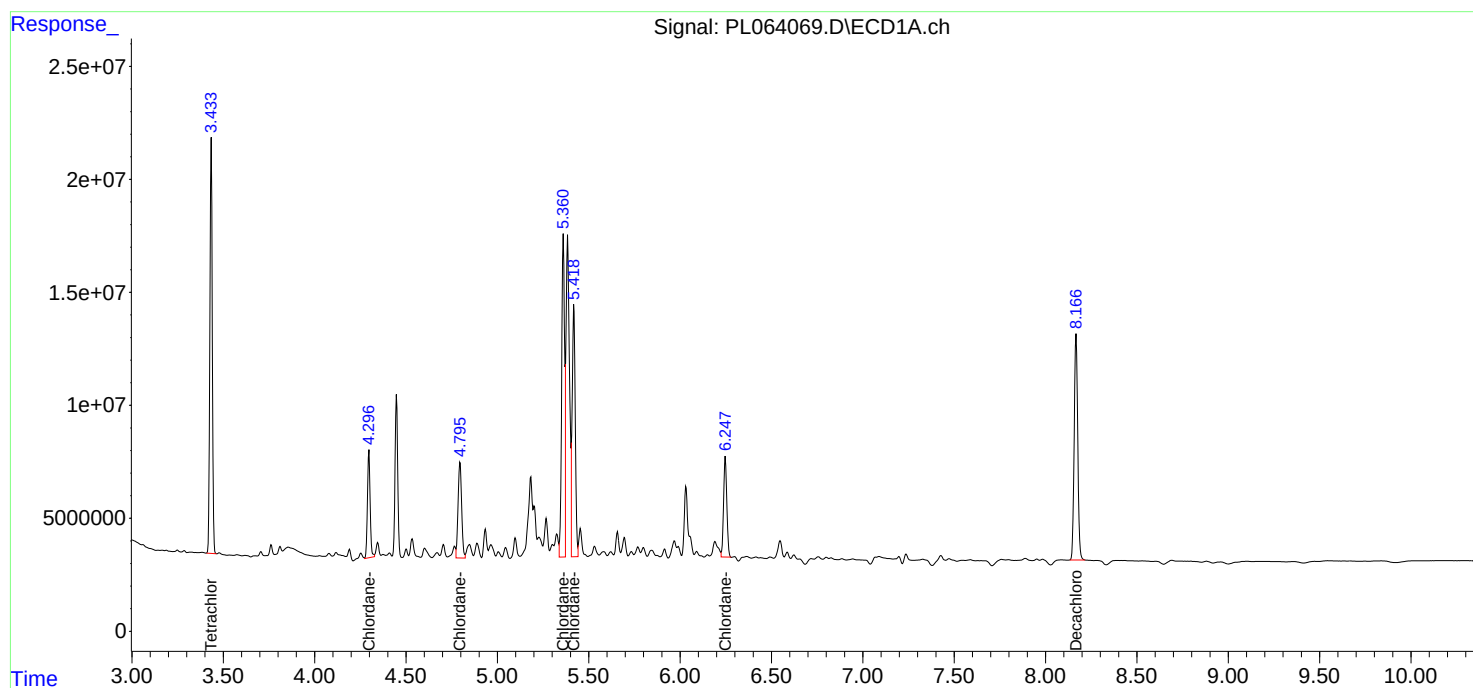


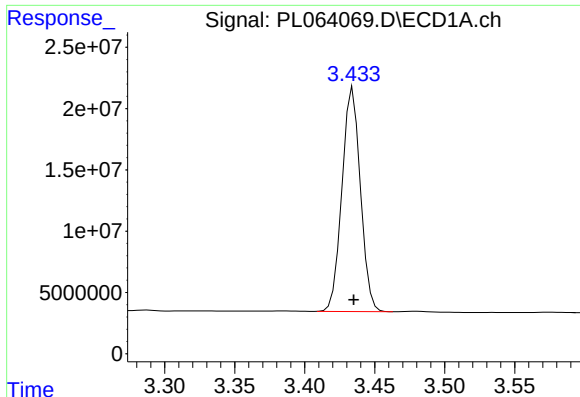

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 167580555
Conc: 55.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011221

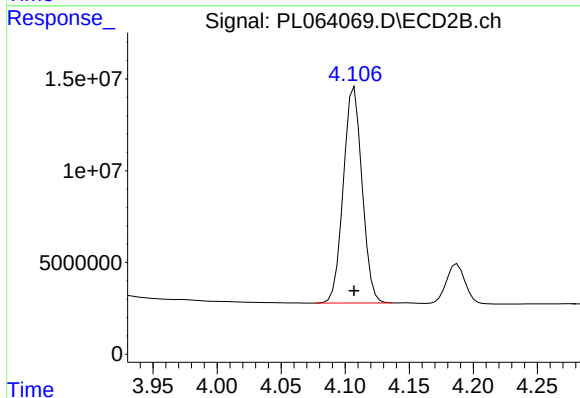


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 119654034
Conc: 46.80 ng/ml

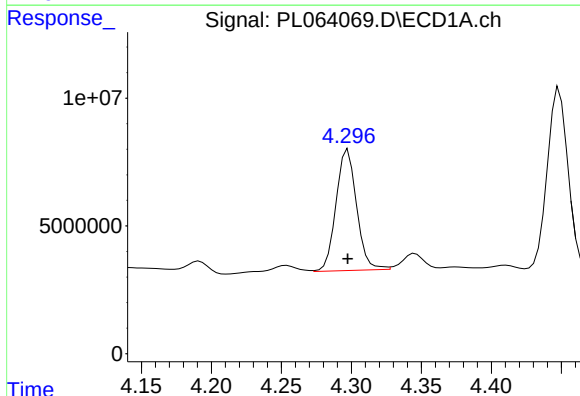


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 48468941
Conc: 453.60 ng/ml

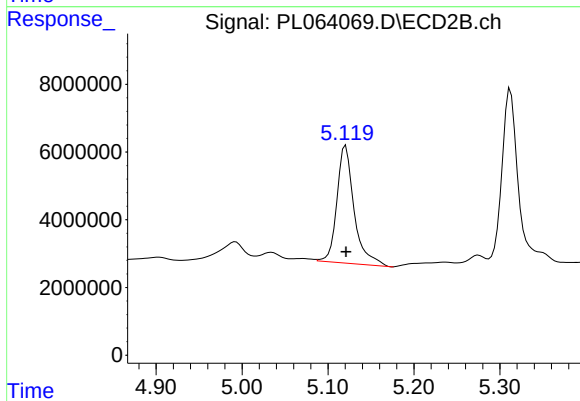

#23 Chlordane-1


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 48193032
Conc: 457.34 ng/ml

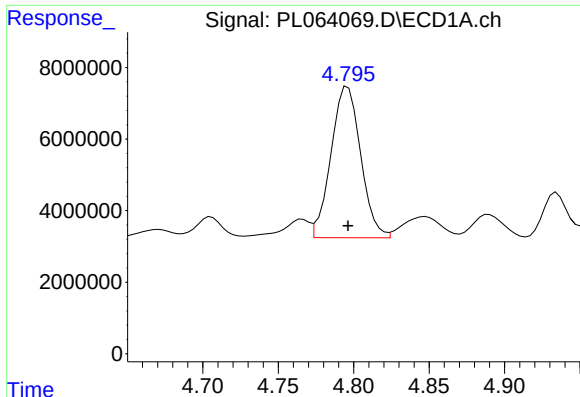

#24 Chlordane-2


R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 57836835
Conc: 432.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011221

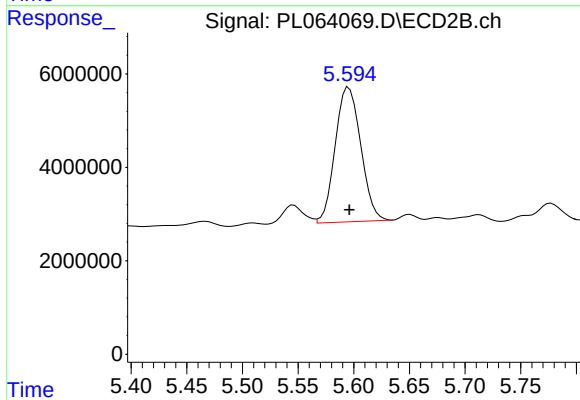


#24 Chlordane-2

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 46049329
Conc: 459.36 ng/ml

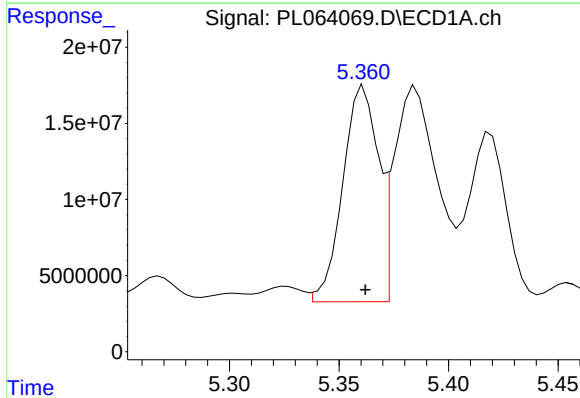


#25 Chlordane-3

R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 159605672
Conc: 444.26 ng/ml

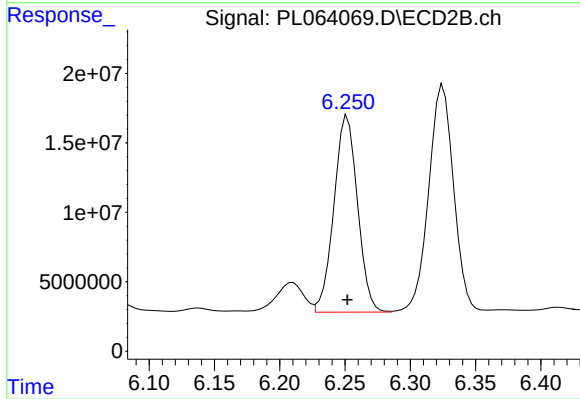

#25 Chlordane-3


R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 178223438
Conc: 449.50 ng/ml

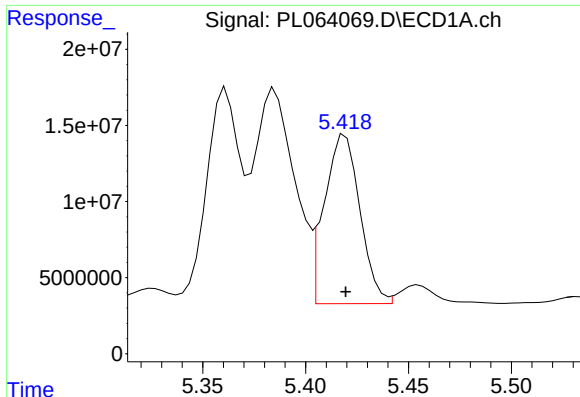

#26 Chlordane-4


R.T.: 5.419 min
Delta R.T.: 0.000 min
Response: 133629430
Conc: 448.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011221

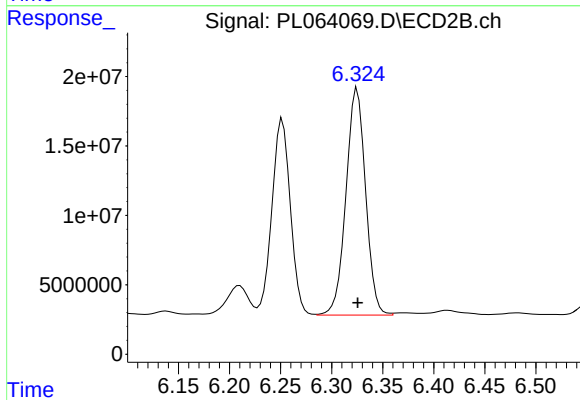


#26 Chlordane-4

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 218301297
Conc: 450.28 ng/ml

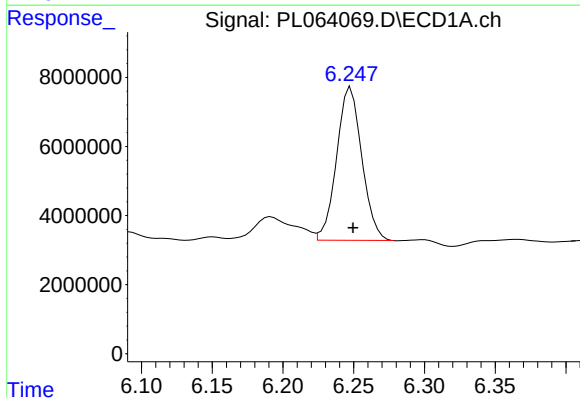


#27 Chlordane-5

R.T.: 6.248 min
Delta R.T.: -0.002 min
Response: 54986789
Conc: 447.51 ng/ml

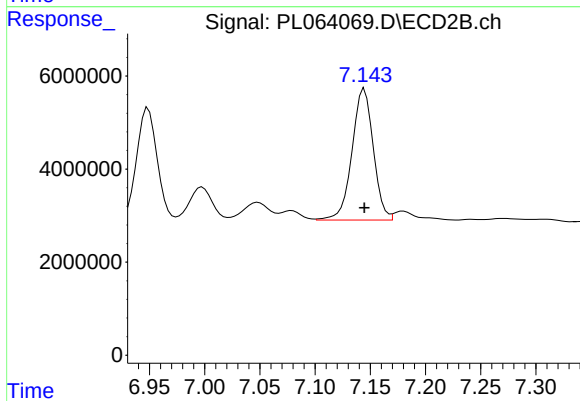

#27 Chlordane-5


R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 37915593
Conc: 451.86 ng/ml

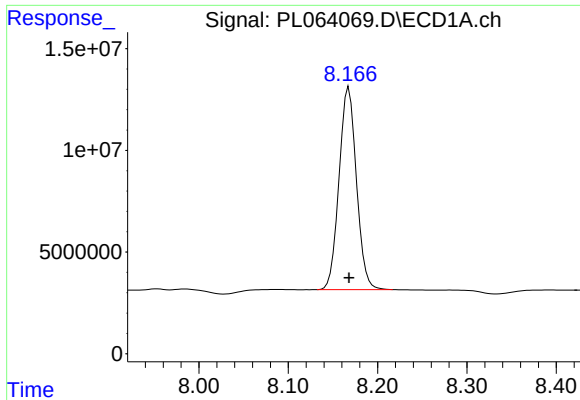

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 134536278
Conc: 44.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011221

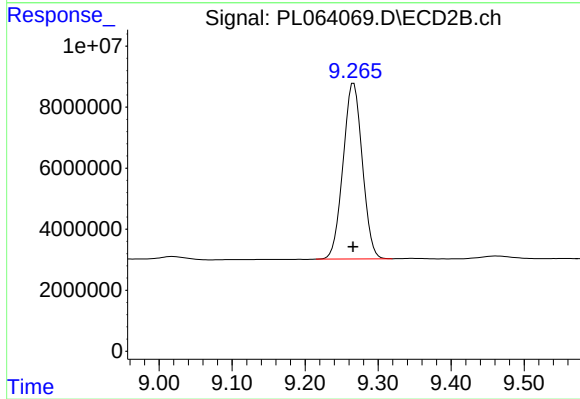

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: 0.000 min
Response: 105407195
Conc: 44.41 ng/ml