

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
 Data File : PL071954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 17:13
 Operator : AR\AJ
 Sample : N1099-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:13:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.493	6310173	17495463	13.660	14.240
28)	SA Decachlor...	10.320	11.386	11599883	18790512	16.044	15.857
Target Compounds							
7)	B delta-BHC	0.000	7.020f	0	421643	N.D.	0.275 #
9)	A Endosulfan I	0.000	8.359	0	125704	N.D.	0.101 #
10)	B gamma-Chl...	0.000	8.232	0	345085	N.D.	0.252 #
11)	B alpha-Chl...	0.000	8.280f	0	54529	N.D.	0.041 #
13)	MA Dieldrin	0.000	8.664f	0	67958	N.D.	0.052 #
25)	Chlordane-3	0.000	8.232	0	345085	N.D.	1.691 #
26)	Chlordane-4	0.000	8.280f	0	54529	N.D.	0.224 #
27)	Chlordane-5	0.000	9.164f	0	540618	N.D.	13.501 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
Data File : PL071954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 17:13
Operator : AR\AJ
Sample : N1099-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:13:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

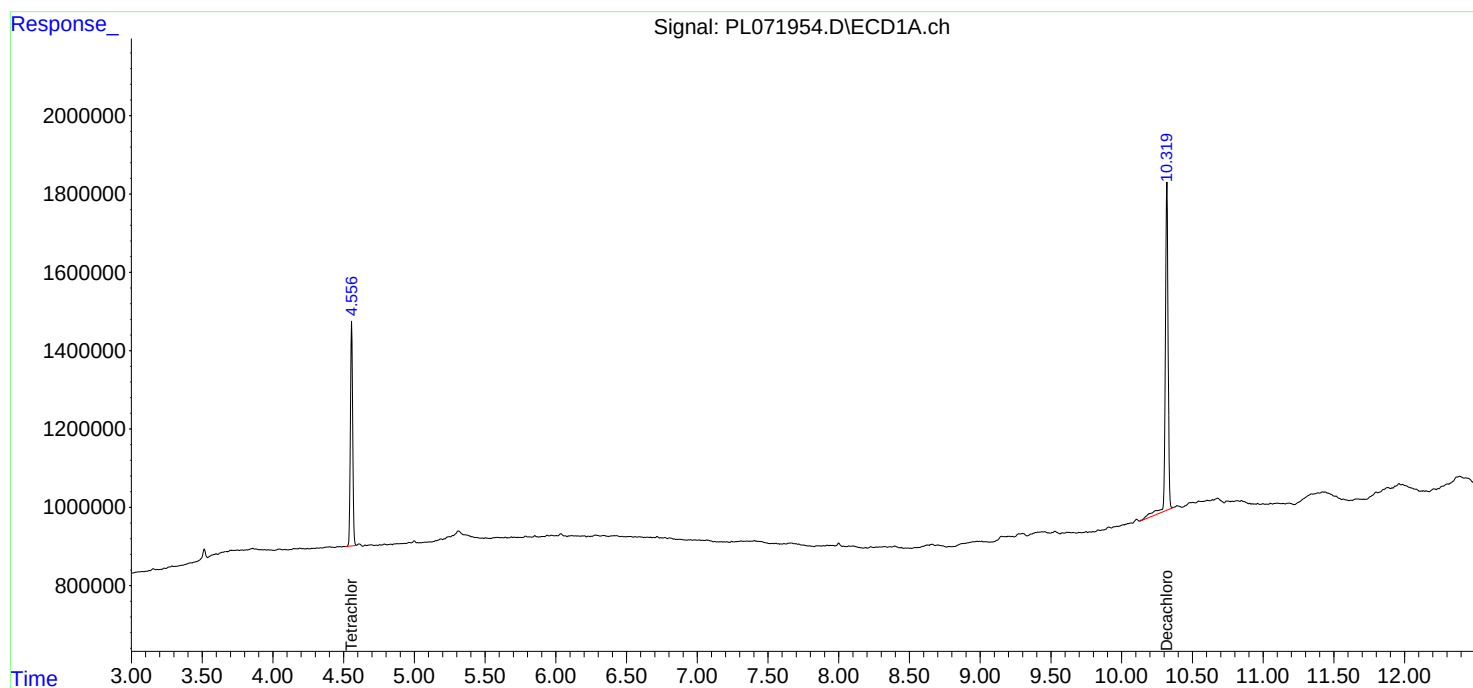


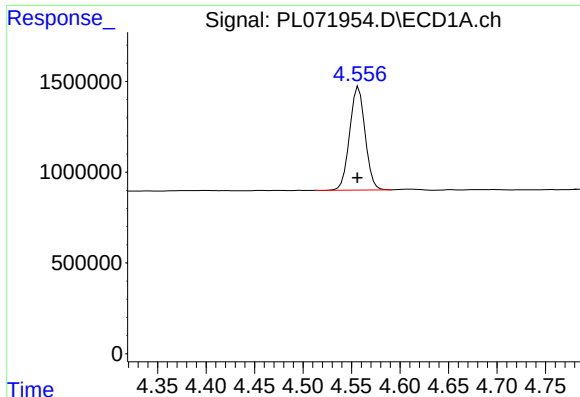

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 6310173
Conc: 13.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

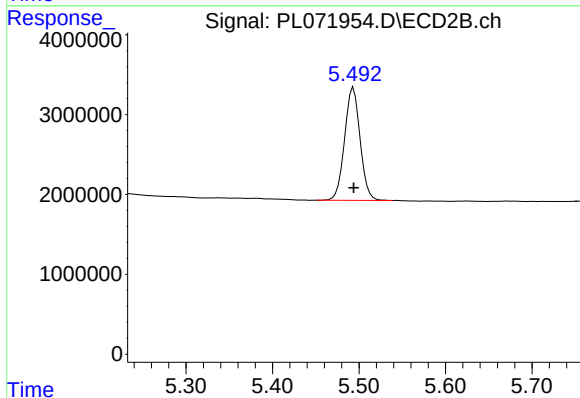


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 17495463
Conc: 14.24 ng/ml

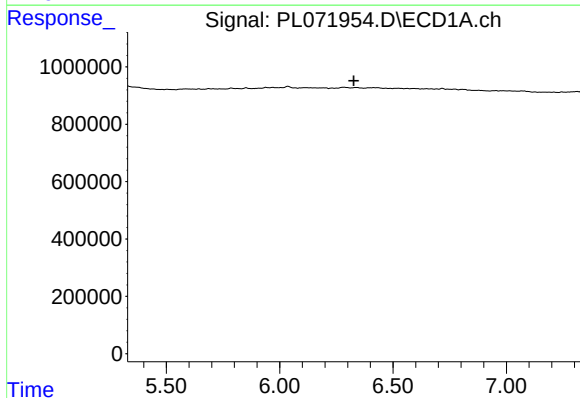


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

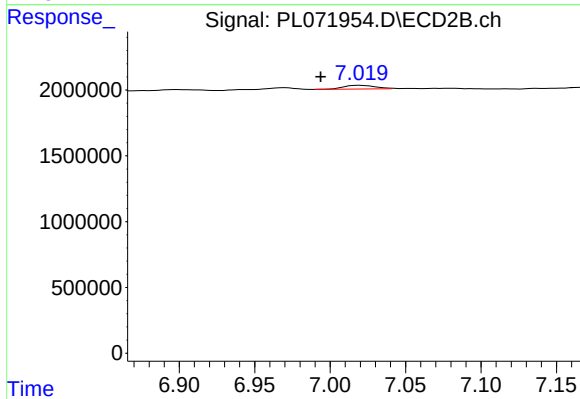

#7 delta-BHC


R.T.: 7.020 min
Delta R.T.: 0.027 min
Response: 421643
Conc: 0.27 ng/ml

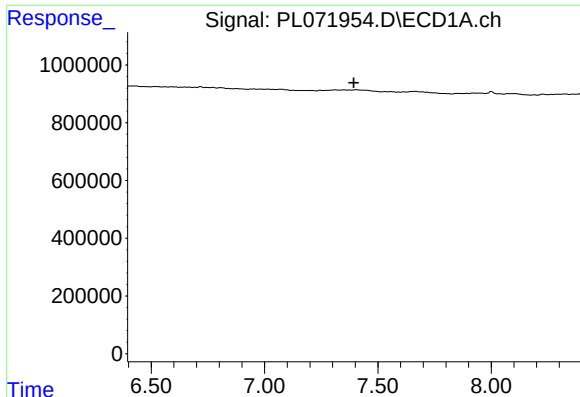

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

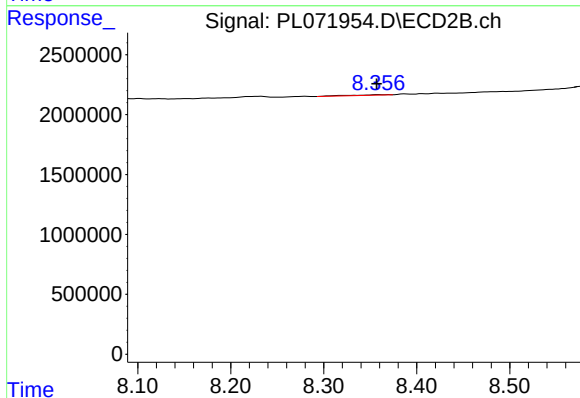


#9 Endosulfan I

R.T.: 8.359 min
Delta R.T.: 0.002 min
Response: 125704
Conc: 0.10 ng/ml

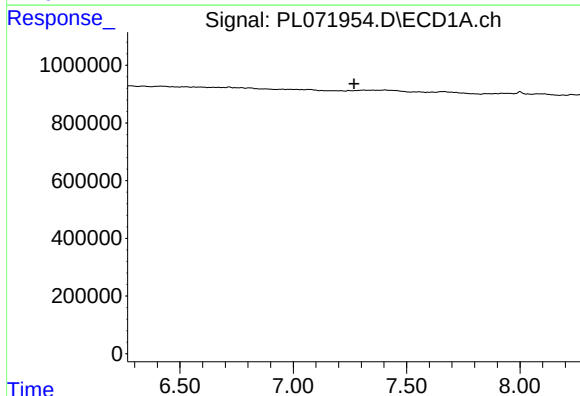


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

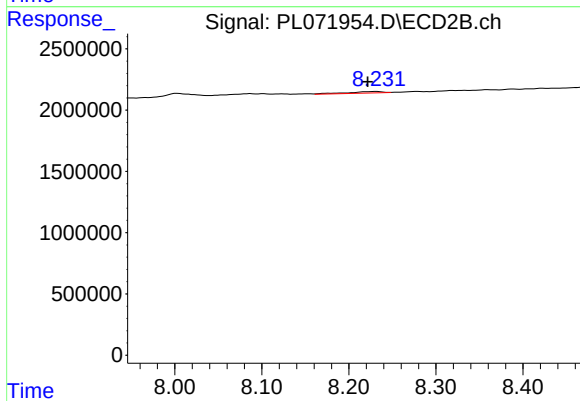

#10 gamma-Chlordane


R.T.: 8.232 min
Delta R.T.: 0.011 min
Response: 345085
Conc: 0.25 ng/ml

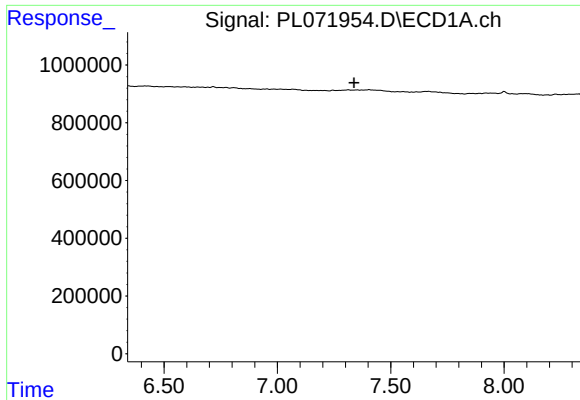

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

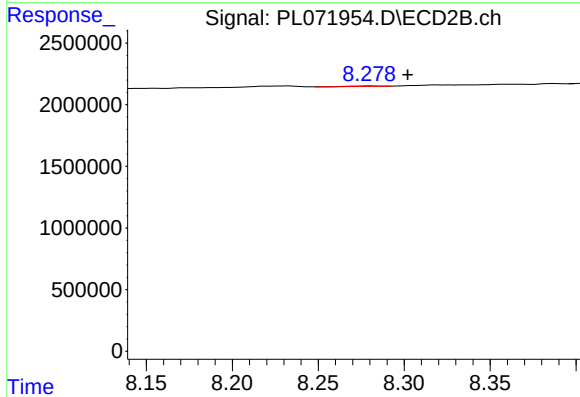


#11 alpha-Chlordane

R.T.: 8.280 min
Delta R.T.: -0.022 min
Response: 54529
Conc: 0.04 ng/ml

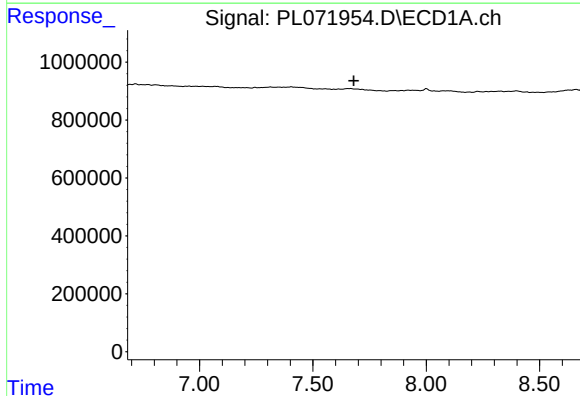


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.680 min
Response: 0
Conc: N.D.

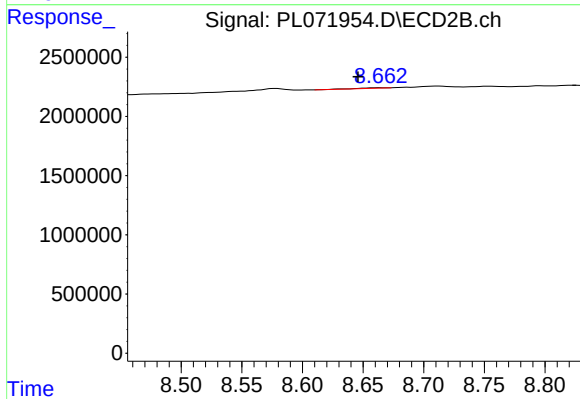

#13 Dieldrin


R.T.: 8.664 min
Delta R.T.: 0.018 min
Response: 67958
Conc: 0.05 ng/ml

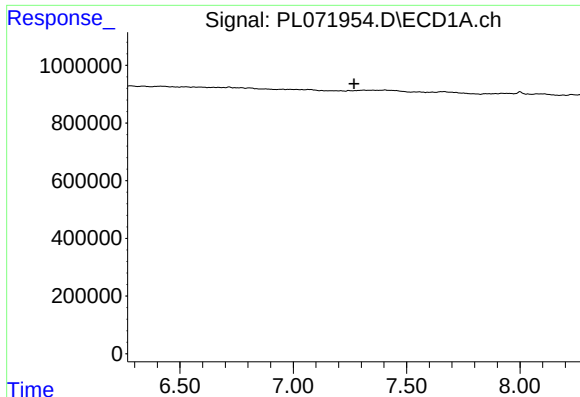

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

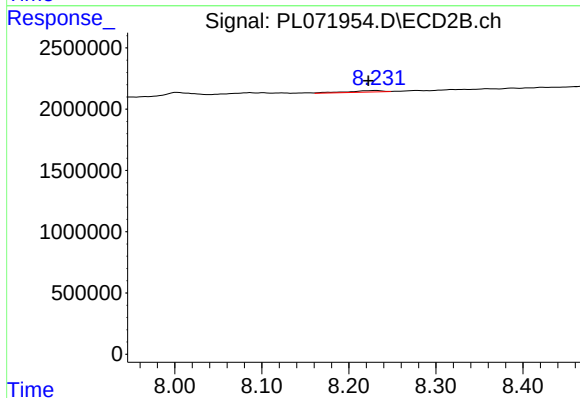


#25 Chlordane-3

R.T.: 8.232 min
Delta R.T.: 0.010 min
Response: 345085
Conc: 1.69 ng/ml

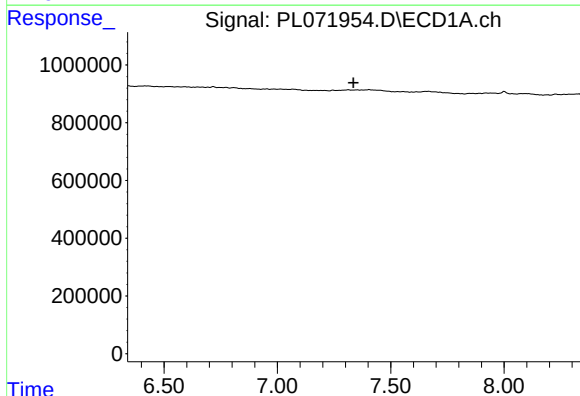


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

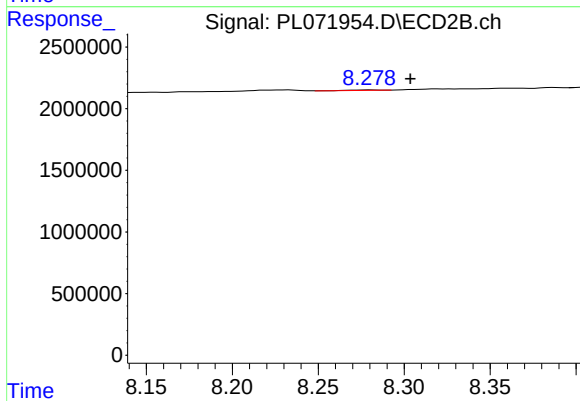

#26 Chlordane-4


R.T.: 8.280 min
Delta R.T.: -0.024 min
Response: 54529
Conc: 0.22 ng/ml

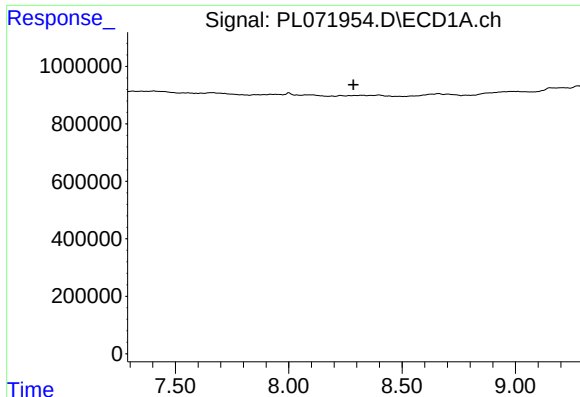

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

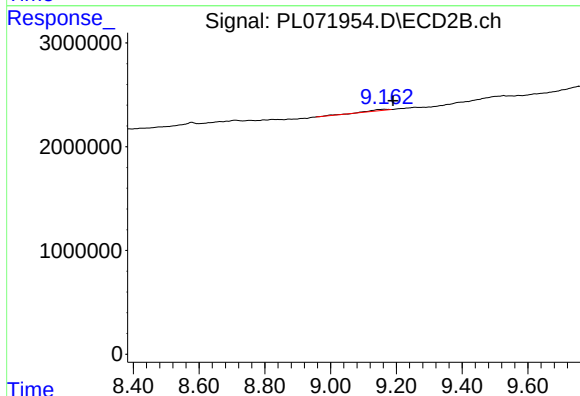


#27 Chlorine-5

R.T.: 9.164 min
Delta R.T.: -0.025 min
Response: 540618
Conc: 13.50 ng/ml

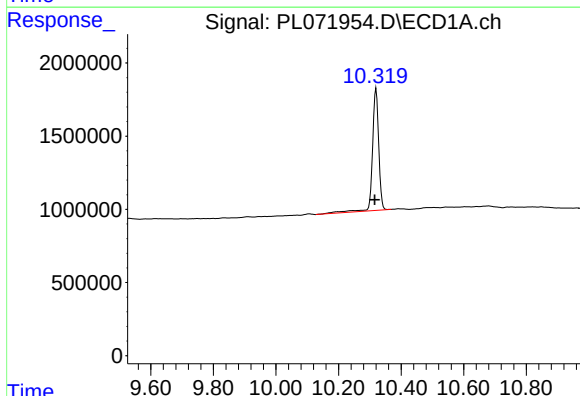

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: 0.004 min
Response: 11599883
Conc: 16.04 ng/ml

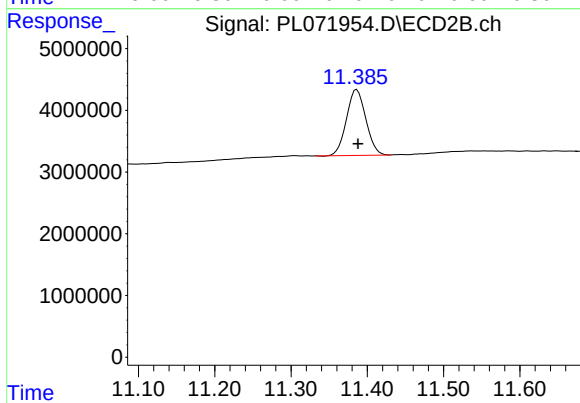

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.002 min
Response: 18790512
Conc: 15.86 ng/ml