

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
 Data File : PL071955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 17:29
 Operator : AR\AJ
 Sample : N1099-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:14:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.493	5856515	16474567	12.678	13.409
28)	SA Decachlor...	10.320	11.386	9925407	17827842	13.728	15.044
Target Compounds							
7)	B delta-BHC	0.000	7.019f	0	332465	N.D.	0.217 #
9)	A Endosulfan I	0.000	8.335f	0	51378	N.D.	0.041 #
10)	B gamma-Chl...	0.000	8.222	0	241936	N.D.	0.177 #
11)	B alpha-Chl...	0.000	8.315	0	184307	N.D.	0.138 #
15)	B Endosulfa...	0.000	9.151f	0	279913	N.D.	0.249 #
16)	A 4,4'-DDD	0.000	9.036	0	97155	N.D.	0.101 #
19)	B Endosulfa...	0.000	9.509f	0	110089	N.D.	0.106 #
25)	Chlordane-3	0.000	8.222	0	241936	N.D.	1.185 #
26)	Chlordane-4	0.000	8.315	0	184307	N.D.	0.757 #
27)	Chlordane-5	0.000	9.183	0	16912	N.D.	0.422 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
Data File : PL071955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 17:29
Operator : AR\AJ
Sample : N1099-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:14:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

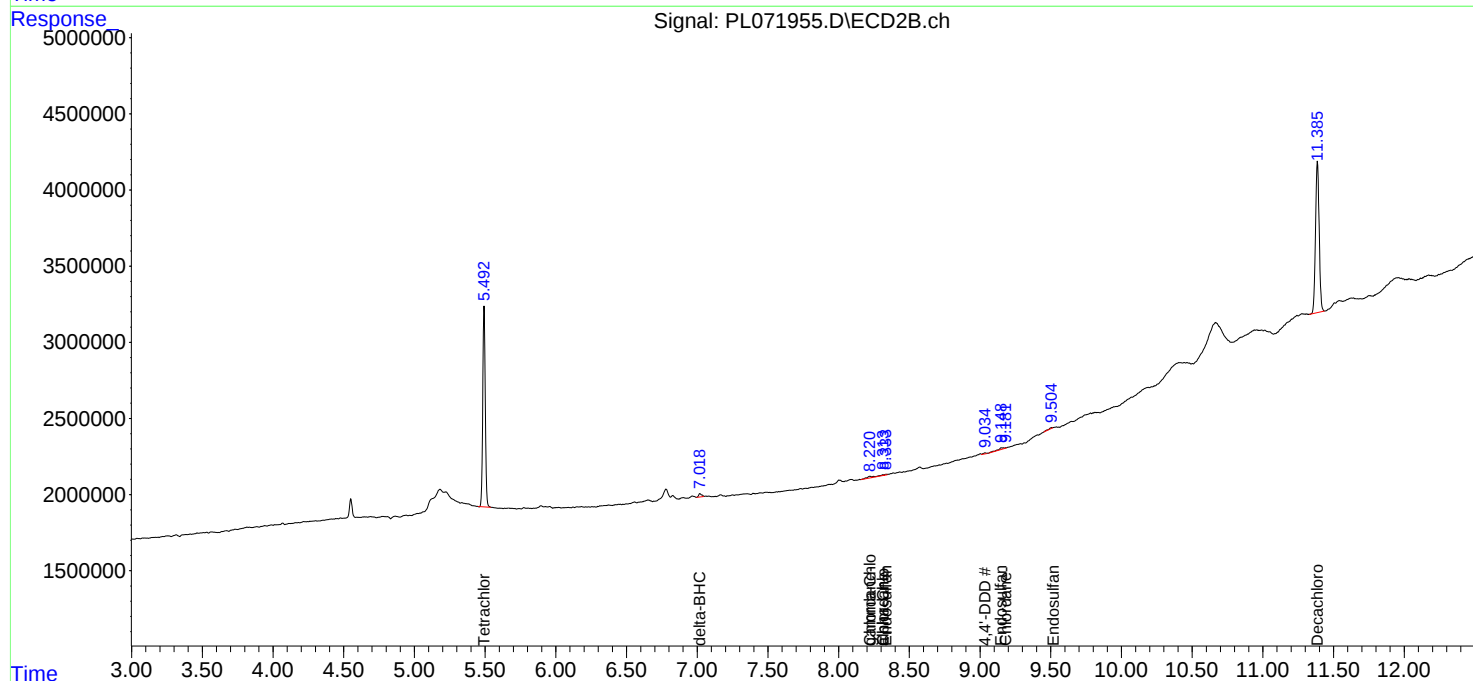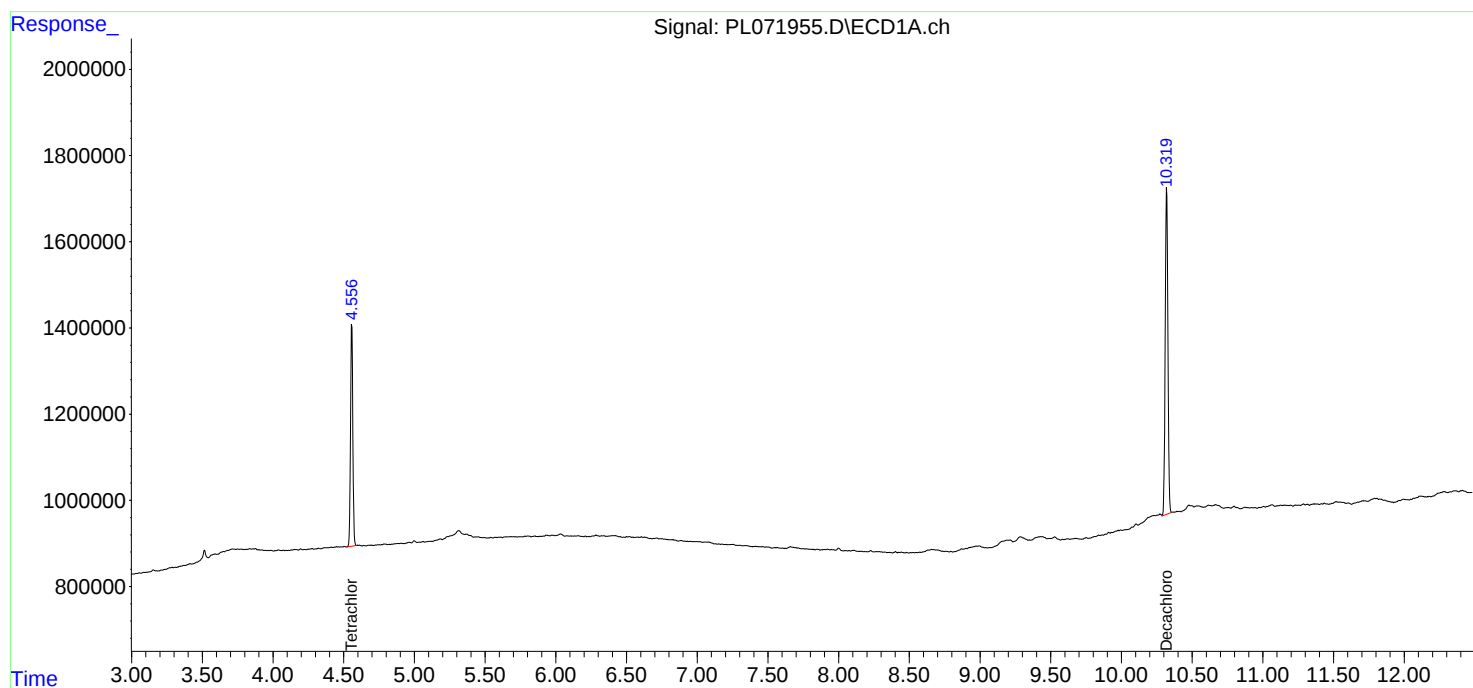


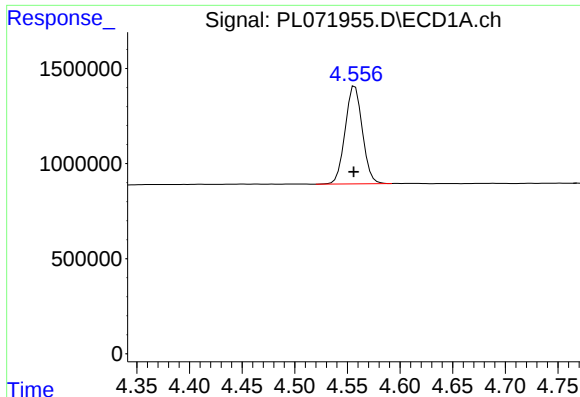

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 5856515
Conc: 12.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

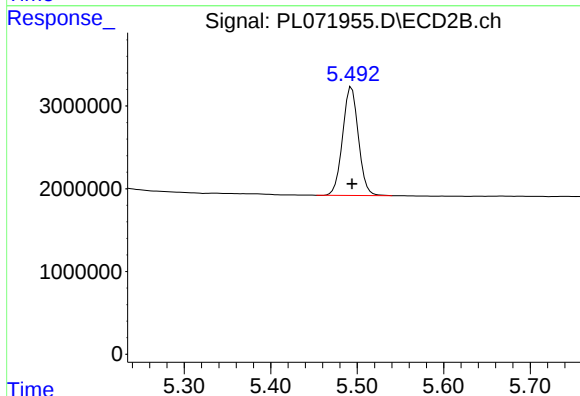


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 16474567
Conc: 13.41 ng/ml

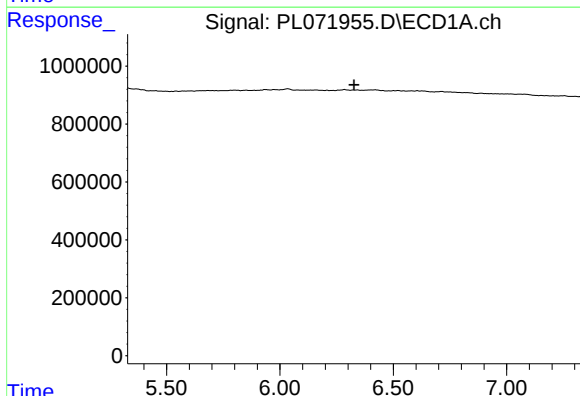


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

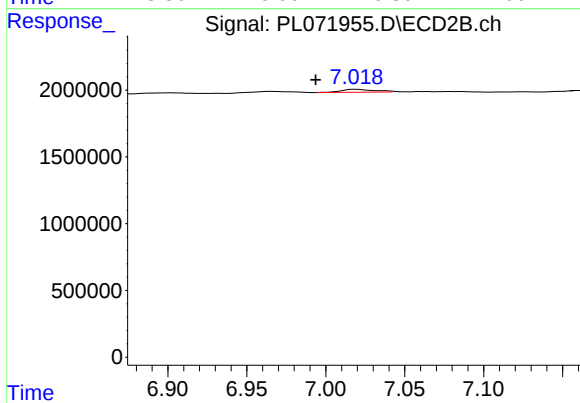

#7 delta-BHC


R.T.: 7.019 min
Delta R.T.: 0.026 min
Response: 332465
Conc: 0.22 ng/ml

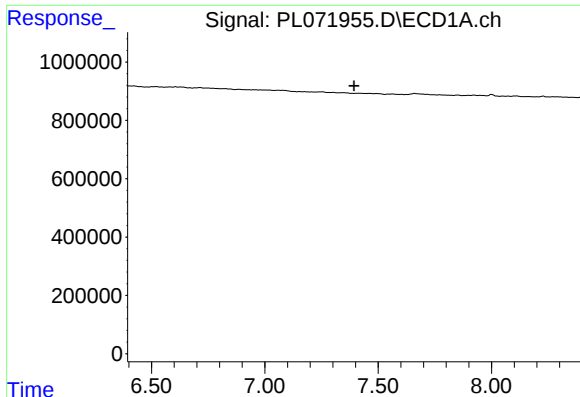

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

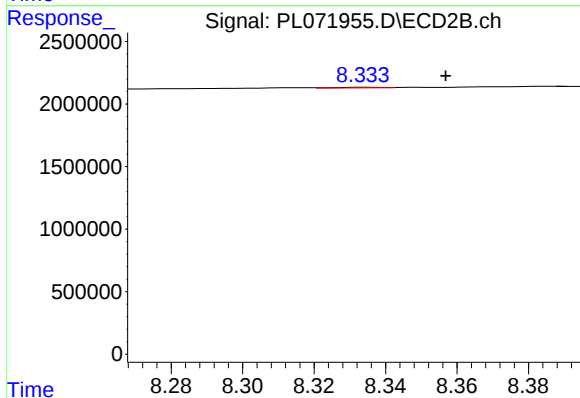


#9 Endosulfan I

R.T.: 8.335 min
Delta R.T.: -0.022 min
Response: 51378
Conc: 0.04 ng/ml

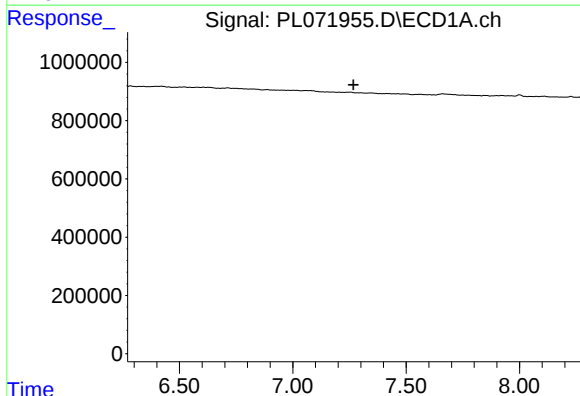


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

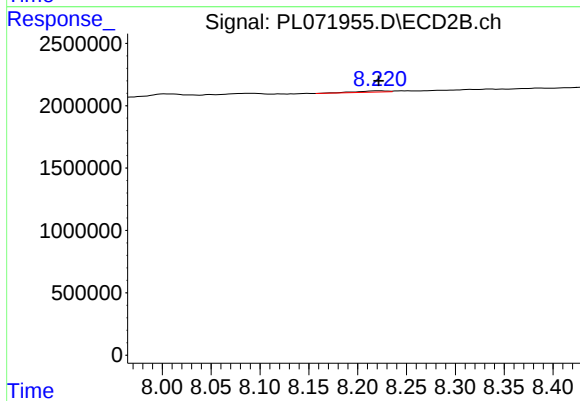

#10 gamma-Chlordane


R.T.: 8.222 min
Delta R.T.: 0.000 min
Response: 241936
Conc: 0.18 ng/ml

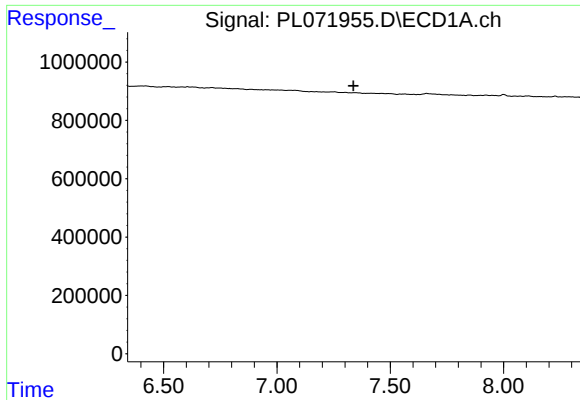

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

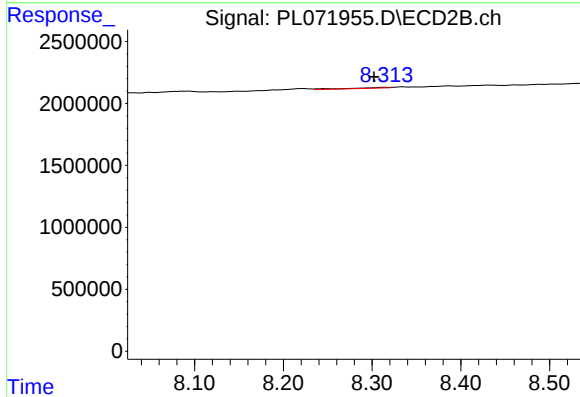


#11 alpha-Chlordane

R.T.: 8.315 min
Delta R.T.: 0.012 min
Response: 184307
Conc: 0.14 ng/ml

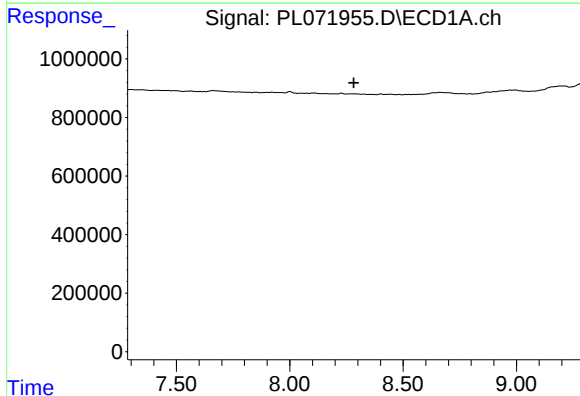


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

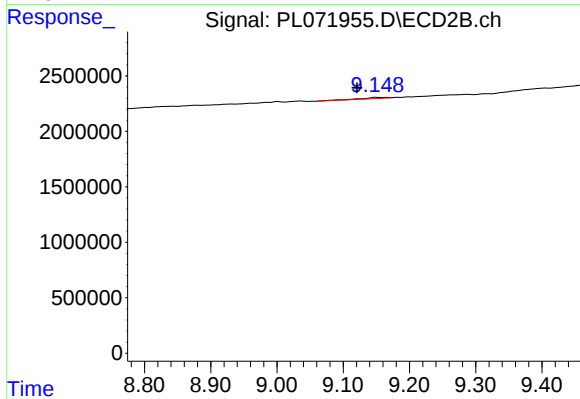

#15 Endosulfan II


R.T.: 9.151 min
Delta R.T.: 0.030 min
Response: 279913
Conc: 0.25 ng/ml

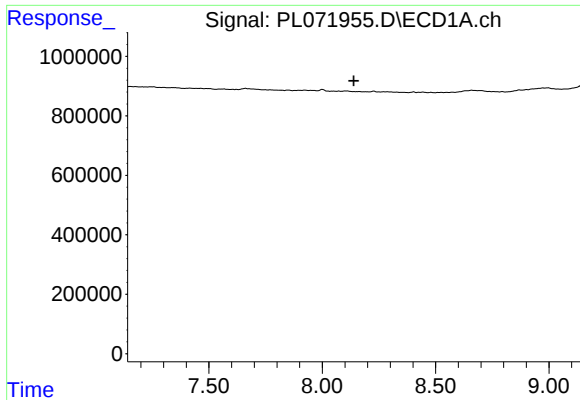

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

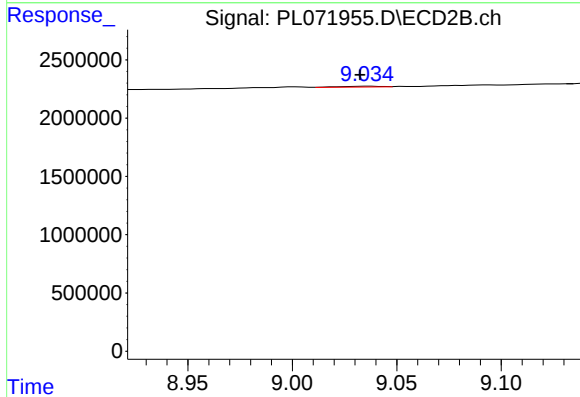


#16 4,4'-DDD

R.T.: 9.036 min
Delta R.T.: 0.003 min
Response: 97155
Conc: 0.10 ng/ml

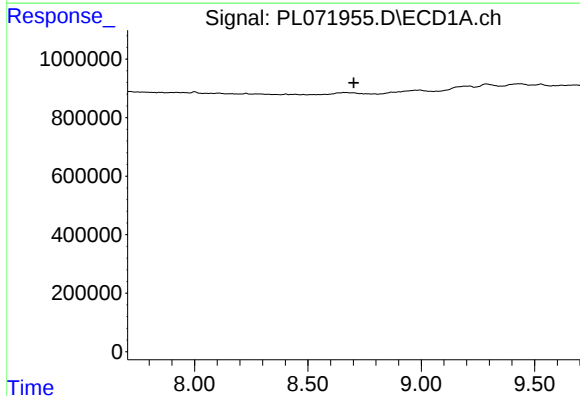


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

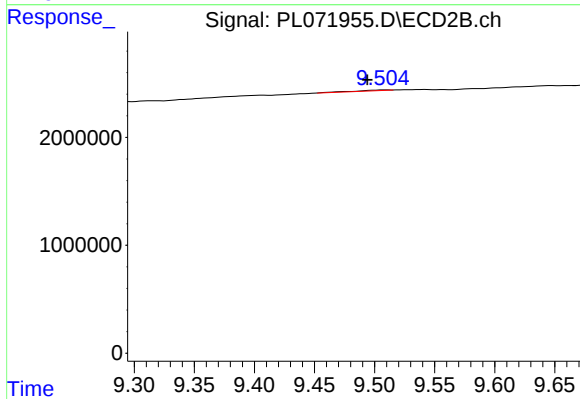

#19 Endosulfan Sulfate


R.T.: 9.509 min
Delta R.T.: 0.015 min
Response: 110089
Conc: 0.11 ng/ml

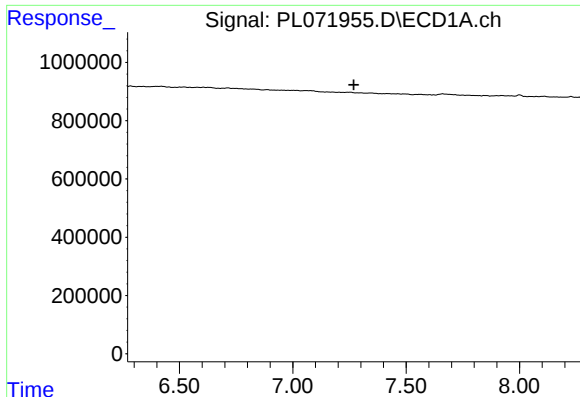

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

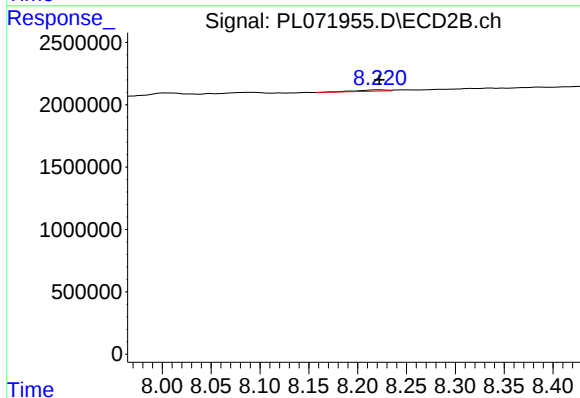


#25 Chlordane-3

R.T.: 8.222 min
Delta R.T.: 0.000 min
Response: 241936
Conc: 1.19 ng/ml

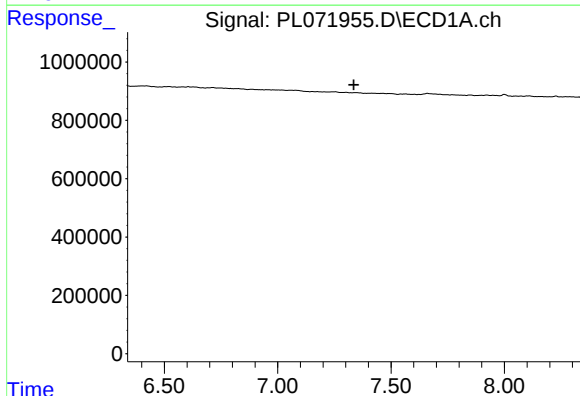


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

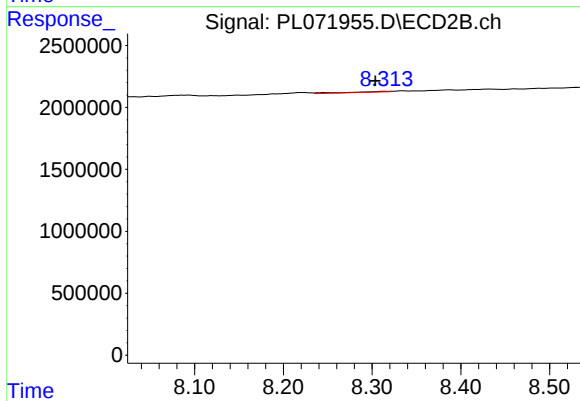

#26 Chlordane-4


R.T.: 8.315 min
Delta R.T.: 0.011 min
Response: 184307
Conc: 0.76 ng/ml

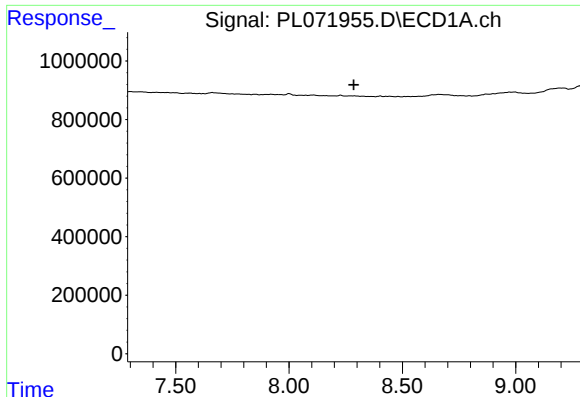

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

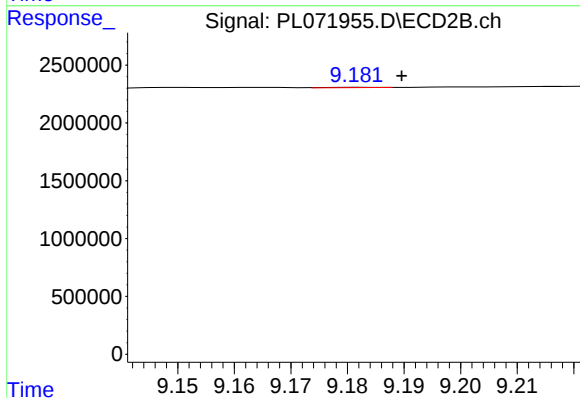


#27 Chlorodane-5

R.T.: 9.183 min
Delta R.T.: -0.007 min
Response: 16912
Conc: 0.42 ng/ml

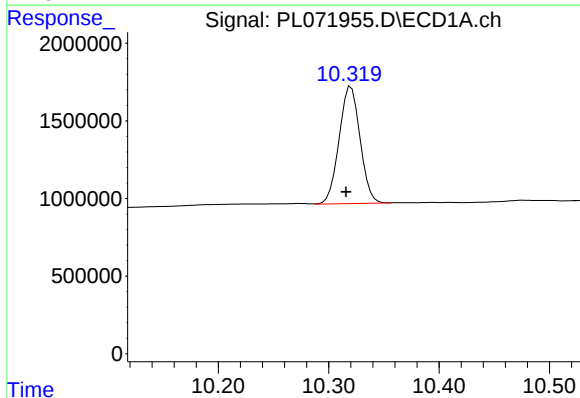

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: 0.004 min
Response: 9925407
Conc: 13.73 ng/ml

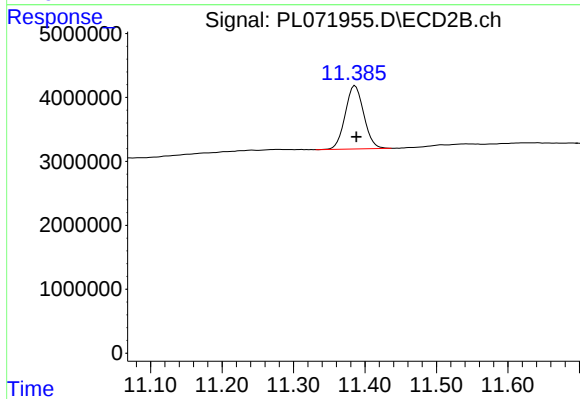

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.002 min
Response: 17827842
Conc: 15.04 ng/ml