

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
 Data File : PL071958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 18:18
 Operator : AR\AJ
 Sample : N1099-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:14:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.493	5502932	15132105	11.912	12.316
28)	SA Decachlor...	10.320	11.388	8745003	14929687	12.095	12.599
Target Compounds							
7)	B delta-BHC	0.000	7.020f	0	613010	N.D.	0.399 #
10)	B gamma-Chl...	0.000	8.242f	0	341035	N.D.	0.249 #
15)	B Endosulfa...	0.000	9.147f	0	664452	N.D.	0.592 #
17)	MA 4,4'-DDT	0.000	9.342	0	53394	N.D.	0.057 #
19)	B Endosulfa...	0.000	9.517f	0	81137	N.D.	0.078 #
20)	A Methoxychlor	0.000	9.867f	0	89985	N.D.	0.183 #
21)	B Endrin ke...	0.000	9.993	0	542516	N.D.	0.481 #
25)	Chlordane-3	0.000	8.242f	0	341035	N.D.	1.671 #
27)	Chlordane-5	0.000	9.191	0	44132	N.D.	1.102 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
Data File : PL071958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 18:18
Operator : AR\AJ
Sample : N1099-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:14:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

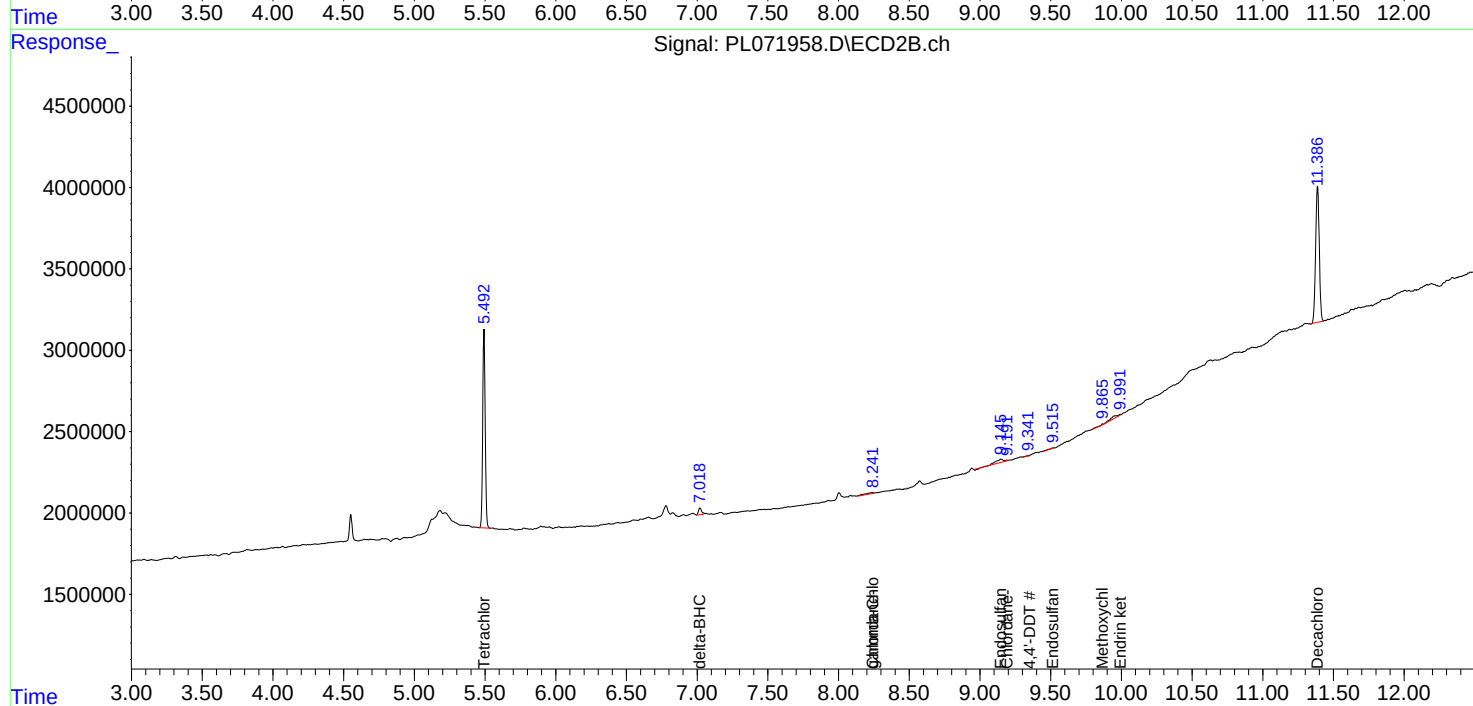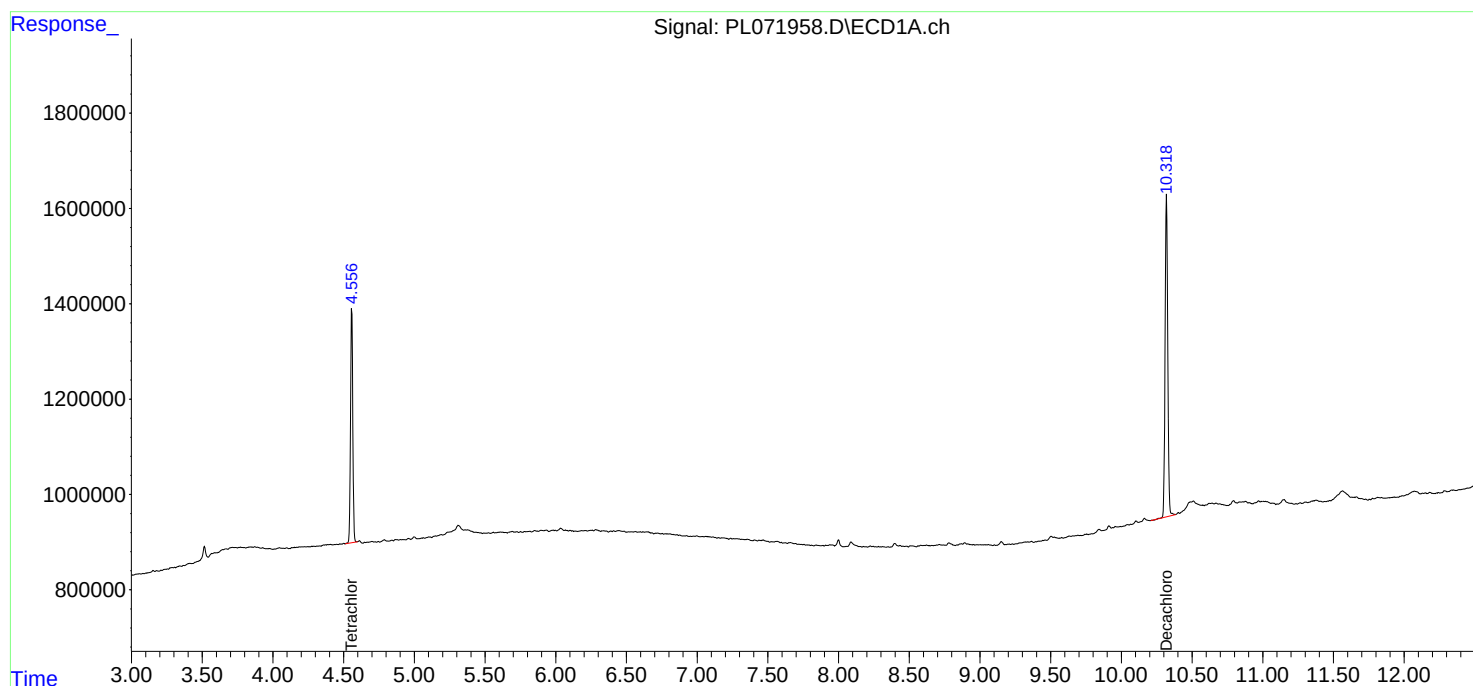


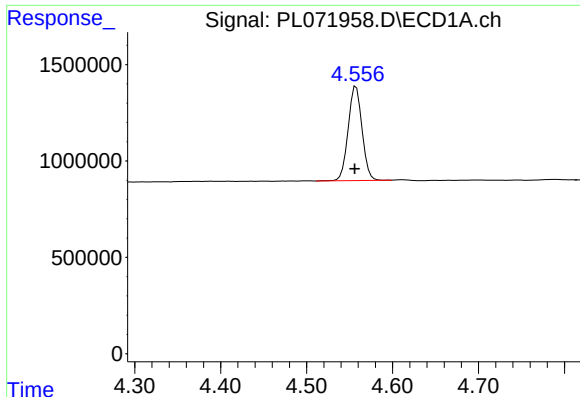

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 5502932
Conc: 11.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

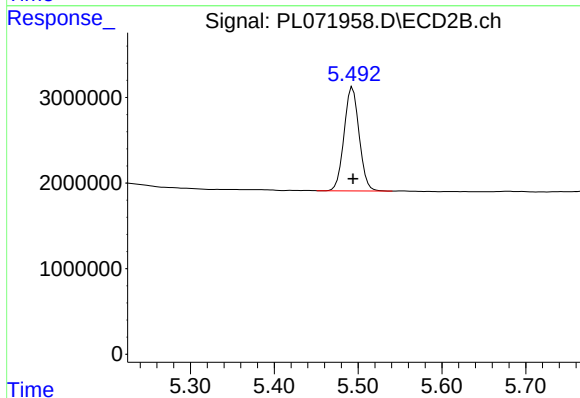


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 15132105
Conc: 12.32 ng/ml

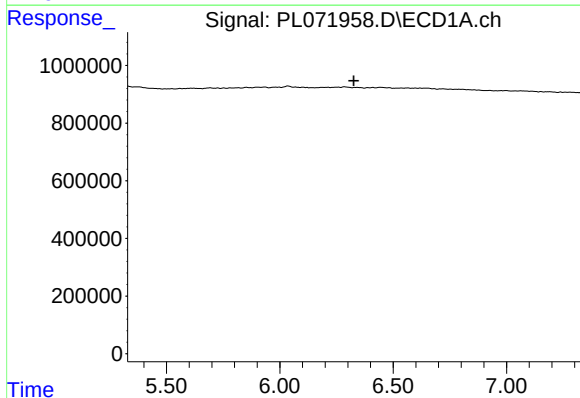


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

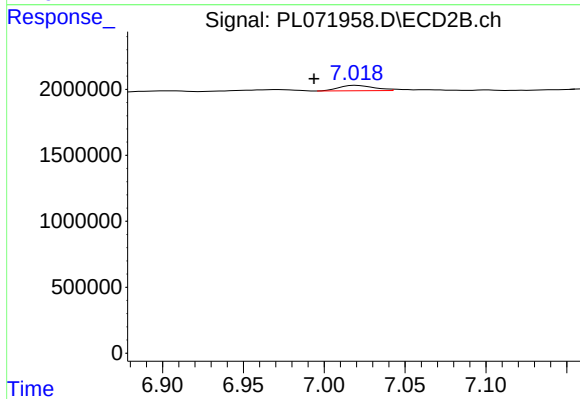

#7 delta-BHC


R.T.: 7.020 min
Delta R.T.: 0.026 min
Response: 613010
Conc: 0.40 ng/ml

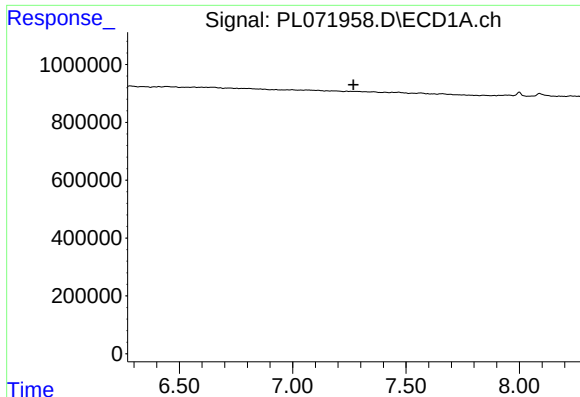

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

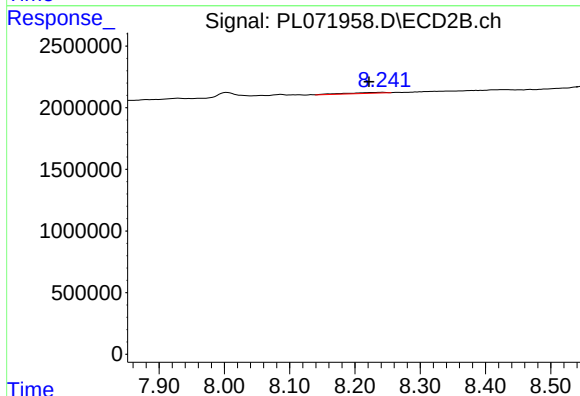


#10 gamma-Chlordane

R.T.: 8.242 min
Delta R.T.: 0.021 min
Response: 341035
Conc: 0.25 ng/ml

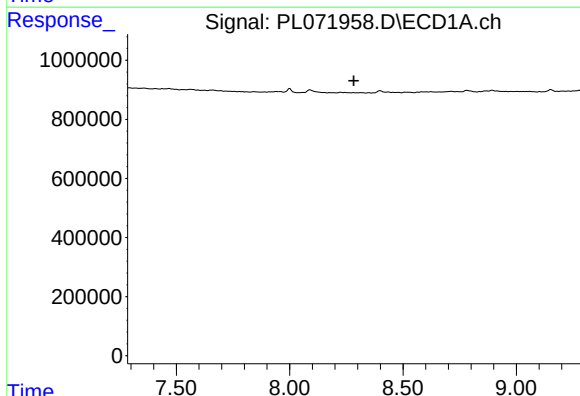


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

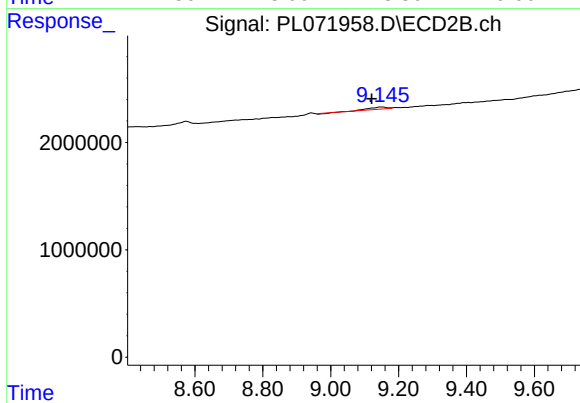

#15 Endosulfan II


R.T.: 9.147 min
Delta R.T.: 0.026 min
Response: 664452
Conc: 0.59 ng/ml

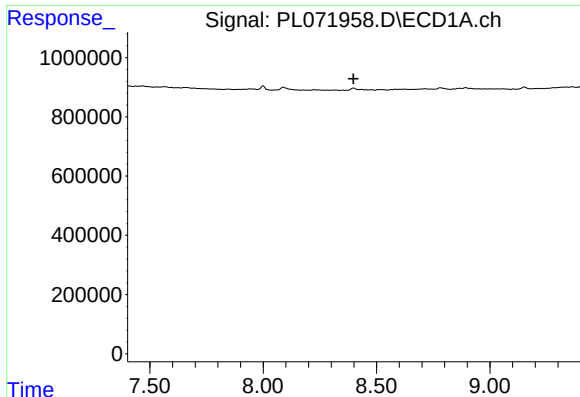

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

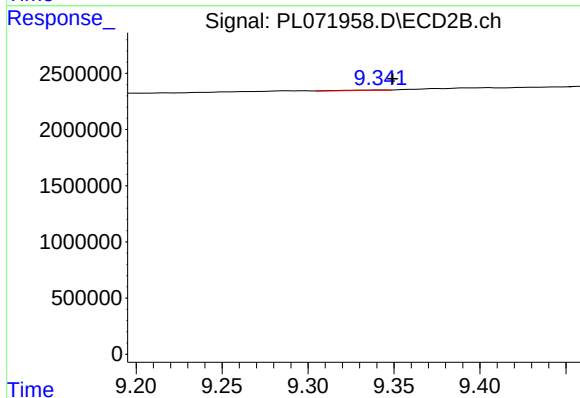


#17 4,4'-DDT

R.T.: 9.342 min
Delta R.T.: -0.007 min
Response: 53394
Conc: 0.06 ng/ml

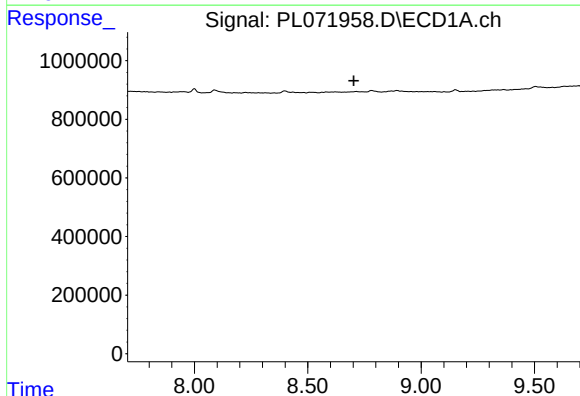


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

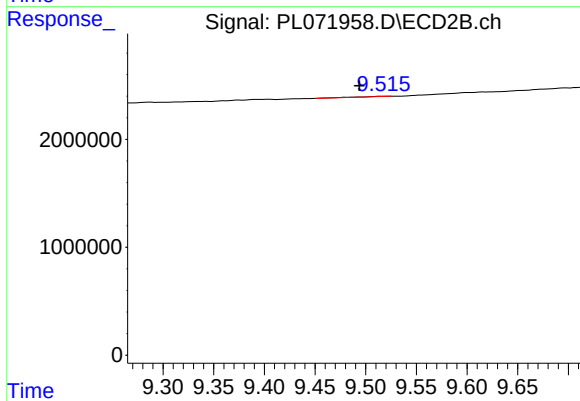

#19 Endosulfan Sulfate


R.T.: 9.517 min
Delta R.T.: 0.024 min
Response: 81137
Conc: 0.08 ng/ml

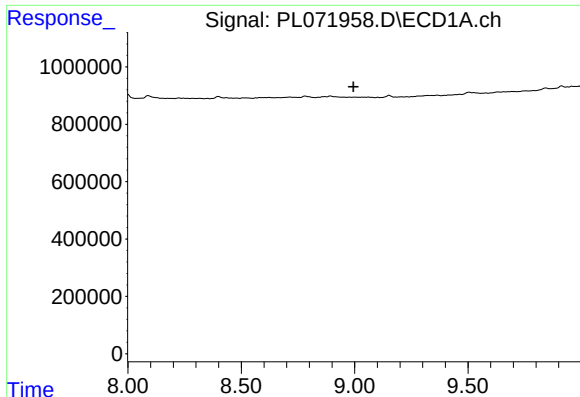

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 8.995 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

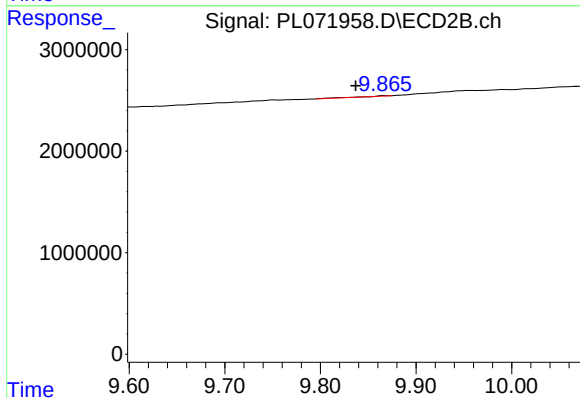


#20 Methoxychlor

R.T.: 9.867 min
Delta R.T.: 0.030 min
Response: 89985
Conc: 0.18 ng/ml

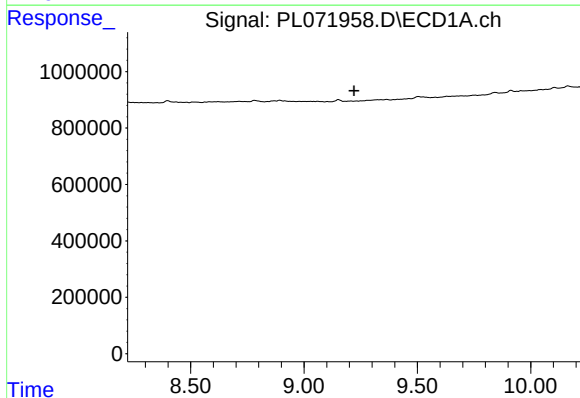


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

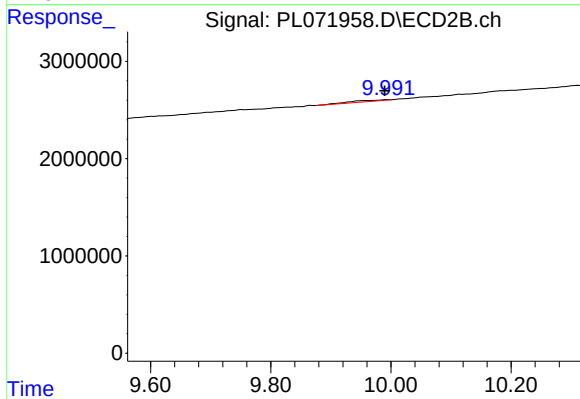

#21 Endrin ketone


R.T.: 9.993 min
Delta R.T.: 0.003 min
Response: 542516
Conc: 0.48 ng/ml

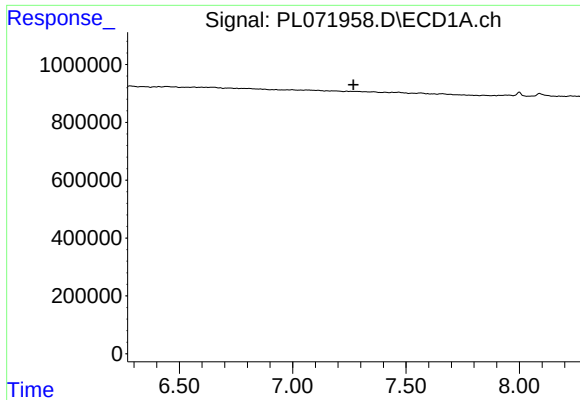

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

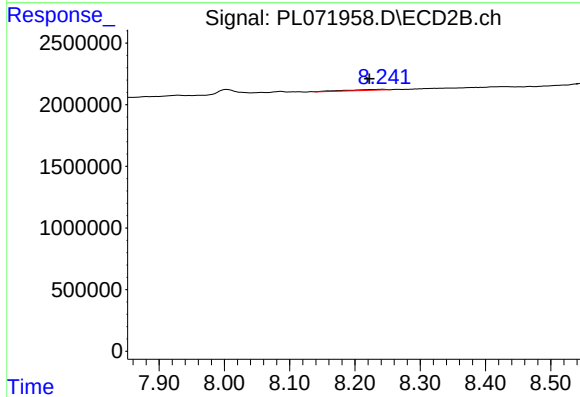


#25 Chlordane-3

R.T.: 8.242 min
Delta R.T.: 0.020 min
Response: 341035
Conc: 1.67 ng/ml

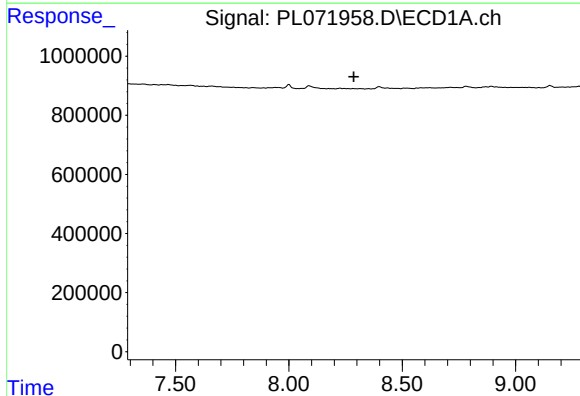


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

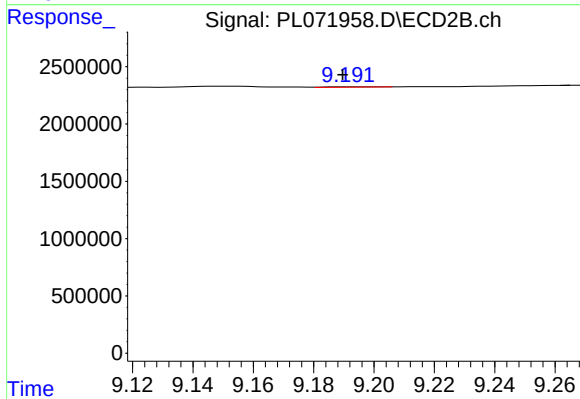

#27 Chlordane-5


R.T.: 9.191 min
Delta R.T.: 0.002 min
Response: 44132
Conc: 1.10 ng/ml

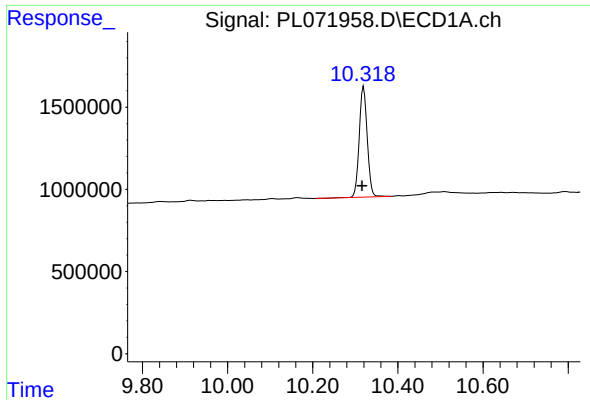

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: 0.004 min
Response: 8745003
Conc: 12.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

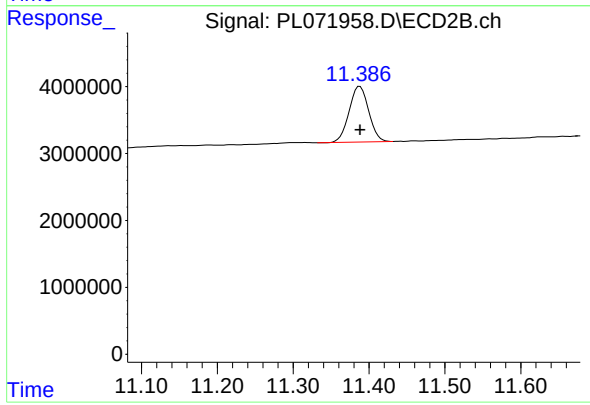

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.000 min
Response: 14929687
Conc: 12.60 ng/ml