

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
 Data File : PL071967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 20:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:17:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.494	9847353	26600044	21.317	21.650
28)	SA Decachlor...	10.320	11.388	13688048	24069229	18.932	20.311
Target Compounds							
7)	B delta-BHC	0.000	6.972f	0	279646	N.D.	0.182 #
9)	A Endosulfan I	0.000	8.339f	0	65950	N.D.	0.053 #
10)	B gamma-Chl...	0.000	8.229	0	1022358	N.D.	0.748 #
11)	B alpha-Chl...	0.000	8.305	0	238347	N.D.	0.179 #
15)	B Endosulfa...	0.000	9.146f	0	3192567	N.D.	2.843 #
21)	B Endrin ke...	0.000	9.983	0	562996	N.D.	0.499 #
25)	Chlordane-3	0.000	8.229	0	1022358	N.D.	5.009 #
26)	Chlordane-4	0.000	8.305	0	238347	N.D.	0.979 #
27)	Chlordane-5	0.000	9.207f	0	118129	N.D.	2.950 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
Data File : PL071967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 20:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:17:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

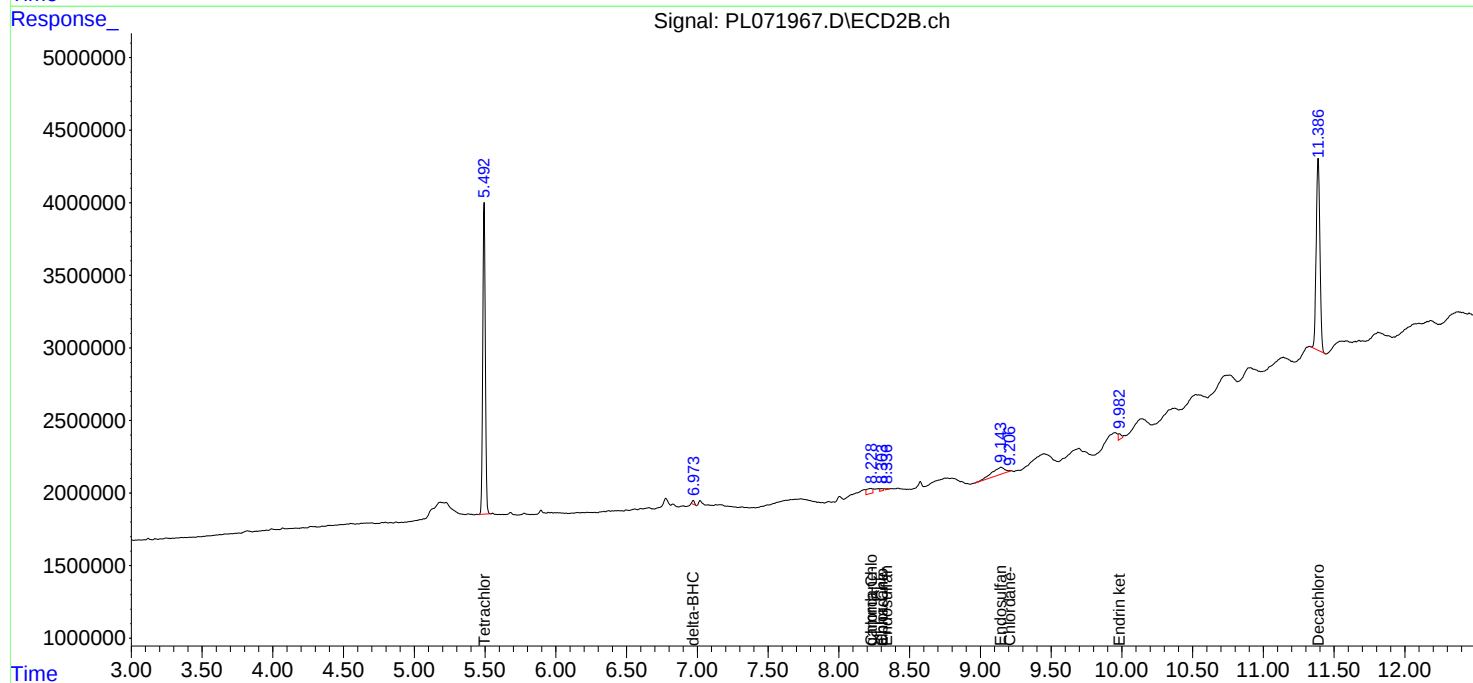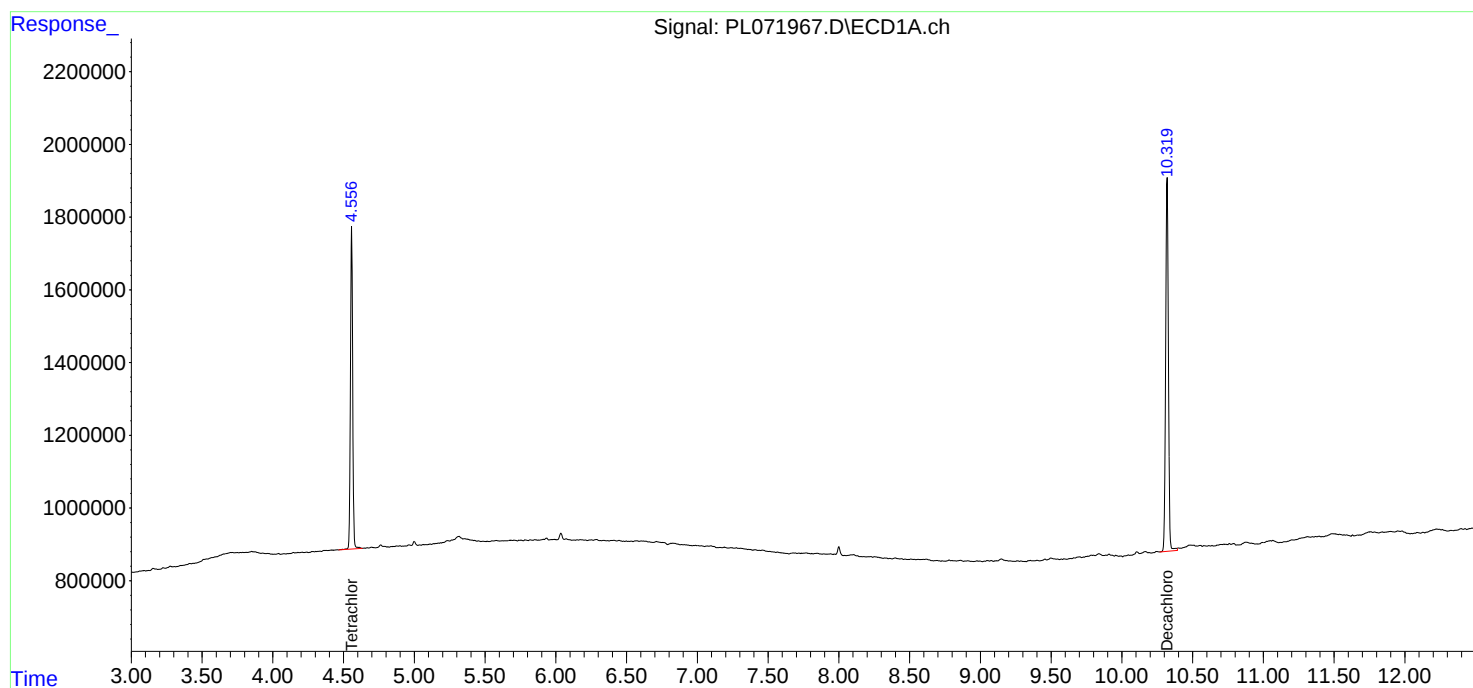


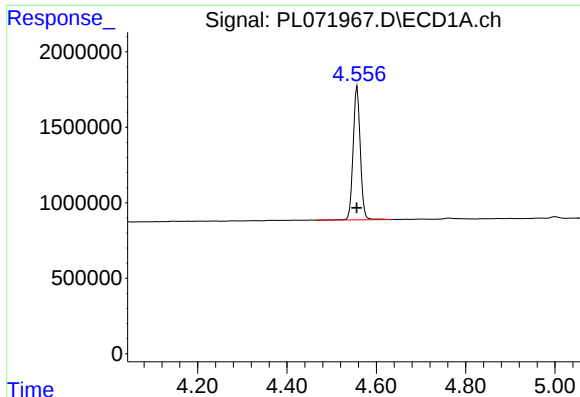

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 9847353
Conc: 21.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

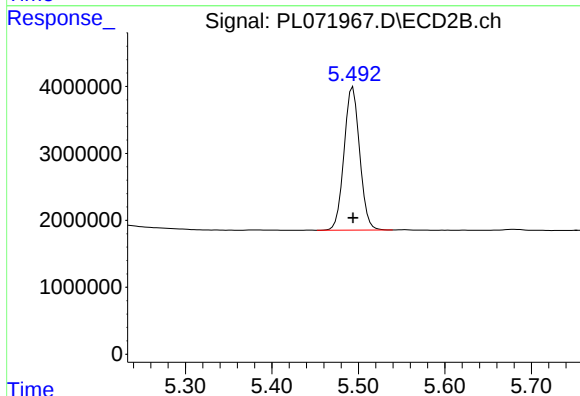


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 26600044
Conc: 21.65 ng/ml

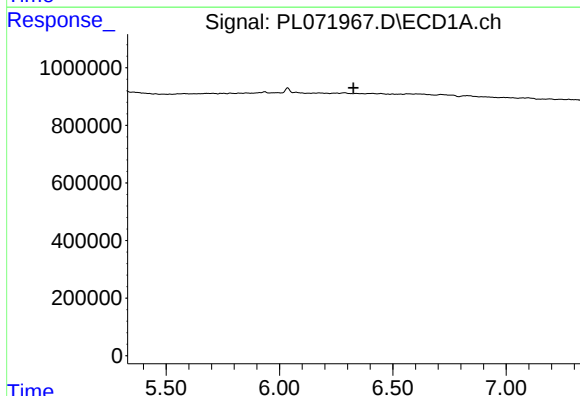


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

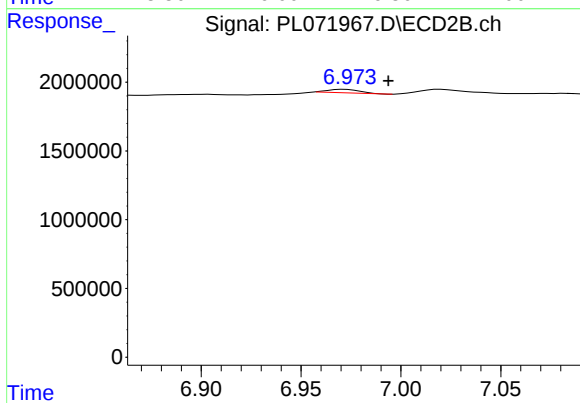

#7 delta-BHC


R.T.: 6.972 min
Delta R.T.: -0.022 min
Response: 279646
Conc: 0.18 ng/ml

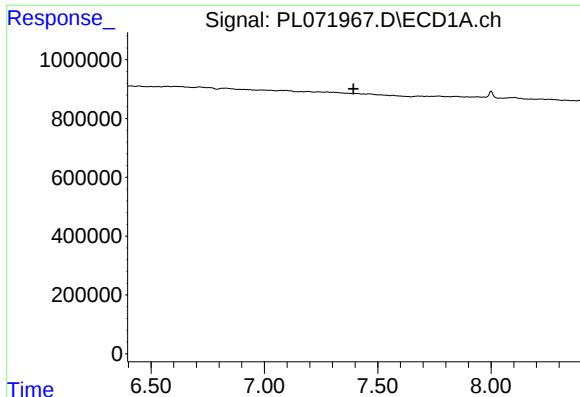

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

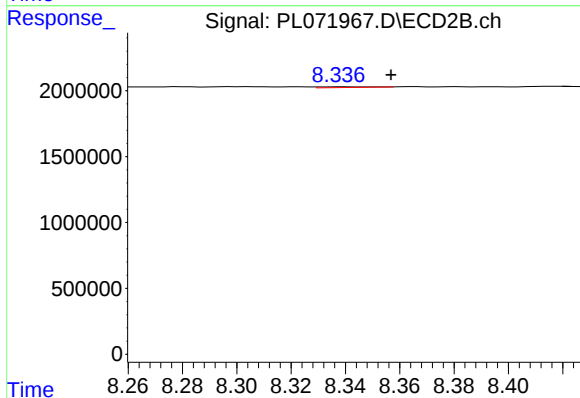


#9 Endosulfan I

R.T.: 8.339 min
Delta R.T.: -0.018 min
Response: 65950
Conc: 0.05 ng/ml

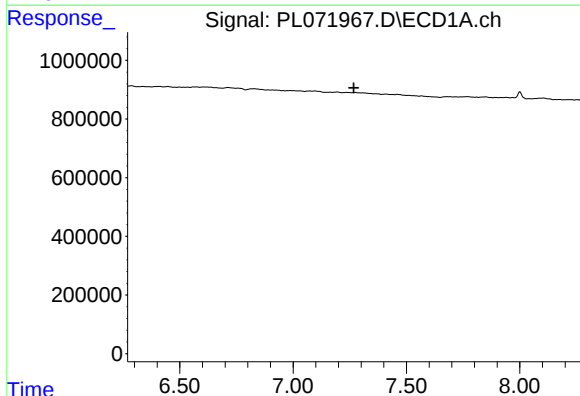


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

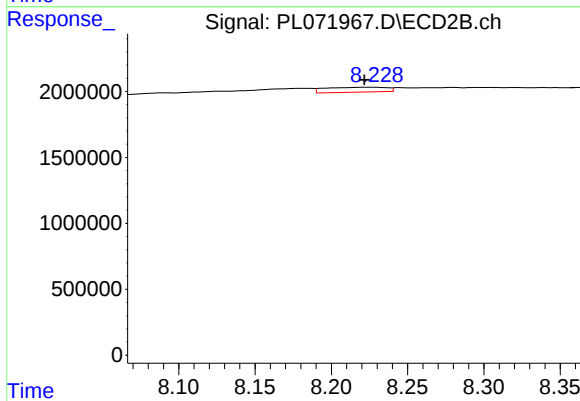

#10 gamma-Chlordane


R.T.: 8.229 min
Delta R.T.: 0.007 min
Response: 1022358
Conc: 0.75 ng/ml

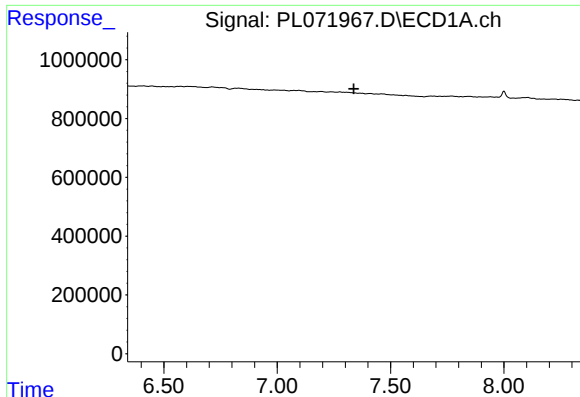

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

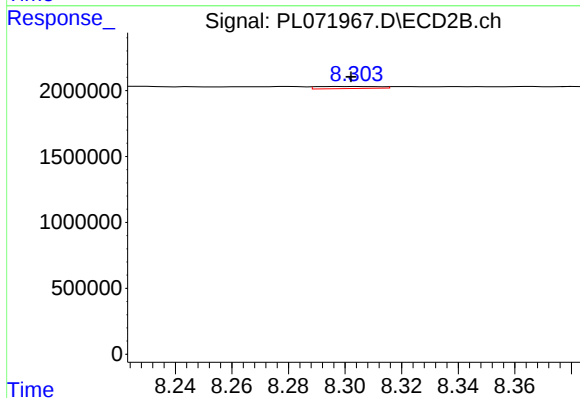


#11 alpha-Chlordane

R.T.: 8.305 min
Delta R.T.: 0.003 min
Response: 238347
Conc: 0.18 ng/ml

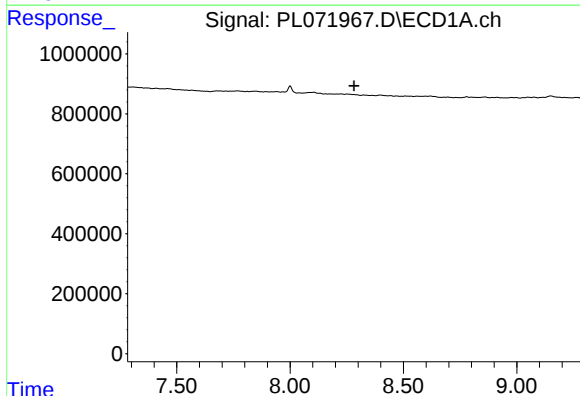


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

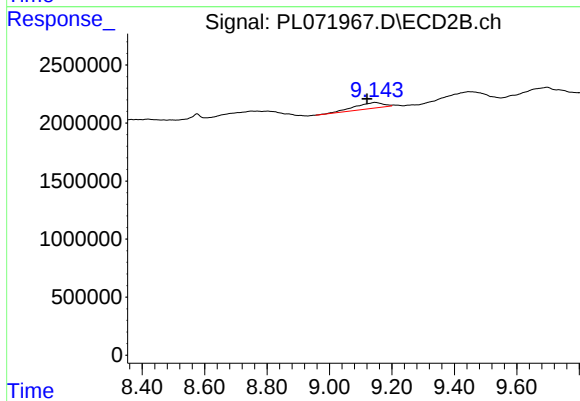

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.025 min
Response: 3192567
Conc: 2.84 ng/ml

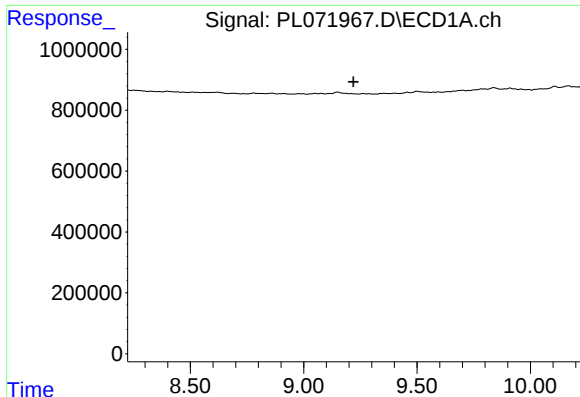

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

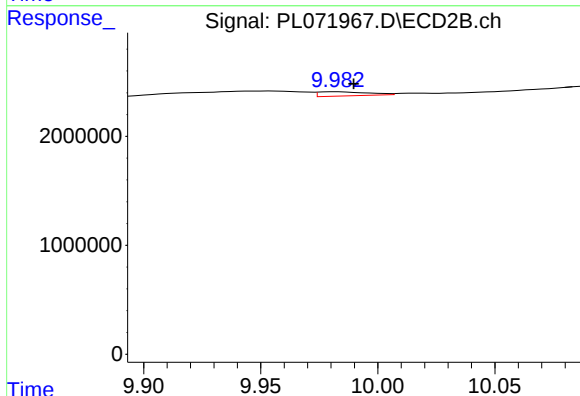


#21 Endrin ketone

R.T.: 9.983 min
Delta R.T.: -0.007 min
Response: 562996
Conc: 0.50 ng/ml

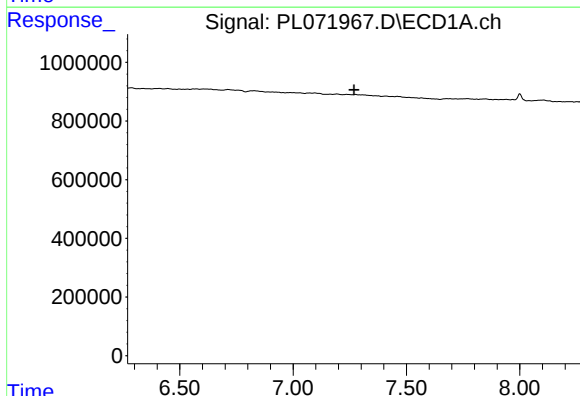


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

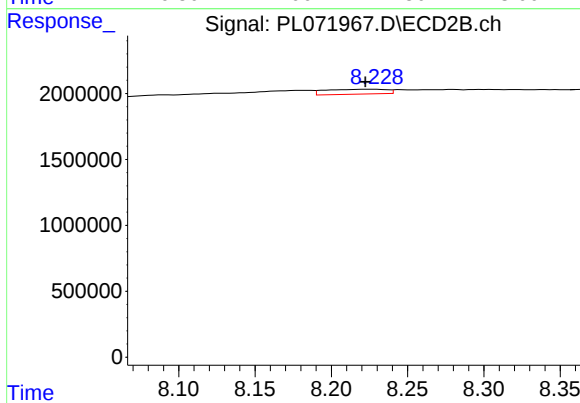

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.006 min
Response: 1022358
Conc: 5.01 ng/ml

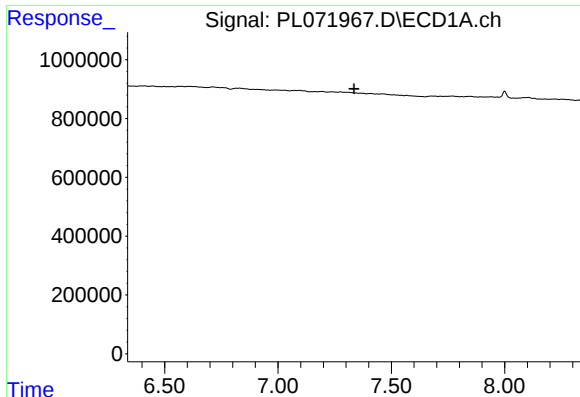

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 7.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

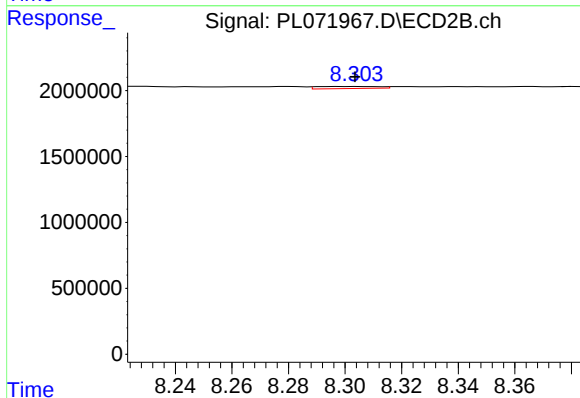


#26 Chlordane-4

R.T.: 8.305 min
Delta R.T.: 0.001 min
Response: 238347
Conc: 0.98 ng/ml

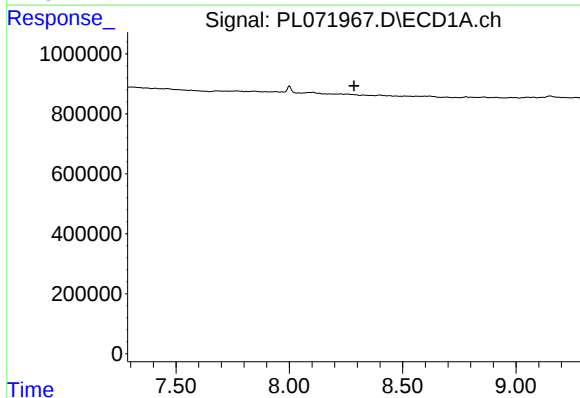


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

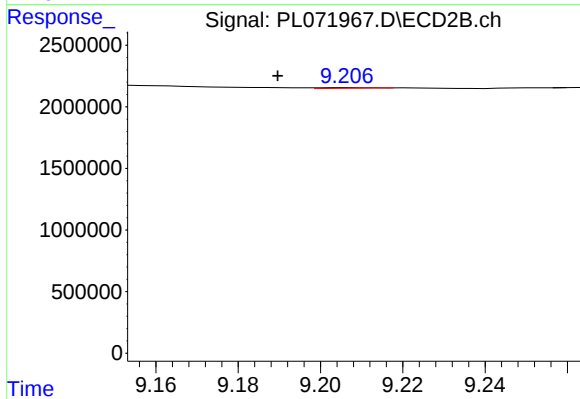

#27 Chlordane-5


R.T.: 9.207 min
Delta R.T.: 0.017 min
Response: 118129
Conc: 2.95 ng/ml

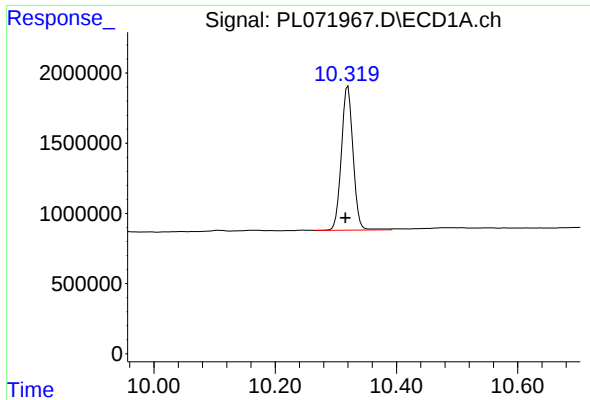

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: 0.004 min
Response: 13688048
Conc: 18.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

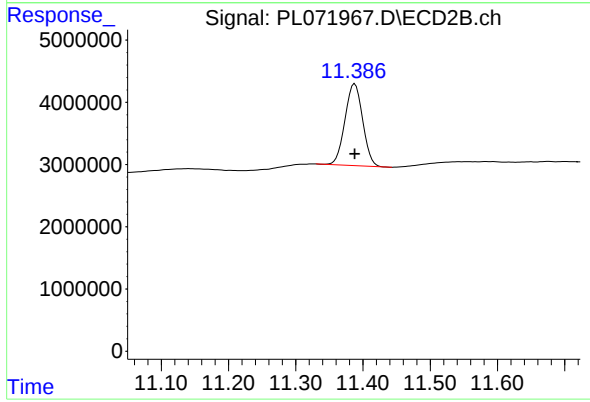

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.000 min
Response: 24069229
Conc: 20.31 ng/ml