

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
 Data File : PL071954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 17:13
 Operator : AR\AJ
 Sample : N1099-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/13/2022
 Supervised By : Ankita Jodhani 01/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:13:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.557	5.493	6310173	17495463	13.660	14.240
28) SA Decachlor...	10.319	11.386	10816522	18790512	14.960m	15.857

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011222\
Data File : PL071954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 17:13
Operator : AR\AJ
Sample : N1099-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/13/2022
Supervised By : Ankita Jodhani 01/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:13:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

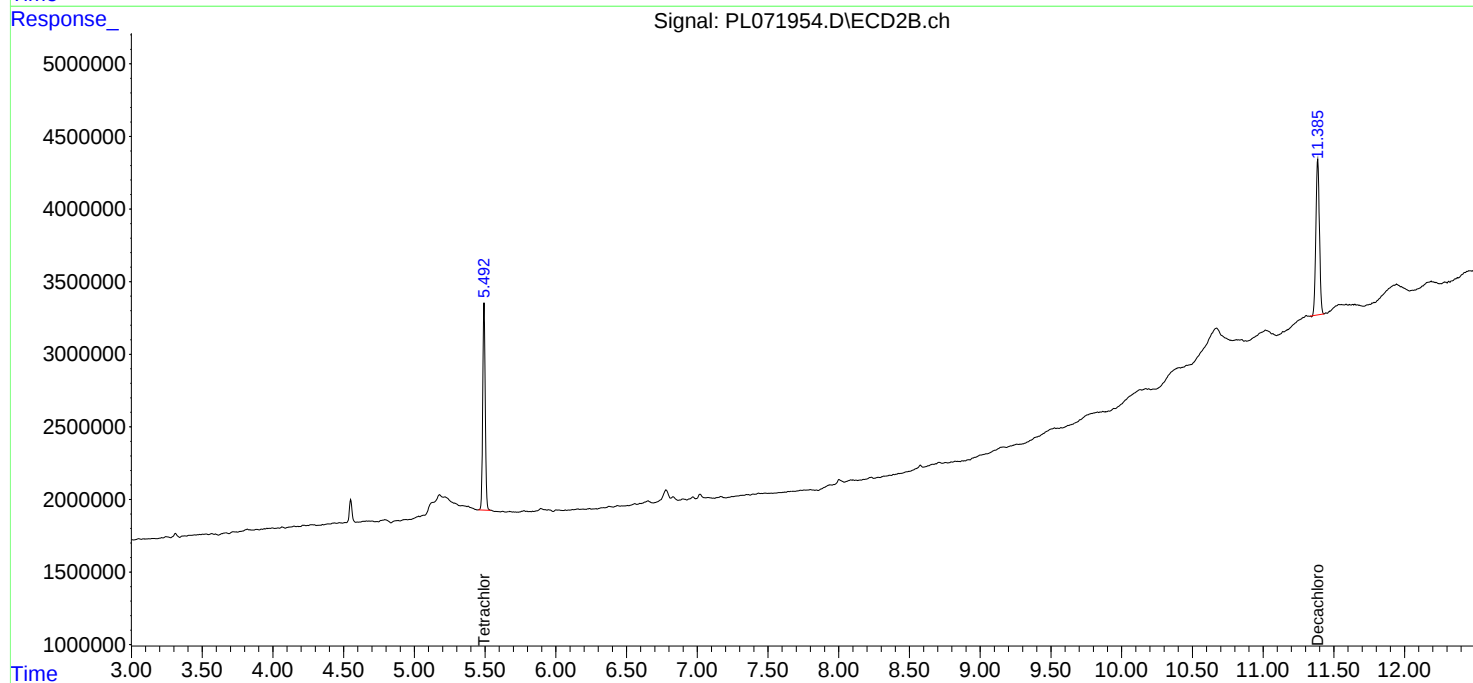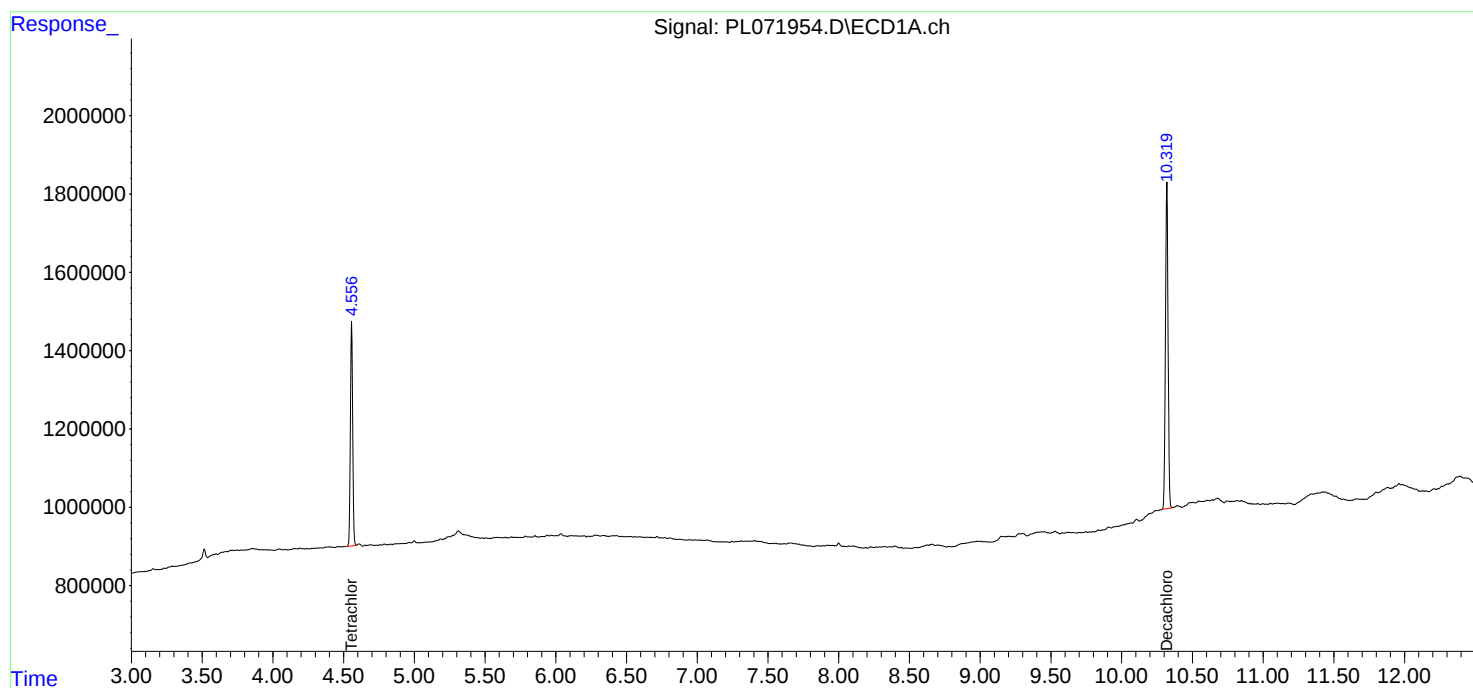

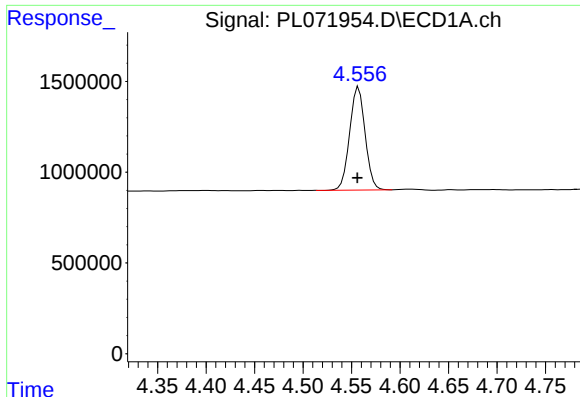


#1 Tetrachloro-m-xylene

R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 6310173
Conc: 13.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/13/2022
Supervised By :Ankita Jodhani 01/13/2022

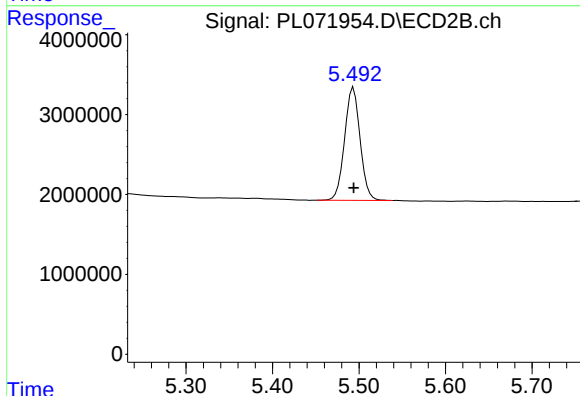


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 17495463
Conc: 14.24 ng/ml

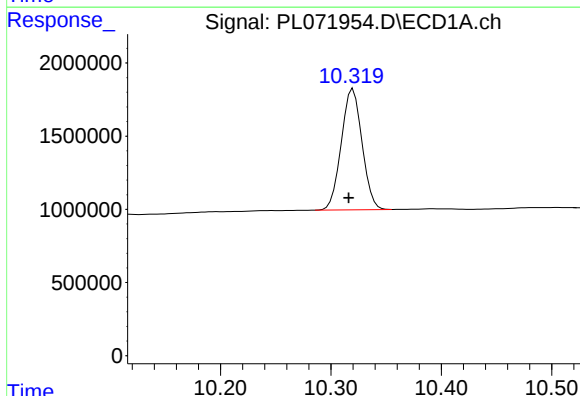

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: 0.003 min
Response: 10816522
Conc: 14.96 ng/ml m

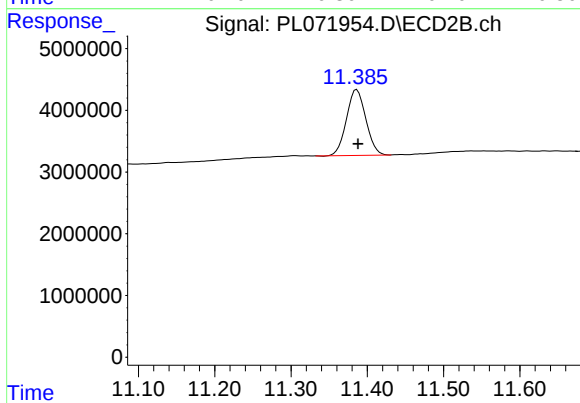

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.002 min
Response: 18790512
Conc: 15.86 ng/ml