

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
 Data File : PL080243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2023 20:54
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 01:48:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 01:47:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.691	45325064	50739390	22.689	22.686
28)	SA Decachlor...	8.787	7.841	32500607	50258139	22.028	22.358
Target Compounds							
9)	A Endosulfan I	5.856	5.014	21645998	27521650	10.685	10.527
10)	B gamma-Chl...	5.729	4.895	23342017	30314387	10.662	10.610
12)	B 4,4'-DDE	5.986	5.152	40685066	49042786	20.976	20.887
13)	MA Dieldrin	6.130	5.279	44108918	58040857	21.466	21.296
19)	B Endosulfa...	6.939	6.250	35145642	46616872	20.164	20.081
20)	A Methoxychlor	7.290	6.536	95556550	126.8E6	107.252	105.451
21)	B Endrin ke...	7.419	6.755	40655938	54213095	21.822	21.531



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011223\
Data File : PL080243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2023 20:54
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 01:48:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 01:47:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

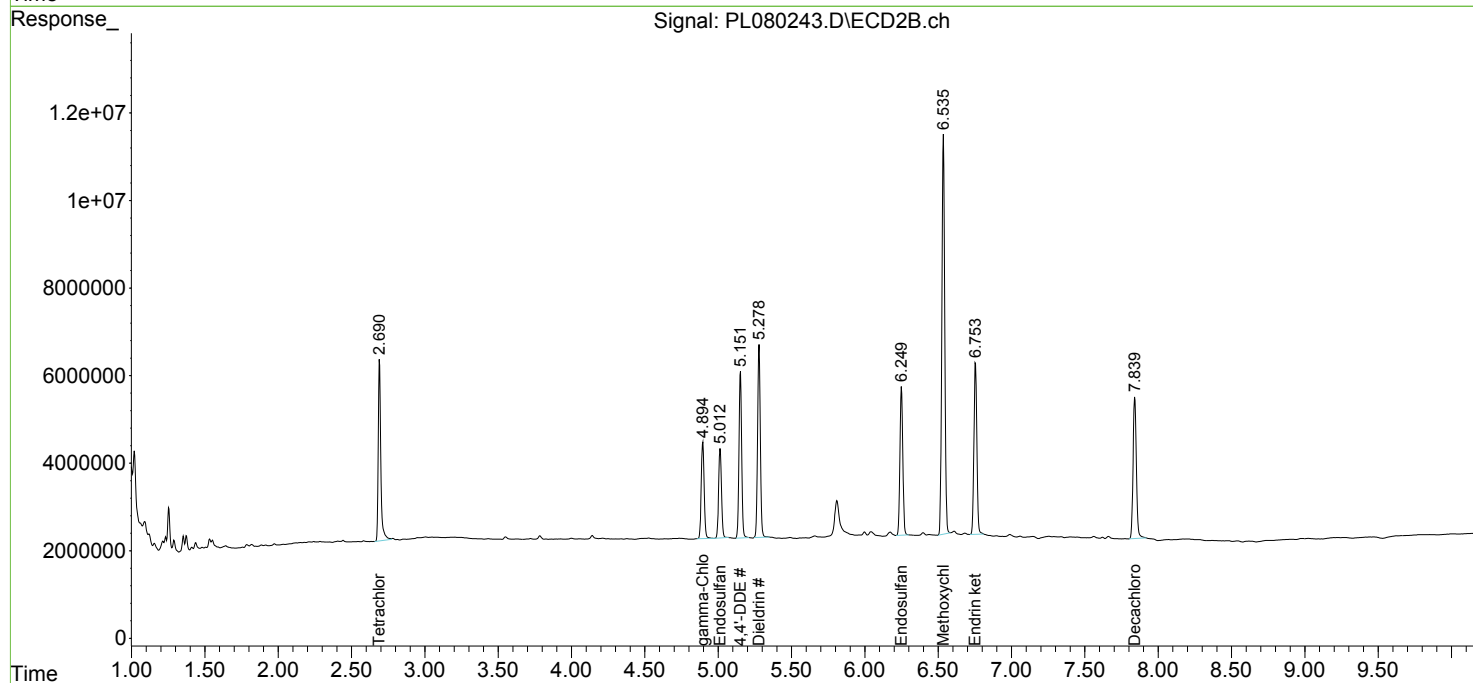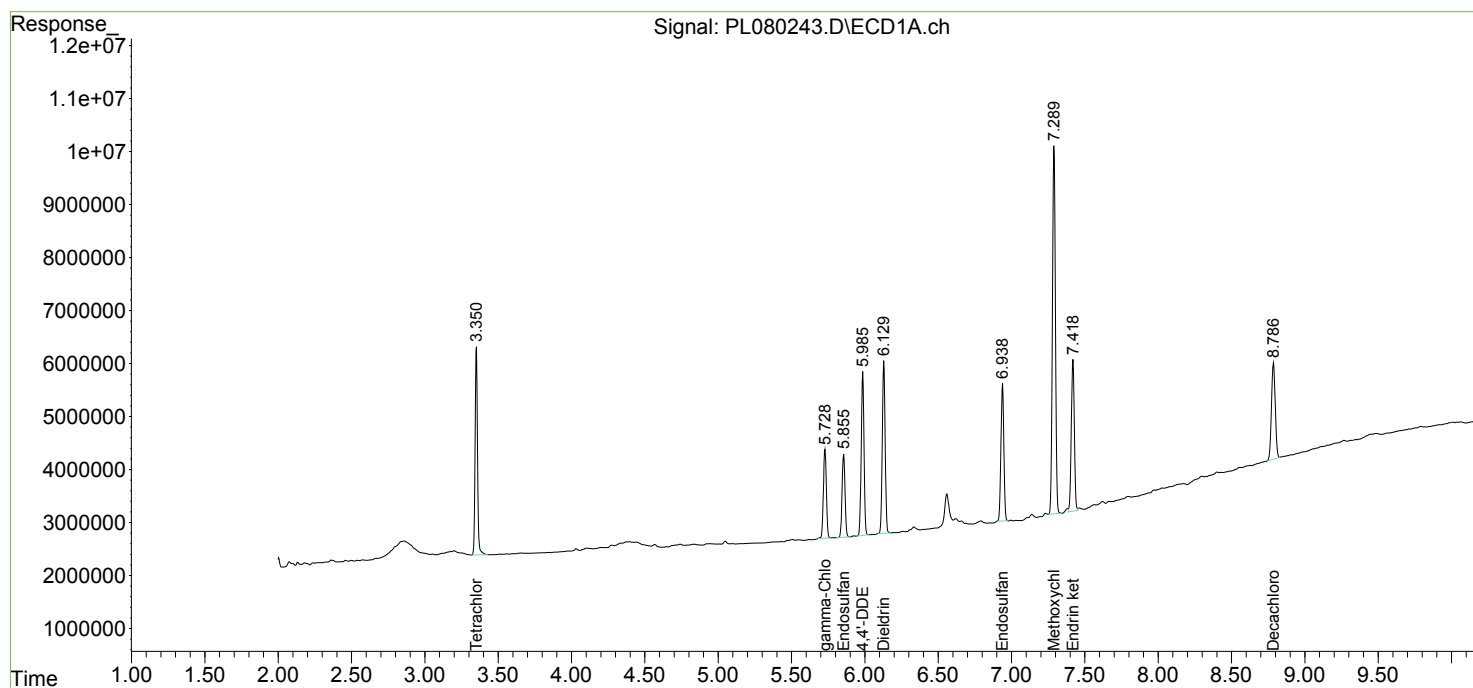


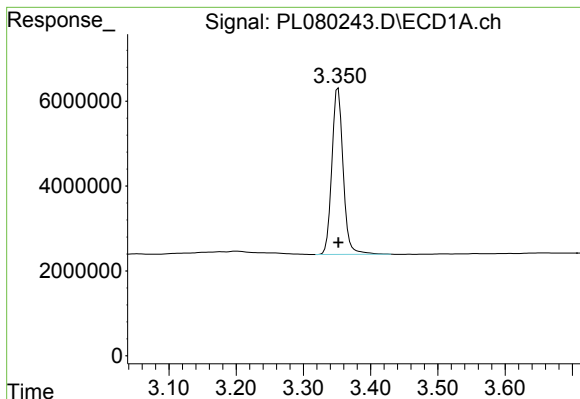

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 45325064
Conc: 22.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

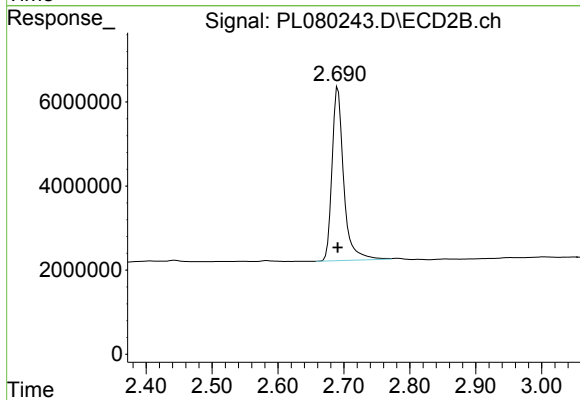


#1 Tetrachloro-m-xylene

R.T.: 2.691 min
Delta R.T.: 0.000 min
Response: 50739390
Conc: 22.69 ng/ml

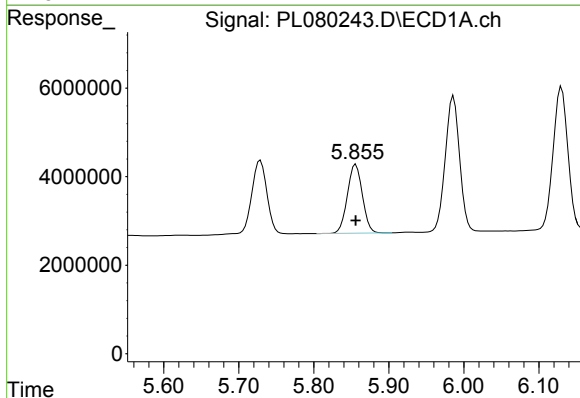


#9 Endosulfan I

R.T.: 5.856 min
Delta R.T.: 0.000 min
Response: 21645998
Conc: 10.69 ng/ml

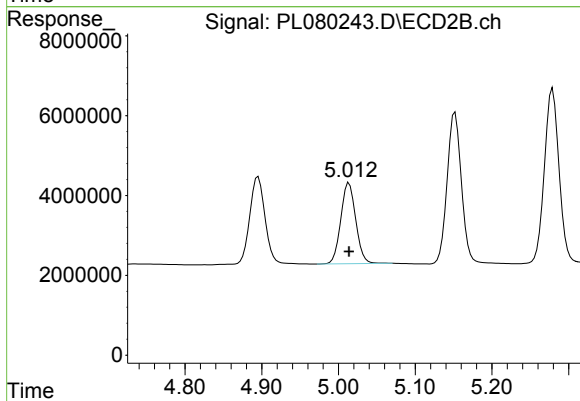

#9 Endosulfan I


R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 27521650
Conc: 10.53 ng/ml

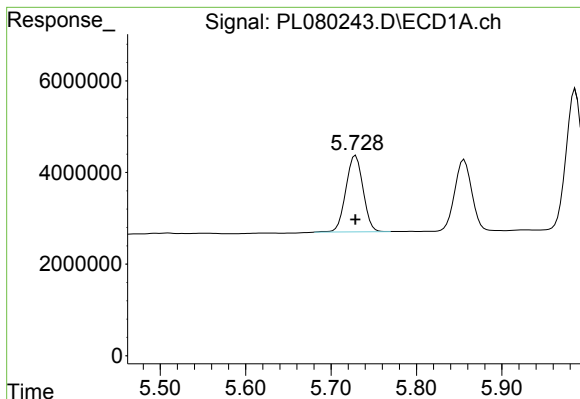

#10 gamma-Chlordane


R.T.: 5.729 min
Delta R.T.: 0.000 min
Response: 23342017
Conc: 10.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

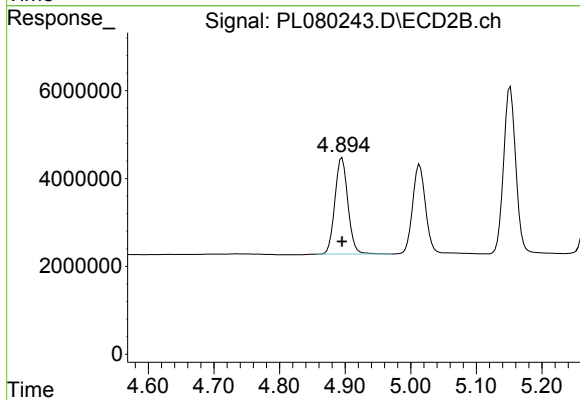


#10 gamma-Chlordane

R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 30314387
Conc: 10.61 ng/ml

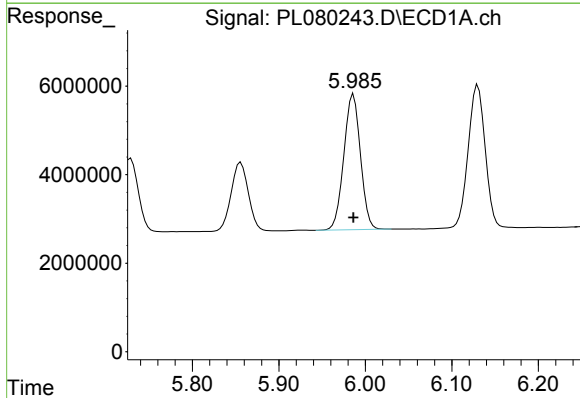


#12 4,4'-DDE

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 40685066
Conc: 20.98 ng/ml

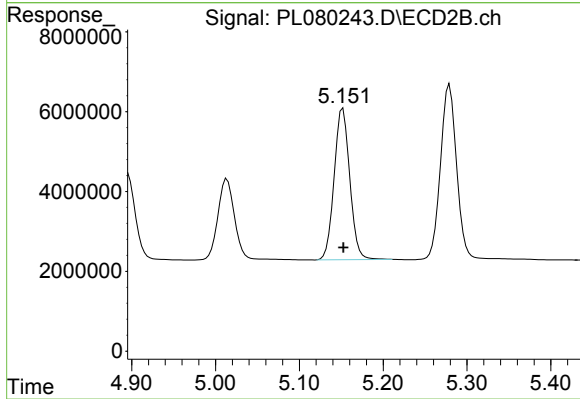

#12 4,4'-DDE


R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 49042786
Conc: 20.89 ng/ml

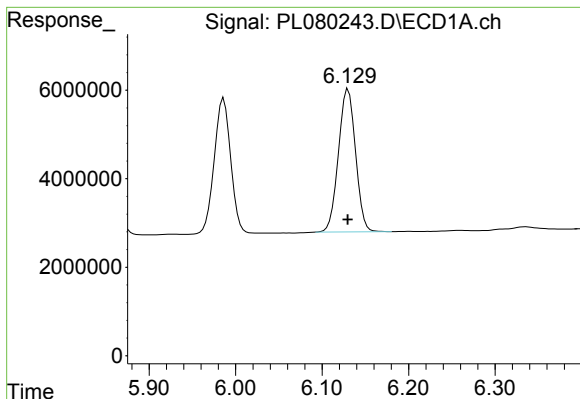

#13 Dieldrin


R.T.: 6.130 min
Delta R.T.: 0.000 min
Response: 44108918
Conc: 21.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

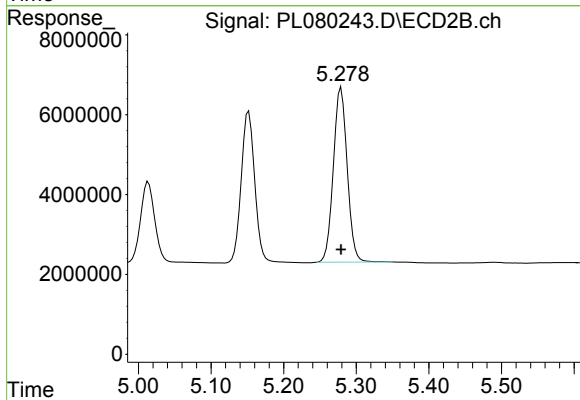


#13 Dieldrin

R.T.: 5.279 min
Delta R.T.: 0.000 min
Response: 58040857
Conc: 21.30 ng/ml

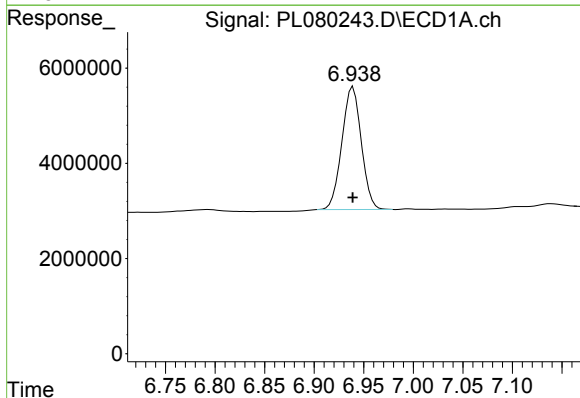


#19 Endosulfan Sulfate

R.T.: 6.939 min
Delta R.T.: 0.000 min
Response: 35145642
Conc: 20.16 ng/ml

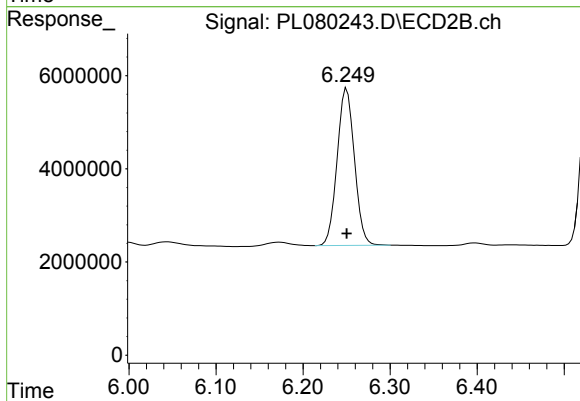

#19 Endosulfan Sulfate


R.T.: 6.250 min
Delta R.T.: 0.000 min
Response: 46616872
Conc: 20.08 ng/ml

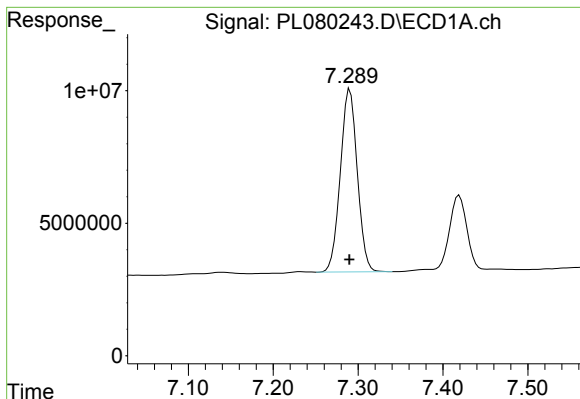

#20 Methoxychlor


R.T.: 7.290 min
Delta R.T.: 0.000 min
Response: 95556550
Conc: 107.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

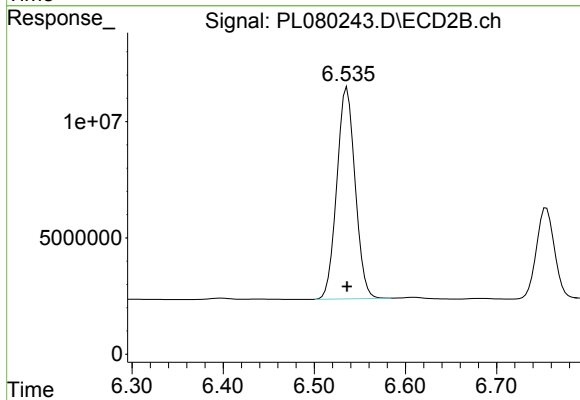


#20 Methoxychlor

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 126752643
Conc: 105.45 ng/ml

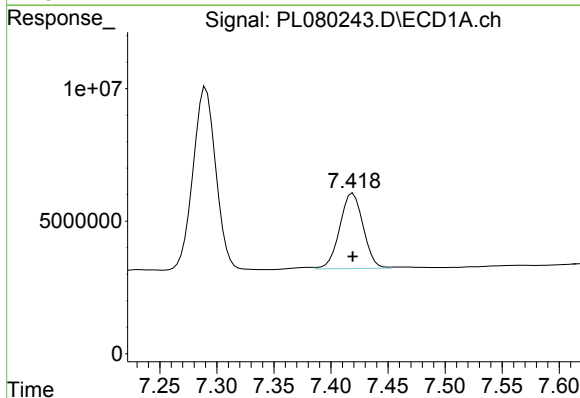


#21 Endrin ketone

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 40655938
Conc: 21.82 ng/ml

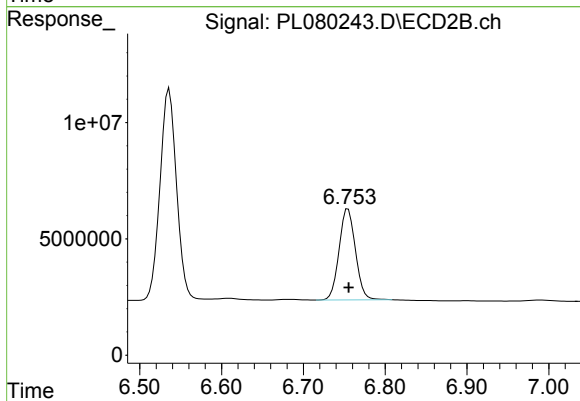

#21 Endrin ketone


R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 54213095
Conc: 21.53 ng/ml

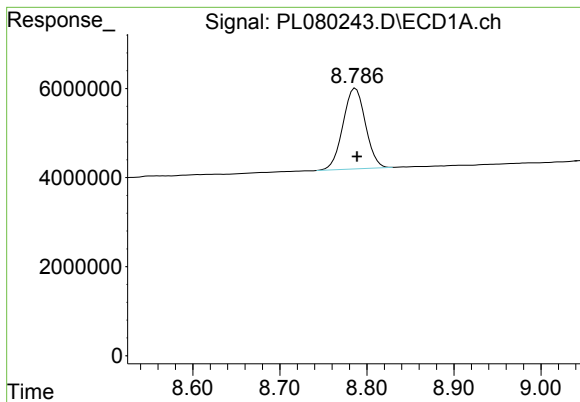

#28 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.002 min
Response: 32500607
Conc: 22.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

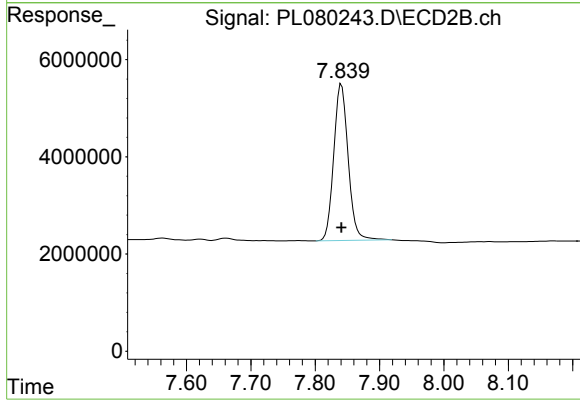

#28 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 50258139
Conc: 22.36 ng/ml